




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011212.D
 Acq On : 01 Aug 2022 22:47
 Operator : CG/JU
 Sample : PB146541BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 02 00:29:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

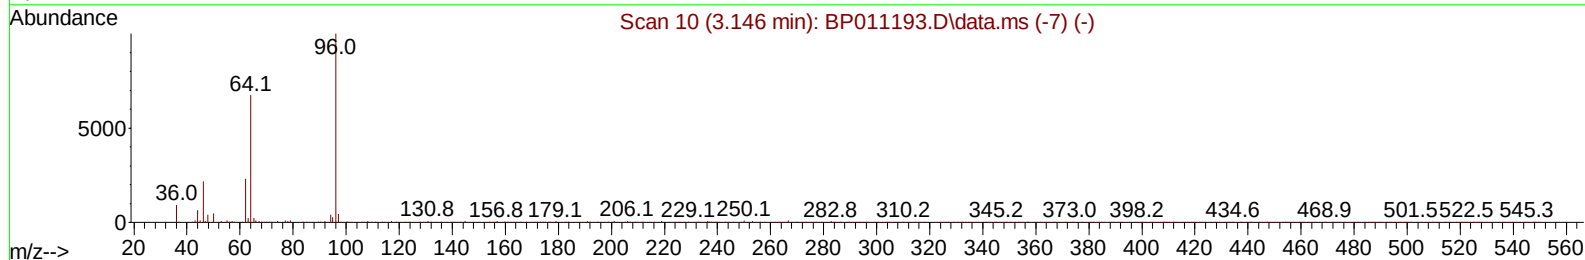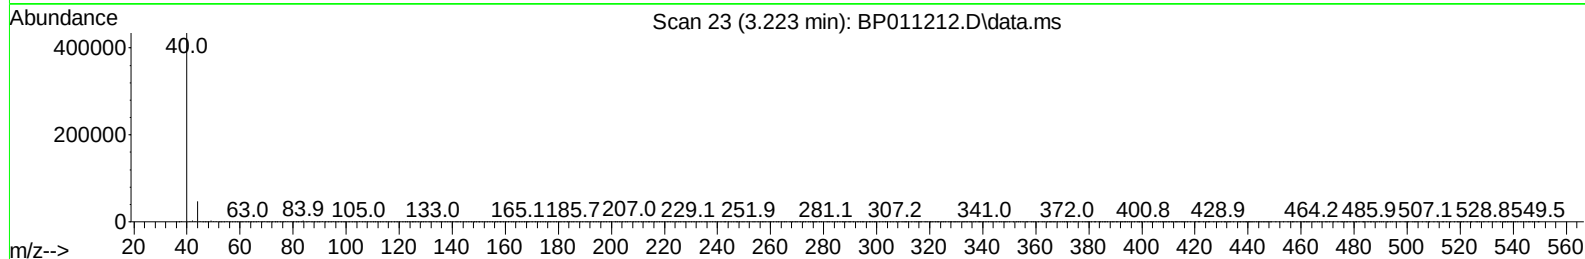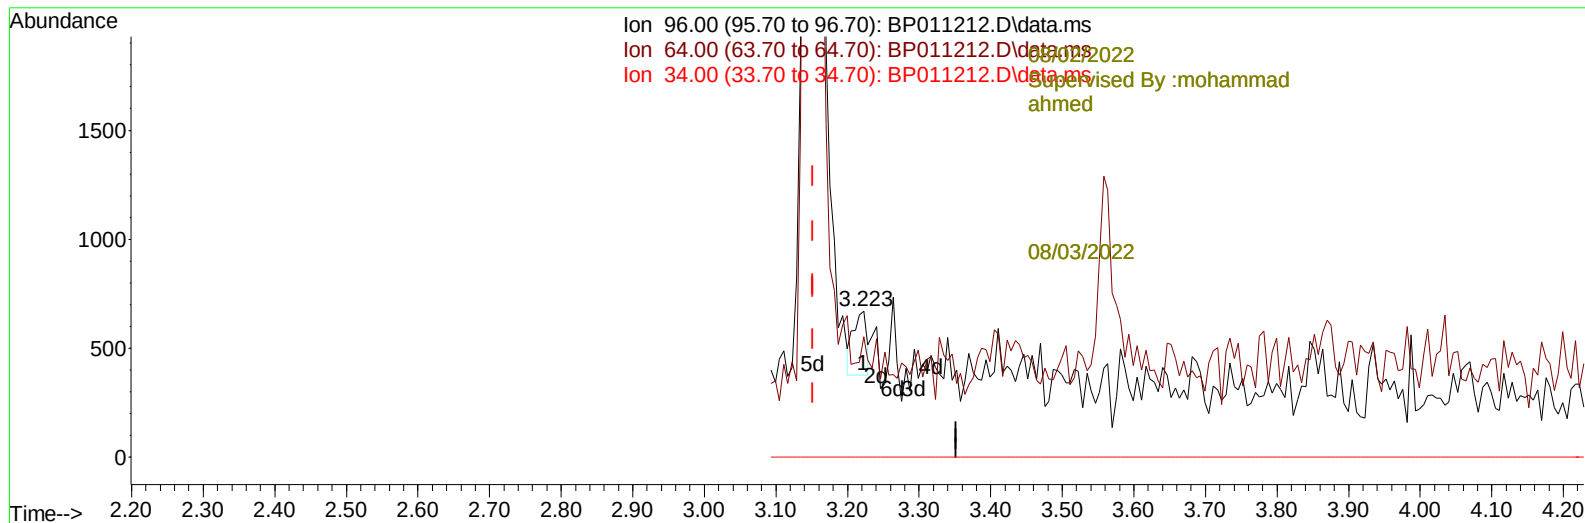

TIC: BP011212.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.223min (+ 0.071) 0.07 ng/uL

response 394

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	82.56
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011212.D
 Acq On : 01 Aug 2022 22:47
 Operator : CG/JU
 Sample : PB146541BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Manual IntegrationsAPPROVED

Quant Time: Aug 02 00:29:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

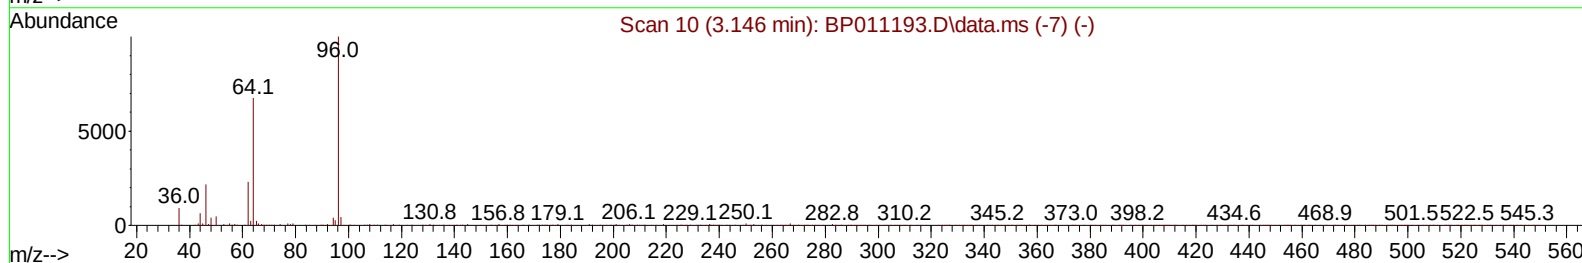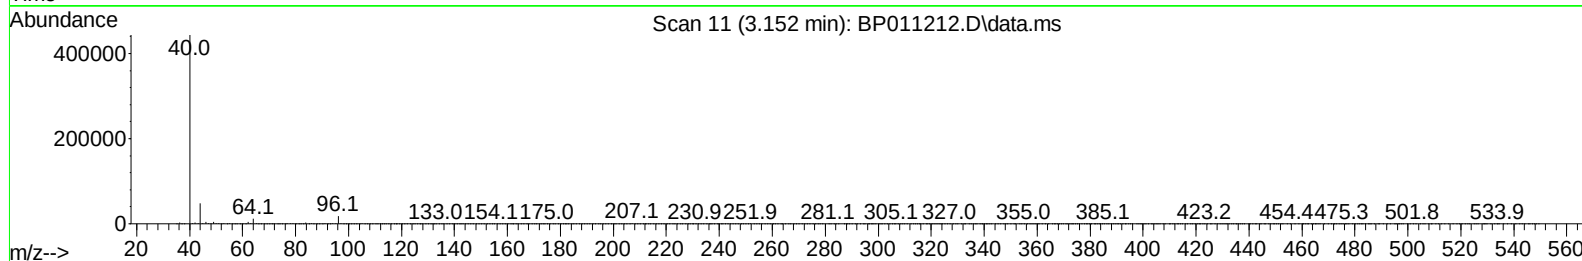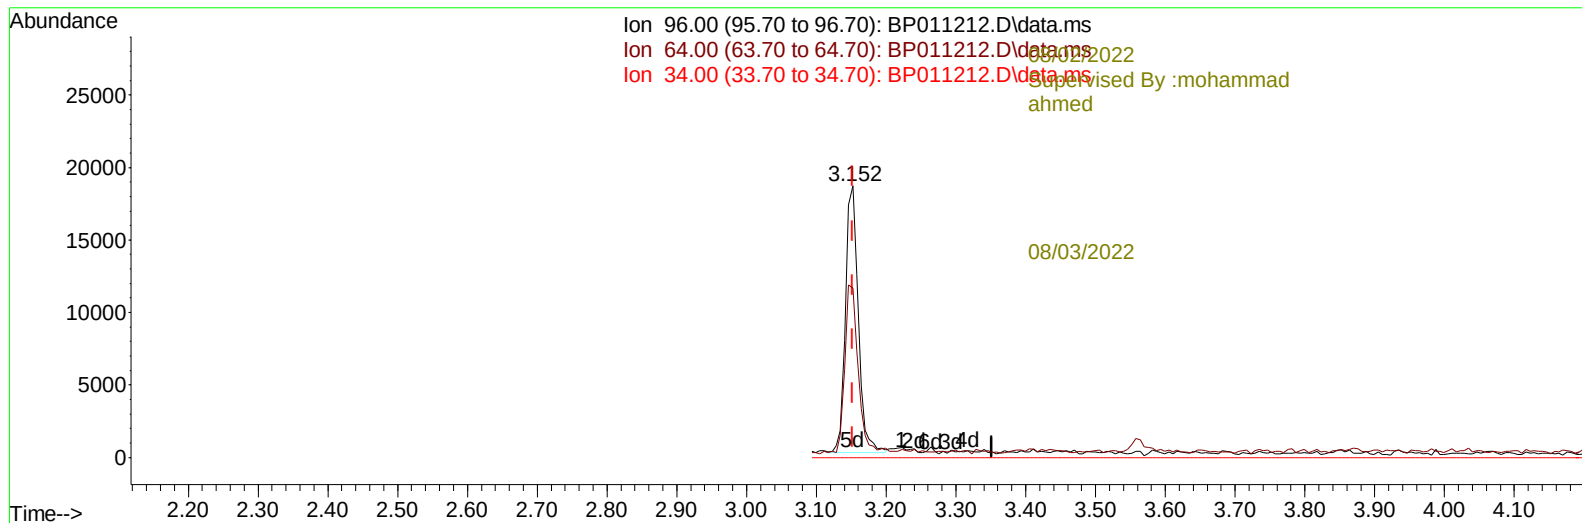

TIC: BP011212.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.152min (+ 0.000) 3.88 ng/uL m

response 23305

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.90	62.46#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011212.D
 Acq On : 01 Aug 2022 22:47
 Operator : CG/JU
 Sample : PB146541BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
 Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 02 00:29:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 28 16:05:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----08/02/2022						
Supervised By :mohammad						
ahmed						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	274862	20.000	ng/ul	0.00
20) Naphthalene-d8	10.440	136	1136953	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	573923	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.087	188	1110943	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.210	240	1094811	20.000	ng/ul	# 0.00
88) Perylene-d12	23.557	264	1172462	20.000	ng/ul	0.0008/03/2022
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	23305m	3.883	ng/uL	0.00
4) Pyridine-d5	3.558	84	326166	19.209	ng/ul	0.00
7) Phenol-d5	6.828	99	714182	29.768	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	498633	29.393	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	583009	30.837	ng/ul	0.00
15) 4-Methylphenol-d8	8.364	113	545474	27.794	ng/ul	0.00
21) Nitrobenzene-d5	8.811	128	271548	30.732	ng/ul	0.00
24) 2-Nitrophenol-d4	9.528	143	268321	31.702	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	440424	29.527	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	684838	28.322	ng/ul	0.00
46) Dimethylphthalate-d6	13.734	166	1269071	32.455	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	1603869	32.640	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	176089	25.036	ng/ul	0.00
60) Fluorene-d10	15.316	176	1052195	32.023	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	110527	19.736	ng/ul	0.00
73) Anthracene-d10	17.187	188	1614411	32.980	ng/ul	0.00
81) Pyrene-d10	19.445	212	1841715	31.306	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	1885365	32.375	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011212.D
Acq On : 01 Aug 2022 22:47
Operator : CG/JU
Sample : PB146541BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2022
Supervised By :mohammad ahmed 08/03/2022

Quant Time: Aug 02 00:29:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 28 16:05:22 2022
Response via : Initial Calibration

