

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011195.D
 Acq On : 01 Aug 2022 12:28
 Operator : CG/JU
 Sample : PB146543BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	77	80	89	rBV	809617	1091013	25.38%	1.865%
2	6.828	630	636	647	rVB	1452844	2218613	51.61%	3.792%
3	6.993	658	664	674	rVB	1226269	1855294	43.16%	3.171%
4	7.181	690	696	706	rVB	1443997	2207169	51.34%	3.772%
5	7.646	769	775	784	rVB	1214645	1844768	42.91%	3.153%
6	8.363	891	897	912	rVB	1644545	2616620	60.87%	4.472%
7	8.810	966	973	981	rBV	1467184	2295562	53.40%	3.924%
8	9.528	1088	1095	1103	rBV	1074001	1695109	39.43%	2.897%
9	10.063	1179	1186	1200	rBV	1449836	2372095	55.18%	4.054%
10	10.440	1243	1250	1262	rVB	1647978	2656955	61.80%	4.541%
11	10.587	1268	1275	1295	rBV	1488977	2537770	59.03%	4.338%
12	12.040	1517	1522	1531	rVB3	21337	42078	0.98%	0.072%
13	12.251	1555	1558	1561	rBV5	4184	6241	0.15%	0.011%
14	13.034	1690	1691	1696	rVB5	4404	4754	0.11%	0.008%
15	13.275	1723	1732	1733	rBV6	5723	8286	0.19%	0.014%
16	13.734	1804	1810	1823	rBV	2139145	2879001	66.97%	4.921%
17	14.004	1848	1856	1871	rBV	2532913	3630684	84.45%	6.206%
18	14.316	1901	1909	1917	rBV	1910453	2702939	62.87%	4.620%
19	14.534	1940	1946	1967	rBV	575854	1036979	24.12%	1.772%
20	15.316	2072	2079	2089	rBV	2852664	3875455	90.15%	6.624%
21	15.445	2095	2101	2112	rBV	594706	834502	19.41%	1.426%
22	15.557	2115	2120	2126	rVB2	28672	40990	0.95%	0.070%
23	16.028	2197	2200	2204	rVB4	3695	5981	0.14%	0.010%
24	16.110	2208	2214	2217	rBV5	10319	15519	0.36%	0.027%
25	16.757	2321	2324	2327	rVV5	4791	5258	0.12%	0.009%
26	16.869	2338	2343	2346	rBV6	4702	8092	0.19%	0.014%
27	17.086	2370	2380	2388	rBV	1788704	2469658	57.45%	4.221%
28	17.186	2390	2397	2409	rVV	2640407	3665353	85.26%	6.265%
29	19.016	2705	2708	2713	rBV3	26830	35538	0.83%	0.061%
30	19.086	2716	2720	2724	rBV	28693	36986	0.86%	0.063%
31	19.445	2775	2781	2789	rBV	3103206	3929075	91.39%	6.716%
32	21.210	3076	3081	3087	rBV	2170436	2638684	61.38%	4.510%
33	23.404	3448	3454	3462	rVB2	2408983	4299027	100.00%	7.348%
34	23.557	3474	3480	3490	rVB2	1486324	2945081	68.51%	5.034%

Sum of corrected areas: 58507129

Instrument :

BNA_P

ClientSampleId :




SBLK543

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011195.D
Acq On : 01 Aug 2022 12:28
Operator : CG/JU
Sample : PB146543BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

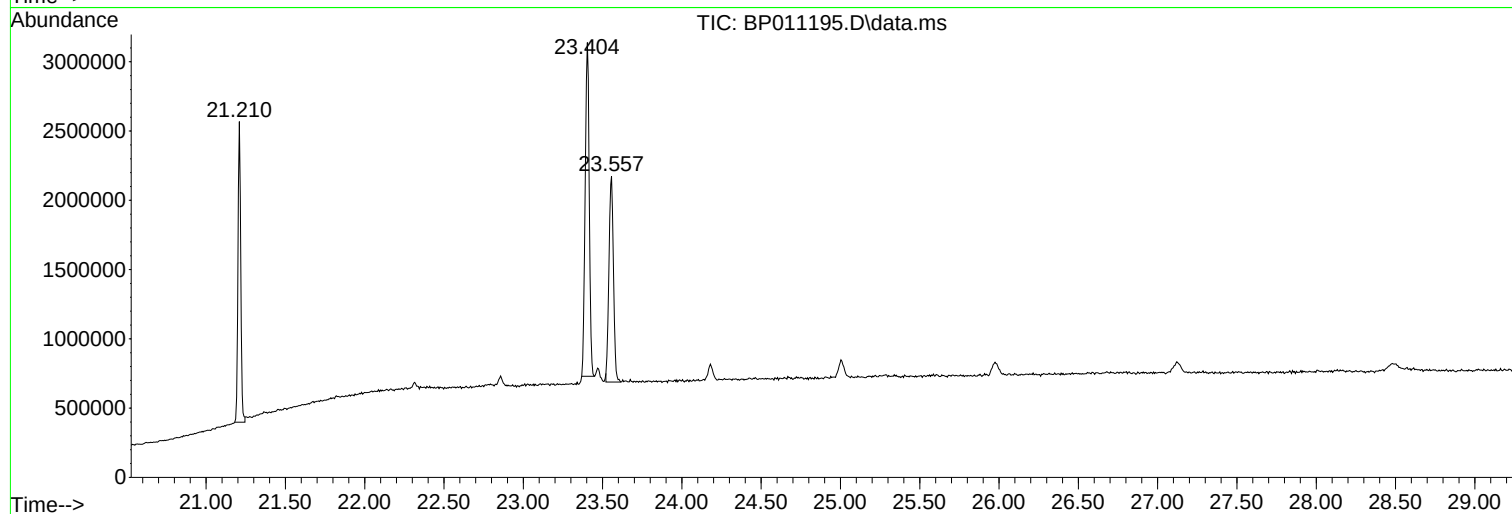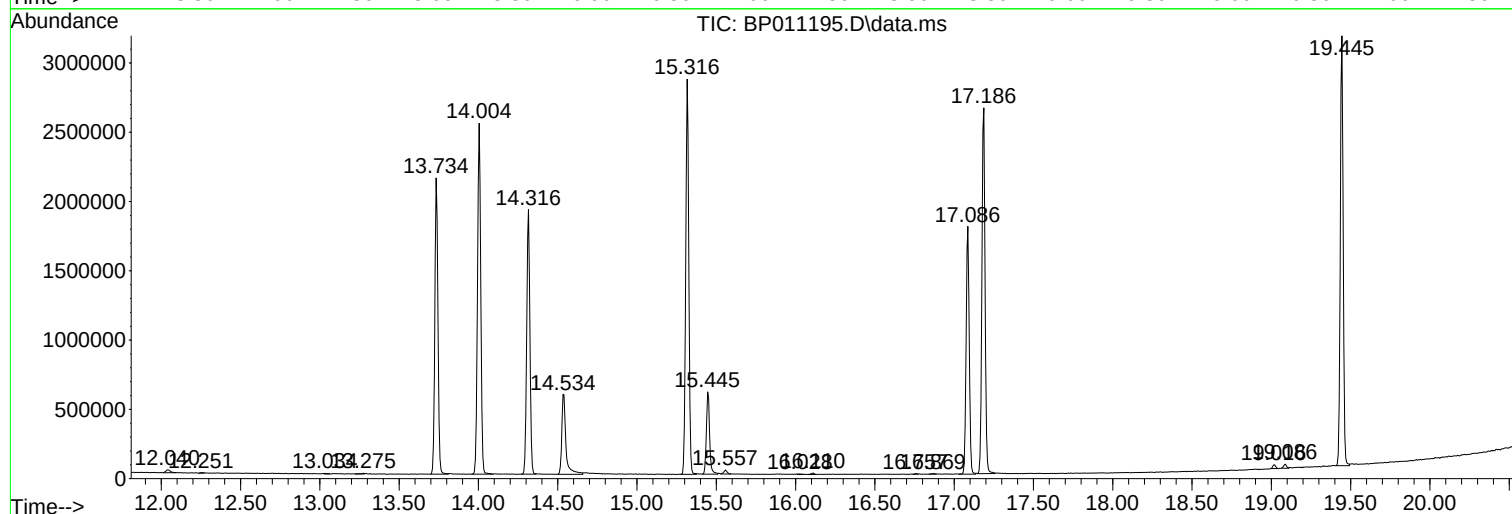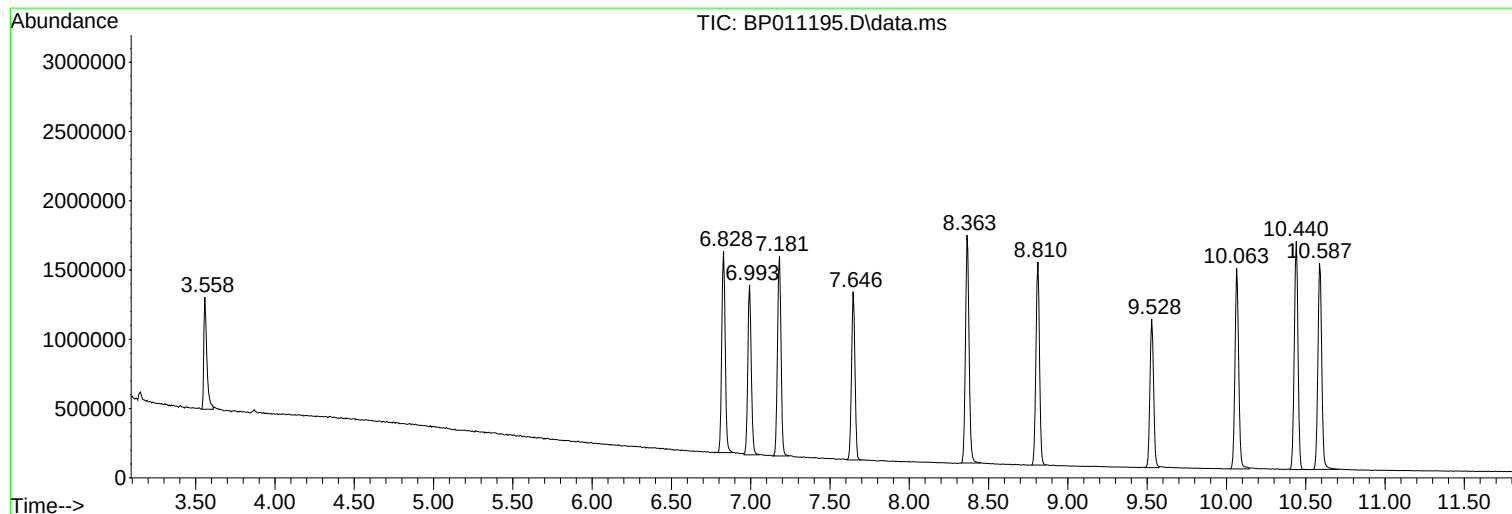

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011195.D
Acq On : 01 Aug 2022 12:28
Operator : CG/JU
Sample : PB146543BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011195.D
Acq On : 01 Aug 2022 12:28
Operator : CG/JU
Sample : PB146543BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc