

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011199.D
 Acq On : 01 Aug 2022 14:45
 Operator : CG/JU
 Sample : N3790-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.569	79	82	92	rBV2	116325	168849	4.81%	0.391%
2	6.828	630	636	651	rVB	829824	1327789	37.85%	3.077%
3	6.993	659	664	674	rVB	666427	1040234	29.66%	2.411%
4	7.181	690	696	707	rVB	802961	1259387	35.90%	2.919%
5	7.646	769	775	783	rVB	1040620	1604560	45.74%	3.719%
6	8.363	891	897	907	rBV	918130	1450285	41.35%	3.361%
7	8.810	967	973	981	rVB	747399	1216093	34.67%	2.818%
8	9.528	1089	1095	1103	rBV	569884	889395	25.36%	2.061%
9	10.063	1180	1186	1198	rBV	837378	1345979	38.37%	3.119%
10	10.440	1243	1250	1260	rVB	1346619	2218658	63.25%	5.142%
11	10.587	1268	1275	1289	rBV	796444	1387028	39.54%	3.215%
12	11.987	1506	1513	1515	rVB7	4455	9658	0.28%	0.022%
13	12.045	1515	1523	1528	rBV4	14026	29839	0.85%	0.069%
14	12.316	1566	1569	1573	rVB3	5195	6173	0.18%	0.014%
15	12.669	1623	1629	1630	rBV3	5030	7659	0.22%	0.018%
16	12.834	1653	1657	1659	rBV4	2363	3513	0.10%	0.008%
17	12.916	1667	1671	1675	rBV5	9293	14310	0.41%	0.033%
18	13.210	1718	1721	1729	rVV8	7099	13694	0.39%	0.032%
19	13.281	1729	1733	1736	rVB6	5537	6962	0.20%	0.016%
20	13.545	1772	1778	1782	rBV9	3639	7670	0.22%	0.018%
21	13.639	1791	1794	1799	rVB6	3668	6478	0.18%	0.015%
22	13.734	1802	1810	1823	rBV	1362384	1838654	52.42%	4.261%
23	14.004	1848	1856	1864	rBV	1529346	2232508	63.65%	5.174%
24	14.192	1884	1888	1890	rBV5	3481	4169	0.12%	0.010%
25	14.222	1890	1893	1898	rVB7	3208	5427	0.15%	0.013%
26	14.310	1900	1908	1922	rVV	1642116	2409343	68.69%	5.584%
27	14.486	1934	1938	1940	rBV5	4642	6229	0.18%	0.014%
28	14.533	1940	1946	1960	rVV	303038	560911	15.99%	1.300%
29	14.751	1978	1983	1989	rBV5	21920	30012	0.86%	0.070%
30	15.133	2043	2048	2049	rBV4	7173	7878	0.22%	0.018%
31	15.151	2049	2051	2056	rVB5	3746	5681	0.16%	0.013%
32	15.316	2071	2079	2088	rBV	1898739	2651682	75.60%	6.146%
33	15.445	2095	2101	2115	rBV	347984	499986	14.25%	1.159%
34	15.557	2115	2120	2126	rVB4	18345	28507	0.81%	0.066%
35	15.892	2173	2177	2182	rBV6	4385	8852	0.25%	0.021%
36	16.028	2194	2200	2203	rBV5	4771	8358	0.24%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011199.D
 Acq On : 01 Aug 2022 14:45
 Operator : CG/JU
 Sample : N3790-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

37	16.110	2211	2214	2216	rVB4	5681	5720	0.16%	0.013%
38	16.228	2224	2234	2240	rBV8	4044	12864	0.37%	0.030%
39	16.363	2252	2257	2260	rVB7	2724	4353	0.12%	0.010%
40	16.757	2321	2324	2328	rVB6	4284	5897	0.17%	0.014%
41	16.863	2338	2342	2345	rBV5	6823	12222	0.35%	0.028%
42	17.022	2364	2369	2373	rBV7	5555	9695	0.28%	0.022%
43	17.086	2373	2380	2387	rVV	1775050	2548854	72.67%	5.907%
44	17.180	2390	2396	2410	rVV	2079291	2890007	82.39%	6.698%
45	17.292	2411	2415	2419	rVB6	21081	28487	0.81%	0.066%
46	17.392	2429	2432	2440	rVB8	4430	6712	0.19%	0.016%
47	17.592	2464	2466	2471	rVB6	2683	3979	0.11%	0.009%
48	17.780	2494	2498	2502	rVB2	32001	37375	1.07%	0.087%
49	17.992	2531	2534	2541	rBV9	7428	15102	0.43%	0.035%
50	18.069	2544	2547	2551	rVB2	10363	10795	0.31%	0.025%
51	18.922	2689	2692	2696	rBV3	39878	43055	1.23%	0.100%
52	19.016	2705	2708	2711	rBV3	26872	31321	0.89%	0.073%
53	19.057	2712	2715	2717	rVV2	16514	16474	0.47%	0.038%
54	19.086	2717	2720	2724	rVV	22772	26720	0.76%	0.062%
55	19.445	2775	2781	2788	rBV	2577536	3383592	96.46%	7.842%
56	20.939	3032	3035	3040	rBV5	88298	136444	3.89%	0.316%
57	21.210	3076	3081	3086	rBV	2454753	2964391	84.51%	6.870%
58	23.404	3448	3454	3461	rVB2	1941258	3507625	100.00%	8.129%
59	23.551	3473	3479	3491	rVB2	1593300	3134068	89.35%	7.264%



Sum of corrected areas: 43148162

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011199.D
Acq On : 01 Aug 2022 14:45
Operator : CG/JU
Sample : N3790-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

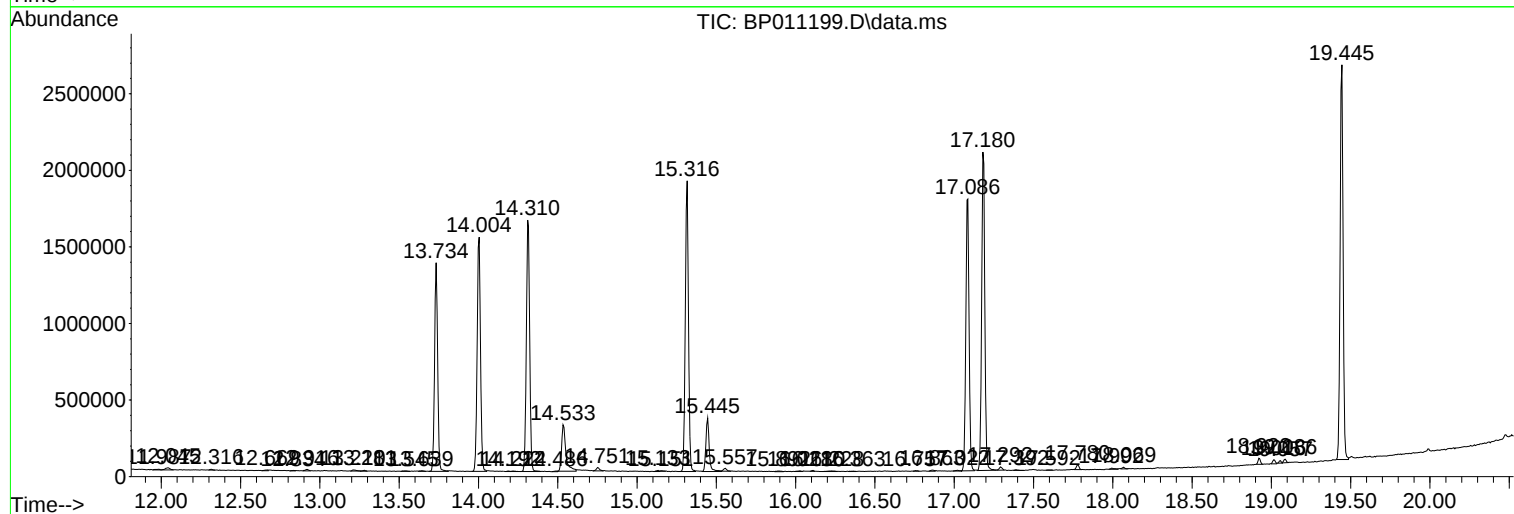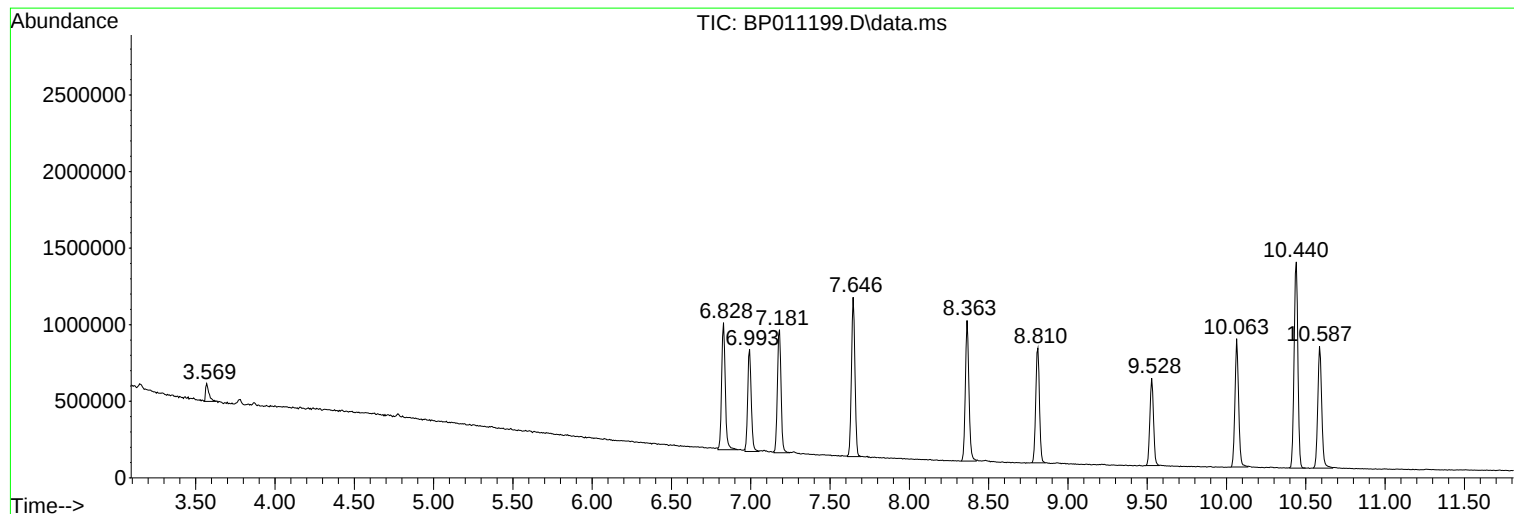

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011199.D
Acq On : 01 Aug 2022 14:45
Operator : CG/JU
Sample : N3790-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011199.D
Acq On : 01 Aug 2022 14:45
Operator : CG/JU
Sample : N3790-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc