

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011207.D
 Acq On : 01 Aug 2022 19:21
 Operator : CG/JU
 Sample : N3792-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.834	632	637	647	rVB	240800	395626	7.37%	0.703%
2	6.993	659	664	672	rVB	994245	1493832	27.83%	2.656%
3	7.181	691	696	708	rVB	920944	1456328	27.13%	2.589%
4	7.652	769	776	786	rVB	1130796	1778327	33.13%	3.161%
5	8.369	892	898	912	rVB	642150	1039112	19.36%	1.847%
6	8.810	967	973	984	rVB	1178446	1905952	35.50%	3.388%
7	9.534	1089	1096	1104	rBV	851941	1391845	25.93%	2.474%
8	10.069	1180	1187	1197	rBV	1124616	1849480	34.45%	3.288%
9	10.440	1243	1250	1260	rVB	1512584	2469119	45.99%	4.389%
10	10.593	1269	1276	1291	rVB	720373	1227846	22.87%	2.183%
11	12.040	1514	1522	1529	rBV2	22640	42826	0.80%	0.076%
12	12.922	1668	1672	1673	rBV3	4319	5601	0.10%	0.010%
13	13.034	1687	1691	1698	rVB9	4550	6413	0.12%	0.011%
14	13.275	1730	1732	1737	rBV6	4558	5686	0.11%	0.010%
15	13.557	1774	1780	1783	rBV7	3122	6498	0.12%	0.012%
16	13.739	1804	1811	1817	rBV	2051209	2866164	53.39%	5.095%
17	13.898	1837	1838	1844	rBV6	2884	5463	0.10%	0.010%
18	14.004	1848	1856	1863	rBV	2297714	3453950	64.34%	6.140%
19	14.228	1890	1894	1897	rVB6	4879	6110	0.11%	0.011%
20	14.316	1902	1909	1917	rBV	1941090	2773048	51.65%	4.930%
21	14.545	1943	1948	1959	rBV	97284	194336	3.62%	0.345%
22	14.763	1981	1985	1989	rVB7	4058	6517	0.12%	0.012%
23	15.133	2043	2048	2050	rBV4	8249	11848	0.22%	0.021%
24	15.186	2054	2057	2061	rVB6	6282	7690	0.14%	0.014%
25	15.322	2073	2080	2089	rBV	2902468	4142554	77.17%	7.364%
26	15.451	2096	2102	2114	rBV	716075	995944	18.55%	1.770%
27	15.563	2114	2121	2127	rVB3	35677	59083	1.10%	0.105%
28	15.898	2172	2178	2181	rBV6	7983	13562	0.25%	0.024%
29	15.975	2184	2191	2192	rBV7	4375	9421	0.18%	0.017%
30	16.004	2192	2196	2197	rBV4	7184	7143	0.13%	0.013%
31	16.051	2202	2204	2210	rVV5	8902	13421	0.25%	0.024%
32	16.116	2210	2215	2222	rVV9	12922	25784	0.48%	0.046%
33	16.563	2289	2291	2295	rVB5	4345	5862	0.11%	0.010%
34	16.816	2331	2334	2336	rBV4	5967	6369	0.12%	0.011%
35	16.857	2339	2341	2342	rBV2	7283	5954	0.11%	0.011%
36	17.086	2374	2380	2386	rBV	2265904	3100691	57.76%	5.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011207.D
 Acq On : 01 Aug 2022 19:21
 Operator : CG/JU
 Sample : N3792-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

37	17.186	2391	2397	2407	rVB2	3285917	4634283	86.32%	8.238%
38	17.275	2410	2412	2414	rBV3	6255	6009	0.11%	0.011%
39	17.780	2495	2498	2502	rVB4	12990	14226	0.26%	0.025%
40	17.998	2532	2535	2539	rBV3	30113	37203	0.69%	0.066%
41	19.445	2776	2781	2788	rBV	4078199	5368417	100.00%	9.543%
42	20.939	3031	3035	3042	rBV	513552	873950	16.28%	1.554%
43	21.210	3077	3081	3087	rBV2	2631700	3224277	60.06%	5.732%
44	22.445	3288	3291	3299	rVB	510044	677457	12.62%	1.204%
45	23.410	3449	3455	3461	rVB2	2765893	5092436	94.86%	9.053%
46	23.557	3475	3480	3490	rVB2	1786238	3540268	65.95%	6.293%




Sum of corrected areas: 56253931

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011207.D
Acq On : 01 Aug 2022 19:21
Operator : CG/JU
Sample : N3792-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

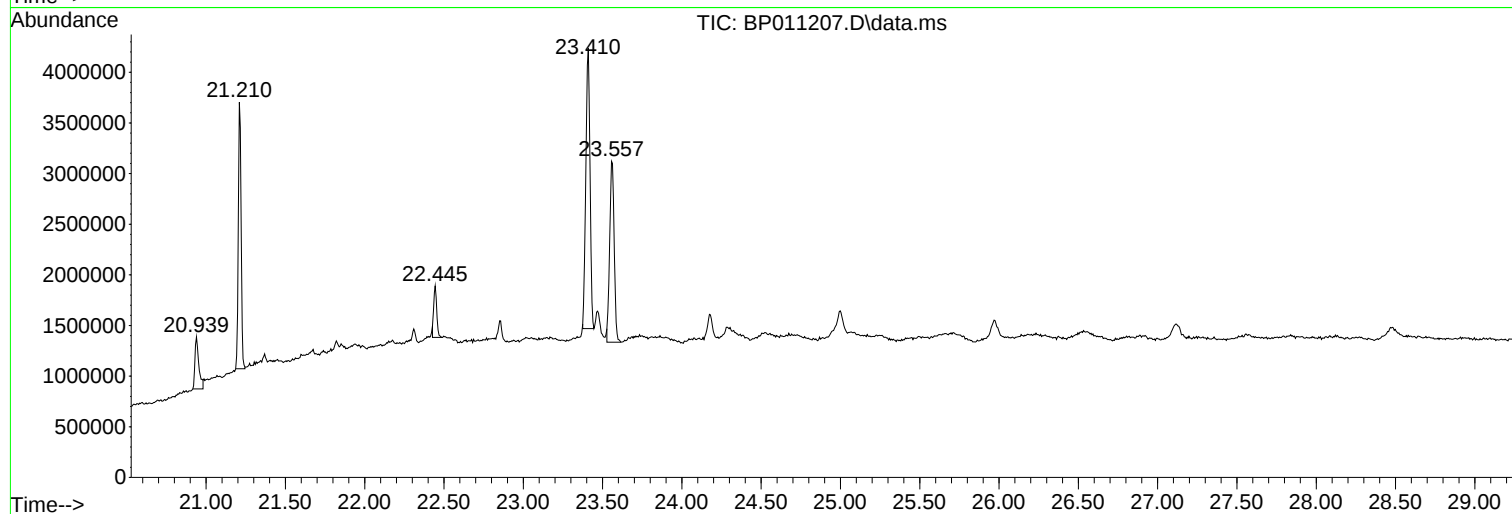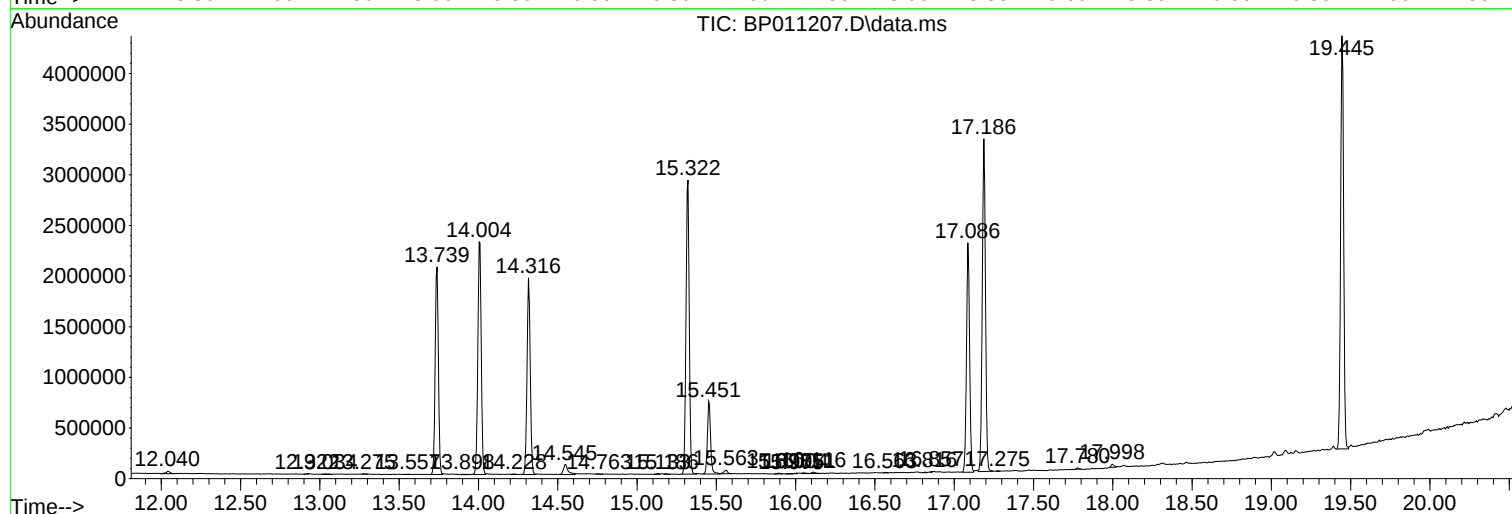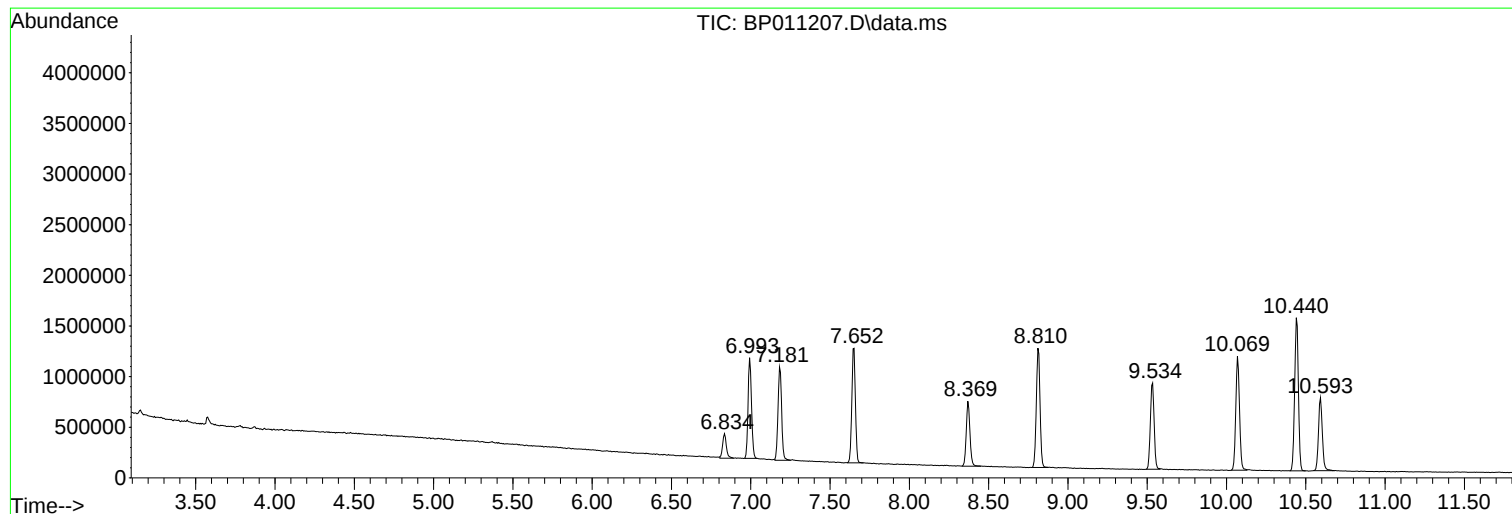

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011207.D
Acq On : 01 Aug 2022 19:21
Operator : CG/JU
Sample : N3792-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic20.939 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.939	5.42 ng/ul	873950	Chrysene-d12	21.210

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	95
2			Z-14-Nonacosene	406	C29H58	1010131-18-9	94
3			Octacosanol	410	C28H58O	000557-61-9	94
4			1-Hexacosene	364	C26H52	018835-33-1	93
5			1-Heptacosanol	396	C27H56O	002004-39-9	91

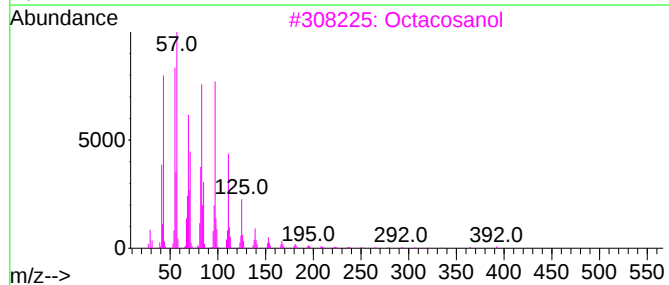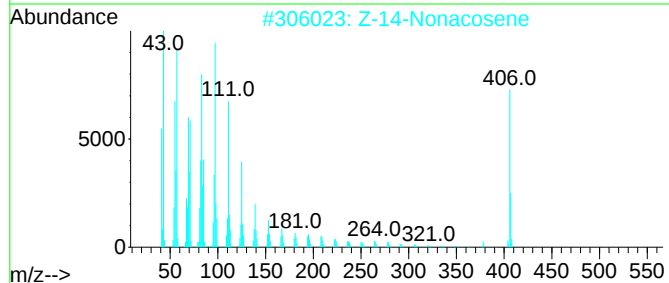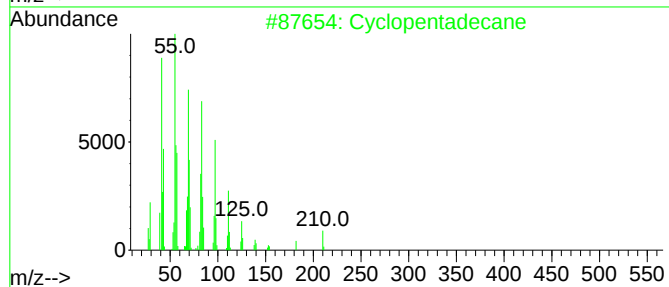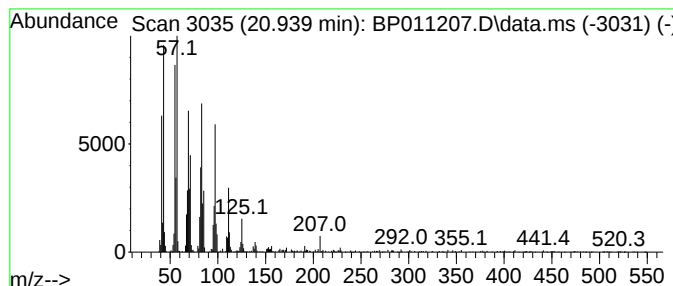

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011207.D
Acq On : 01 Aug 2022 19:21
Operator : CG/JU
Sample : N3792-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	20.939	5.4	ng/u1	873950	5	21.210	3224280	20.0
5,9,13,17-Tetra...	22.445	3.8	ng/u1	677457	6	23.562	3540270	20.0