

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011208.D
 Acq On : 01 Aug 2022 19:55
 Operator : CG/JU
 Sample : N3792-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBUN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	79	81	89	rVB	156573	233616	3.80%	0.408%
2	6.834	632	637	648	rVB	270262	440827	7.17%	0.771%
3	6.993	659	664	673	rVB	1065105	1591714	25.88%	2.783%
4	7.181	690	696	708	rVB	992182	1538486	25.02%	2.690%
5	7.646	770	775	783	rVB	940489	1449443	23.57%	2.534%
6	8.369	892	898	912	rVB	720079	1160234	18.87%	2.029%
7	8.810	967	973	984	rVB	1248316	2026966	32.96%	3.544%
8	9.528	1089	1095	1107	rBV	899937	1455413	23.66%	2.545%
9	10.069	1180	1187	1204	rBV	1192194	1968991	32.02%	3.443%
10	10.440	1243	1250	1259	rVB	1279271	2084490	33.89%	3.645%
11	10.593	1269	1276	1290	rVB	1056368	1793454	29.16%	3.136%
12	12.040	1517	1522	1530	rVB3	26085	48472	0.79%	0.085%
13	12.928	1666	1673	1680	rBV10	6552	14742	0.24%	0.026%
14	13.034	1688	1691	1697	rVB8	3562	6345	0.10%	0.011%
15	13.275	1729	1732	1736	rBV6	5607	8542	0.14%	0.015%
16	13.734	1803	1810	1817	rBV	2212573	3068331	49.89%	5.365%
17	14.004	1847	1856	1869	rBV	2522925	3737367	60.77%	6.535%
18	14.316	1902	1909	1916	rBV	1678978	2353835	38.27%	4.116%
19	14.545	1941	1948	1961	rBV	125757	256530	4.17%	0.449%
20	15.134	2044	2048	2050	rBV3	6842	9455	0.15%	0.017%
21	15.186	2054	2057	2061	rVB5	7803	9502	0.15%	0.017%
22	15.316	2073	2079	2092	rBV	3140671	4519590	73.49%	7.903%
23	15.451	2095	2102	2115	rBV	906638	1207228	19.63%	2.111%
24	15.557	2115	2120	2127	rVB	39018	60982	0.99%	0.107%
25	15.892	2171	2177	2179	rBV7	5582	10224	0.17%	0.018%
26	16.016	2193	2198	2201	rBV7	7524	12200	0.20%	0.021%
27	16.051	2201	2204	2209	rVV7	8231	13245	0.22%	0.023%
28	16.110	2209	2214	2219	rVB7	15883	24193	0.39%	0.042%
29	16.563	2287	2291	2296	rVB8	4454	7653	0.12%	0.013%
30	16.763	2321	2325	2330	rVB7	8604	12360	0.20%	0.022%
31	16.863	2338	2342	2347	rVB8	8025	14931	0.24%	0.026%
32	17.086	2373	2380	2387	rBV	1846998	2580467	41.96%	4.512%
33	17.186	2391	2397	2408	rVV2	3837632	5318031	86.47%	9.299%
34	17.275	2410	2412	2418	rVV7	4049	6826	0.11%	0.012%
35	17.386	2429	2431	2435	rVB4	6316	8268	0.13%	0.014%
36	17.604	2465	2468	2469	rBV3	6140	6288	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011208.D
Acq On : 01 Aug 2022 19:55
Operator : CG/JU
Sample : N3792-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Title : SVOA CALIBRATION

37	17.775	2494	2497	2502	rVB3	17306	21692	0.35%	0.038%
38	17.998	2531	2535	2541	rBV4	34151	52065	0.85%	0.091%
39	19.016	2705	2708	2712	rBV3	53972	62701	1.02%	0.110%
40	19.086	2717	2720	2724	rVV	47784	58307	0.95%	0.102%
41	19.445	2775	2781	2788	rBV	4786013	6150121	100.00%	10.754%
42	20.939	3032	3035	3042	rVB	223399	316217	5.14%	0.553%
43	21.210	3077	3081	3087	rVB2	2211561	2651020	43.11%	4.636%
44	23.404	3448	3454	3461	rVB2	3245437	6029927	98.05%	10.544%
45	23.557	3474	3480	3487	rVB2	1457911	2787599	45.33%	4.874%




Sum of corrected areas: 57188890

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011208.D
Acq On : 01 Aug 2022 19:55
Operator : CG/JU
Sample : N3792-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

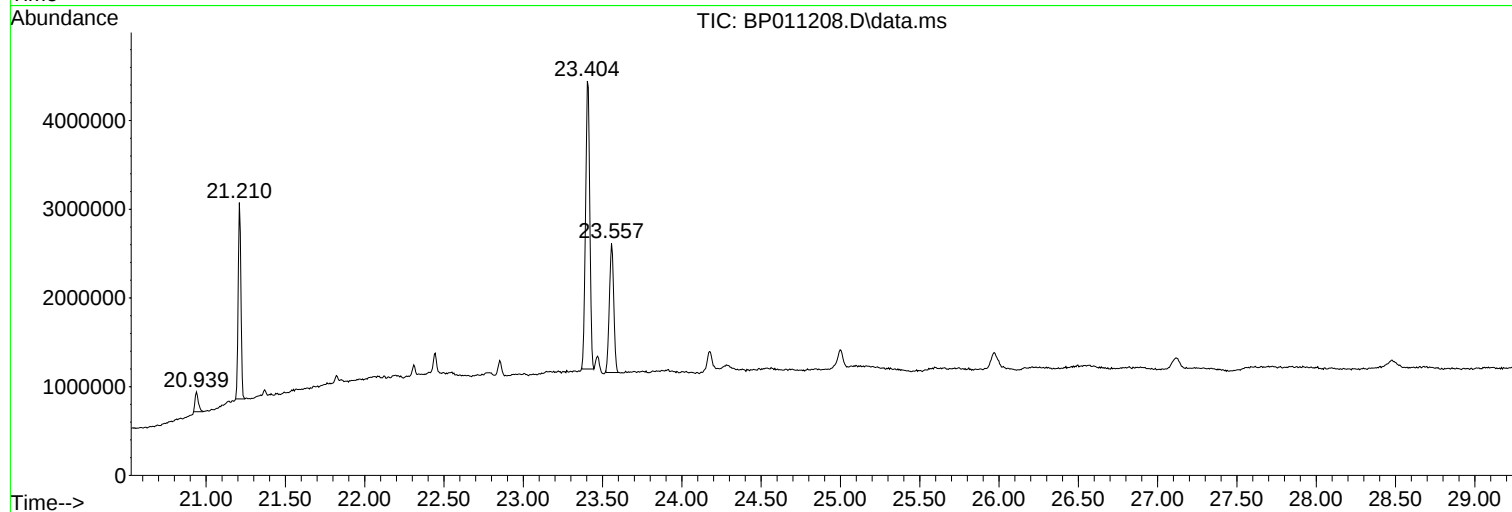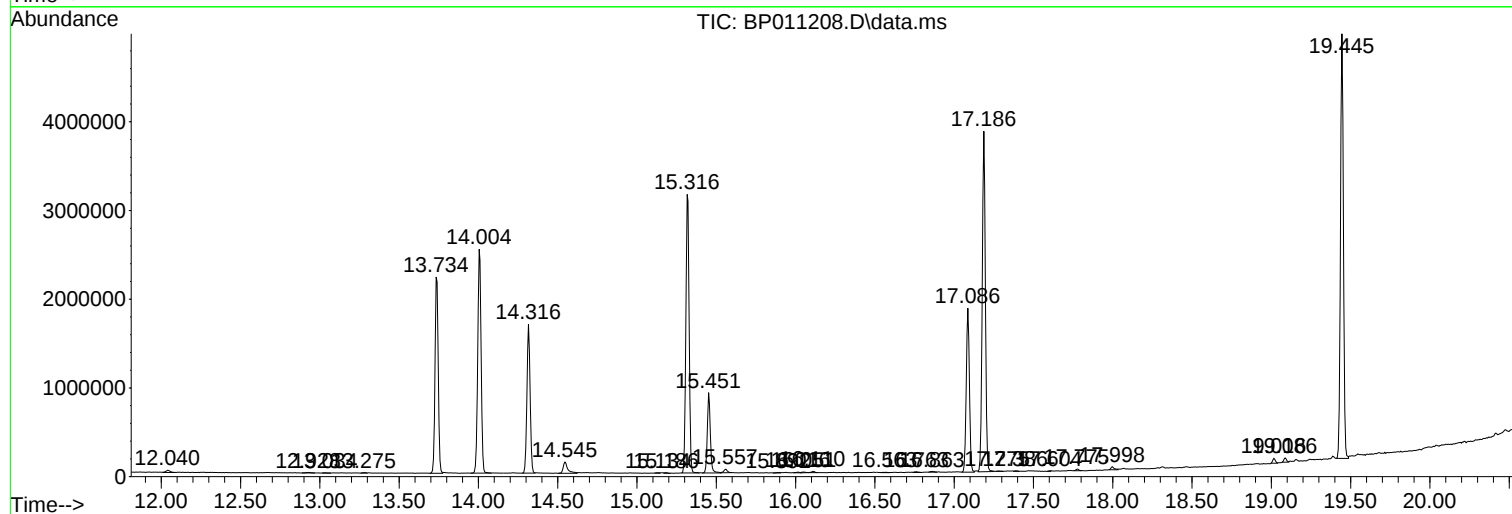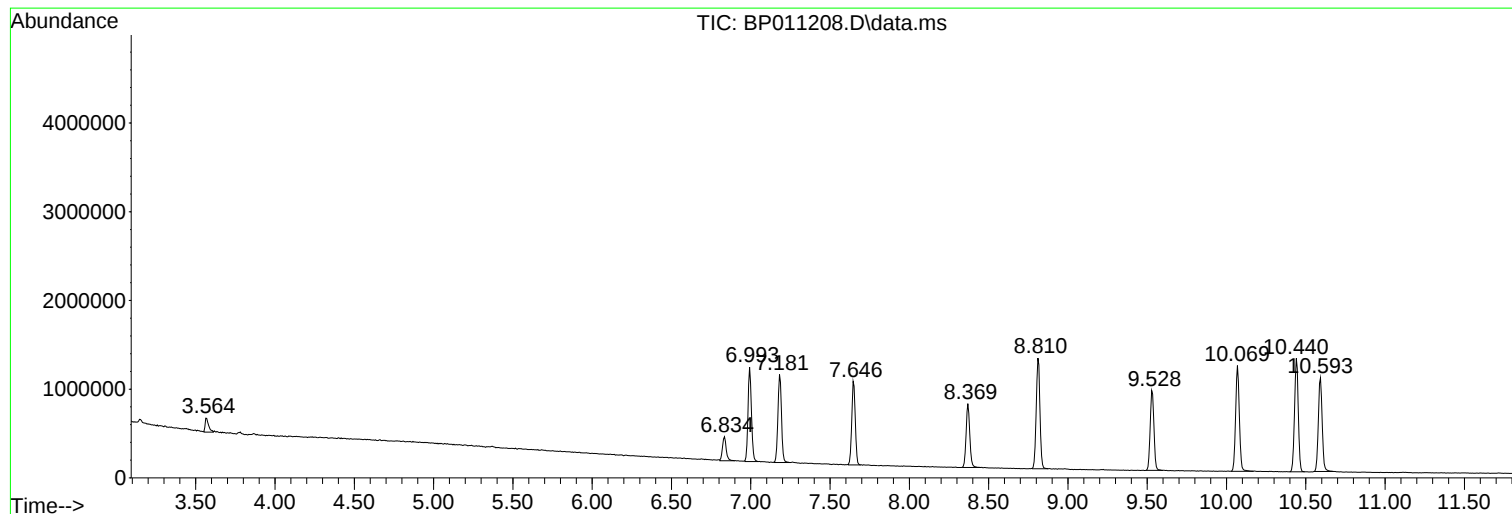

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011208.D
Acq On : 01 Aug 2022 19:55
Operator : CG/JU
Sample : N3792-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.939	2.39 ng/ul	316217	Chrysene-d12	21.210

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Pentacos-1-ene	350	C25H50	016980-85-1	93
2		Cyclooctacosane	392	C28H56	000297-24-5	93
3		1-Docosene	308	C22H44	001599-67-3	91
4		1-Hexacosanol	382	C26H54O	000506-52-5	90
5		Octacosanol	410	C28H58O	000557-61-9	90

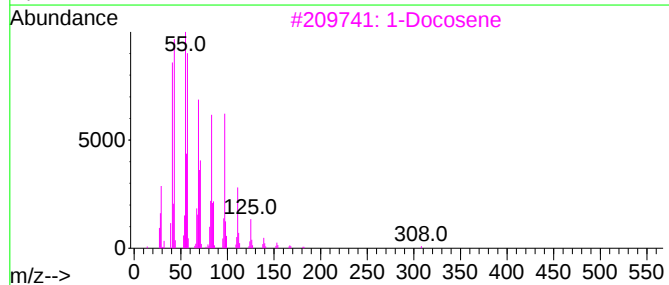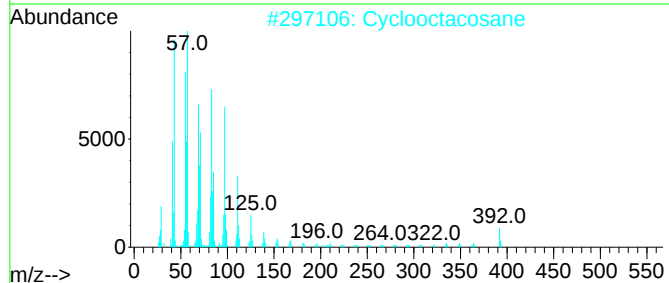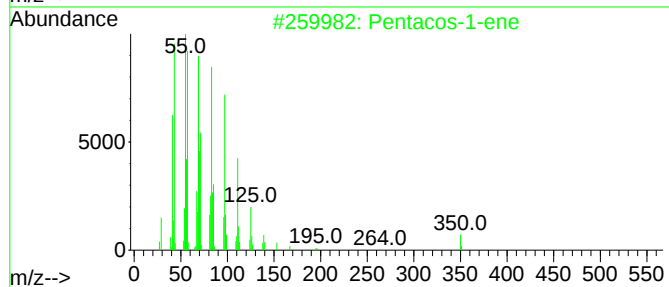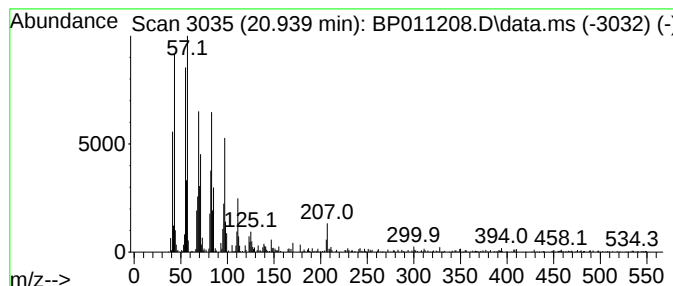

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011208.D
Acq On : 01 Aug 2022 19:55
Operator : CG/JU
Sample : N3792-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBUN3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.939	2.4	ng/u1	316217	5	21.210	2651020	20.0