

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011211.D
 Acq On : 01 Aug 2022 22:12
 Operator : CG/JU
 Sample : PB146356BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK356

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	77	80	90	rVB	697615	933954	17.15%	1.415%
2	6.828	631	636	647	rVB	1433043	2234734	41.04%	3.387%
3	6.993	658	664	675	rVB	1212251	1847401	33.92%	2.800%
4	7.181	690	696	706	rVB	1506835	2294030	42.12%	3.477%
5	7.646	769	775	784	rVB	1247289	1882875	34.57%	2.854%
6	8.364	891	897	914	rVB	1600743	2631745	48.33%	3.988%
7	8.811	966	973	986	rVB	1426217	2248192	41.28%	3.407%
8	9.528	1088	1095	1105	rBV	1086748	1735919	31.88%	2.631%
9	10.063	1180	1186	1200	rBV	1455307	2440537	44.82%	3.699%
10	10.440	1242	1250	1260	rVB	1609294	2628897	48.27%	3.984%
11	10.587	1268	1275	1294	rBV	1505180	2531839	46.49%	3.837%
12	12.040	1517	1522	1528	rBV4	22417	39932	0.73%	0.061%
13	13.275	1729	1732	1736	rVB4	6844	8717	0.16%	0.013%
14	13.734	1804	1810	1824	rBV	2352667	3145276	57.76%	4.767%
15	14.004	1849	1856	1867	rBV	2783251	3917309	71.93%	5.937%
16	14.316	1902	1909	1919	rVB	1970506	2882892	52.94%	4.369%
17	14.540	1940	1947	1968	rBV	912146	1461497	26.84%	2.215%
18	15.316	2072	2079	2093	rVV	3227469	4443920	81.60%	6.735%
19	15.451	2095	2102	2114	rVV	804468	1113725	20.45%	1.688%
20	15.557	2115	2120	2128	rVB2	34626	58676	1.08%	0.089%
21	16.016	2193	2198	2204	rBV10	5392	9155	0.17%	0.014%
22	16.110	2208	2214	2219	rBV7	11538	16350	0.30%	0.025%
23	16.757	2318	2324	2329	rBV10	6698	11911	0.22%	0.018%
24	16.869	2339	2343	2347	rBV7	6113	11984	0.22%	0.018%
25	17.087	2373	2380	2390	rBV	2191269	3072772	56.42%	4.657%
26	17.187	2390	2397	2410	rVV	3269246	4646585	85.32%	7.042%
27	19.016	2704	2708	2713	rVB2	43900	53397	0.98%	0.081%
28	19.087	2716	2720	2724	rBV	41945	58108	1.07%	0.088%
29	19.445	2775	2781	2788	rBV	3912066	5251308	96.43%	7.958%
30	21.210	3076	3081	3086	rBV	2813231	3395807	62.36%	5.146%
31	23.404	3447	3454	3460	rBV2	2835505	5445790	100.00%	8.253%
32	23.551	3473	3479	3490	rVB2	1770221	3528453	64.79%	5.347%




Sum of corrected areas: 65983687

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011211.D
Acq On : 01 Aug 2022 22:12
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

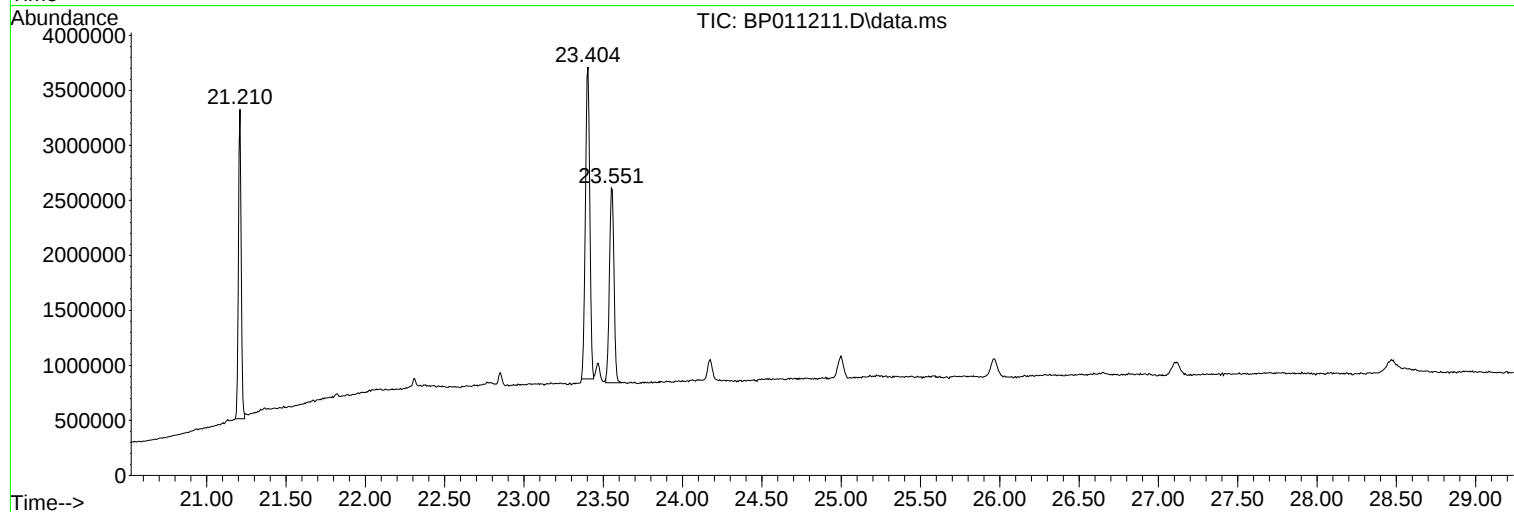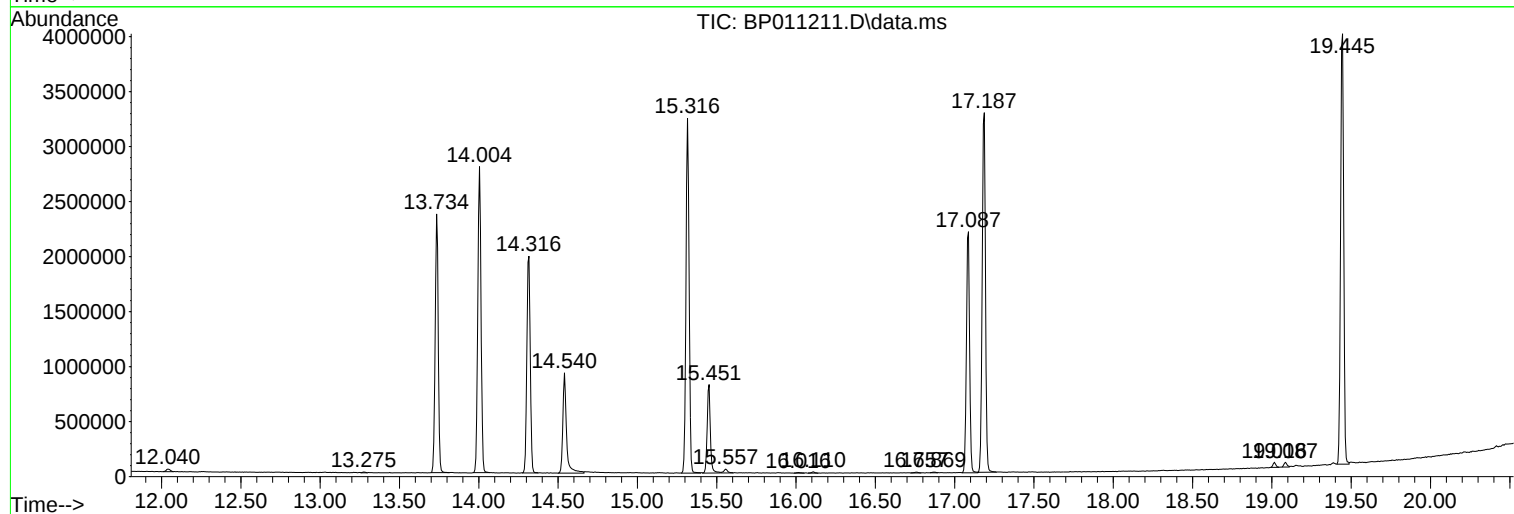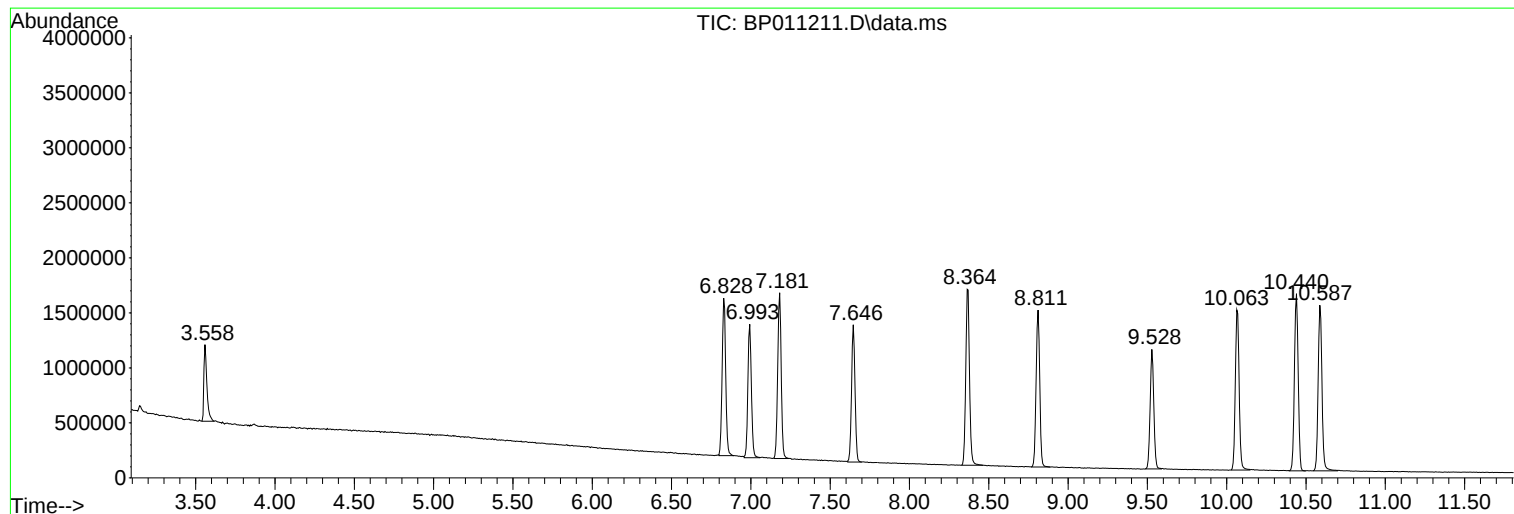

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011211.D
Acq On : 01 Aug 2022 22:12
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011211.D
Acq On : 01 Aug 2022 22:12
Operator : CG/JU
Sample : PB146356BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK356

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc