

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011212.D
 Acq On : 01 Aug 2022 22:47
 Operator : CG/JU
 Sample : PB146541BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK541

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	77	80	94	rVB	664631	908847	16.54%	1.430%
2	6.828	631	636	653	rVB	1390218	2175848	39.59%	3.423%
3	6.993	658	664	673	rVB	1145280	1745851	31.77%	2.747%
4	7.181	690	696	706	rVB	1432910	2207424	40.16%	3.473%
5	7.646	769	775	784	rVB	1180433	1805888	32.86%	2.841%
6	8.364	891	897	913	rVB	1510591	2485257	45.22%	3.910%
7	8.811	966	973	984	rVB	1334059	2128078	38.72%	3.348%
8	9.528	1089	1095	1106	rVB	1021538	1607277	29.24%	2.529%
9	10.063	1180	1186	1200	rVB	1341430	2292670	41.71%	3.607%
10	10.440	1243	1250	1258	rVB	1506261	2450113	44.58%	3.855%
11	10.587	1268	1275	1291	rBV	1384807	2358765	42.92%	3.711%
12	12.040	1517	1522	1534	rVB3	24131	48492	0.88%	0.076%
13	13.034	1685	1691	1694	rVB6	4936	9309	0.17%	0.015%
14	13.287	1727	1734	1736	rBV6	5125	8165	0.15%	0.013%
15	13.734	1803	1810	1819	rBV	2231914	2981031	54.24%	4.690%
16	14.004	1848	1856	1868	rBV	2644370	3721079	67.70%	5.855%
17	14.316	1902	1909	1919	rVB	1893108	2689905	48.94%	4.232%
18	14.540	1941	1947	1966	rBV	898712	1431130	26.04%	2.252%
19	15.316	2071	2079	2092	rBV	3067254	4257341	77.46%	6.698%
20	15.451	2095	2102	2115	rVV	767507	1056323	19.22%	1.662%
21	15.557	2115	2120	2125	rVB2	30395	45306	0.82%	0.071%
22	15.893	2172	2177	2180	rVB6	4398	6219	0.11%	0.010%
23	16.010	2194	2197	2200	rBV4	3929	6364	0.12%	0.010%
24	16.104	2210	2213	2218	rVB4	8637	12362	0.22%	0.019%
25	16.757	2318	2324	2329	rBV10	5132	9060	0.16%	0.014%
26	16.863	2338	2342	2350	rVB6	5740	11556	0.21%	0.018%
27	17.087	2371	2380	2389	rBV	2130113	2956857	53.80%	4.652%
28	17.187	2390	2397	2412	rVV	3214120	4542889	82.66%	7.148%
29	18.287	2580	2584	2586	rBV5	4663	7708	0.14%	0.012%
30	19.016	2704	2708	2713	rBV3	42642	59605	1.08%	0.094%
31	19.087	2716	2720	2729	rVV	39470	64977	1.18%	0.102%
32	19.445	2775	2781	2789	rBV	4069467	5228140	95.12%	8.226%
33	21.210	3076	3081	3087	rBV	2676063	3301937	60.08%	5.195%
34	23.404	3447	3454	3461	rBV2	2915989	5496118	100.00%	8.647%
35	23.551	3473	3479	3488	rVB2	1696386	3440801	62.60%	5.414%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011212.D
Acq On : 01 Aug 2022 22:47
Operator : CG/JU
Sample : PB146541BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Title : SVOA CALIBRATION




Sum of corrected areas: 63558692

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011212.D
Acq On : 01 Aug 2022 22:47
Operator : CG/JU
Sample : PB146541BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

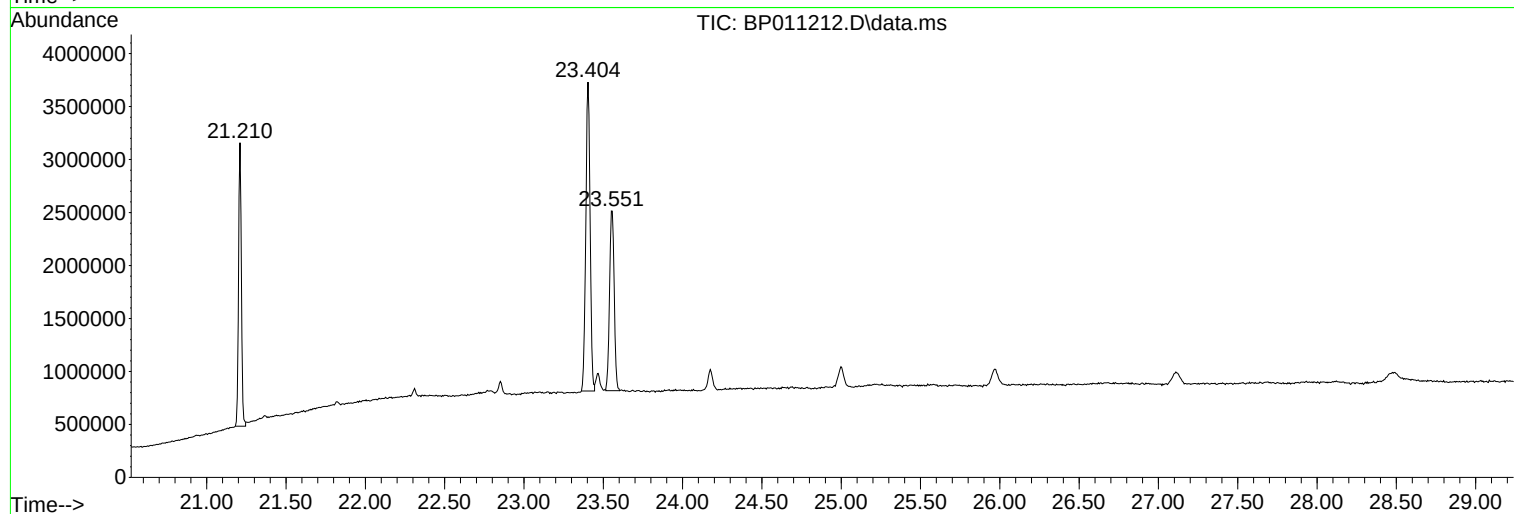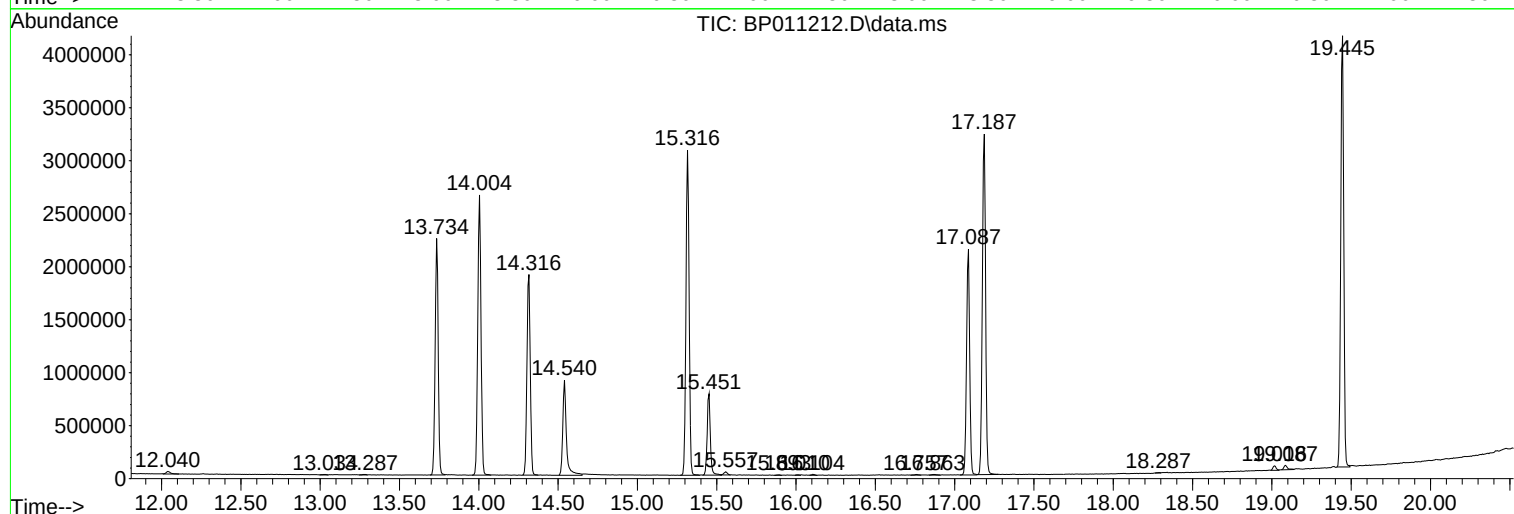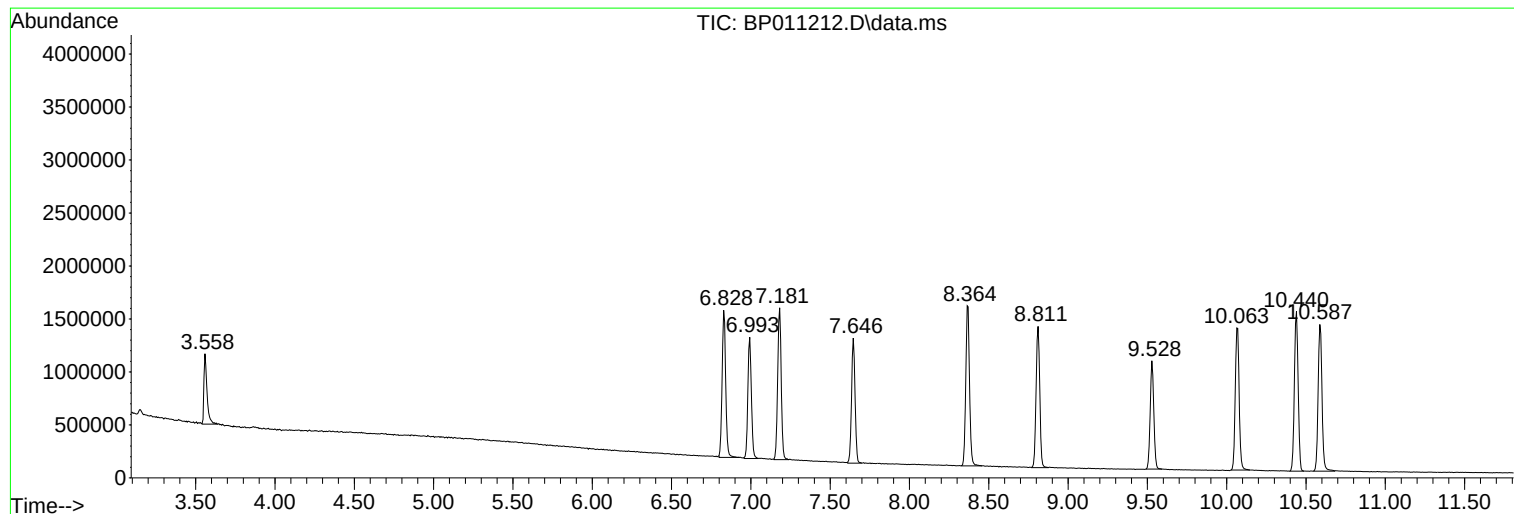

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011212.D
Acq On : 01 Aug 2022 22:47
Operator : CG/JU
Sample : PB146541BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011212.D
Acq On : 01 Aug 2022 22:47
Operator : CG/JU
Sample : PB146541BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK541

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------