

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011220.D
 Acq On : 02 Aug 2022 08:23
 Operator : CG/JU
 Sample : PB146570BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK570

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	77	80	94	rVB	697255	977392	18.63%	1.612%
2	6.834	631	637	648	rVB	1299082	2021317	38.54%	3.334%
3	6.993	659	664	677	rVB	1076852	1657022	31.59%	2.733%
4	7.181	690	696	710	rVB	1325659	2077387	39.61%	3.426%
5	7.652	770	776	785	rVB	1013877	1566200	29.86%	2.583%
6	8.369	892	898	915	rVB	1489617	2356433	44.93%	3.887%
7	8.816	967	974	985	rVB	1251887	2012227	38.36%	3.319%
8	9.534	1089	1096	1108	rBV	946261	1509171	28.77%	2.489%
9	10.069	1180	1187	1197	rBV	1337000	2206799	42.07%	3.640%
10	10.446	1244	1251	1259	rVB	1329404	2184542	41.65%	3.603%
11	10.593	1269	1276	1298	rVB	1314453	2198477	41.92%	3.626%
12	12.046	1518	1523	1529	rVB2	23169	40982	0.78%	0.068%
13	13.281	1729	1733	1737	rVB6	4650	6943	0.13%	0.011%
14	13.740	1805	1811	1822	rVB	2117806	2896682	55.23%	4.778%
15	14.010	1849	1857	1869	rBV	2455579	3623627	69.09%	5.977%
16	14.322	1902	1910	1919	rBV	1725652	2466787	47.03%	4.069%
17	14.545	1941	1948	1962	rBV	875110	1418494	27.04%	2.340%
18	15.322	2074	2080	2088	rVB	2919511	4183245	79.76%	6.900%
19	15.457	2096	2103	2116	rBV	779131	1054730	20.11%	1.740%
20	15.563	2116	2121	2129	rVB2	31809	53236	1.01%	0.088%
21	16.016	2194	2198	2200	rBV4	4992	6836	0.13%	0.011%
22	16.039	2200	2202	2207	rVB5	5931	8109	0.15%	0.013%
23	16.116	2211	2215	2222	rBV8	9938	16471	0.31%	0.027%
24	16.204	2223	2230	2232	rBV6	5953	12645	0.24%	0.021%
25	16.434	2265	2269	2272	rVB6	4496	6717	0.13%	0.011%
26	16.563	2282	2291	2296	rBV6	9907	22630	0.43%	0.037%
27	16.769	2322	2326	2331	rBV8	6043	9270	0.18%	0.015%
28	16.875	2340	2344	2352	rVB7	5305	12058	0.23%	0.020%
29	17.022	2363	2369	2372	rBV7	7550	14778	0.28%	0.024%
30	17.092	2374	2381	2391	rVV	1995310	2744900	52.33%	4.527%
31	17.192	2391	2398	2409	rVV2	3318944	4572188	87.17%	7.541%
32	17.486	2442	2448	2454	rBV6	9145	22012	0.42%	0.036%
33	17.657	2472	2477	2481	rBV4	6369	8326	0.16%	0.014%
34	17.722	2483	2488	2495	rVV5	15028	30688	0.59%	0.051%
35	17.781	2495	2498	2501	rVB4	5809	7170	0.14%	0.012%
36	18.063	2541	2546	2550	rBV7	12204	21642	0.41%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011220.D
Acq On : 02 Aug 2022 08:23
Operator : CG/JU
Sample : PB146570BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Title : SVOA CALIBRATION

37	18.528	2622	2625	2629	rBV4	7393	7749	0.15%	0.013%
38	19.028	2706	2710	2715	rVB3	42378	58385	1.11%	0.096%
39	19.092	2718	2721	2723	rBV	36337	44992	0.86%	0.074%
40	19.451	2776	2782	2790	rBV	3939006	5245014	100.00%	8.651%
41	21.222	3078	3083	3087	rBV	2333665	2983310	56.88%	4.920%
42	23.421	3450	3457	3464	rBV2	2770177	5209059	99.31%	8.592%
43	23.568	3476	3482	3493	rVB2	1582670	3053619	58.22%	5.036%




Sum of corrected areas: 60630261

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011220.D
Acq On : 02 Aug 2022 08:23
Operator : CG/JU
Sample : PB146570BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

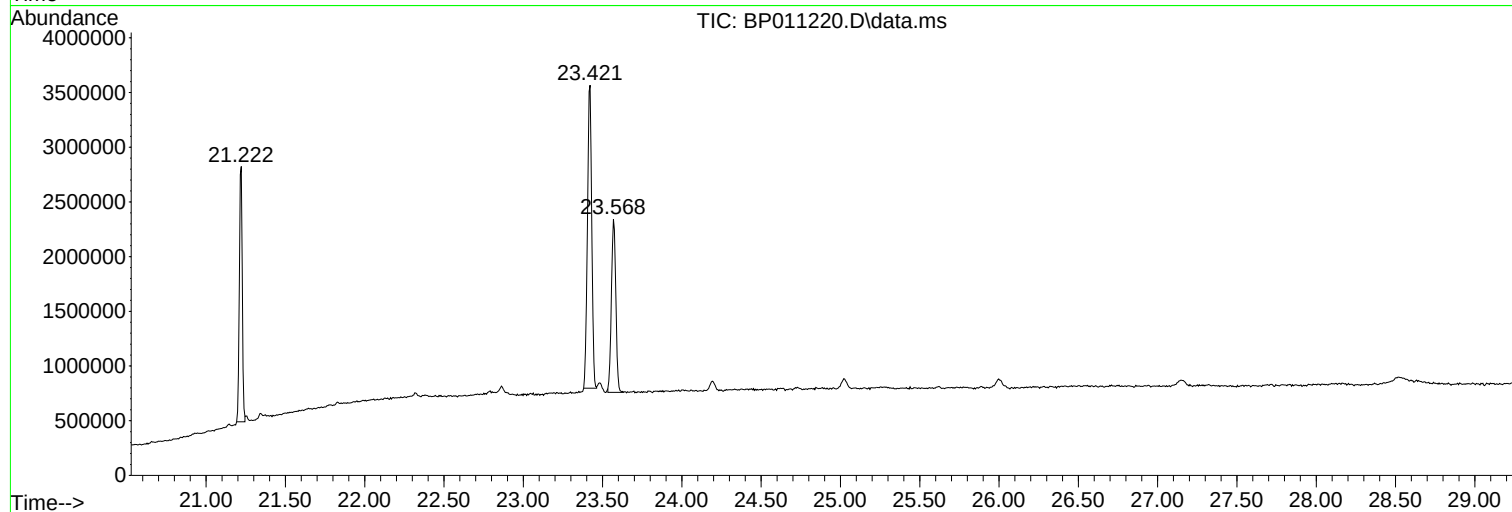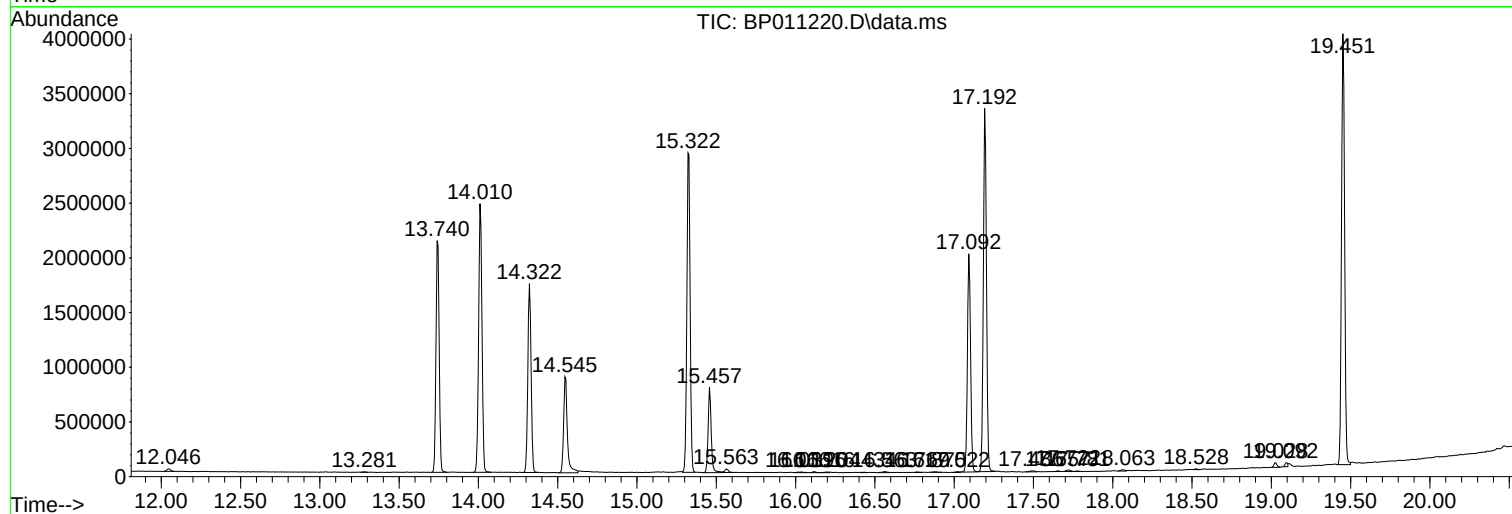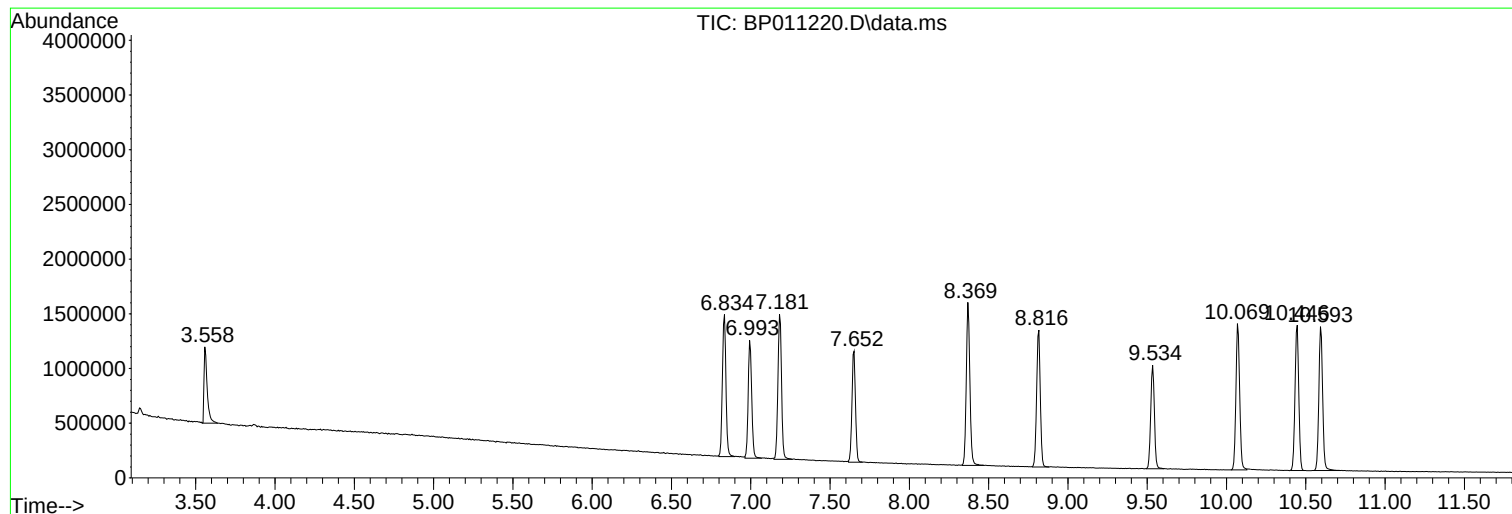

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011220.D
Acq On : 02 Aug 2022 08:23
Operator : CG/JU
Sample : PB146570BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011220.D
Acq On : 02 Aug 2022 08:23
Operator : CG/JU
Sample : PB146570BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc