

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
 Data File : BP011222.D
 Acq On : 02 Aug 2022 09:31
 Operator : CG/JU
 Sample : N3900-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	96	98	110	rVB2	99530	166185	3.29%	0.346%
2	6.828	648	653	664	rVB	188804	306640	6.07%	0.639%
3	6.987	675	680	688	rVB	836600	1292010	25.55%	2.691%
4	7.175	707	712	722	rVB	724834	1149319	22.73%	2.394%
5	7.646	786	792	800	rVB	1014325	1543406	30.53%	3.215%
6	8.363	908	914	929	rVB	514691	849859	16.81%	1.770%
7	8.810	983	990	997	rBV	991538	1594783	31.54%	3.322%
8	9.528	1106	1112	1126	rVB	684097	1083372	21.43%	2.257%
9	10.063	1197	1203	1216	rBV	908529	1486646	29.40%	3.097%
10	10.440	1260	1267	1276	rVB	1343359	2173318	42.99%	4.527%
11	10.587	1285	1292	1309	rBV	869381	1489279	29.46%	3.102%
12	12.040	1535	1539	1545	rVB4	15216	25334	0.50%	0.053%
13	12.916	1685	1688	1694	rVB7	5747	8266	0.16%	0.017%
14	13.134	1721	1725	1731	rVB4	12892	18771	0.37%	0.039%
15	13.275	1743	1749	1753	rVB8	4817	9269	0.18%	0.019%
16	13.734	1820	1827	1837	rBV	1797960	2429886	48.06%	5.062%
17	14.004	1866	1873	1886	rBV	1983485	2823539	55.85%	5.882%
18	14.228	1907	1911	1915	rVB5	5165	7010	0.14%	0.015%
19	14.316	1919	1926	1936	rBV	1615813	2368267	46.84%	4.934%
20	14.545	1958	1965	1975	rBV2	55154	125919	2.49%	0.262%
21	14.751	1992	2000	2001	rBV8	4154	7240	0.14%	0.015%
22	15.128	2060	2064	2067	rBV5	5242	7579	0.15%	0.016%
23	15.316	2088	2096	2112	rBV	2440033	3382576	66.90%	7.047%
24	15.451	2113	2119	2132	rVV	617141	812202	16.06%	1.692%
25	15.557	2132	2137	2142	rVB3	22714	33972	0.67%	0.071%
26	16.110	2227	2231	2235	rBV7	9046	10888	0.22%	0.023%
27	16.763	2338	2342	2345	rBV5	5905	9160	0.18%	0.019%
28	16.863	2355	2359	2366	rBV8	5964	14328	0.28%	0.030%
29	17.086	2389	2397	2403	rBV	1859261	2508507	49.62%	5.226%
30	17.186	2407	2414	2423	rBV	3008026	4104236	81.18%	8.550%
31	18.292	2594	2602	2603	rBV8	5800	13051	0.26%	0.027%
32	19.022	2721	2726	2731	rBV2	39703	58331	1.15%	0.122%
33	19.086	2734	2737	2741	rVV	31467	41987	0.83%	0.087%
34	19.445	2792	2798	2806	rBV	3833877	4825724	95.45%	10.053%
35	19.769	2850	2853	2859	rBV3	68185	93231	1.84%	0.194%
36	20.945	3049	3053	3060	rBV4	158742	294787	5.83%	0.614%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011222.D
Acq On : 02 Aug 2022 09:31
Operator : CG/JU
Sample : N3900-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C98

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Title : SVOA CALIBRATION

37	21.210	3094	3098	3108	rBV2	2301339	2791131	55.21%	5.814%
38	23.404	3465	3471	3478	rBV2	2644188	5055847	100.00%	10.532%
39	23.557	3491	3497	3506	rVB2	1524727	2987590	59.09%	6.224%




Sum of corrected areas: 48003445

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011222.D
Acq On : 02 Aug 2022 09:31
Operator : CG/JU
Sample : N3900-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

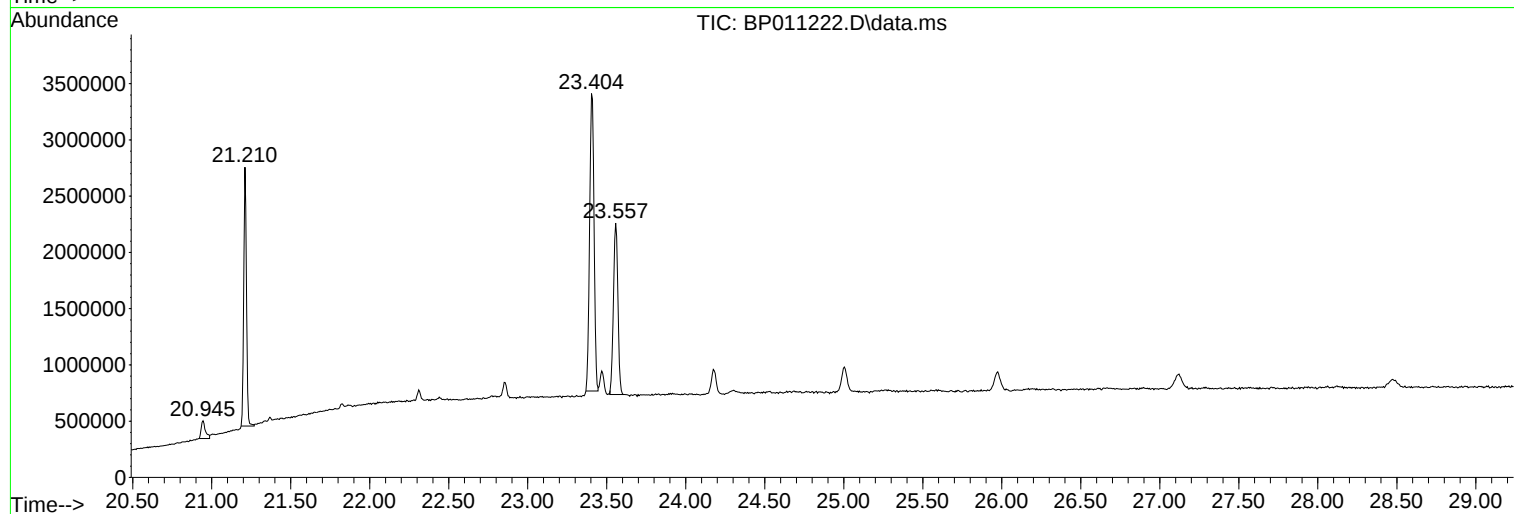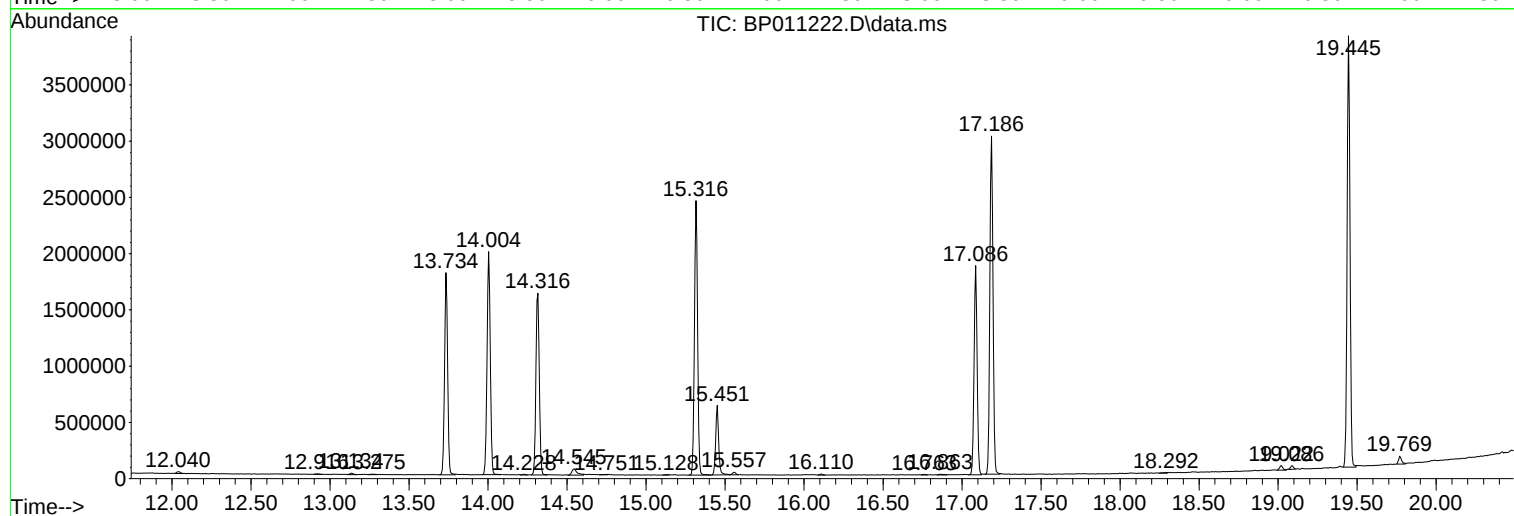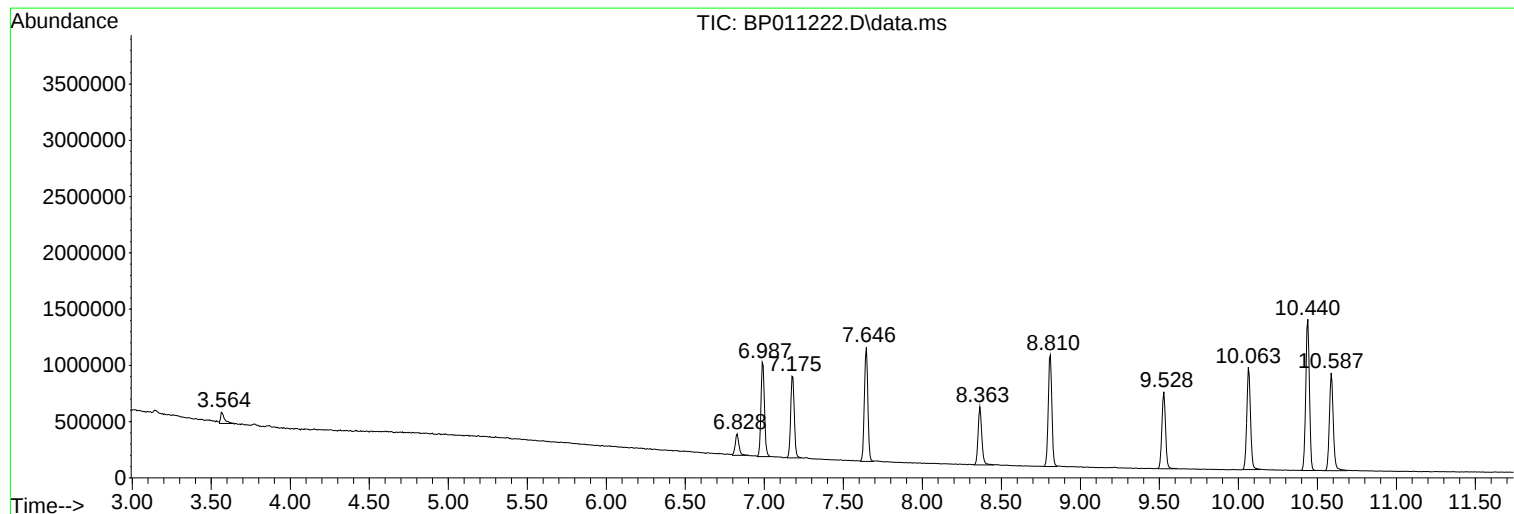

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011222.D
Acq On : 02 Aug 2022 09:31
Operator : CG/JU
Sample : N3900-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.945	2.11 ng/ul	294787	Chrysene-d12	21.210

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		9-Tricosene, (Z)-	322	C23H46	027519-02-4	97
2		9-Tricosene, (Z)-	322	C23H46	027519-02-4	97
3		Octadecane, 1-(ethenyloxy)-	296	C20H40O	000930-02-9	94
4		Ethyl triacontyl ether	467	C32H66O	1000406-37-1	93
5		Behenic alcohol	326	C22H46O	000661-19-8	93

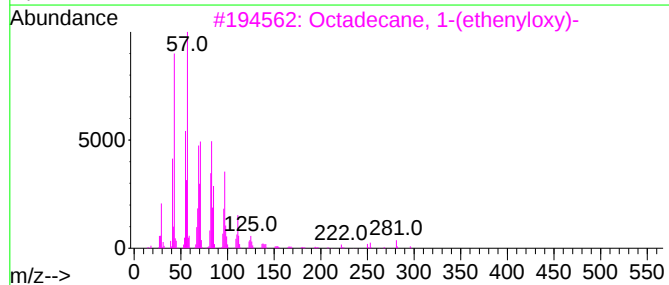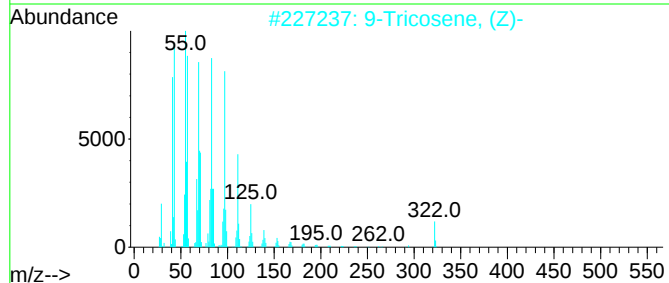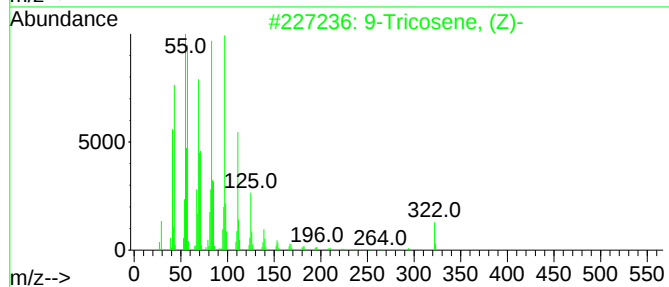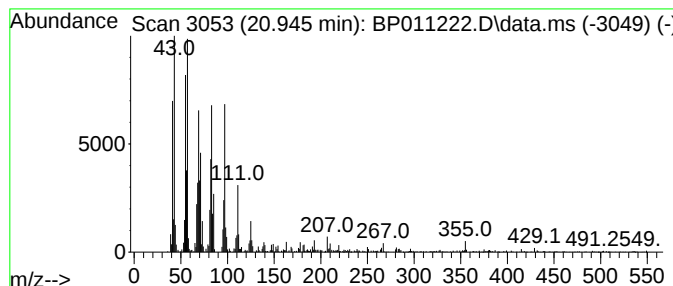

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080122\
Data File : BP011222.D
Acq On : 02 Aug 2022 09:31
Operator : CG/JU
Sample : N3900-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.945	2.1	ng/u1	294787	5	21.210	2791130	20.0