
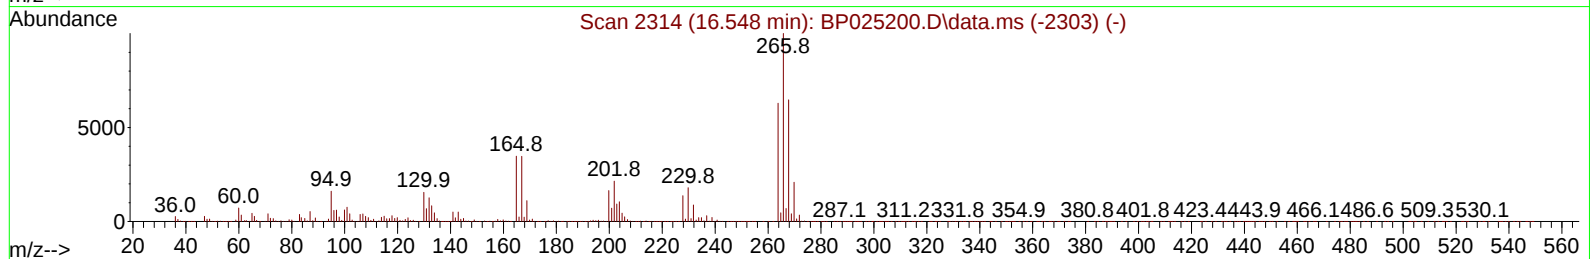
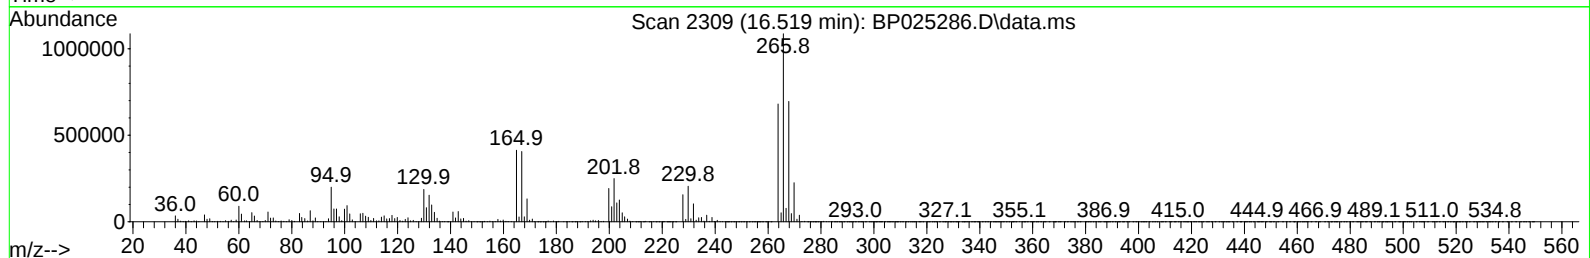


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080125\
Data File : BP025286.D
Acq On : 01 Aug 2025 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 10:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

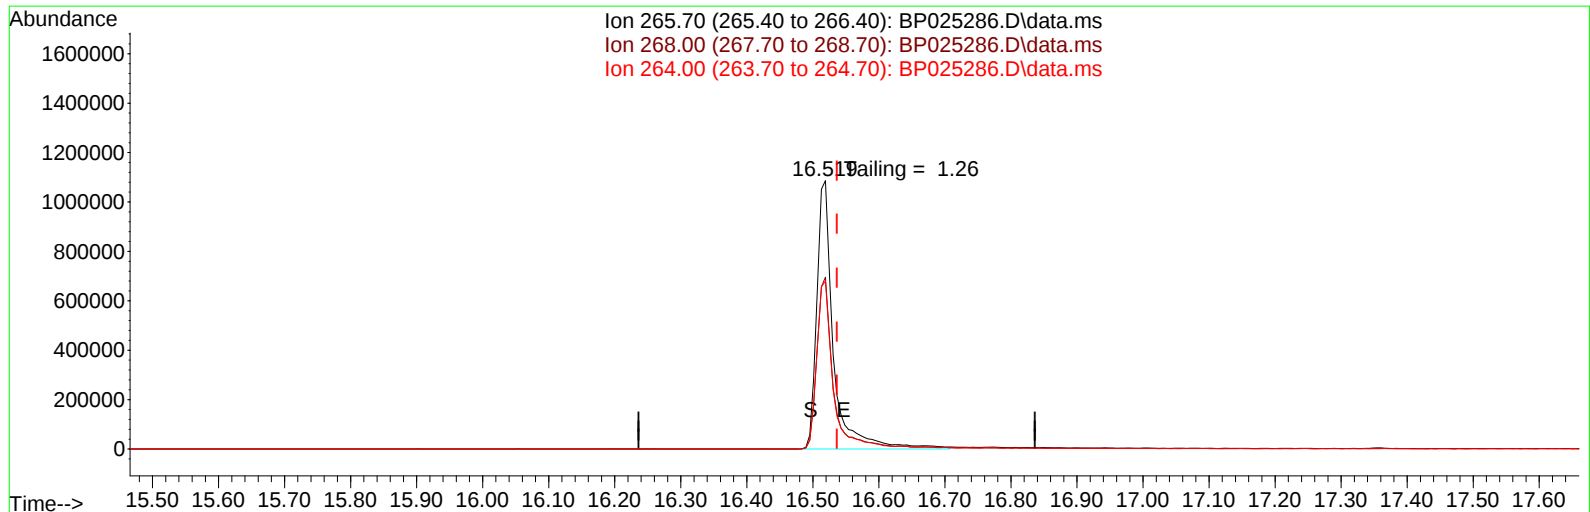

TIC: BP025286.D\data.ms

(70) Pentachlorophenol (C)




16.519min (-0.017) 142404.63 ng

response 1884342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.03
264.00	62.90	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080125\
Data File : BP025286.D
Acq On : 01 Aug 2025 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 10:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

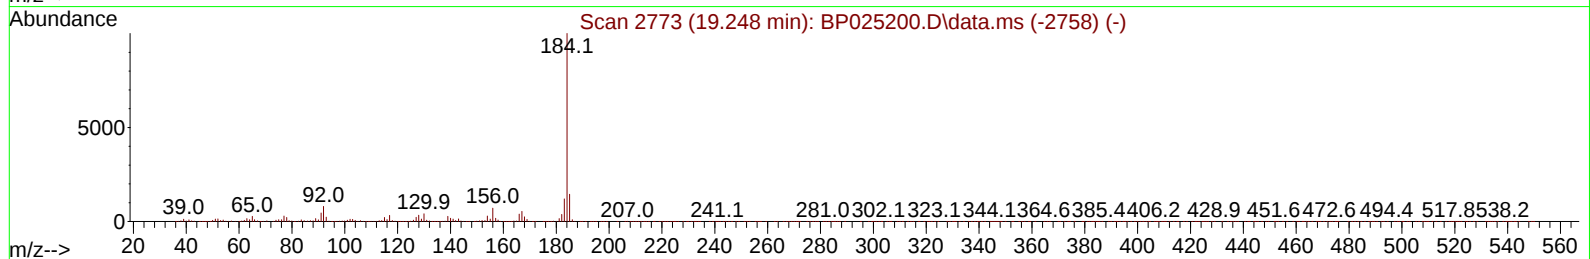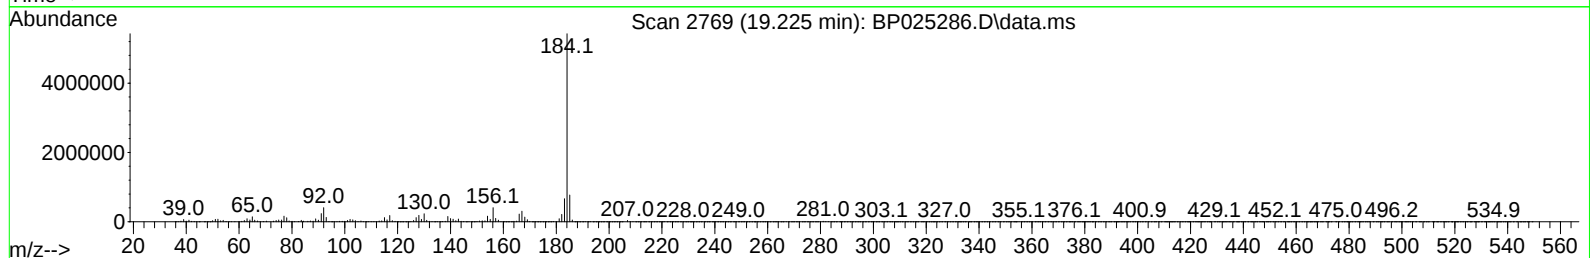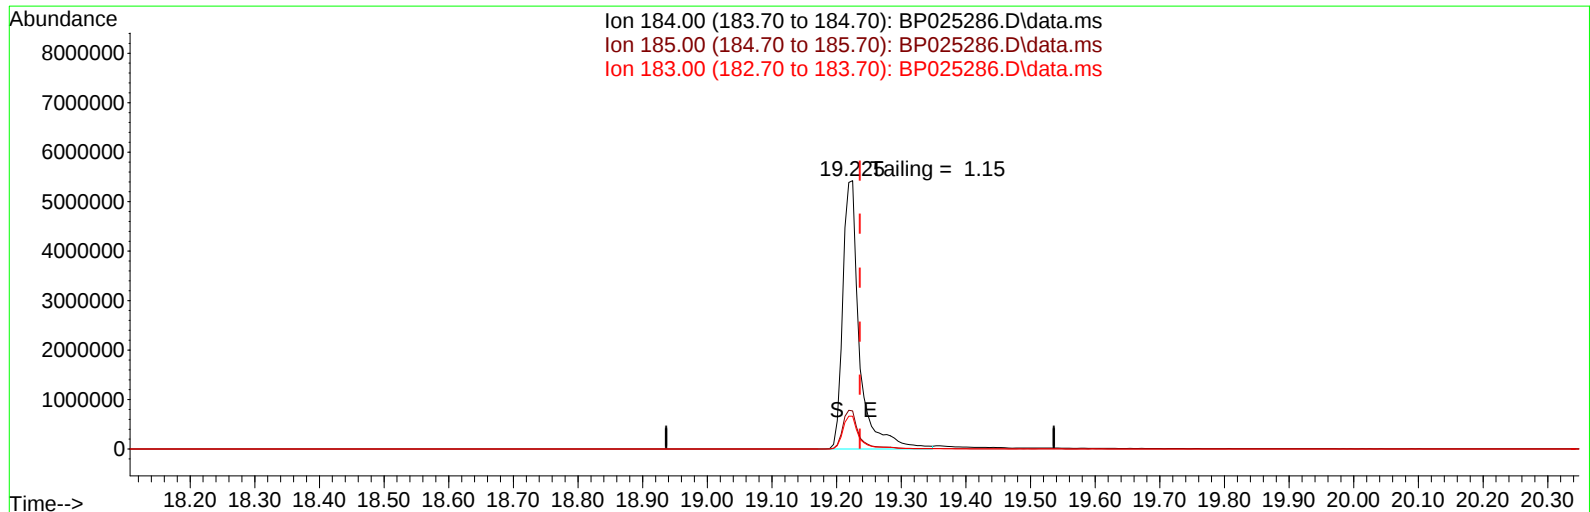

TIC: BP025286.D\data.ms

(77) Benzidine

19.225min (-0.012) 72346.12 ng

response 9788858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	12.00	12.22
0.00	0.00	0.00