


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080125\
Data File : BP025286.D
Acq On : 01 Aug 2025 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 29 15:28:11 2025

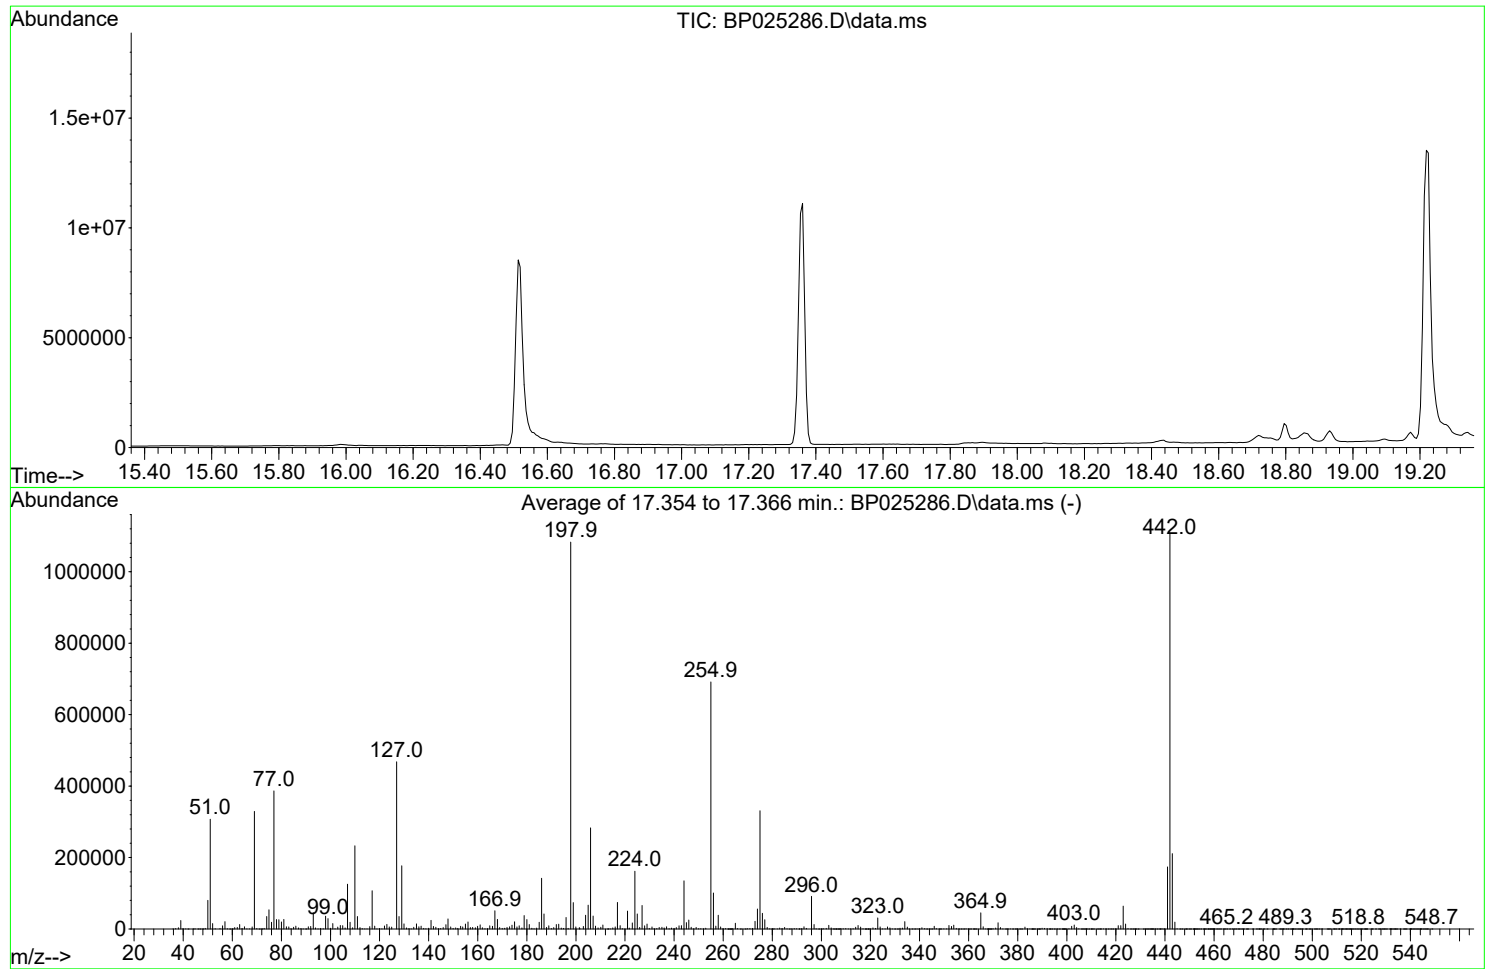

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2440

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	5833	PASS
69	69	100	100	100.0	329093	PASS
70	69	0.00	2	0.5	1599	PASS
197	198	0.00	2	0.2	1967	PASS
198	198	100	100	100.0	1082951	PASS
199	198	5	9	6.8	73932	PASS
365	198	1	100	4.2	45112	PASS
441	443	0.01	150	82.4	173803	PASS
442	442	100	100	100.0	1105195	PASS
443	442	15	24	19.1	210897	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2025	BNA_P	<u>BP025286.D</u>
Compound Name	Response	Retention Time
DDT	4266243	20.53
DDD	119250	20.066
DDE	8464	19.525
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
127714	4393957	2.91

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080125\
Data File : BP025286.D
Acq On : 01 Aug 2025 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 01 10:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

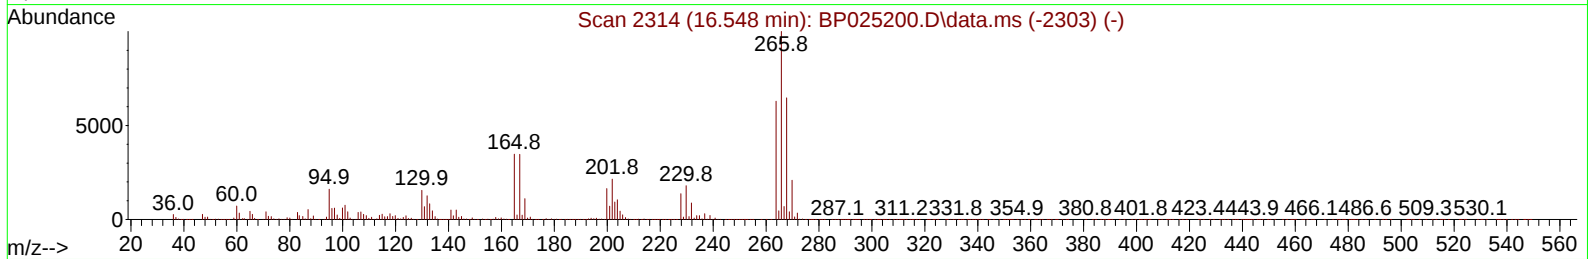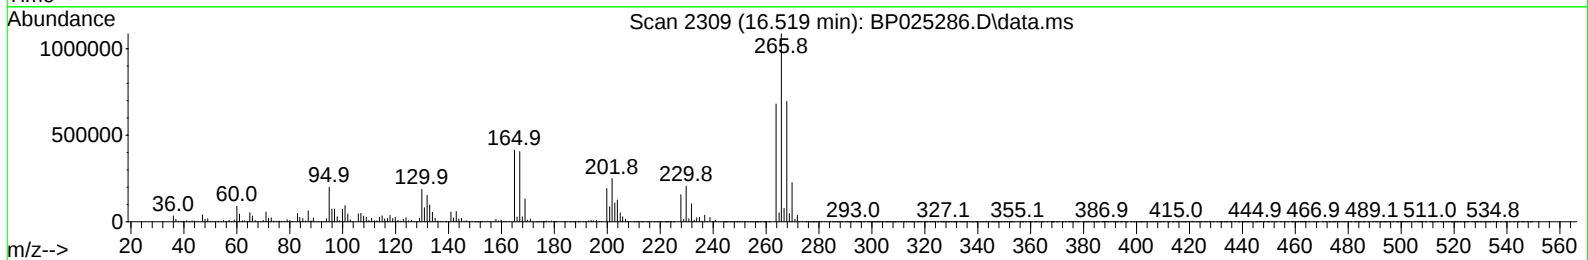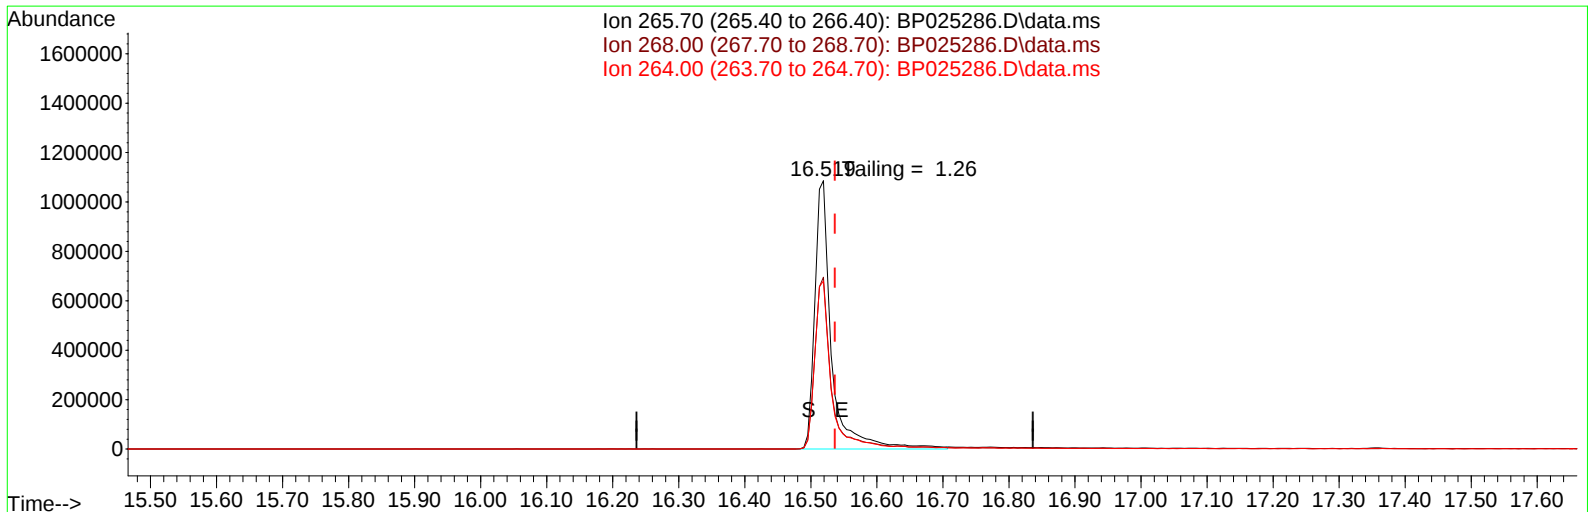

TIC: BP025286.D\data.ms

(70) Pentachlorophenol (C)

16.519min (-0.017) 142404.63 ng




response 1884342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.03
264.00	62.90	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080125\
Data File : BP025286.D
Acq On : 01 Aug 2025 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 01 10:52:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 29 15:28:11 2025
Response via : Initial Calibration

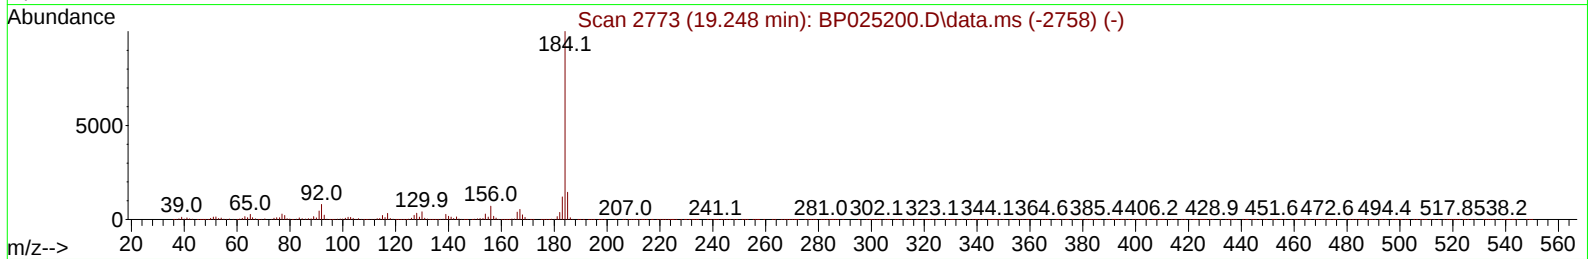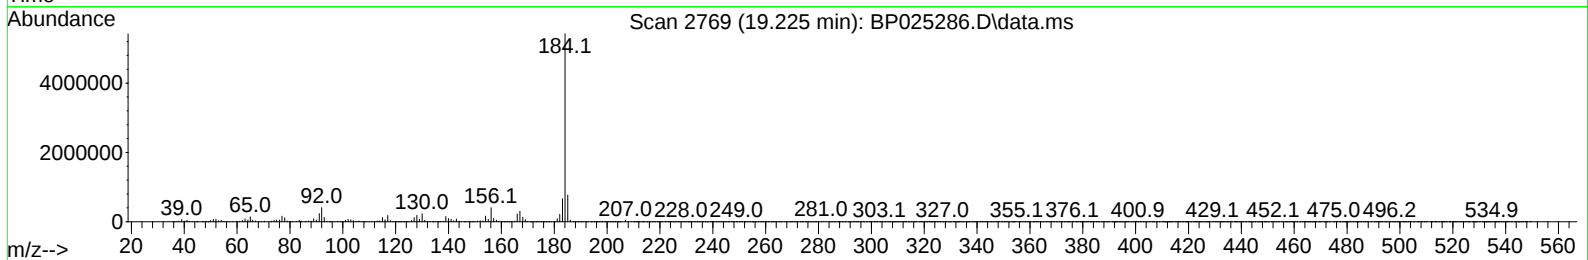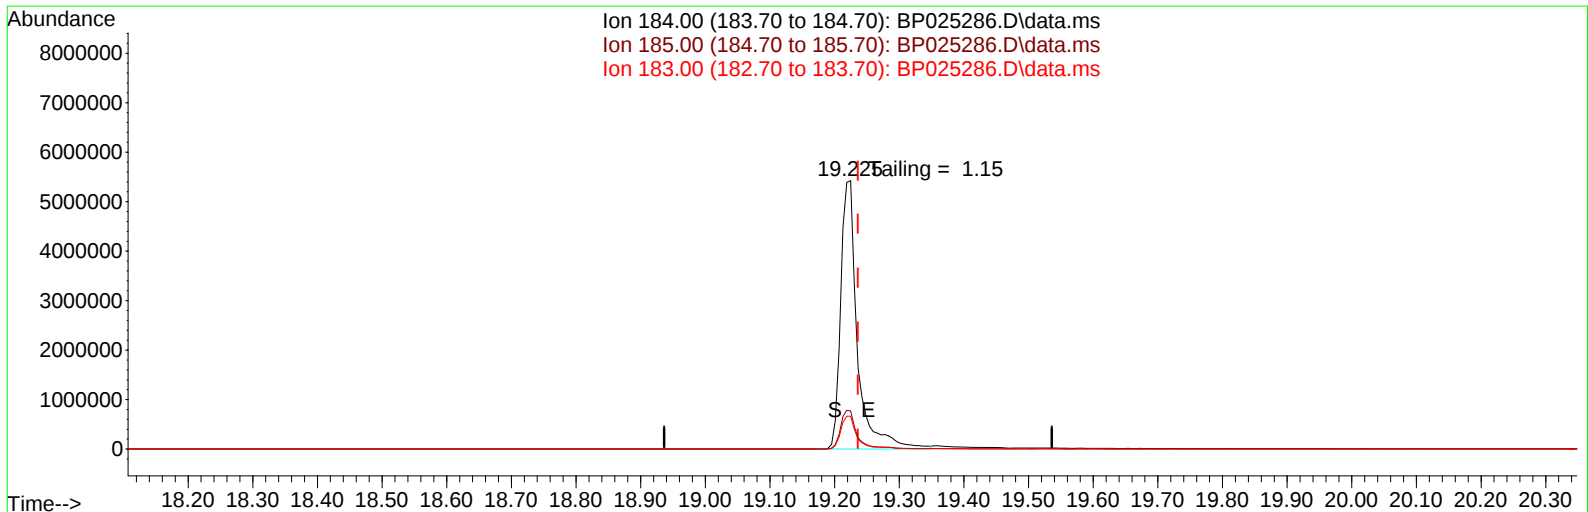

TIC: BP025286.D\data.ms

(77) Benzidine

19.225min (-0.012) 72346.12 ng

response 9788858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.19
183.00	12.00	12.22
0.00	0.00	0.00