
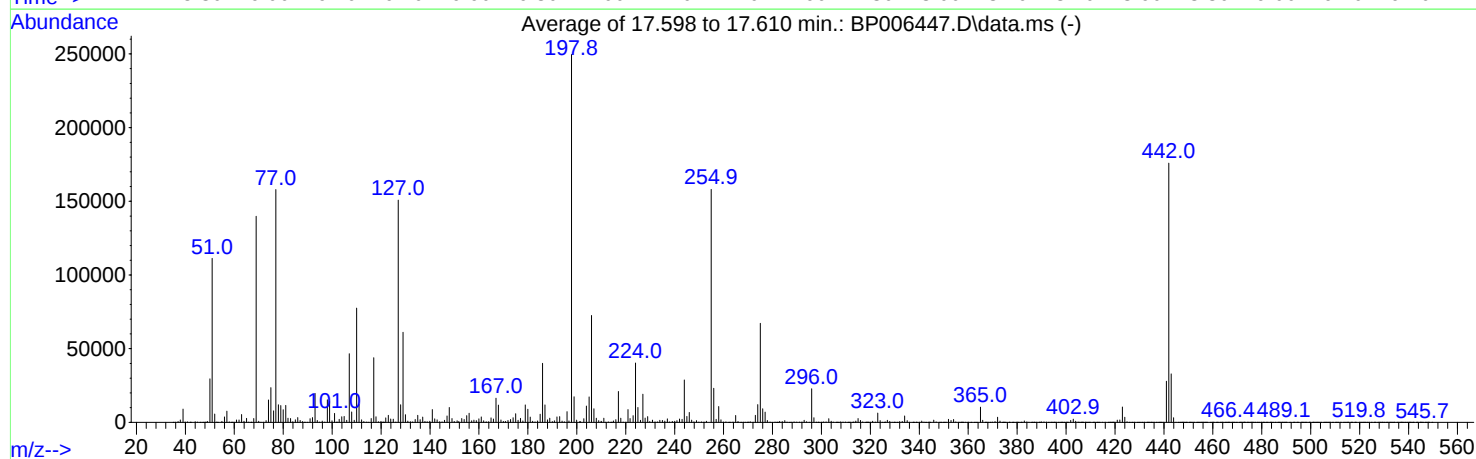


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP080221\  
 Data File : BP006447.D  
 Acq On : 02 Aug 2021 12:21  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP080221.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 02 19:55:20 2021

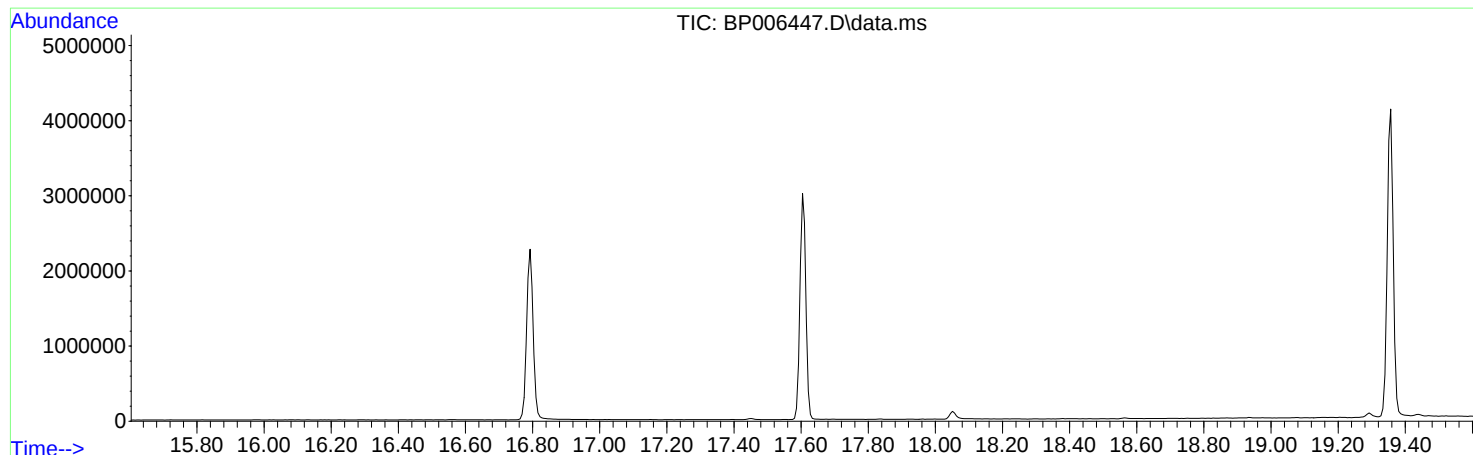


AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2455

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 44.6         | 111256     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 2636       | PASS                |
| 69             | 198             | 0.00            | 100             | 56.0         | 139796     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 777        | PASS                |
| 127            | 198             | 10              | 80              | 60.4         | 150814     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 993        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 249613     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 17342      | PASS                |
| 275            | 198             | 10              | 60              | 26.9         | 67235      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 10265      | PASS                |
| 441            | 198             | 0.01            | 100             | 11.2         | 27867      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 175916     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 32944      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP080221\  
Data File : BP006447.D  
Acq On : 02 Aug 2021 12:21  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Aug 02 16:02:04 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP080221.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 02 15:59:11 2021  
Response via : Initial Calibration

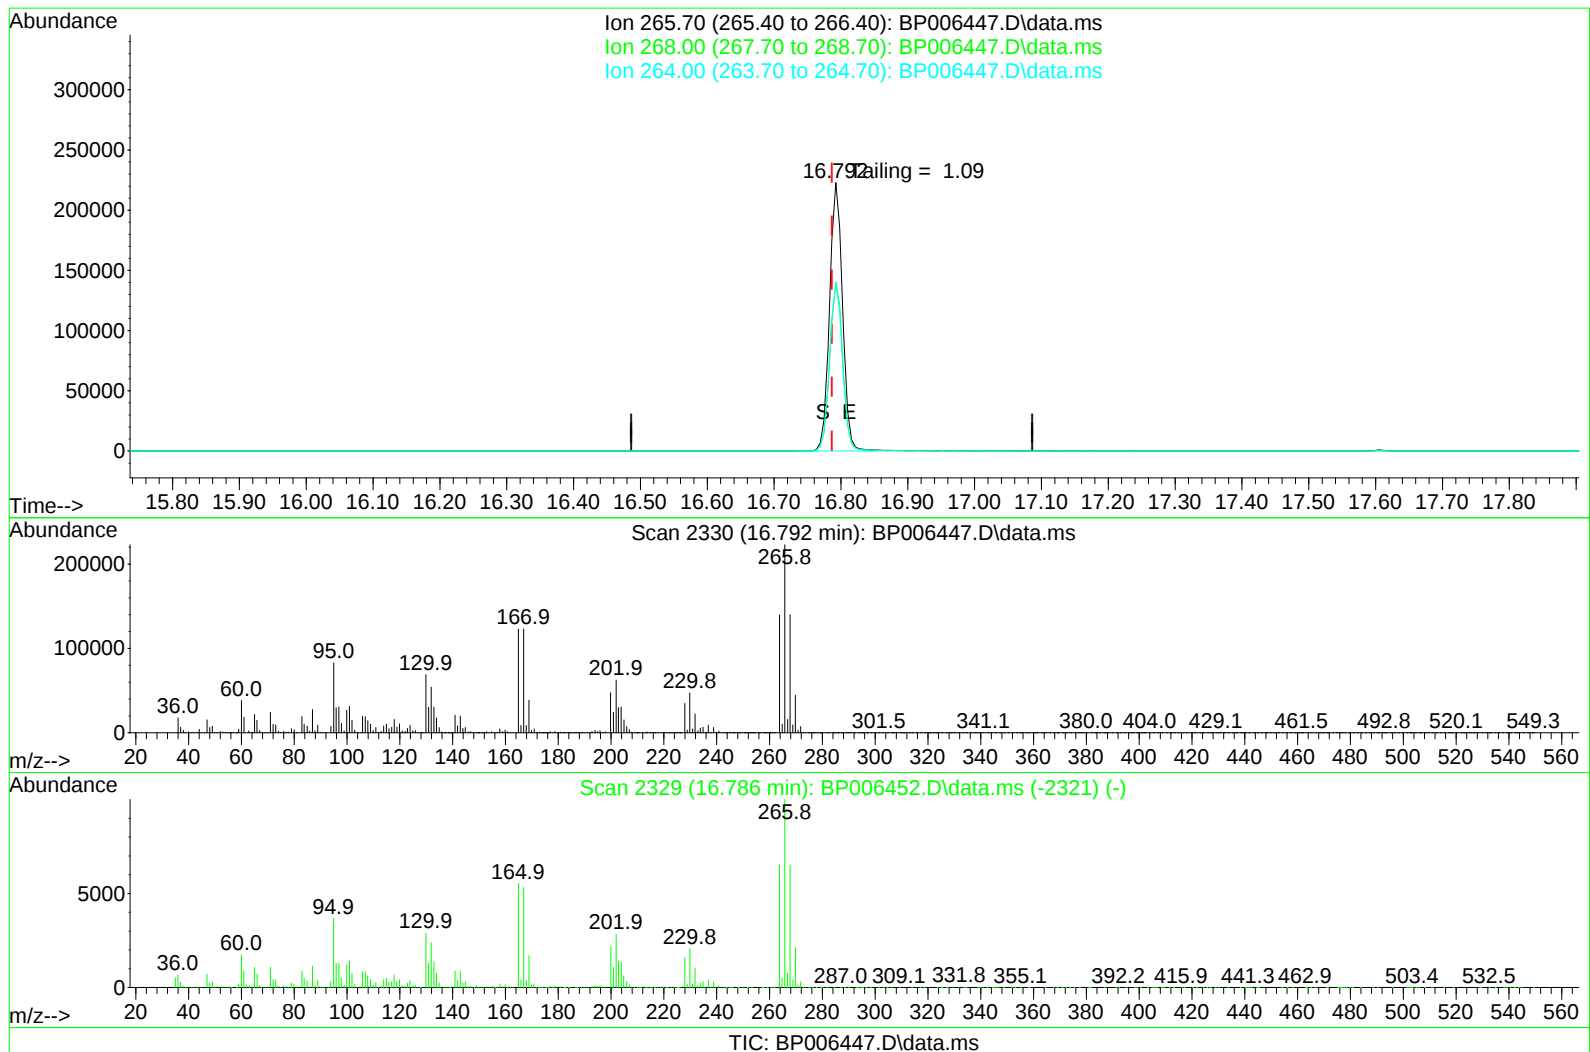

(70) Pentachlorophenol (C)

16.792min (+ 0.006) 2808661.94 ng




response 301279

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 62.82  |
| 264.00 | 62.90  | 62.73  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP080221\  
 Data File : BP006447.D  
 Acq On : 02 Aug 2021 12:21  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 02 16:02:04 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP080221.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 02 15:59:11 2021  
 Response via : Initial Calibration

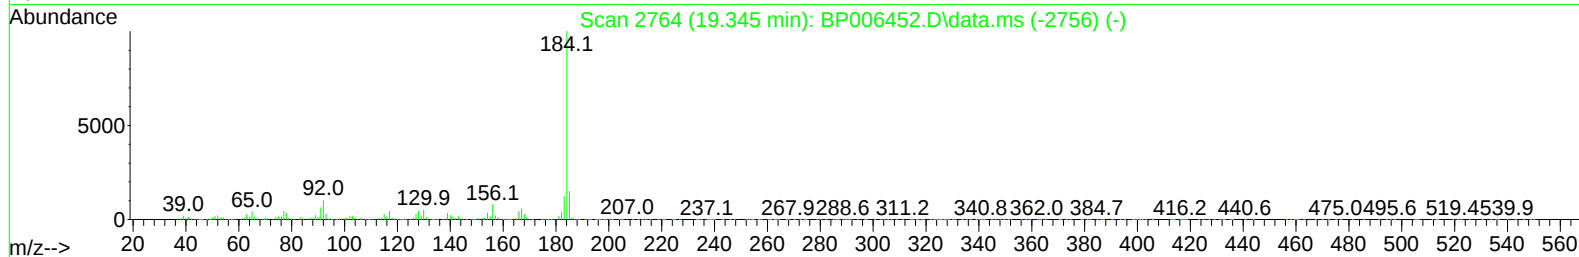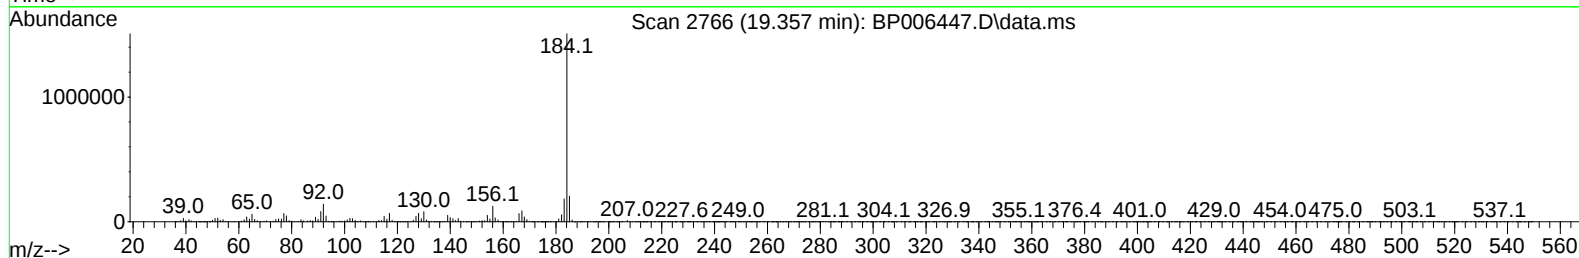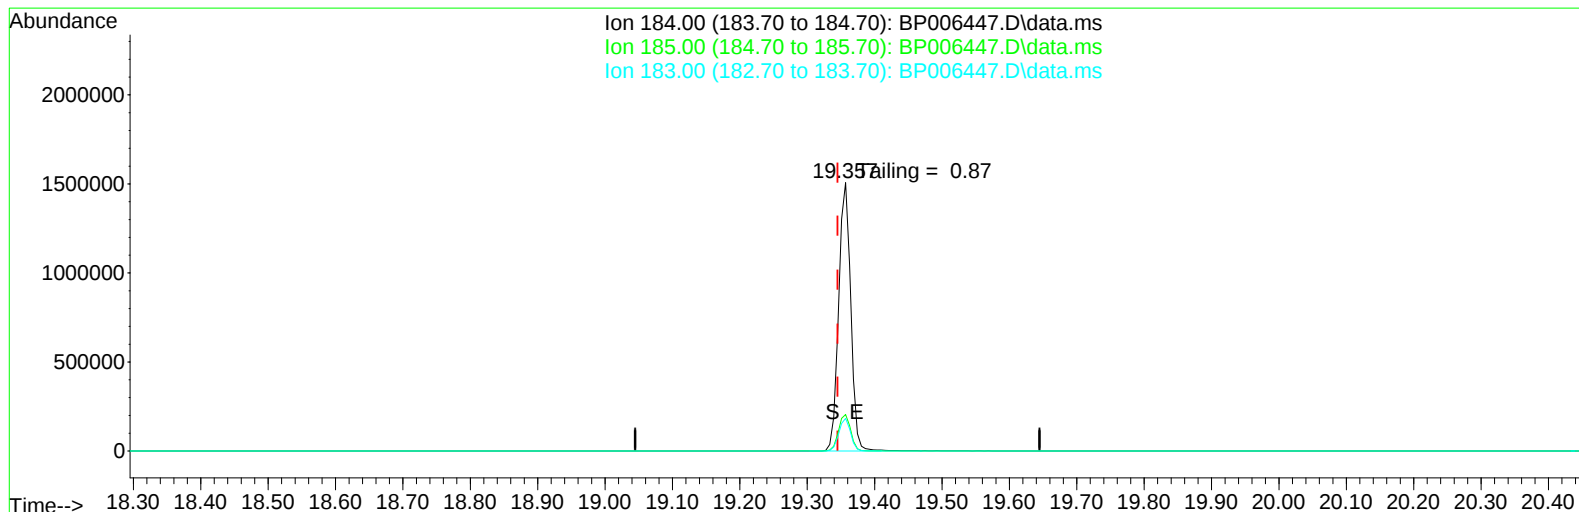

TIC: BP006447.D\data.ms

**(77) Benzidine**

**19.357min (+ 0.012) 5542529.71 ng**

**response 1880677**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.70  | 13.61  |
| 183.00 | 11.90  | 12.16  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/8/2021      | BNA_P            | <u>BP006447.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 908012           | 20.56              |
| DDD           | 2670             | 20.18              |
| DDE           | 1000             | 19.63              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3670          | 911682           | 0.40               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP