
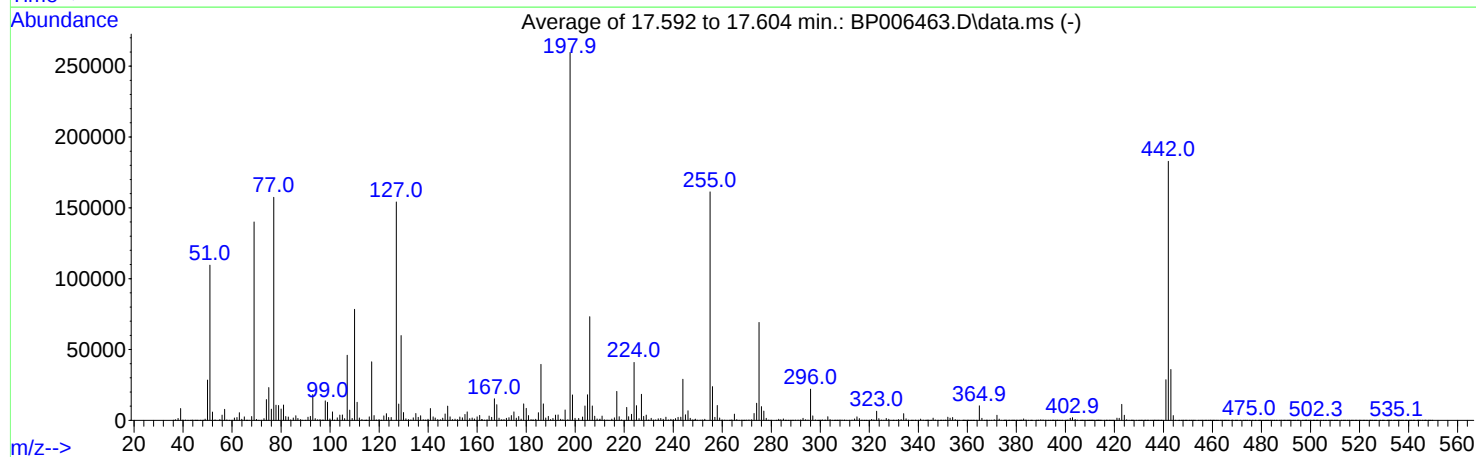


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080221\
 Data File : BP006463.D
 Acq On : 02 Aug 2021 22:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 19:55:20 2021

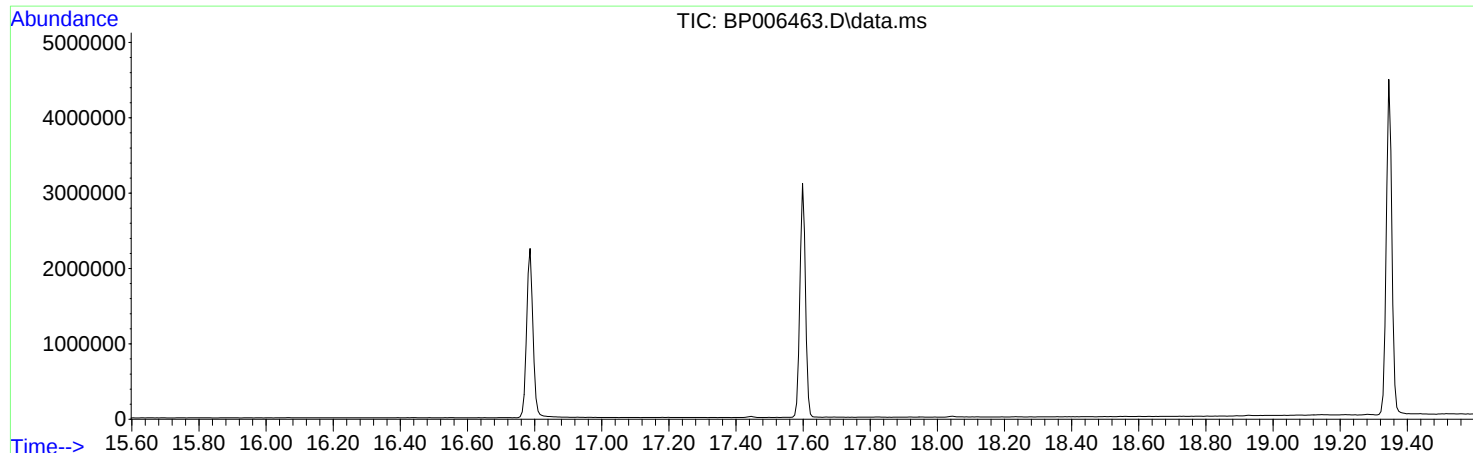




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	109565	PASS
68	69	0.00	2	1.9	2694	PASS
69	198	0.00	100	53.9	140005	PASS
70	69	0.00	2	0.5	726	PASS
127	198	10	80	59.4	154121	PASS
197	198	0.00	2	0.2	458	PASS
198	198	100	100	100.0	259637	PASS
199	198	5	9	6.9	17911	PASS
275	198	10	60	26.6	69129	PASS
365	198	1	100	3.9	10231	PASS
441	198	0.01	100	11.0	28685	PASS
442	442	100	100	100.0	182871	PASS
443	442	15	24	19.6	35933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080221\
Data File : BP006463.D
Acq On : 02 Aug 2021 22:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:02:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 19:55:20 2021
Response via : Initial Calibration

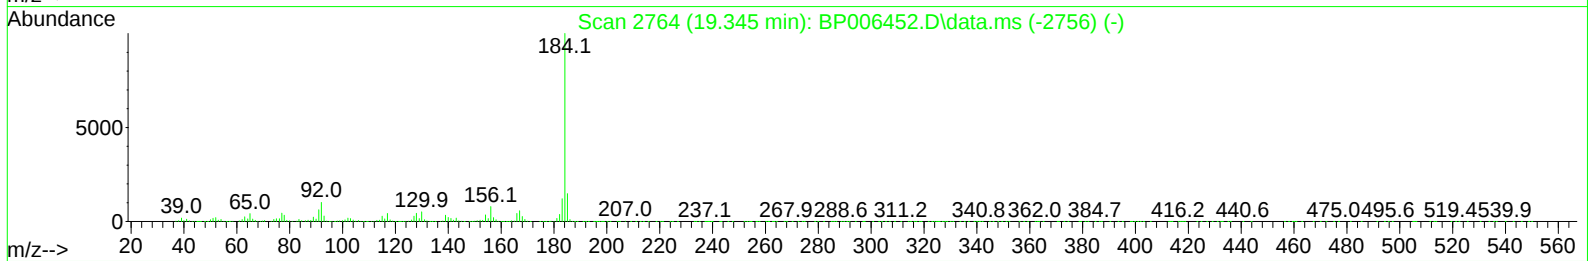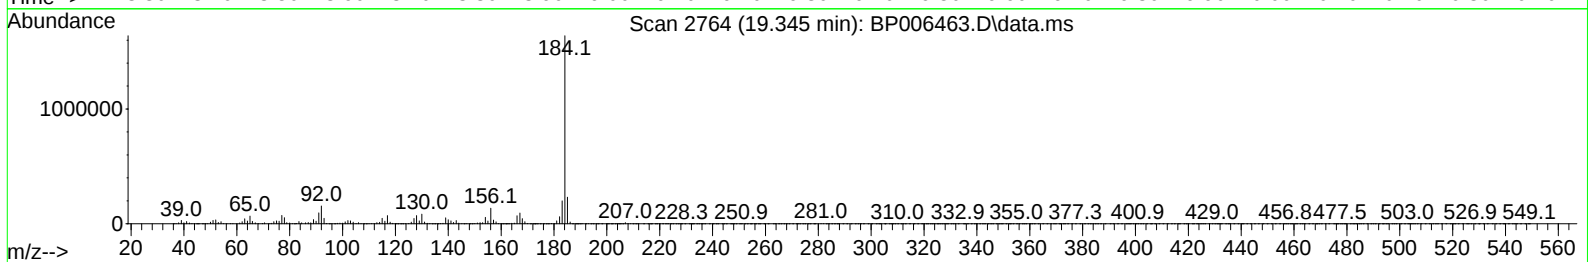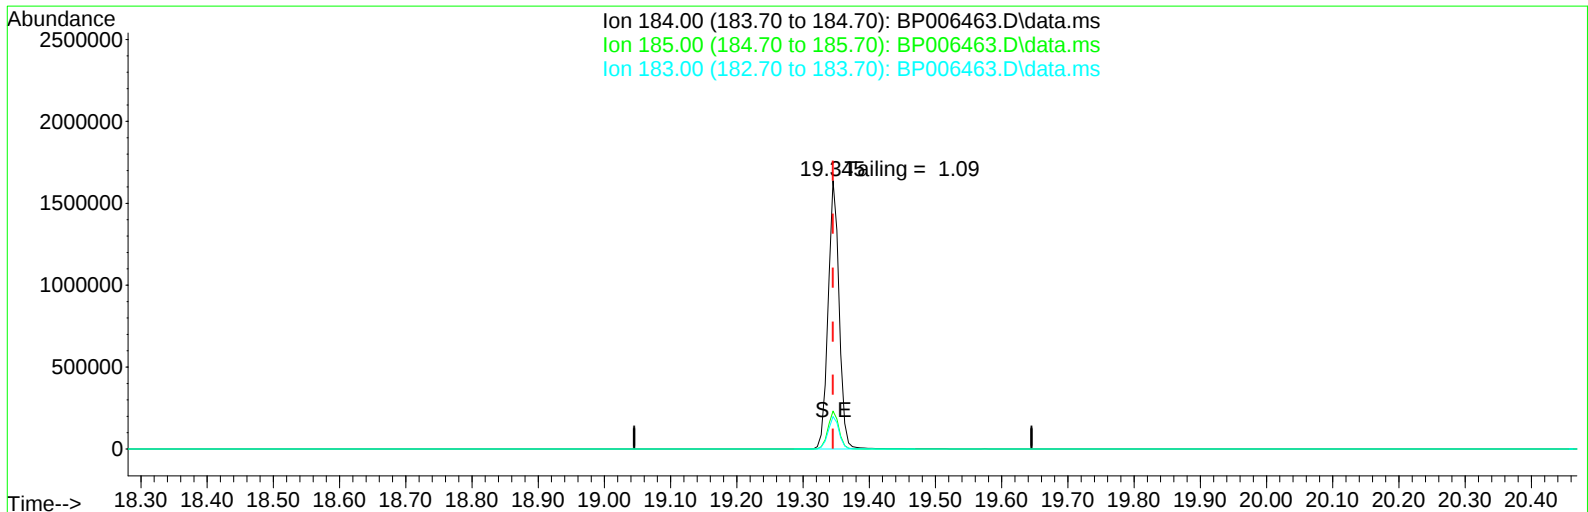

TIC: BP006463.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 47869.81 ng




response 1900493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.12
183.00	11.90	12.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080221\
Data File : BP006463.D
Acq On : 02 Aug 2021 22:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:02:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 19:55:20 2021
Response via : Initial Calibration

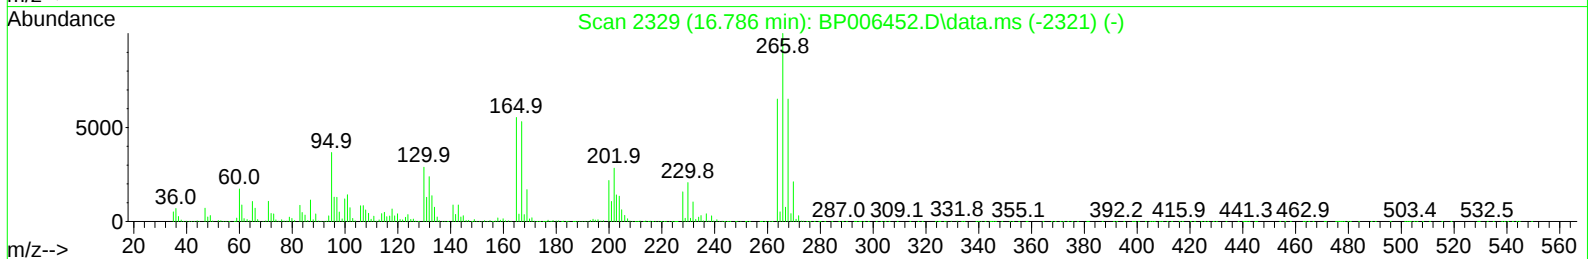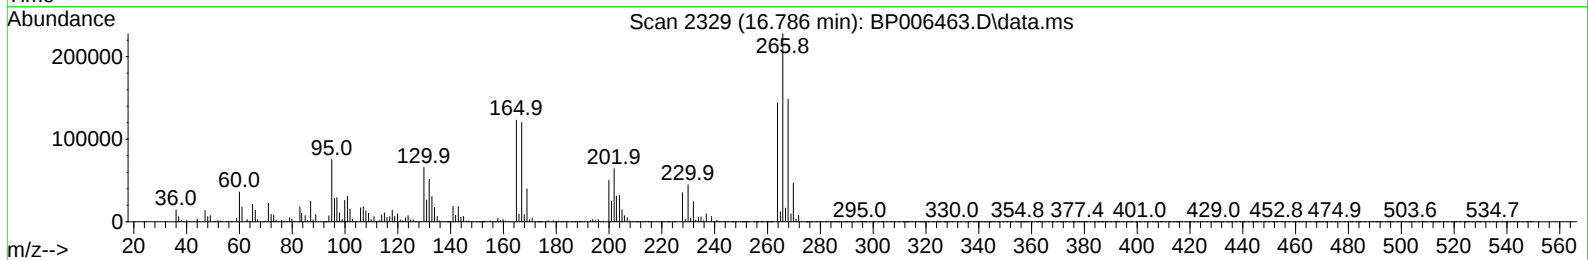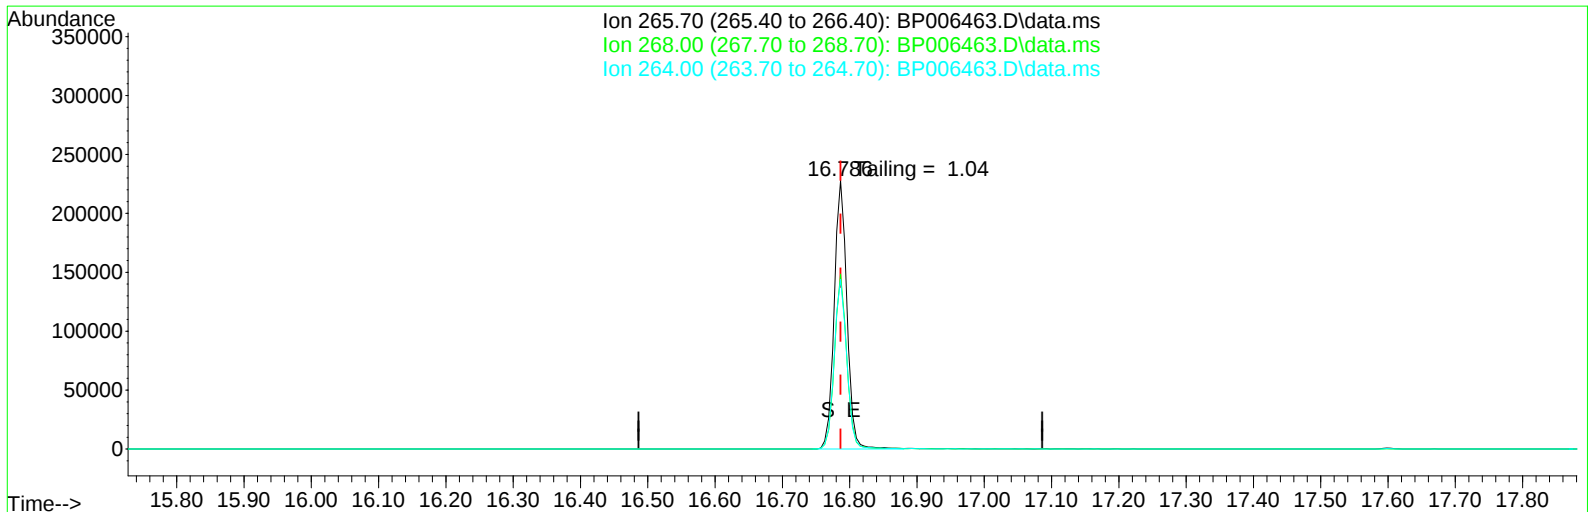

TIC: BP006463.D\data.ms

(70) Pentachlorophenol (C)

16.786min (+ 0.000) 102715.13 ng

response 299408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.19
264.00	62.90	63.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2021	BNA_P	<u>BP006463.D</u>
Compound Name	Response	Retention Time
DDT	908622	20.551
DDD	6474	20.122
DDE	1095	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7569	916191	0.83

Instrument :
BNA_P
ClientSampleId :
DFTPP