

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080222\
 Data File : BP011227.D
 Acq On : 02 Aug 2022 15:57
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020726

Quant Time: Aug 02 23:17:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:11:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.646	152	228669	20.000	ng/u1	0.04
20) Naphthalene-d8	10.440	136	1037536	20.000	ng/u1	0.04
38) Acenaphthene-d10	14.316	164	544948	20.000	ng/u1	0.04
64) Phenanthrene-d10	17.086	188	976571	20.000	ng/u1	0.04
79) Chrysene-d12	21.210	240	911684	20.000	ng/u1	0.04
88) Perylene-d12	23.551	264	1032731	20.000	ng/u1	0.06
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	30782	6.165	ng/uL	0.05
4) Pyridine-d5	3.552	84	160817	11.384	ng/u1	0.05
7) Phenol-d5	6.828	99	379474	19.012	ng/u1	0.04
9) Bis-(2-Chloroethyl)eth...	6.987	67	283192	20.066	ng/u1	0.04
11) 2-Chlorophenol-d4	7.175	132	317531	20.188	ng/u1	0.04
15) 4-Methylphenol-d8	8.363	113	315704	19.336	ng/u1	0.04
21) Nitrobenzene-d5	8.810	128	153648	19.055	ng/u1	0.04
24) 2-Nitrophenol-d4	9.528	143	145111	18.788	ng/u1	0.04
28) 2,4-Dichlorophenol-d3	10.063	165	271824	19.970	ng/u1	0.04
31) 4-Chloroaniline-d4	10.587	131	407567	18.470	ng/u1	0.04
46) Dimethylphthalate-d6	13.734	166	729829	19.657	ng/u1	0.04
49) Acenaphthylene-d8	14.004	160	944267	20.239	ng/u1	0.04
54) 4-Nitrophenol-d4	14.539	143	114456	17.138	ng/u1	0.04
60) Fluorene-d10	15.316	176	622743	19.961	ng/u1	0.04
65) 4,6-Dinitro-2-methylph...	15.451	200	80243	16.300	ng/u1	0.04
73) Anthracene-d10	17.186	188	872711	20.281	ng/u1	0.04
81) Pyrene-d10	19.445	212	937863	19.144	ng/u1	0.04
92) Benzo(a)pyrene-d12	23.398	264	1021150	19.907	ng/u1	0.05
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.175	88	22003	4.257	ng/uL	95
5) Pyridine	3.569	79	161990	11.117	ng/u1	100
6) Benzaldehyde	6.793	77	160238	16.643	ng/u1	100
8) Phenol	6.852	94	411482	19.216	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.081	93	345135	19.879	ng/u1	99
12) 2-Chlorophenol	7.210	128	333260	20.379	ng/u1	99
13) 2-Methylphenol	8.099	108	313098	19.728	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.175	45	361860	12.444	ng/u1	99
16) Acetophenone	8.475	105	531479	20.927	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.463	70	261730	19.495	ng/u1	98
18) 4-Methylphenol	8.428	108	341424	19.975	ng/u1	97
19) Hexachloroethane	8.710	117	155188	21.126	ng/u1	98
22) Nitrobenzene	8.852	77	413455	19.944	ng/u1	97
23) Isophorone	9.381	82	738957	19.701	ng/u1	98
25) 2-Nitrophenol	9.557	139	169616	19.543	ng/u1	94
26) 2,4-Dimethylphenol	9.628	107	376785	20.209	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.869	93	463075	19.649	ng/u1	98
29) 2,4-Dichlorophenol	10.093	162	282089	20.038	ng/u1	99
30) Naphthalene	10.487	128	1105243	20.248	ng/u1	100
32) 4-Chloroaniline	10.610	127	423985	19.337	ng/u1	99
33) Hexachlorobutadiene	10.769	225	174989	20.353	ng/u1	98
34) Caprolactam	11.410	113	75743	16.178	ng/u1	97
35) 4-Chloro-3-methylphenol	11.751	107	316327	20.041	ng/u1	99
36) 2-Methylnaphthalene	12.110	142	686855	19.884	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080222\
 Data File : BP011227.D
 Acq On : 02 Aug 2022 15:57
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020726

Quant Time: Aug 02 23:17:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:11:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.334	142	694878	20.080	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.487	216	299581	19.759	ng/ul	97
40) Hexachlorocyclopentadiene	12.457	237	202092	20.218	ng/ul	98
41) 2,4,6-Trichlorophenol	12.740	196	191422	20.106	ng/ul	100
42) 2,4,5-Trichlorophenol	12.810	196	201292	19.973	ng/ul	99
43) 1,1'-Biphenyl	13.140	154	873972	20.072	ng/ul	99
44) 2-Chloronaphthalene	13.181	162	652552	20.047	ng/ul	99
45) 2-Nitroaniline	13.398	65	157901	16.691	ng/ul	96
47) Dimethylphthalate	13.787	163	733392	19.614	ng/ul	99
48) 2,6-Dinitrotoluene	13.904	165	114542	17.531	ng/ul	99
50) Acenaphthylene	14.034	152	1063606	20.406	ng/ul	100
51) 3-Nitroaniline	14.240	138	97076	13.758	ng/ul	93
52) Acenaphthene	14.381	153	685603	20.138	ng/ul	99
53) 2,4-Dinitrophenol	14.445	184	65004	17.641	ng/ul	95
55) 4-Nitrophenol	14.557	109	105035	18.304	ng/ul	95
56) Dibenzofuran	14.716	168	929601	20.088	ng/ul	99
57) 2,4-Dinitrotoluene	14.698	165	179697	19.712	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	14.951	232	146640	20.010	ng/ul	98
59) Diethylphthalate	15.157	149	754003	20.176	ng/ul	99
61) Fluorene	15.375	166	725103	20.150	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.375	204	325217	19.857	ng/ul	99
63) 4-Nitroaniline	15.410	138	61536	10.258	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.463	198	86845	17.370	ng/ul	97
67) N-Nitrosodiphenylamine	15.592	169	588542	19.611	ng/ul	99
68) 4-Bromophenyl-phenylether	16.275	248	181286	19.345	ng/ul	98
69) Hexachlorobenzene	16.381	284	208586	19.457	ng/ul	99
70) Atrazine	16.563	200	165534	17.540	ng/ul	99
71) Pentachlorophenol	16.733	266	113132	18.381	ng/ul	99
72) Phenanthrene	17.128	178	1068226	19.987	ng/ul	99
74) Anthracene	17.222	178	1072500	20.284	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.098	216	304446	18.083	ng/uL	98
76) Pentachlorobenzene	14.634	250	267219	19.258	ng/uL	99
77) Carbazole	17.498	167	941352	20.095	ng/ul	98
78) Di-n-butylphthalate	18.069	149	1136494	20.288	ng/ul	99
80) Fluoranthene	19.116	202	1147818	18.968	ng/ul	99
82) Pyrene	19.475	202	1184515	19.048	ng/ul	97
83) Butylbenzylphthalate	20.369	149	454501	18.252	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.133	252	248478	15.626	ng/ul	99
85) Benzo(a)anthracene	21.192	228	1137908	20.078	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.133	149	763010	20.275	ng/ul	99
87) Chrysene	21.245	228	1120002	19.879	ng/ul	99
89) Di-n-octyl phthalate	22.045	149	1372749	19.340	ng/ul	100
90) Benzo(b)fluoranthene	22.839	252	1293937	19.875	ng/ul	99
91) Benzo(k)fluoranthene	22.886	252	1191783	19.288	ng/ul	99
93) Benzo(a)pyrene	23.445	252	1268932	19.982	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	25.974	276	1528090	19.532	ng/ul	98
95) Dibenzo(a,h)anthracene	25.992	278	1300236	19.377	ng/ul	98
96) Benzo(g,h,i)perylene	26.715	276	1317987	19.478	ng/ul	100





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 4.257 ng/uL
RT: 3.175 min Scan# 31
Delta R.T. 0.047 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion: 88 Resp: 22003
Ion Ratio Lower Upper
88 100
43 38.8 29.6 44.4
58 66.4 49.1 73.7

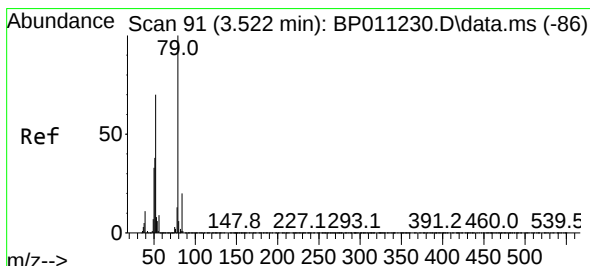

#5
Pyridine
Concen: 11.117 ng/uL
RT: 3.569 min Scan# 99
Delta R.T. 0.047 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion: 79 Resp: 161990
Ion Ratio Lower Upper
79 100
52 72.5 57.8 86.6
51 39.5 31.5 47.3









#6
Benzaldehyde
Concen: 16.643 ng/ul
RT: 6.793 min Scan# 640
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion: 77 Resp: 160238
Ion Ratio Lower Upper
77 100
105 90.4 72.0 108.0
106 86.8 69.4 104.0



#8
Phenol
Concen: 19.216 ng/ul
RT: 6.852 min Scan# 657
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion: 94 Resp: 411482
Ion Ratio Lower Upper
94 100
65 32.7 24.7 37.1
66 42.1 32.6 49.0





#10

Bis(2-Chloroethyl)ether

Concen: 19.879 ng/ul

RT: 7.081 min Scan# 696

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion: 93 Resp: 345135

Ion Ratio Lower Upper

93 100

63 87.2 71.0 106.6

95 32.4 26.0 39.0



#12

2-Chlorophenol

Concen: 20.379 ng/ul

RT: 7.210 min Scan# 718

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:128 Resp: 333260


Ion Ratio Lower Upper

128 100

64 54.0 43.8 65.6

130 31.2 25.4 38.2









#13
2-Methylphenol
Concen: 19.728 ng/ul
RT: 8.099 min Scan# 80
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:108 Resp: 313098
Ion Ratio Lower Upper
108 100
107 89.4 71.8 107.6



#14
2,2'-oxybis(1-Chloropropane)
Concen: 12.444 ng/ul
RT: 8.175 min Scan# 882
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion: 45 Resp: 361860
Ion Ratio Lower Upper
45 100
77 12.6 9.9 14.9
79 8.8 7.2 10.8









#16
 Acetophenone
 Concen: 20.927 ng/ul
 RT: 8.475 min Scan# 911
 Delta R.T. 0.041 min
 Lab File: BP011227.D
 Acq: 02 Aug 2022 15:57




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020726


Tgt Ion:105 Resp: 531479
 Ion Ratio Lower Upper
 105 100
 77 79.9 65.4 98.0
 51 33.3 26.5 39.7



#17
 N-Nitroso-di-n-propylamine
 Concen: 19.495 ng/ul
 RT: 8.463 min Scan# 931
 Delta R.T. 0.041 min
 Lab File: BP011227.D
 Acq: 02 Aug 2022 15:57

Tgt Ion: 70 Resp: 261730
 Ion Ratio Lower Upper
 70 100
 42 67.6 55.5 83.3
 101 8.8 7.1 10.7
 130 18.3 14.8 22.2









#18
4-Methylphenol
Concen: 19.975 ng/ul
RT: 8.428 min Scan# 919
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:108 Resp: 341424
Ion Ratio Lower Upper
108 100
107 113.9 88.2 132.4



#19
Hexachloroethane
Concen: 21.126 ng/ul
RT: 8.710 min Scan# 973
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:117 Resp: 155188
Ion Ratio Lower Upper
117 100
201 76.3 62.2 93.2
199 48.5 39.8 59.6









#22
Nitrobenzene
Concen: 19.944 ng/ul
RT: 8.852 min Scan# 990
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion: 77 Resp: 413455
Ion Ratio Lower Upper
77 100
123 41.1 31.4 47.0
65 13.7 10.6 15.8



#23
Isophorone
Concen: 19.701 ng/ul
RT: 9.381 min Scan# 1087
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion: 82 Resp: 738957
Ion Ratio Lower Upper
82 100
95 6.9 5.8 8.8
138 16.6 12.6 18.8









#25
2-Nitrophenol
Concen: 19.543 ng/ul
RT: 9.557 min Scan# 1117
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:139 Resp: 169616
Ion Ratio Lower Upper
139 100
65 64.8 46.7 70.1
109 31.0 24.2 36.2



#26
2,4-Dimethylphenol
Concen: 20.209 ng/ul
RT: 9.628 min Scan# 1129
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:107 Resp: 376785
Ion Ratio Lower Upper
107 100
121 49.0 40.3 60.5
122 82.5 67.7 101.5









#27
Bis(2-Chloroethoxy)methane
Concen: 19.649 ng/ul
RT: 9.869 min Scan# 1163
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion: 93 Resp: 463075
Ion Ratio Lower Upper
93 100
95 32.5 25.2 37.8
123 10.9 8.4 12.6



#29
2,4-Dichlorophenol
Concen: 20.038 ng/ul
RT: 10.093 min Scan# 1208
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:162 Resp: 282089
Ion Ratio Lower Upper
162 100
164 65.5 52.6 79.0
98 41.1 34.2 51.4









#30
Naphthalene
Concen: 20.248 ng/ul
RT: 10.487 min Scan# 11
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:128 Resp: 1105243
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.4
127 12.9 10.4 15.6



#32
4-Chloroaniline
Concen: 19.337 ng/ul
RT: 10.610 min Scan# 1296
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:127 Resp: 423985
Ion Ratio Lower Upper
127 100
129 32.8 26.6 40.0









#33
Hexachlorobutadiene
Concen: 20.353 ng/ul
RT: 10.769 min Scan# 11
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:225 Resp: 174989
Ion Ratio Lower Upper
225 100
223 61.7 51.2 76.8
227 62.3 50.6 75.8



#34
Caprolactam
Concen: 16.178 ng/ul
RT: 11.410 min Scan# 1432
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:113 Resp: 75743
Ion Ratio Lower Upper
113 100
55 211.8 164.2 246.4
56 155.8 127.0 190.6









#35
4-Chloro-3-methylphenol
Concen: 20.041 ng/ul
RT: 11.751 min Scan# 1483
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:107 Resp: 316327
Ion Ratio Lower Upper
107 100
144 24.6 19.0 28.4
142 75.0 59.8 89.8



#36
2-Methylnaphthalene
Concen: 19.884 ng/ul
RT: 12.110 min Scan# 1551
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:142 Resp: 686855
Ion Ratio Lower Upper
142 100
141 88.8 71.8 107.8









#37
1-Methylnaphthalene
Concen: 20.080 ng/ul
RT: 12.334 min Scan# 11
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:142 Resp: 694878
Ion Ratio Lower Upper
142 100
141 93.5 74.1 111.1
116 4.2 3.4 5.0



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.759 ng/ul
RT: 12.487 min Scan# 1615
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:216 Resp: 299581
Ion Ratio Lower Upper
216 100
214 79.7 61.1 91.7
179 23.6 18.6 27.8
108 23.5 19.1 28.7





#40

Hexachlorocyclopentadiene

Concen: 20.218 ng/ul

RT: 12.457 min Scan# 1610

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:237 Resp: 202092

Ion Ratio Lower Upper

237 100

235 64.9 50.4 75.6

272 12.0 9.9 14.9



#41

2,4,6-Trichlorophenol

Concen: 20.106 ng/ul

RT: 12.740 min Scan# 1658

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:196 Resp: 191422


Ion Ratio Lower Upper

196 100

198 94.2 75.5 113.3

200 30.0 24.4 36.6





#42

2,4,5-Trichlorophenol

Concen: 19.973 ng/ul

RT: 12.810 min Scan# 1663

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:196 Resp: 201292

Ion Ratio Lower Upper

196 100

198 95.6 76.8 115.2

200 30.8 25.0 37.6



#43

1,1'-Biphenyl

Concen: 20.072 ng/ul

RT: 13.140 min Scan# 1726

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:154 Resp: 873972


Ion Ratio Lower Upper

154 100

153 40.3 31.9 47.9

76 15.9 12.2 18.2





#44

2-Chloronaphthalene

Concen: 20.047 ng/ul

RT: 13.181 min Scan# 1733

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:162 Resp: 652552

Ion Ratio Lower Upper

162 100

164 33.0 25.6 38.4

127 43.7 34.6 51.8



#45

2-Nitroaniline

Concen: 16.691 ng/ul

RT: 13.398 min Scan# 1770

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion: 65 Resp: 157901


Ion Ratio Lower Upper

65 100

92 62.5 51.4 77.2

138 79.6 67.4 101.0









#47
Dimethylphthalate
Concen: 19.614 ng/ul
RT: 13.787 min Scan# 1836
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:163 Resp: 733392
Ion Ratio Lower Upper
163 100
194 3.7 2.9 4.3
164 9.9 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 17.531 ng/ul
RT: 13.904 min Scan# 1856
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:165 Resp: 114542
Ion Ratio Lower Upper
165 100
89 83.2 65.8 98.6
121 31.4 24.2 36.2





#50

Acenaphthylene

Concen: 20.406 ng/ul

RT: 14.034 min Scan# 11

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:152 Resp: 1063606

Ion Ratio Lower Upper

152 100

151 20.2 15.8 23.8

153 13.1 10.5 15.7



#51

3-Nitroaniline

Concen: 13.758 ng/ul

RT: 14.240 min Scan# 1913

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:138 Resp: 97076


Ion Ratio Lower Upper

138 100

108 11.1 9.9 14.9

92 124.8 106.8 160.2





#52

Acenaphthene

Concen: 20.138 ng/ul

RT: 14.381 min Scan# 1937

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:153 Resp: 685603

Ion Ratio Lower Upper

153 100

152 49.1 39.5 59.3

154 87.7 68.6 103.0



#53

2,4-Dinitrophenol

Concen: 17.641 ng/ul

RT: 14.445 min Scan# 1948

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:184 Resp: 65004


Ion Ratio Lower Upper

184 100

63 99.4 75.0 112.6

154 68.8 53.1 79.7









#55
4-Nitrophenol
Concen: 18.304 ng/ul
RT: 14.557 min Scan# 1994
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:109 Resp: 105035
Ion Ratio Lower Upper
109 100
139 123.7 100.6 150.8
65 143.2 122.6 184.0



#56
Dibenzofuran
Concen: 20.088 ng/ul
RT: 14.716 min Scan# 1994
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:168 Resp: 929601
Ion Ratio Lower Upper
168 100
139 42.0 34.2 51.2









#57
2,4-Dinitrotoluene
Concen: 19.712 ng/ul
RT: 14.698 min Scan# 1985
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:165 Resp: 179697
Ion Ratio Lower Upper
165 100
63 64.1 50.6 75.8
182 2.4 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 20.010 ng/ul
RT: 14.951 min Scan# 2034
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:232 Resp: 146640
Ion Ratio Lower Upper
232 100
131 62.9 50.4 75.6
130 3.1 2.6 3.8
166 37.2 31.9 47.9









#59
Diethylphthalate
Concen: 20.176 ng/ul
RT: 15.157 min Scan# 2106
Delta R.T. 0.029 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:149 Resp: 754003
Ion Ratio Lower Upper
149 100
177 19.9 16.1 24.1
150 13.0 9.4 14.0



#61
Fluorene
Concen: 20.150 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:166 Resp: 725103
Ion Ratio Lower Upper
166 100
165 97.7 77.7 116.5
167 13.7 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 19.857 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:204 Resp: 325217
Ion Ratio Lower Upper
204 100
206 32.8 27.3 40.9
141 72.8 57.7 86.5



#63
4-Nitroaniline
Concen: 10.258 ng/ul
RT: 15.410 min Scan# 2112
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:138 Resp: 61536
Ion Ratio Lower Upper
138 100
92 64.7 55.9 83.9
108 85.5 67.1 100.7









#66
 4,6-Dinitro-2-methylphenol
 Concen: 17.370 ng/ul
 RT: 15.463 min Scan# 2115
 Delta R.T. 0.035 min
 Lab File: BP011227.D
 Acq: 02 Aug 2022 15:57




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020726


Tgt Ion:198 Resp: 86845
 Ion Ratio Lower Upper
 198 100
 182 9.5 7.4 11.0
 77 37.9 28.6 42.8



#67
 N-Nitrosodiphenylamine
 Concen: 19.611 ng/ul
 RT: 15.592 min Scan# 2143
 Delta R.T. 0.035 min
 Lab File: BP011227.D
 Acq: 02 Aug 2022 15:57

Tgt Ion:169 Resp: 588542
 Ion Ratio Lower Upper
 169 100
 168 68.5 53.6 80.4
 167 37.1 30.0 45.0









#68
4-Bromophenyl-phenylether
Concen: 19.345 ng/ul
RT: 16.275 min Scan# 21
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:248 Resp: 181286
Ion Ratio Lower Upper
248 100
250 94.1 77.3 115.9
141 96.9 76.4 114.6



#69
Hexachlorobenzene
Concen: 19.457 ng/ul
RT: 16.381 min Scan# 2277
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:284 Resp: 208586
Ion Ratio Lower Upper
284 100
142 48.1 39.5 59.3
249 31.6 25.1 37.7





#70

Atrazine

Concen: 17.540 ng/ul

RT: 16.563 min Scan# 21

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:200 Resp: 165534

Ion Ratio Lower Upper

200 100

173 27.0 22.6 34.0

215 45.2 36.5 54.7



#71

Pentachlorophenol

Concen: 18.381 ng/ul

RT: 16.733 min Scan# 2337

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:266 Resp: 113132


Ion Ratio Lower Upper

266 100

264 66.3 52.2 78.2

268 64.1 50.6 75.8





#72

Phenanthrene

Concen: 19.987 ng/ul

RT: 17.128 min Scan# 2404

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:178 Resp: 1068226

Ion Ratio Lower Upper

178 100

179 15.3 12.1 18.1

176 19.5 15.4 23.2



#74

Anthracene

Concen: 20.284 ng/ul

RT: 17.222 min Scan# 2420

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:178 Resp: 1072500


Ion Ratio Lower Upper

178 100

179 15.0 12.3 18.5

176 18.5 14.7 22.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 18.083 ng/uL

RT: 13.098 min Scan# 1

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:216 Resp: 304446

Ion Ratio Lower Upper

216 100

214 78.8 62.0 93.0

218 50.0 38.2 57.4



#76

Pentachlorobenzene

Concen: 19.258 ng/uL

RT: 14.634 min Scan# 1980

Delta R.T. 0.041 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:250 Resp: 267219


Ion Ratio Lower Upper

250 100

248 62.1 49.2 73.8

252 63.2 50.8 76.2





#77

Carbazole

Concen: 20.095 ng/ul

RT: 17.498 min Scan# 2461

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:167 Resp: 941352

Ion Ratio Lower Upper

167 100

166 22.7 17.1 25.7

139 14.6 11.5 17.3



#78

Di-n-butylphthalate

Concen: 20.288 ng/ul

RT: 18.069 min Scan# 2564

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:149 Resp: 1136494


Ion Ratio Lower Upper

149 100

150 8.9 7.4 11.0

104 6.1 5.1 7.7









#80
Fluoranthene
Concen: 18.968 ng/ul
RT: 19.116 min Scan# 21
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:202 Resp: 1147818
Ion Ratio Lower Upper
202 100
101 14.5 11.9 17.9
100 11.4 9.3 13.9



#82
Pyrene
Concen: 19.048 ng/ul
RT: 19.475 min Scan# 2803
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:202 Resp: 1184515
Ion Ratio Lower Upper
202 100
101 16.6 14.3 21.5
100 13.9 11.8 17.6









#83
Butylbenzylphthalate
Concen: 18.252 ng/ul
RT: 20.369 min Scan# 2949
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:149 Resp: 454501
Ion Ratio Lower Upper
149 100
91 77.2 64.2 96.4
206 18.0 14.0 21.0



#84
3,3'-Dichlorobenzidine
Concen: 15.626 ng/ul
RT: 21.133 min Scan# 3085
Delta R.T. 0.029 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:252 Resp: 248478
Ion Ratio Lower Upper
252 100
254 64.6 51.8 77.6
126 15.7 11.4 17.0





#85

Benzo(a)anthracene

Concen: 20.078 ng/ul

RT: 21.192 min Scan# 3095

Delta R.T. 0.035 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:228 Resp: 1137908

Ion Ratio Lower Upper

228 100

229 19.6 15.8 23.6

226 26.7 21.8 32.6



#86

Bis(2-ethylhexyl)phthalate

Concen: 20.275 ng/ul

RT: 21.133 min Scan# 3085

Delta R.T. 0.029 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:149 Resp: 763010


Ion Ratio Lower Upper

149 100

167 25.8 20.4 30.6

279 3.1 2.9 4.3









#87
Chrysene
Concen: 19.879 ng/ul
RT: 21.245 min Scan# 3104
Delta R.T. 0.035 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:228 Resp: 1120002
Ion Ratio Lower Upper
228 100
226 30.1 23.8 35.6
229 19.7 15.7 23.5



#89
Di-n-octyl phthalate
Concen: 19.340 ng/ul
RT: 22.045 min Scan# 3240
Delta R.T. 0.041 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:149 Resp: 1372749









#90
Benzo(b)fluoranthene
Concen: 19.875 ng/ul
RT: 22.839 min Scan# 31
Delta R.T. 0.047 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57




Instrument :
BNA_P
ClientSampleId :
SSTD020726


Tgt Ion:252 Resp: 1293937
Ion Ratio Lower Upper
252 100
253 22.2 17.4 26.0
125 13.5 10.8 16.2



#91
Benzo(k)fluoranthene
Concen: 19.288 ng/ul
RT: 22.886 min Scan# 3383
Delta R.T. 0.047 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:252 Resp: 1191783
Ion Ratio Lower Upper
252 100
253 21.5 17.6 26.4
125 13.7 11.0 16.6





#93

Benzo(a)pyrene

Concen: 19.982 ng/ul

RT: 23.445 min Scan# 3469

Delta R.T. 0.053 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57

Instrument :

BNA_P

ClientSampleId :

SSTD020726





Tgt Ion:252 Resp: 1268932

Ion Ratio Lower Upper

252 100

253 21.7 17.4 26.2

125 15.3 12.5 18.7



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.532 ng/ul

RT: 25.974 min Scan# 3908

Delta R.T. 0.082 min

Lab File: BP011227.D

Acq: 02 Aug 2022 15:57




Tgt Ion:276 Resp: 1528090


Ion Ratio Lower Upper

276 100

138 30.6 25.5 38.3

277 24.4 19.8 29.8









#95
Dibenzo(a,h)anthracene
Concen: 19.377 ng/ul
RT: 25.992 min Scan# 3911
Delta R.T. 0.082 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Instrument :
BNA_P
ClientSampleId :
SSTD020726

Tgt Ion:278 Resp: 1300236
Ion Ratio Lower Upper
278 100
139 21.5 18.5 27.7
279 24.1 19.6 29.4



#96
Benzo(g,h,i)perylene
Concen: 19.478 ng/ul
RT: 26.715 min Scan# 4034
Delta R.T. 0.088 min
Lab File: BP011227.D
Acq: 02 Aug 2022 15:57

Tgt Ion:276 Resp: 1317987
Ion Ratio Lower Upper
276 100
138 28.7 22.8 34.2
277 23.2 18.5 27.7

