

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080222\
 Data File : BP011234.D
 Acq On : 02 Aug 2022 20:11
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV637

Quant Time: Aug 03 00:10:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.604	152	218288	20.000	ng/u1	0.00
20) Naphthalene-d8	10.398	136	996748	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	542413	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	1018464	20.000	ng/u1	0.00
79) Chrysene-d12	21.174	240	991048	20.000	ng/u1	0.00
88) Perylene-d12	23.492	264	1058684	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	17498	6.481	ng/uL	0.00
4) Pyridine-d5	3.505	84	134027	18.405	ng/u1	0.00
7) Phenol-d5	6.787	99	366750	20.161	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.952	67	284359	21.663	ng/u1	0.00
11) 2-Chlorophenol-d4	7.134	132	303241	20.451	ng/u1	0.00
15) 4-Methylphenol-d8	8.328	113	305883	20.435	ng/u1	0.00
21) Nitrobenzene-d5	8.769	128	147743	20.608	ng/u1	0.00
24) 2-Nitrophenol-d4	9.487	143	134760	20.053	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	262382	20.474	ng/u1	0.00
31) 4-Chloroaniline-d4	10.545	131	408449	20.602	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	761307	20.493	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	958086	20.498	ng/u1	0.00
54) 4-Nitrophenol-d4	14.504	143	127271	20.146	ng/u1	0.00
60) Fluorene-d10	15.281	176	639421	20.228	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	87785	18.563	ng/u1	0.00
73) Anthracene-d10	17.145	188	927048	20.711	ng/u1	0.00
81) Pyrene-d10	19.410	212	1019899	20.354	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.345	264	1060003	20.093	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.128	88	17812	7.154	ng/uL	100
5) Pyridine	3.522	79	130846	17.744	ng/u1	99
6) Benzaldehyde	6.752	77	213662	24.027	ng/u1	98
8) Phenol	6.816	94	381379	19.551	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.040	93	319499	19.962	ng/u1	98
12) 2-Chlorophenol	7.169	128	305578	19.841	ng/u1	98
13) 2-Methylphenol	8.057	108	293572	19.891	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.134	45	306218	11.227	ng/u1	100
16) Acetophenone	8.434	105	507275	20.912	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.422	70	237478	20.119	ng/u1	99
18) 4-Methylphenol	8.387	108	316631	20.004	ng/u1	98
19) Hexachloroethane	8.669	117	147263	19.940	ng/u1	98
22) Nitrobenzene	8.810	77	394623	20.086	ng/u1	99
23) Isophorone	9.340	82	699384	20.005	ng/u1	99
25) 2-Nitrophenol	9.516	139	155281	19.968	ng/u1	95
26) 2,4-Dimethylphenol	9.587	107	351562	19.983	ng/u1	99
27) Bis(2-Chloroethoxy)met...	9.828	93	433924	19.714	ng/u1	99
29) 2,4-Dichlorophenol	10.051	162	264802	19.772	ng/u1	99
30) Naphthalene	10.445	128	1047273	19.903	ng/u1	99
32) 4-Chloroaniline	10.569	127	410962	20.466	ng/u1	99
33) Hexachlorobutadiene	10.728	225	165688	19.806	ng/u1	98
34) Caprolactam	11.369	113	74294	18.729	ng/u1	98
35) 4-Chloro-3-methylphenol	11.710	107	301296	19.893	ng/u1	99
36) 2-Methylnaphthalene	12.075	142	663337	20.175	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080222\
 Data File : BP011234.D
 Acq On : 02 Aug 2022 20:11
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 9 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SICV637


Quant Time: Aug 03 00:10:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.292	142	653188	19.777	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.445	216	293230	19.767	ng/ul	98
40) Hexachlorocyclopentadiene	12.422	237	164697	17.572	ng/ul	100
41) 2,4,6-Trichlorophenol	12.698	196	182265	19.612	ng/ul	99
42) 2,4,5-Trichlorophenol	12.769	196	194475	19.500	ng/ul	99
43) 1,1'-Biphenyl	13.104	154	850773	19.652	ng/ul	99
44) 2-Chloronaphthalene	13.139	162	629706	19.499	ng/ul	98
45) 2-Nitroaniline	13.363	65	147811	19.028	ng/ul	98
47) Dimethylphthalate	13.745	163	737085	19.667	ng/ul	100
48) 2,6-Dinitrotoluene	13.869	165	134303	23.873	ng/ul	94
50) Acenaphthylene	13.998	152	1056792	20.009	ng/ul	99
51) 3-Nitroaniline	14.198	138	141615	22.822	ng/ul	99
52) Acenaphthene	14.339	153	674382	19.740	ng/ul	97
53) 2,4-Dinitrophenol	14.410	184	55585	16.639	ng/ul	98
55) 4-Nitrophenol	14.516	109	108745	19.075	ng/ul	98
56) Dibenzofuran	14.681	168	927564	19.840	ng/ul	98
57) 2,4-Dinitrotoluene	14.663	165	185388	20.925	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	14.910	232	149589	19.864	ng/ul	98
59) Diethylphthalate	15.128	149	740280	19.140	ng/ul	99
61) Fluorene	15.333	166	734589	19.721	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.333	204	322204	19.587	ng/ul	97
63) 4-Nitroaniline	15.369	138	107608	20.727	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.428	198	90932	18.595	ng/ul	100
67) N-Nitrosodiphenylamine	15.557	169	599330	20.133	ng/ul	100
68) 4-Bromophenyl-phenylether	16.239	248	181652	19.772	ng/ul	97
69) Hexachlorobenzene	16.339	284	211940	19.748	ng/ul	98
70) Atrazine	16.528	200	159967	17.964	ng/ul	99
71) Pentachlorophenol	16.698	266	114612	18.233	ng/ul	99
72) Phenanthrene	17.086	178	1100721	19.740	ng/ul	99
74) Anthracene	17.180	178	1117876	20.158	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.063	216	295830	18.981	ng/uL	98
76) Pentachlorobenzene	14.592	250	267377	20.124	ng/uL	99
77) Carbazole	17.463	167	1018214	20.472	ng/ul	100
78) Di-n-butylphthalate	18.033	149	1138796	18.458	ng/ul	100
80) Fluoranthene	19.080	202	1201669	19.609	ng/ul	99
82) Pyrene	19.433	202	1258460	19.679	ng/ul	100
83) Butylbenzylphthalate	20.333	149	415956	17.034	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.104	252	274757	16.951	ng/ul	99
85) Benzo(a)anthracene	21.157	228	1223031	19.745	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.104	149	722071	17.307	ng/ul	99
87) Chrysene	21.210	228	1177326	19.311	ng/ul	99
89) Di-n-octyl phthalate	22.004	149	1280898	17.745	ng/ul	100
90) Benzo(b)fluoranthene	22.786	252	1293698	19.181	ng/ul	99
91) Benzo(k)fluoranthene	22.833	252	1271833	20.099	ng/ul	99
93) Benzo(a)pyrene	23.392	252	1261968	19.221	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	25.886	276	1500982	19.156	ng/ul	100
95) Dibenzo(a,h)anthracene	25.909	278	1288821	19.397	ng/ul	98
96) Benzo(g,h,i)perylene	26.621	276	1299628	19.355	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 03 00:10:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration







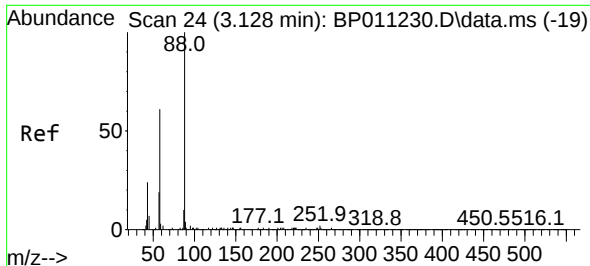

#2
 1,4-Dioxane
 Concen: 7.154 ng/uL
 RT: 3.128 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BP011234.D
 Acq: 02 Aug 2022 20:11




Instrument :
 BNA_P
 ClientSampleId :
 SICV637


Tgt Ion: 88 Resp: 17812
 Ion Ratio Lower Upper
 88 100
 43 37.0 29.6 44.4
 58 61.7 49.1 73.7

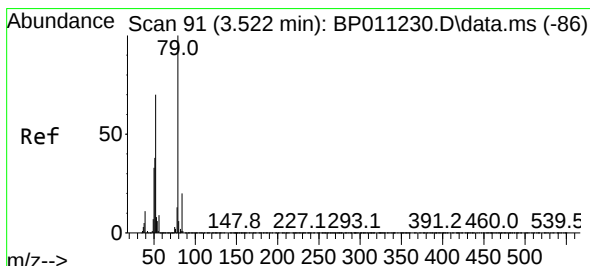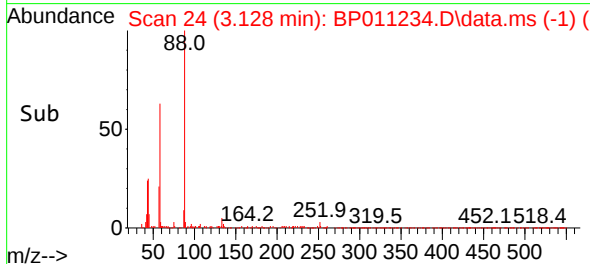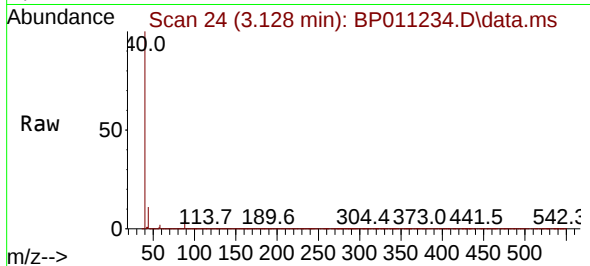

#5
 Pyridine
 Concen: 17.744 ng/uL
 RT: 3.522 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BP011234.D
 Acq: 02 Aug 2022 20:11

Tgt Ion: 79 Resp: 130846
 Ion Ratio Lower Upper
 79 100
 52 70.9 57.8 86.6
 51 39.0 31.5 47.3


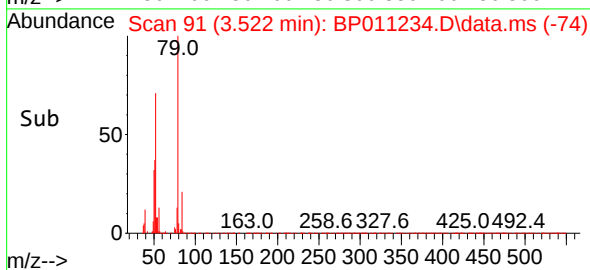

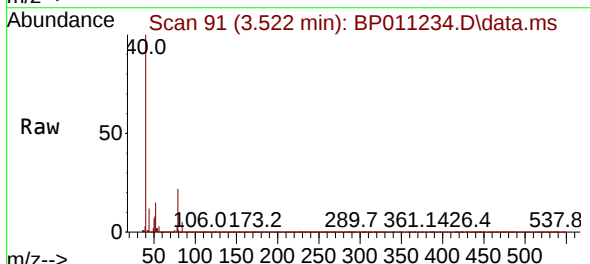




#6
Benzaldehyde
Concen: 24.027 ng/ul
RT: 6.752 min Scan# 640
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion: 77 Resp: 213662
Ion Ratio Lower Upper
77 100
105 92.3 72.0 108.0
106 87.8 69.4 104.0



#8
Phenol
Concen: 19.551 ng/ul
RT: 6.816 min Scan# 651
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion: 94 Resp: 381379
Ion Ratio Lower Upper
94 100
65 30.8 24.7 37.1
66 38.6 32.6 49.0

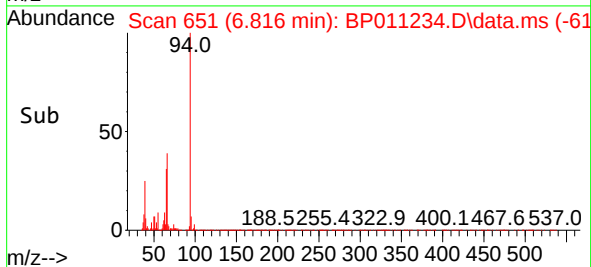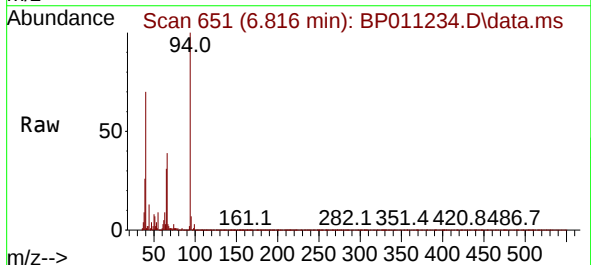



#10

Bis(2-Chloroethyl)ether

Concen: 19.962 ng/ul

RT: 7.040 min Scan# 689

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion: 93 Resp: 319499

Ion Ratio Lower Upper

93 100

63 86.0 71.0 106.6

95 32.3 26.0 39.0

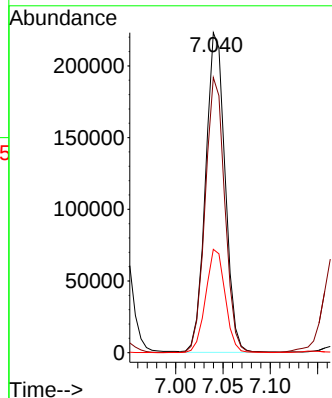

#12

2-Chlorophenol

Concen: 19.841 ng/ul

RT: 7.169 min Scan# 711

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion:128 Resp: 305578


Ion Ratio Lower Upper

128 100

64 53.3 43.8 65.6

130 32.3 25.4 38.2

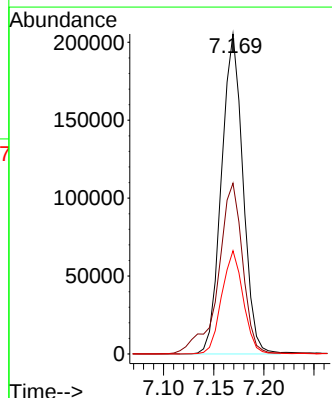



#13

2-Methylphenol

Concen: 19.891 ng/ul

RT: 8.057 min Scan# 862

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :





SICV637

Tgt Ion:108 Resp: 293572

Ion Ratio Lower Upper

108 100

107 89.5 71.8 107.6

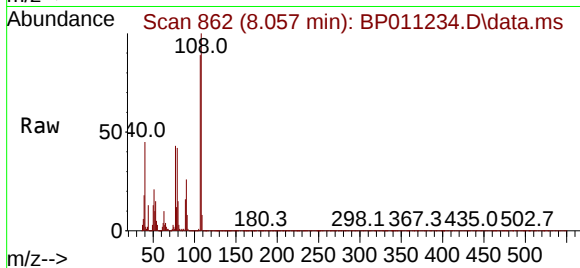

#14

2,2'-oxybis(1-Chloropropane)

Concen: 11.227 ng/ul

RT: 8.134 min Scan# 875

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion: 45 Resp: 306218


Ion Ratio Lower Upper

45 100

77 12.4 9.9 14.9

79 9.0 7.2 10.8



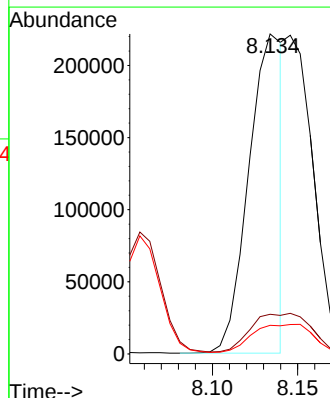





#16
Acetophenone
Concen: 20.912 ng/ul
RT: 8.434 min Scan# 911
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:105 Resp: 507275
Ion Ratio Lower Upper
105 100
77 81.8 65.4 98.0
51 33.6 26.5 39.7



#17
N-Nitroso-di-n-propylamine
Concen: 20.119 ng/ul
RT: 8.422 min Scan# 924
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion: 70 Resp: 237478
Ion Ratio Lower Upper
70 100
42 68.8 55.5 83.3
101 9.5 7.1 10.7
130 18.4 14.8 22.2









#18
4-Methylphenol
Concen: 20.004 ng/ul
RT: 8.387 min Scan# 918
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:108 Resp: 316631
Ion Ratio Lower Upper
108 100
107 112.4 88.2 132.4



#19
Hexachloroethane
Concen: 19.940 ng/ul
RT: 8.669 min Scan# 966
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:117 Resp: 147263
Ion Ratio Lower Upper
117 100
201 75.5 62.2 93.2
199 49.0 39.8 59.6



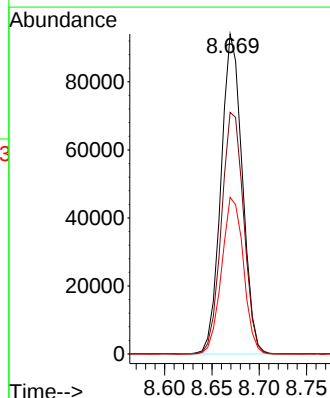





#22
Nitrobenzene
Concen: 20.086 ng/ul
RT: 8.810 min Scan# 990
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion: 77 Resp: 394623
Ion Ratio Lower Upper
77 100
123 40.0 31.4 47.0
65 13.5 10.6 15.8



#23
Isophorone
Concen: 20.005 ng/ul
RT: 9.340 min Scan# 1080
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion: 82 Resp: 699384
Ion Ratio Lower Upper
82 100
95 7.1 5.8 8.8
138 16.2 12.6 18.8









#25
2-Nitrophenol
Concen: 19.968 ng/ul
RT: 9.516 min Scan# 1111
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:139 Resp: 155281
Ion Ratio Lower Upper
139 100
65 63.4 46.7 70.1
109 30.6 24.2 36.2



#26
2,4-Dimethylphenol
Concen: 19.983 ng/ul
RT: 9.587 min Scan# 1122
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:107 Resp: 351562
Ion Ratio Lower Upper
107 100
121 49.3 40.3 60.5
122 84.1 67.7 101.5





#27

Bis(2-Chloroethoxy)methane

Concen: 19.714 ng/ul

RT: 9.828 min Scan# 1163

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion: 93 Resp: 433924

Ion Ratio Lower Upper

93 100

95 31.3 25.2 37.8

123 10.8 8.4 12.6

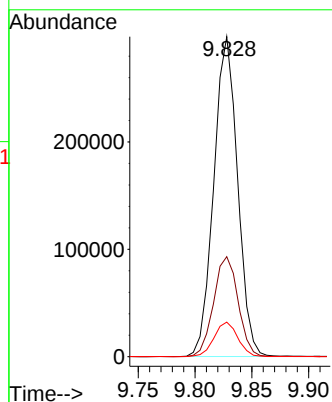

#29

2,4-Dichlorophenol

Concen: 19.772 ng/ul

RT: 10.051 min Scan# 1201

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion:162 Resp: 264802


Ion Ratio Lower Upper

162 100

164 65.3 52.6 79.0

98 41.1 34.2 51.4









#30
Naphthalene
Concen: 19.903 ng/ul
RT: 10.445 min Scan# 1268
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:128 Resp: 1047273
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 13.2 10.4 15.6

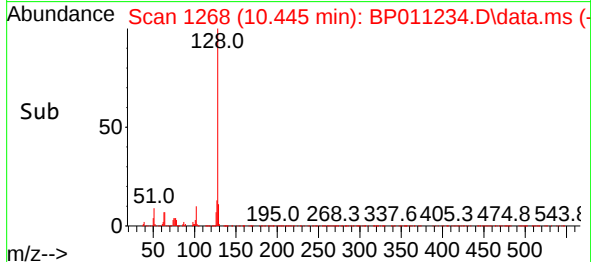

#32
4-Chloroaniline
Concen: 20.466 ng/ul
RT: 10.569 min Scan# 1289
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:127 Resp: 410962
Ion Ratio Lower Upper
127 100
129 32.6 26.6 40.0


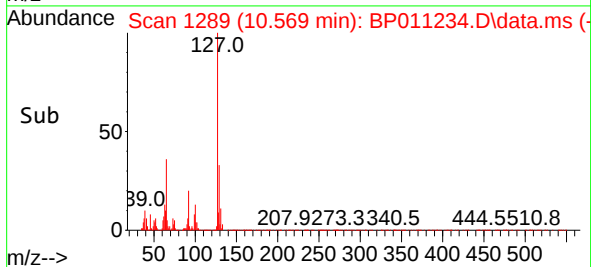

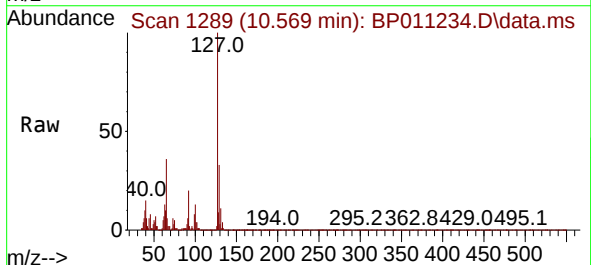




#33
Hexachlorobutadiene
Concen: 19.806 ng/ul
RT: 10.728 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:225 Resp: 165688
Ion Ratio Lower Upper
225 100
223 61.3 51.2 76.8
227 62.1 50.6 75.8



#34
Caprolactam
Concen: 18.729 ng/ul
RT: 11.369 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:113 Resp: 74294
Ion Ratio Lower Upper
113 100
55 204.3 164.2 246.4
56 154.4 127.0 190.6









#35
4-Chloro-3-methylphenol
Concen: 19.893 ng/ul
RT: 11.710 min Scan# 1483
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:107 Resp: 301296
Ion Ratio Lower Upper
107 100
144 24.7 19.0 28.4
142 75.5 59.8 89.8



#36
2-Methylnaphthalene
Concen: 20.175 ng/ul
RT: 12.075 min Scan# 1545
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:142 Resp: 663337
Ion Ratio Lower Upper
142 100
141 89.6 71.8 107.8









#37
1-Methylnaphthalene
Concen: 19.777 ng/ul
RT: 12.292 min Scan# 1582
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:142 Resp: 653188
Ion Ratio Lower Upper
142 100
141 92.7 74.1 111.1
116 3.9 3.4 5.0



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.767 ng/ul
RT: 12.445 min Scan# 1608
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:216 Resp: 293230
Ion Ratio Lower Upper
216 100
214 78.6 61.1 91.7
179 23.8 18.6 27.8
108 23.4 19.1 28.7









#40
Hexachlorocyclopentadiene
Concen: 17.572 ng/ul
RT: 12.422 min Scan# 1604
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:237 Resp: 164697
Ion Ratio Lower Upper
237 100
235 62.7 50.4 75.6
272 12.5 9.9 14.9

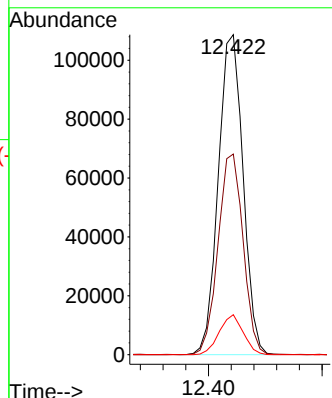

#41
2,4,6-Trichlorophenol
Concen: 19.612 ng/ul
RT: 12.698 min Scan# 1651
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:196 Resp: 182265
Ion Ratio Lower Upper
196 100
198 93.9 75.5 113.3
200 30.8 24.4 36.6



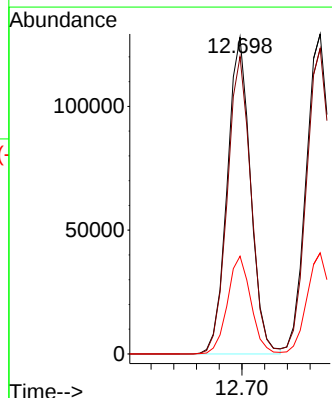





#42
2,4,5-Trichlorophenol
Concen: 19.500 ng/ul
RT: 12.769 min Scan# 1663
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:196 Resp: 194475
Ion Ratio Lower Upper
196 100
198 95.5 76.8 115.2
200 31.6 25.0 37.6



#43
1,1'-Biphenyl
Concen: 19.652 ng/ul
RT: 13.104 min Scan# 1720
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:154 Resp: 850773
Ion Ratio Lower Upper
154 100
153 39.6 31.9 47.9
76 15.8 12.2 18.2





#44

2-Chloronaphthalene

Concen: 19.499 ng/ul

RT: 13.139 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion:162 Resp: 629706

Ion Ratio Lower Upper

162 100

164 32.9 25.6 38.4

127 44.3 34.6 51.8

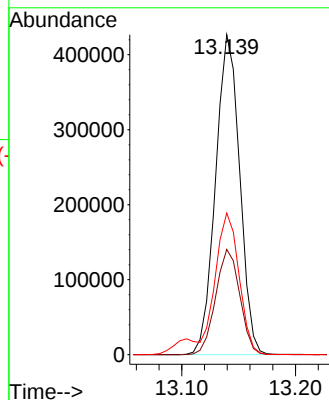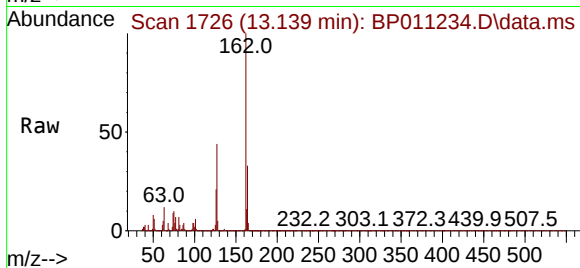

#45

2-Nitroaniline

Concen: 19.028 ng/ul

RT: 13.363 min Scan# 1764

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion: 65 Resp: 147811


Ion Ratio Lower Upper

65 100

92 65.5 51.4 77.2

138 87.1 67.4 101.0


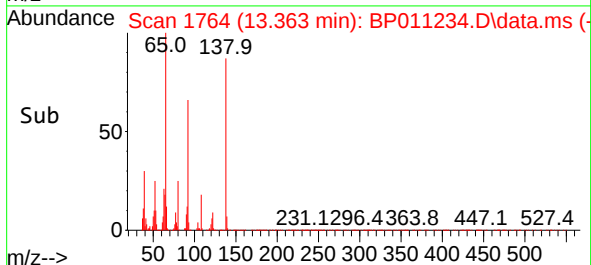
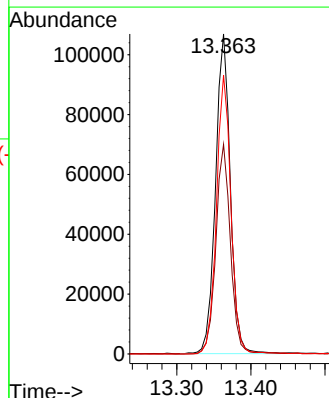
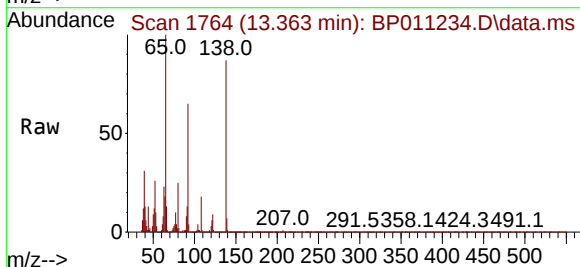




#47
Dimethylphthalate
Concen: 19.667 ng/ul
RT: 13.745 min Scan# 1829
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:163 Resp: 737085
Ion Ratio Lower Upper
163 100
194 3.5 2.9 4.3
164 10.3 8.2 12.4

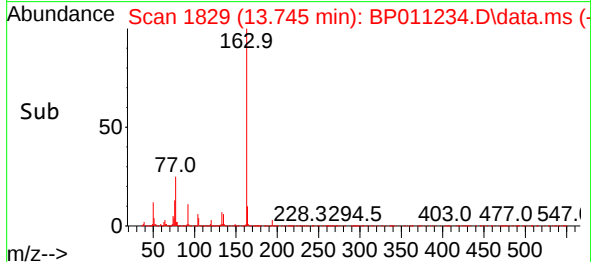

#48
2,6-Dinitrotoluene
Concen: 23.873 ng/ul
RT: 13.869 min Scan# 1850
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:165 Resp: 134303
Ion Ratio Lower Upper
165 100
89 76.6 65.8 98.6
121 26.6 24.2 36.2









#50
Acenaphthylene
Concen: 20.009 ng/ul
RT: 13.998 min Scan# 1872
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:152 Resp: 1056792
Ion Ratio Lower Upper
152 100
151 20.1 15.8 23.8
153 13.3 10.5 15.7

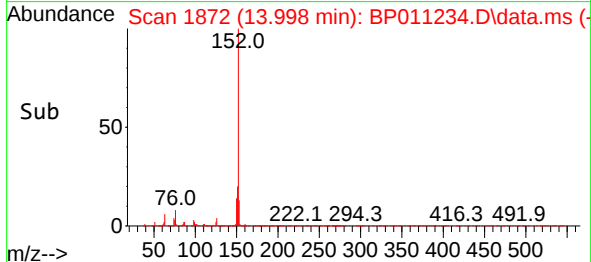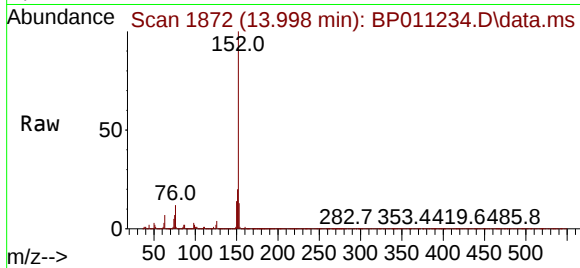

#51
3-Nitroaniline
Concen: 22.822 ng/ul
RT: 14.198 min Scan# 1906
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:138 Resp: 141615
Ion Ratio Lower Upper
138 100
108 11.3 9.9 14.9
92 132.3 106.8 160.2


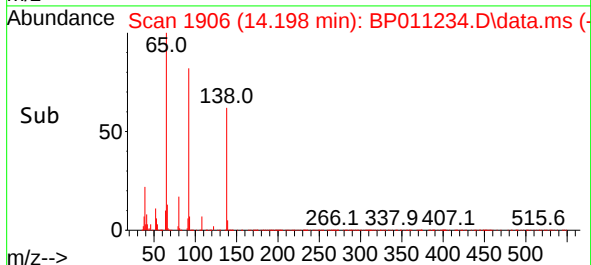
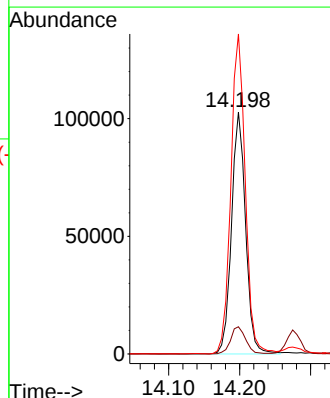
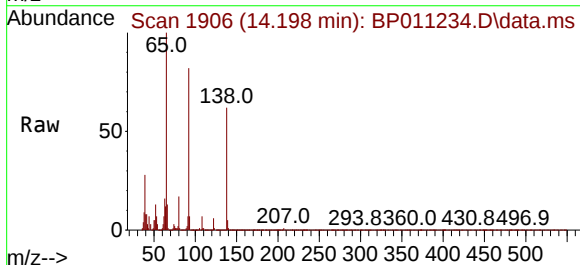




#52
Acenaphthene
Concen: 19.740 ng/ul
RT: 14.339 min Scan# 1930
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:153 Resp: 674382
Ion Ratio Lower Upper
153 100
152 50.5 39.5 59.3
154 88.7 68.6 103.0



#53
2,4-Dinitrophenol
Concen: 16.639 ng/ul
RT: 14.410 min Scan# 1942
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:184 Resp: 55585
Ion Ratio Lower Upper
184 100
63 91.3 75.0 112.6
154 67.0 53.1 79.7



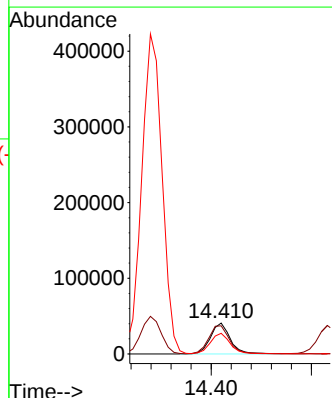





#55
4-Nitrophenol
Concen: 19.075 ng/ul
RT: 14.516 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:109 Resp: 108745
Ion Ratio Lower Upper
109 100
139 128.3 100.6 150.8
65 155.5 122.6 184.0



#56
Dibenzofuran
Concen: 19.840 ng/ul
RT: 14.681 min Scan# 1988
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:168 Resp: 927564
Ion Ratio Lower Upper
168 100
139 41.5 34.2 51.2









#57
2,4-Dinitrotoluene
Concen: 20.925 ng/ul
RT: 14.663 min Scan# 1985
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:165 Resp: 185388
Ion Ratio Lower Upper
165 100
63 62.9 50.6 75.8
182 2.8 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 19.864 ng/ul
RT: 14.910 min Scan# 2027
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:232 Resp: 149589
Ion Ratio Lower Upper
232 100
131 64.9 50.4 75.6
130 3.2 2.6 3.8
166 39.2 31.9 47.9









#59
Diethylphthalate
Concen: 19.140 ng/ul
RT: 15.128 min Scan# 2064
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:149 Resp: 740280
Ion Ratio Lower Upper
149 100
177 20.6 16.1 24.1
150 12.5 9.4 14.0



#61
Fluorene
Concen: 19.721 ng/ul
RT: 15.333 min Scan# 2099
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:166 Resp: 734589
Ion Ratio Lower Upper
166 100
165 97.1 77.7 116.5
167 13.6 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 19.587 ng/ul
RT: 15.333 min Scan# 20
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:204 Resp: 322204
Ion Ratio Lower Upper
204 100
206 33.9 27.3 40.9
141 75.6 57.7 86.5

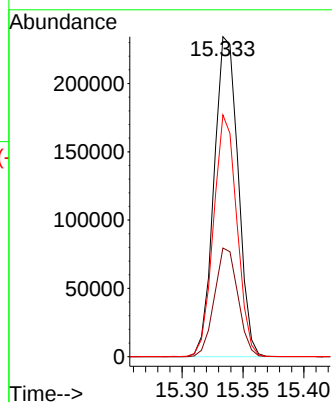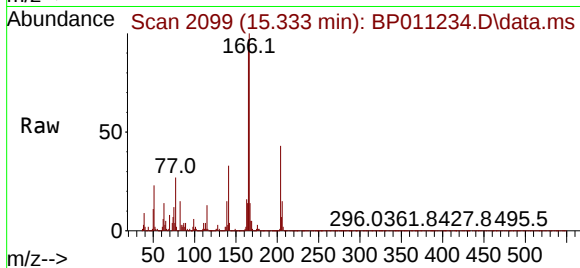

#63
4-Nitroaniline
Concen: 20.727 ng/ul
RT: 15.369 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:138 Resp: 107608
Ion Ratio Lower Upper
138 100
92 66.0 55.9 83.9
108 88.2 67.1 100.7









#66
 4,6-Dinitro-2-methylphenol
 Concen: 18.595 ng/ul
 RT: 15.428 min Scan# 2115
 Delta R.T. -0.000 min
 Lab File: BP011234.D
 Acq: 02 Aug 2022 20:11




Instrument :
 BNA_P
 ClientSampleId :
 SICV637


Tgt Ion:198 Resp: 90932
 Ion Ratio Lower Upper
 198 100
 182 8.6 7.4 11.0
 77 35.6 28.6 42.8



#67
 N-Nitrosodiphenylamine
 Concen: 20.133 ng/ul
 RT: 15.557 min Scan# 2137
 Delta R.T. -0.000 min
 Lab File: BP011234.D
 Acq: 02 Aug 2022 20:11

Tgt Ion:169 Resp: 599330
 Ion Ratio Lower Upper
 169 100
 168 67.2 53.6 80.4
 167 37.4 30.0 45.0









#68
4-Bromophenyl-phenylether
Concen: 19.772 ng/ul
RT: 16.239 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:248 Resp: 181652
Ion Ratio Lower Upper
248 100
250 98.1 77.3 115.9
141 91.9 76.4 114.6



#69
Hexachlorobenzene
Concen: 19.748 ng/ul
RT: 16.339 min Scan# 2270
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:284 Resp: 211940
Ion Ratio Lower Upper
284 100
142 47.7 39.5 59.3
249 31.6 25.1 37.7









#70
Atrazine
Concen: 17.964 ng/ul
RT: 16.528 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:200 Resp: 159967
Ion Ratio Lower Upper
200 100
173 27.3 22.6 34.0
215 45.8 36.5 54.7



#71
Pentachlorophenol
Concen: 18.233 ng/ul
RT: 16.698 min Scan# 2331
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:266 Resp: 114612
Ion Ratio Lower Upper
266 100
264 64.3 52.2 78.2
268 63.7 50.6 75.8









#72
Phenanthrene
Concen: 19.740 ng/u1
RT: 17.086 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:178 Resp: 1100721
Ion Ratio Lower Upper
178 100
179 15.5 12.1 18.1
176 19.2 15.4 23.2



#74
Anthracene
Concen: 20.158 ng/u1
RT: 17.180 min Scan# 2413
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:178 Resp: 1117876
Ion Ratio Lower Upper
178 100
179 15.5 12.3 18.5
176 18.9 14.7 22.1









#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.981 ng/uL
RT: 13.063 min Scan# 1713
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:216 Resp: 295830
Ion Ratio Lower Upper
216 100
214 78.4 62.0 93.0
218 49.4 38.2 57.4



#76
Pentachlorobenzene
Concen: 20.124 ng/uL
RT: 14.592 min Scan# 1973
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:250 Resp: 267377
Ion Ratio Lower Upper
250 100
248 62.3 49.2 73.8
252 62.0 50.8 76.2



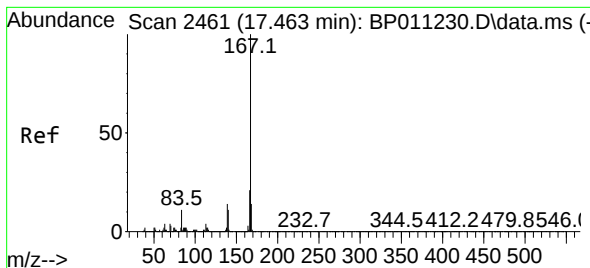

#77

Carbazole

Concen: 20.472 ng/ul

RT: 17.463 min Scan# 2461

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :





BNA_P

ClientSampleId :

SICV637

Tgt Ion:167 Resp: 1018214

Ion	Ratio	Lower	Upper
167	100		
166	21.5	17.1	25.7
139	14.3	11.5	17.3

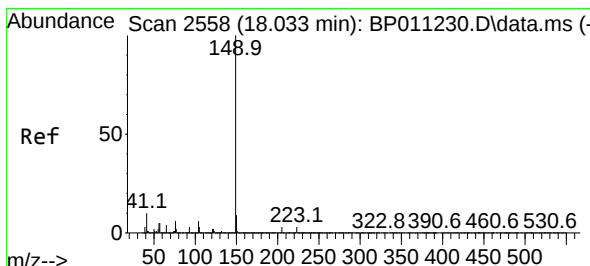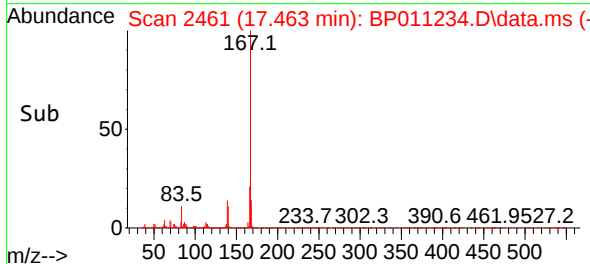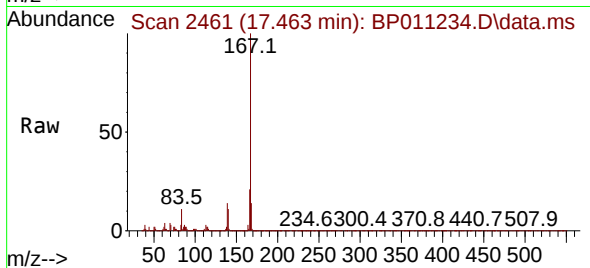

#78

Di-n-butylphthalate

Concen: 18.458 ng/ul

RT: 18.033 min Scan# 2558




Delta R.T. -0.000 min


Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Tgt Ion:149 Resp: 1138796

Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.4	11.0
104	6.4	5.1	7.7


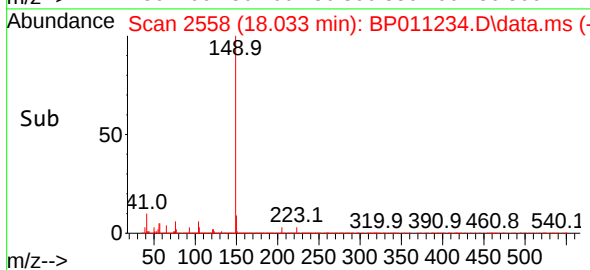

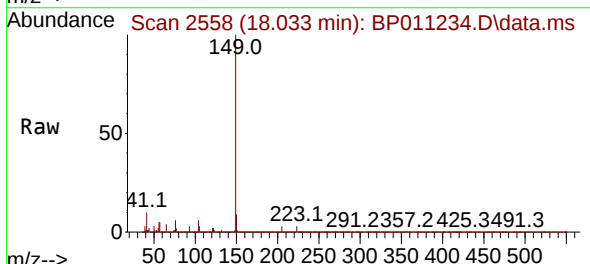




#80
Fluoranthene
Concen: 19.609 ng/u1
RT: 19.080 min Scan# 2736
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:202 Resp: 1201669
Ion Ratio Lower Upper
202 100
101 15.2 11.9 17.9
100 11.5 9.3 13.9



#82
Pyrene
Concen: 19.679 ng/u1
RT: 19.433 min Scan# 2796
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:202 Resp: 1258460
Ion Ratio Lower Upper
202 100
101 18.0 14.3 21.5
100 15.0 11.8 17.6









#83
Butylbenzylphthalate
Concen: 17.034 ng/ul
RT: 20.333 min Scan# 2949
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:149 Resp: 415956
Ion Ratio Lower Upper
149 100
91 79.4 64.2 96.4
206 17.7 14.0 21.0

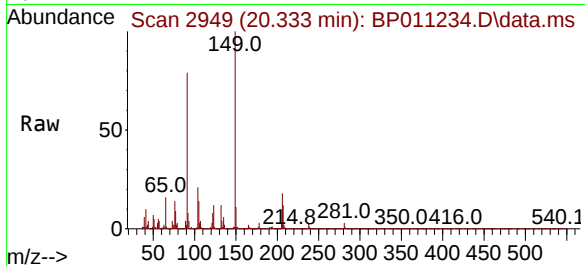

#84
3,3'-Dichlorobenzidine
Concen: 16.951 ng/ul
RT: 21.104 min Scan# 3080
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:252 Resp: 274757
Ion Ratio Lower Upper
252 100
254 65.5 51.8 77.6
126 13.9 11.4 17.0

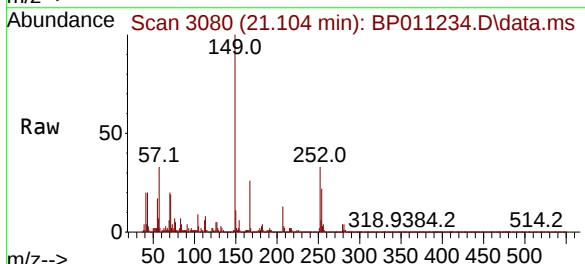



#85

Benzo(a)anthracene

Concen: 19.745 ng/ul

RT: 21.157 min Scan# 3089

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion:228 Resp: 1223031

Ion Ratio Lower Upper

228 100

229 20.4 15.8 23.6

226 27.0 21.8 32.6

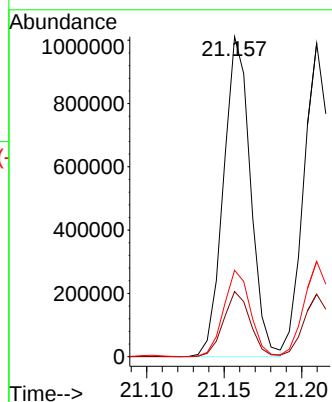

#86

Bis(2-ethylhexyl)phthalate

Concen: 17.307 ng/ul

RT: 21.104 min Scan# 3080

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion:149 Resp: 722071


Ion Ratio Lower Upper

149 100

167 25.9 20.4 30.6

279 3.5 2.9 4.3









#87
Chrysene
Concen: 19.311 ng/ul
RT: 21.210 min Scan# 3098
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:228 Resp: 1177326
Ion Ratio Lower Upper
228 100
226 30.4 23.8 35.6
229 20.0 15.7 23.5

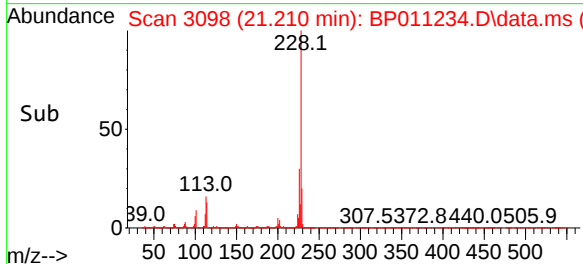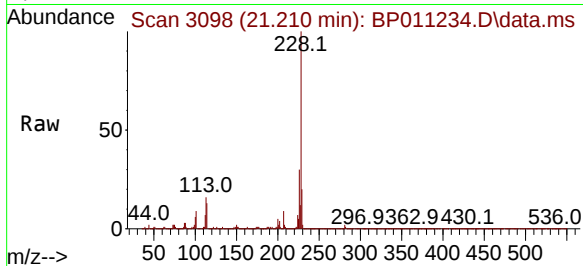

#89
Di-n-octyl phthalate
Concen: 17.745 ng/ul
RT: 22.004 min Scan# 3233
Delta R.T. -0.000 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:149 Resp: 1280898


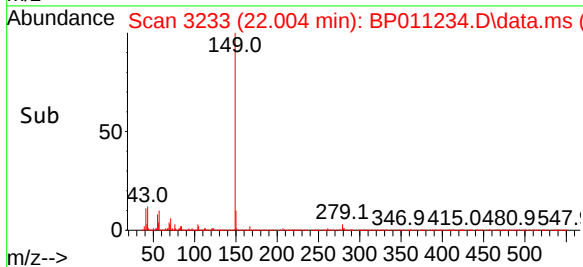

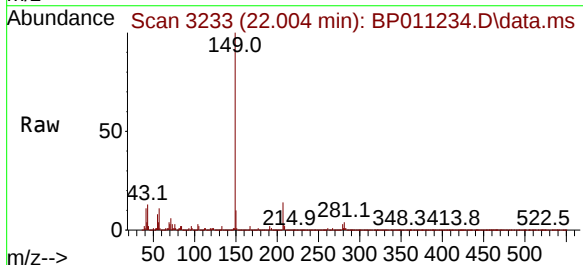




#90
Benzo(b)fluoranthene
Concen: 19.181 ng/ul
RT: 22.786 min Scan# 31
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11




Instrument :
BNA_P
ClientSampleId :
SICV637


Tgt Ion:252 Resp: 1293698
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.0
125 14.0 10.8 16.2



#91
Benzo(k)fluoranthene
Concen: 20.099 ng/ul
RT: 22.833 min Scan# 3374
Delta R.T. -0.006 min
Lab File: BP011234.D
Acq: 02 Aug 2022 20:11

Tgt Ion:252 Resp: 1271833
Ion Ratio Lower Upper
252 100
253 21.6 17.6 26.4
125 14.6 11.0 16.6





#93

Benzo(a)pyrene

Concen: 19.221 ng/ul

RT: 23.392 min Scan# 3469

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion:252 Resp: 1261968

Ion Ratio Lower Upper

252 100

253 21.4 17.4 26.2

125 14.5 12.5 18.7

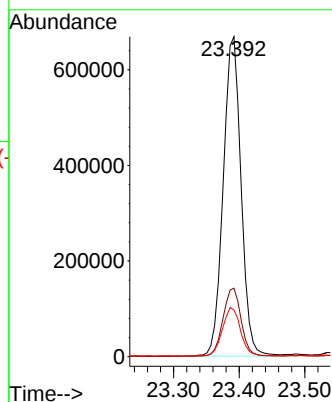

#94

Indeno(1,2,3-cd)pyrene

Concen: 19.156 ng/ul

RT: 25.886 min Scan# 3893

Delta R.T. -0.006 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11




Tgt Ion:276 Resp: 1500982


Ion Ratio Lower Upper

276 100

138 31.7 25.5 38.3

277 24.8 19.8 29.8



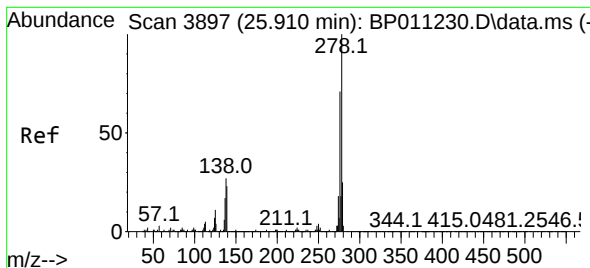

#95

Dibenzo(a,h)anthracene

Concen: 19.397 ng/ul

RT: 25.909 min Scan# 3897

Delta R.T. -0.000 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Instrument :

BNA_P

ClientSampleId :

SICV637





Tgt Ion:278 Resp: 1288821

Ion Ratio Lower Upper

278 100

139 21.4 18.5 27.7

279 24.2 19.6 29.4

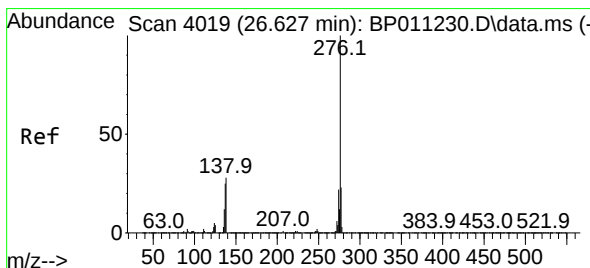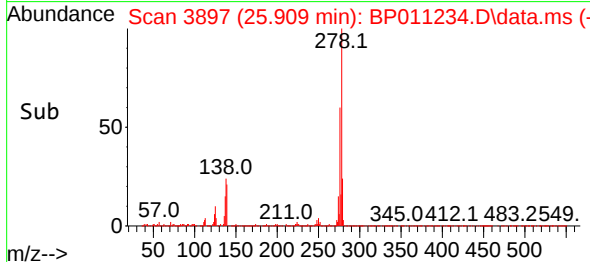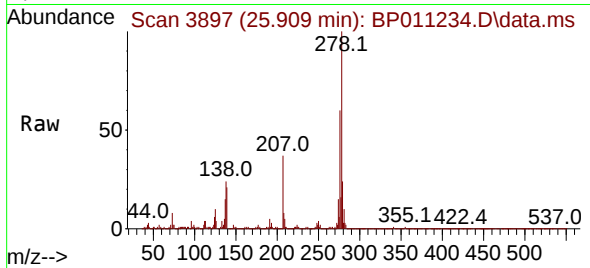

#96

Benzo(g,h,i)perylene

Concen: 19.355 ng/ul

RT: 26.621 min Scan# 4018

Delta R.T. -0.006 min

Lab File: BP011234.D

Acq: 02 Aug 2022 20:11

Tgt Ion:276 Resp: 1299628

Ion Ratio Lower Upper

276 100

138 29.2 22.8 34.2

277 23.7 18.5 27.7

