

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080322\
 Data File : BP011237.D
 Acq On : 03 Aug 2022 09:47
 Operator : CG/JU
 Sample : PB146573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	85	88	100	rVB	334137	491547	12.19%	1.066%
2	6.781	640	645	654	rVB	836764	1291105	32.02%	2.799%
3	6.946	668	673	685	rVB	752391	1163910	28.86%	2.523%
4	7.134	700	705	718	rVB	890740	1346947	33.40%	2.920%
5	7.599	779	784	793	rVB	791074	1226756	30.42%	2.660%
6	8.322	901	907	918	rBV	1053904	1625808	40.32%	3.525%
7	8.763	976	982	997	rVB	922252	1477814	36.65%	3.204%
8	9.487	1099	1105	1119	rVB	585157	933359	23.15%	2.024%
9	10.022	1189	1196	1210	rBV	969695	1566112	38.84%	3.395%
10	10.393	1252	1259	1267	rVB	1175877	1867466	46.31%	4.049%
11	10.546	1278	1285	1298	rBV	1006908	1668552	41.38%	3.617%
12	12.004	1529	1533	1539	rVB3	11888	20669	0.51%	0.045%
13	13.698	1814	1821	1832	rBV	1792925	2320281	57.54%	5.030%
14	13.787	1834	1836	1842	rVB4	4304	5370	0.13%	0.012%
15	13.963	1857	1866	1876	rBV	2012502	2856514	70.84%	6.193%
16	14.275	1912	1919	1928	rBV	1639750	2287235	56.72%	4.959%
17	14.498	1949	1957	1970	rBV	525363	816808	20.26%	1.771%
18	14.704	1991	1992	1997	rVB4	3619	4352	0.11%	0.009%
19	15.045	2046	2050	2053	rVB5	2360	4070	0.10%	0.009%
20	15.275	2083	2089	2103	rBV	2407129	3380495	83.83%	7.329%
21	15.410	2106	2112	2126	rVV	516574	685878	17.01%	1.487%
22	15.516	2126	2130	2136	rVB3	19103	29281	0.73%	0.063%
23	15.839	2183	2185	2191	rVB7	2146	4165	0.10%	0.009%
24	16.069	2218	2224	2231	rVB7	5564	11504	0.29%	0.025%
25	16.828	2350	2353	2356	rBV5	3833	5517	0.14%	0.012%
26	17.045	2383	2390	2400	rBV	1795420	2403398	59.60%	5.211%
27	17.145	2400	2407	2422	rVV2	2572743	3479158	86.28%	7.543%
28	17.692	2496	2500	2504	rBV7	2634	5804	0.14%	0.013%
29	18.239	2588	2593	2594	rBV5	3605	4554	0.11%	0.010%
30	18.980	2715	2719	2724	rBV3	23961	31483	0.78%	0.068%
31	19.051	2727	2731	2735	rBV2	21871	33485	0.83%	0.073%
32	19.404	2786	2791	2800	rBV	2887823	3778073	93.69%	8.191%
33	21.174	3087	3092	3099	rBV	2036904	2581579	64.02%	5.597%
34	23.345	3454	3461	3469	rBV2	2227828	4032413	100.00%	8.742%
35	23.492	3480	3486	3494	rVB2	1438474	2683602	66.55%	5.818%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080322\
Data File : BP011237.D
Acq On : 03 Aug 2022 09:47
Operator : CG/JU
Sample : PB146573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK573

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46125064

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080322\
Data File : BP011237.D
Acq On : 03 Aug 2022 09:47
Operator : CG/JU
Sample : PB146573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

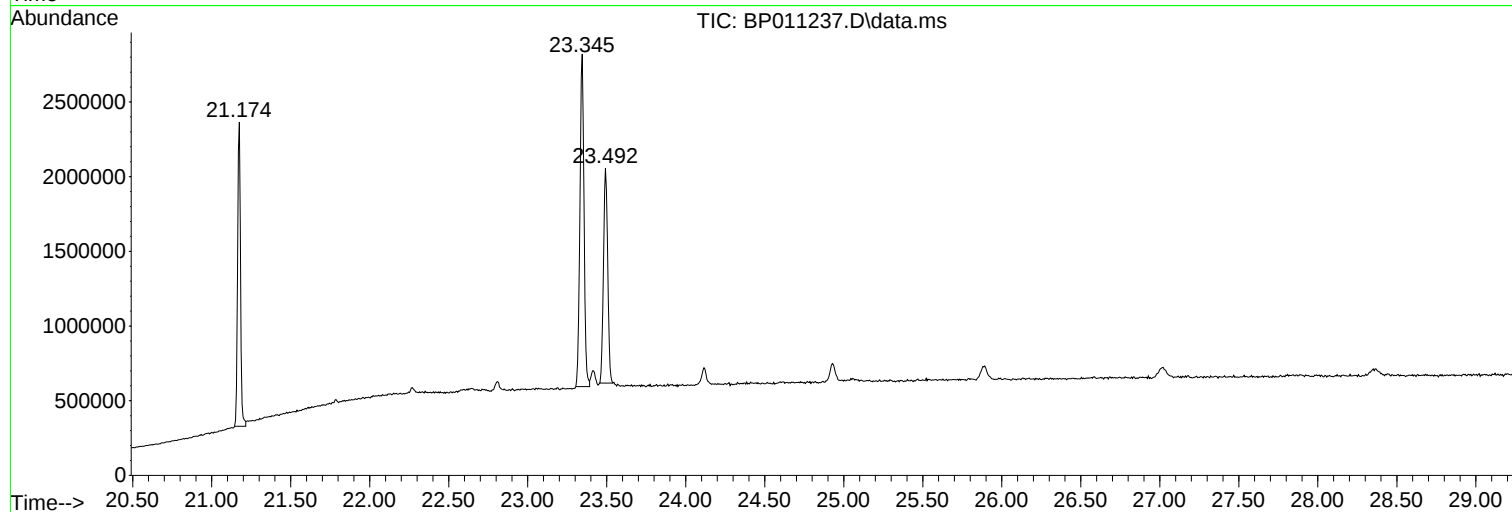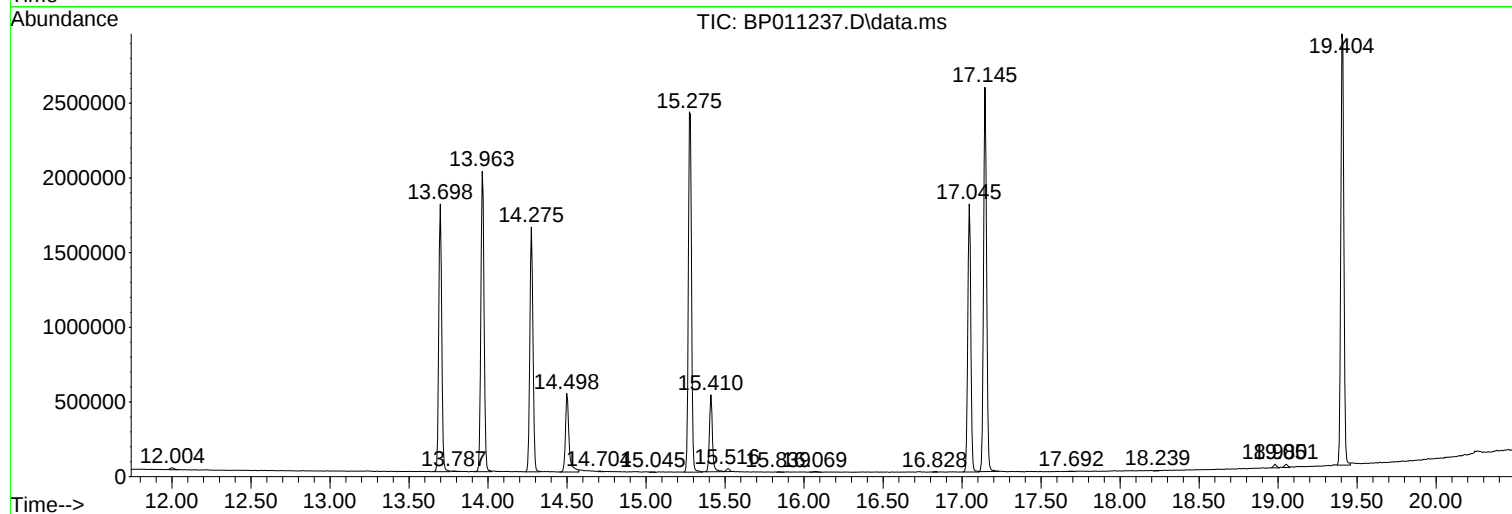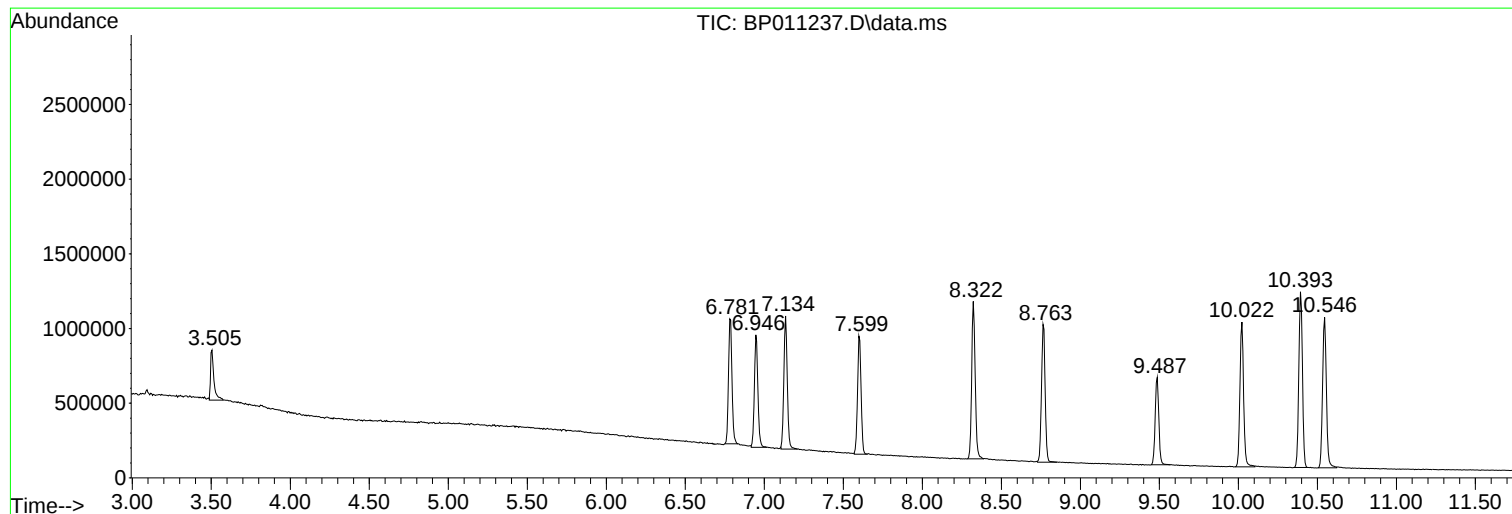

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080322\
Data File : BP011237.D
Acq On : 03 Aug 2022 09:47
Operator : CG/JU
Sample : PB146573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080322\
Data File : BP011237.D
Acq On : 03 Aug 2022 09:47
Operator : CG/JU
Sample : PB146573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc