




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021340.D
Acq On : 03 Aug 2024 11:38
Operator : CG/JU
Sample : P3278-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZP7

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:20:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

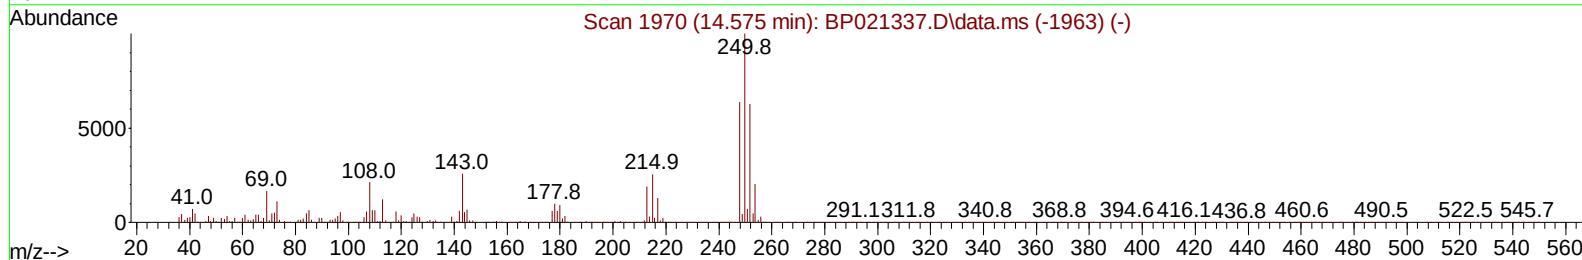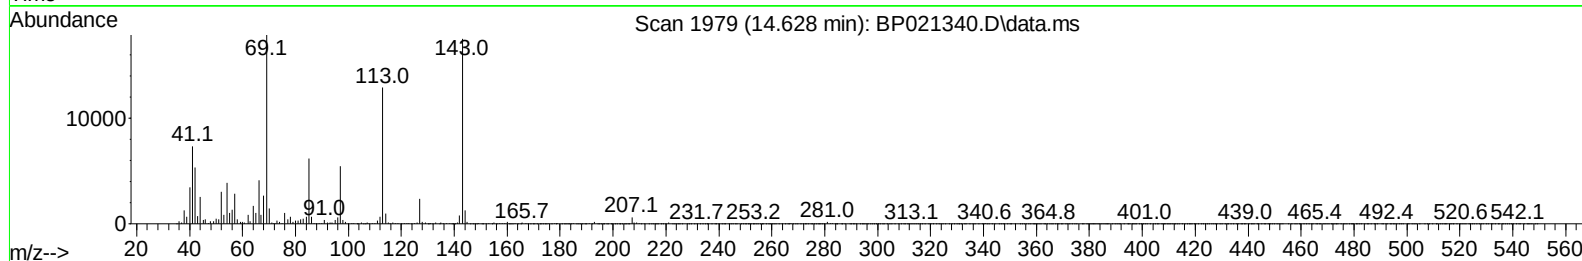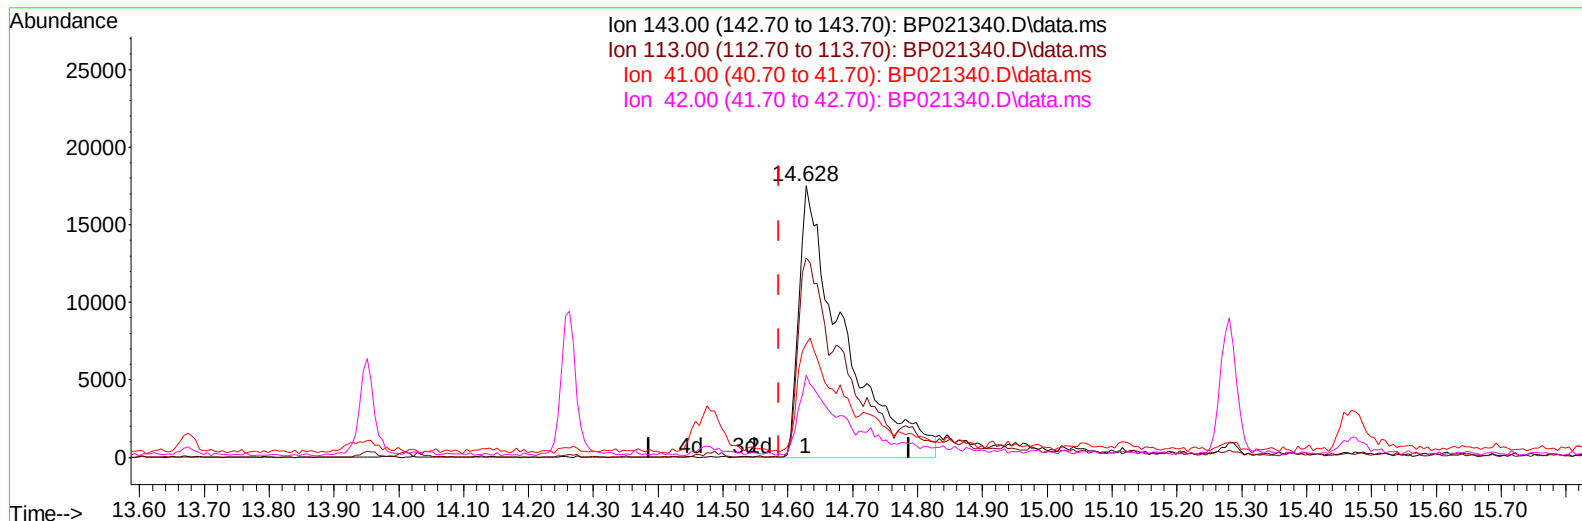

TIC: BP021340.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.628min (+ 0.042) 16.91 ng/ul m

response 84248

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	73.49
41.00	37.90	41.97
42.00	27.10	30.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021340.D
 Acq On : 03 Aug 2024 11:38
 Operator : CG/JU
 Sample : P3278-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZP7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/05/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Aug 04 23:37:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	174373	20.000	ng/ul	0.00
20) Naphthalene-d8	10.381	136	722203	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.263	164	481703	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.081	188	1084093	20.000	ng/ul	-0.01
79) Chrysene-d12	21.527	240	1060858	20.000	ng/ul	0.00
88) Perylene-d12	24.816	264	1209778	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	11152	2.910	ng/uL	-0.01
4) Pyridine-d5	3.587	84	149000	13.431	ng/ul	0.00
7) Phenol-d5	6.858	99	232437	16.350	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.981	67	140854	16.349	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	191298	16.332	ng/ul	0.00
15) 4-Methylphenol-d8	8.375	113	198961	16.851	ng/ul	0.01
21) Nitrobenzene-d5	8.793	128	94710	16.884	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	111147	17.312	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	182982	15.761	ng/ul	0.01
31) 4-Chloroaniline-d4	10.563	131	275230	17.895	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	732004	20.904	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	769925	19.581	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.628	143	84248m	16.910	ng/ul	0.04
60) Fluorene-d10	15.281	176	625607	21.777	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	81042	12.355	ng/ul	0.01
73) Anthracene-d10	17.187	188	1021424	21.213	ng/ul	0.00
81) Pyrene-d10	19.575	212	1252761	19.101	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.586	264	1331996	22.324	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021340.D
Acq On : 03 Aug 2024 11:38
Operator : CG/JU
Sample : P3278-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZP7

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:37:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

