




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021345.D
Acq On : 03 Aug 2024 15:24
Operator : CG/JU
Sample : P3278-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZQ8

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:21:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

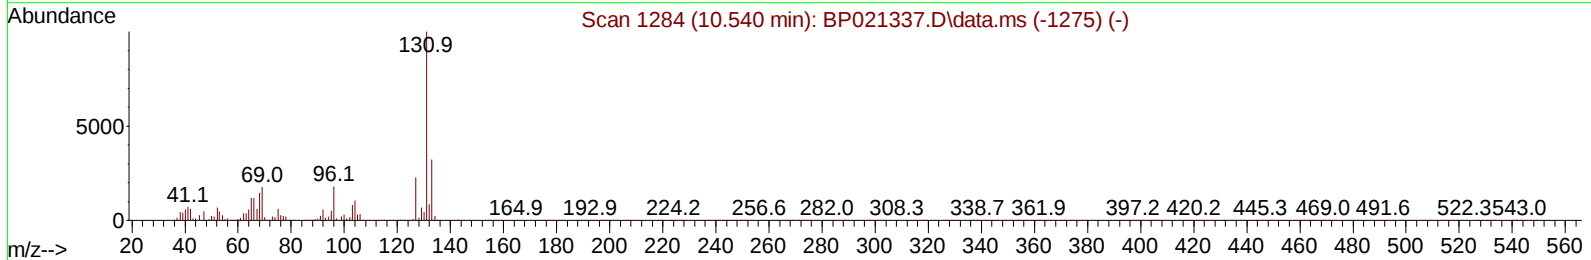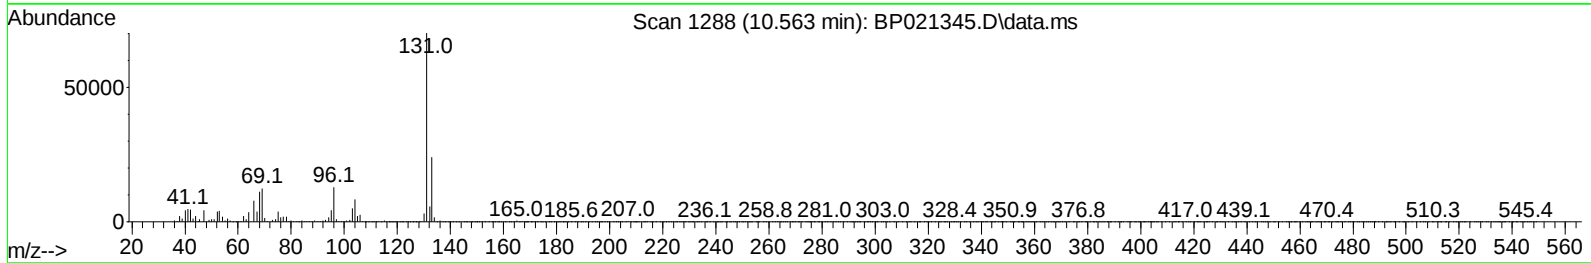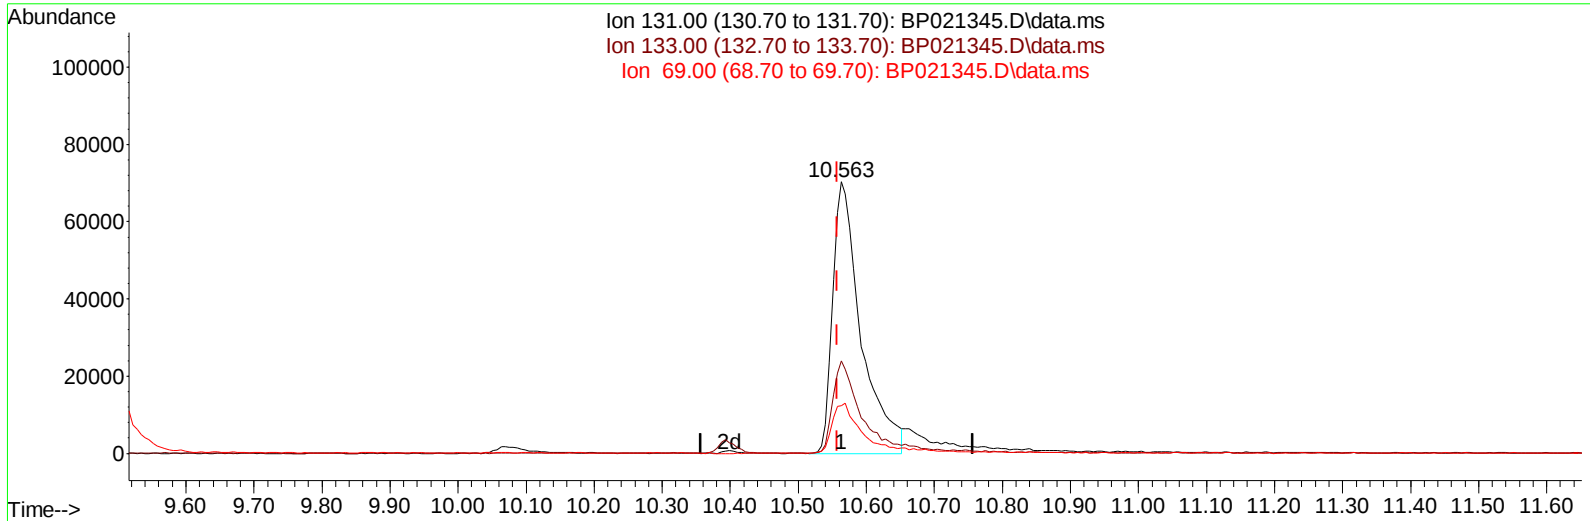

TIC: BP021345.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.563min (+ 0.006) 12.96 ng/u1

response 202896

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	34.16
69.00	17.40	17.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021345.D
 Acq On : 03 Aug 2024 15:24
 Operator : CG/JU
 Sample : P3278-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZQ8

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:21:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
 Supervised By :mohammad ahmed 08/05/2024

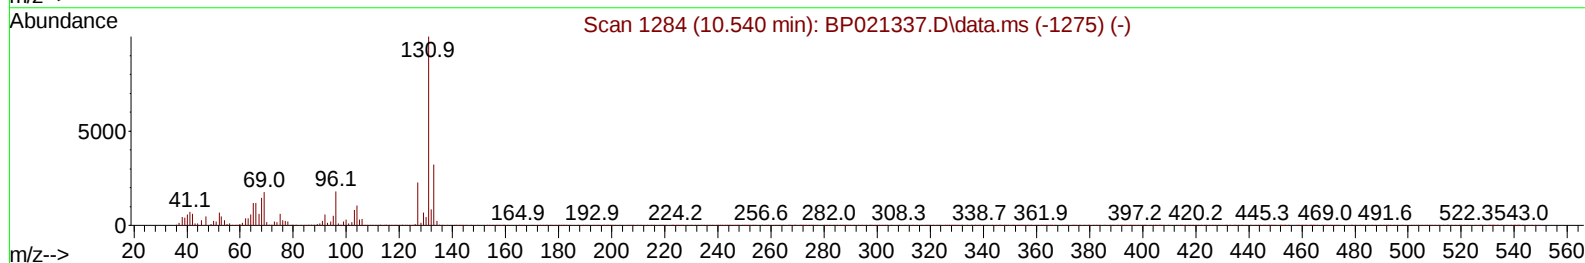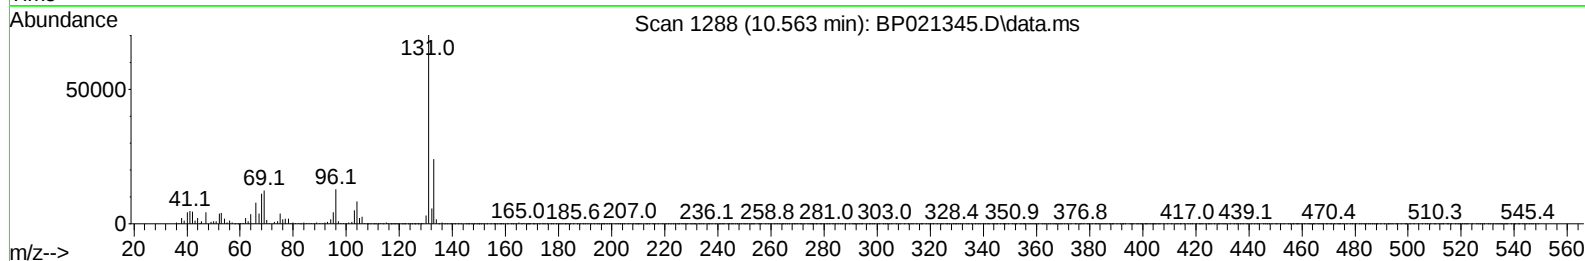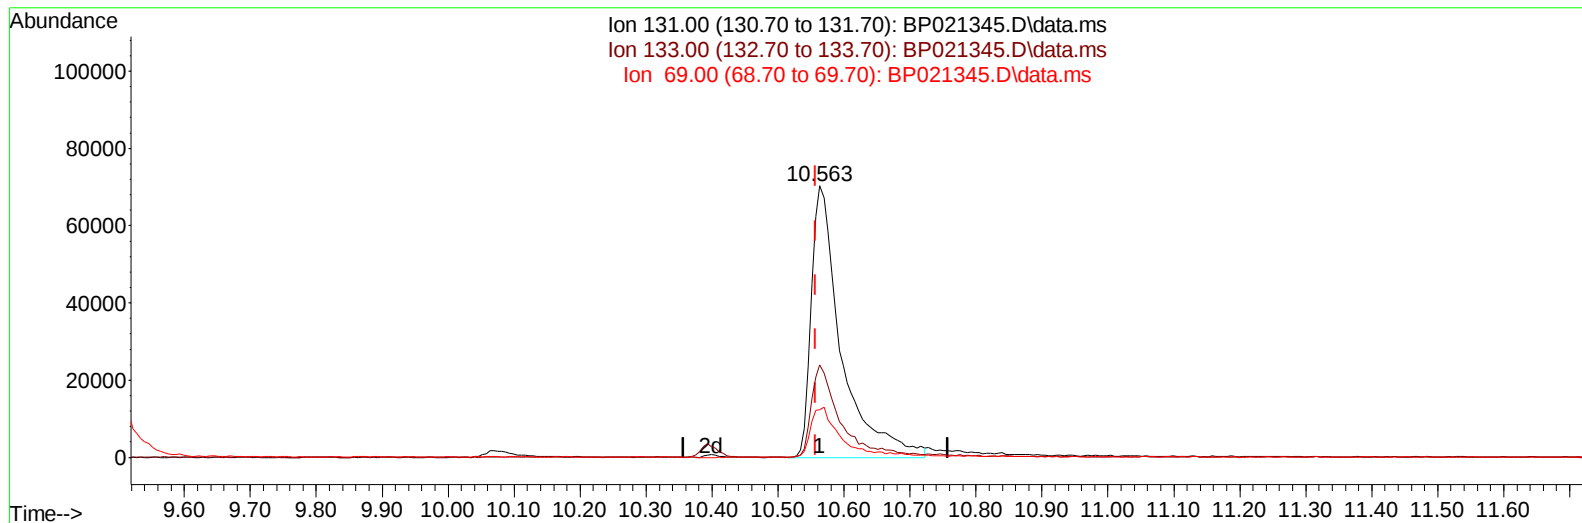

TIC: BP021345.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.563min (+ 0.006) 14.05 ng/ul m

response 219925

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	34.16
69.00	17.40	17.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021345.D
Acq On : 03 Aug 2024 15:24
Operator : CG/JU
Sample : P3278-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZQ8

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:21:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

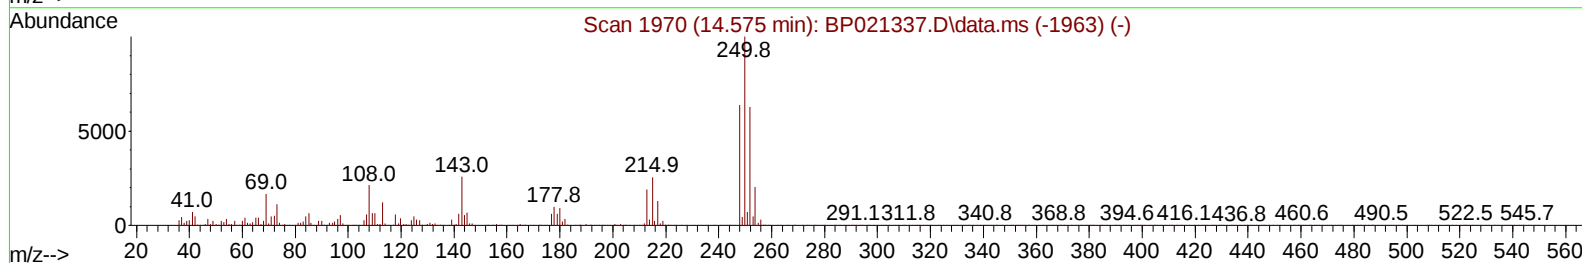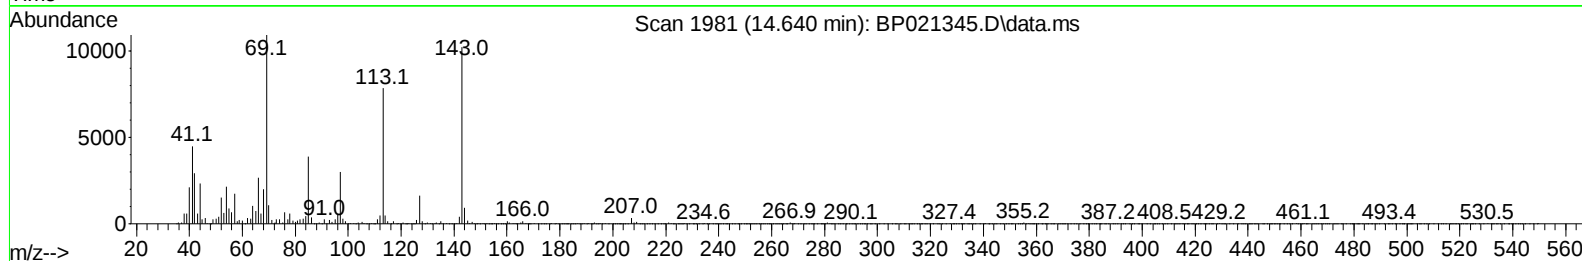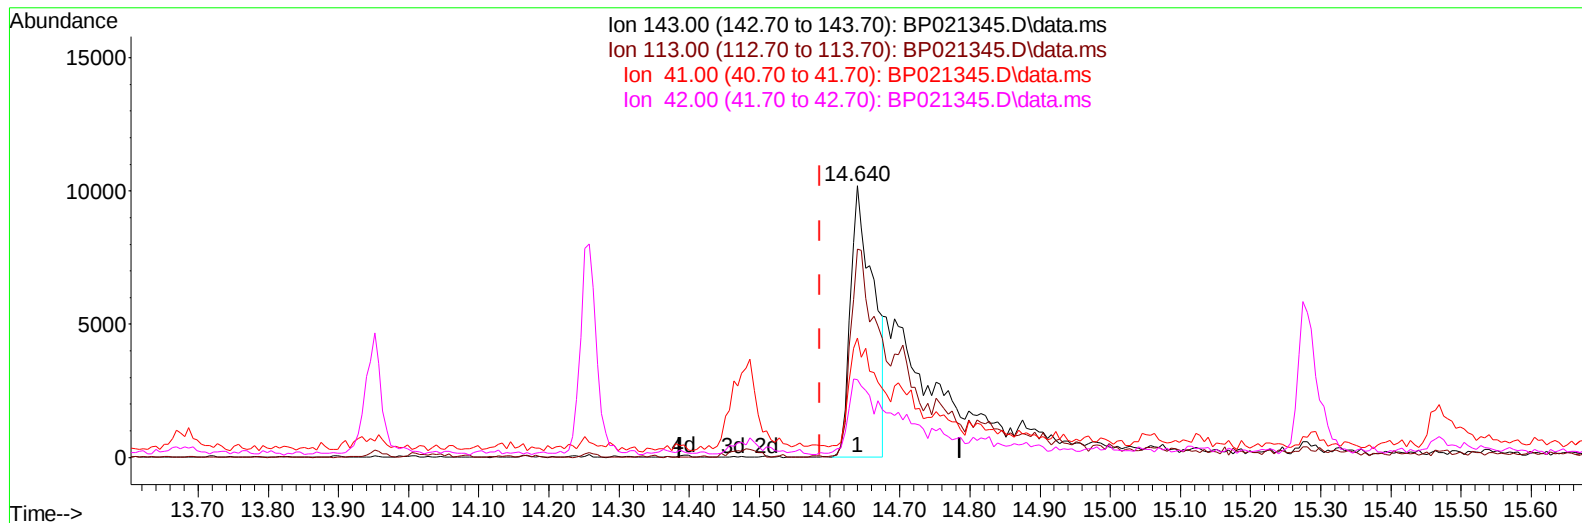

TIC: BP021345.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.640min (+ 0.053) 5.27 ng/u1

response 23260

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	76.80
41.00	37.90	43.90
42.00	27.10	28.70




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021345.D
Acq On : 03 Aug 2024 15:24
Operator : CG/JU
Sample : P3278-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZQ8

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:21:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

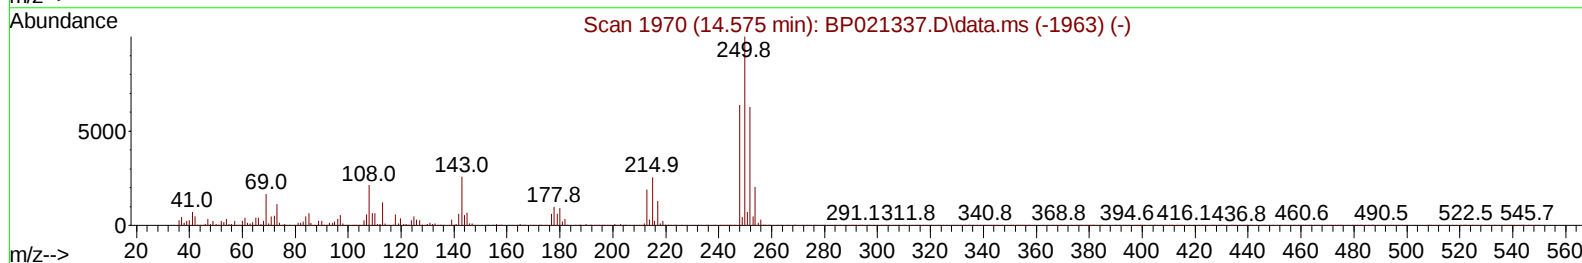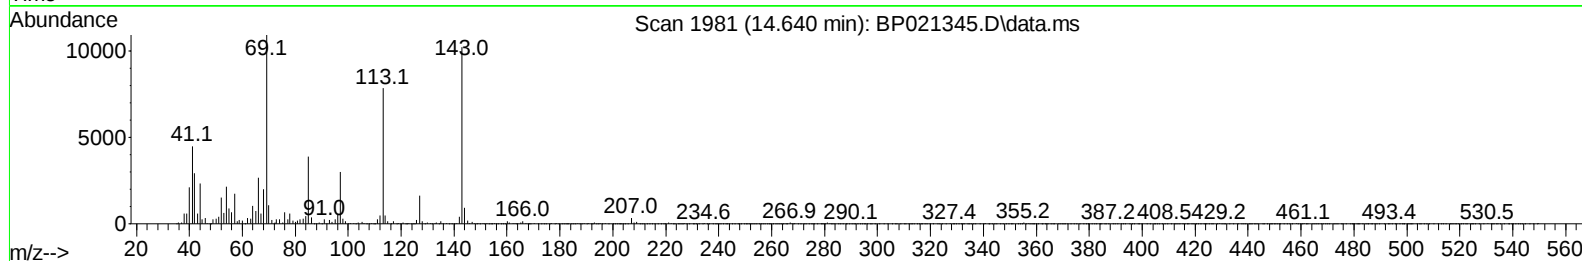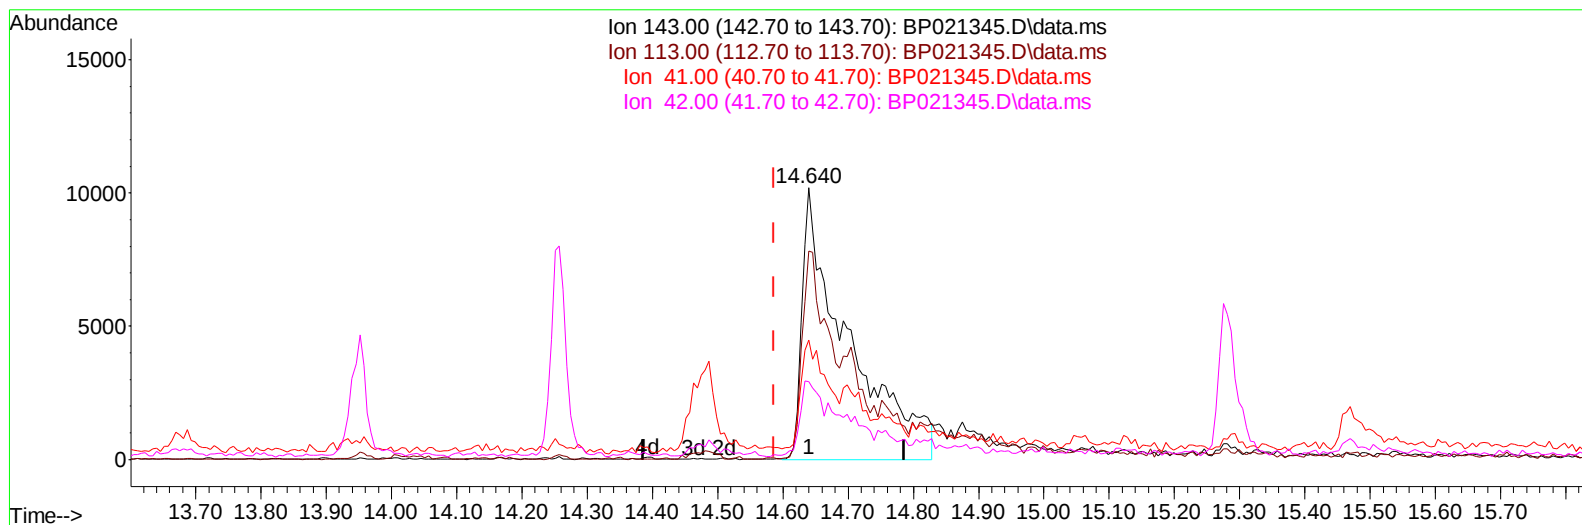

TIC: BP021345.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.640min (+ 0.053) 11.08 ng/ul m

response 48963

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	76.80
41.00	37.90	43.90
42.00	27.10	28.70

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021345.D
 Acq On : 03 Aug 2024 15:24
 Operator : CG/JU
 Sample : P3278-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZQ8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/05/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Aug 04 23:51:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	195815	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.393	136	735117	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	427062	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.087	188	877604	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	999702	20.000	ng/ul	0.00
88) Perylene-d12	24.821	264	1235980	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	12687	2.948	ng/uL	-0.01
4) Pyridine-d5	3.587	84	160314	12.869	ng/ul	0.00
7) Phenol-d5	6.858	99	218125	13.663	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.981	67	137130	14.174	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	186323	14.166	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	175693	13.251	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	79517	13.927	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	94535	14.466	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	158267	13.393	ng/ul	0.02
31) 4-Chloroaniline-d4	10.563	131	219925m	14.048	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	488973	15.750	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	562104	16.125	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.640	143	48963m	11.085	ng/ul	0.05
60) Fluorene-d10	15.281	176	431448	16.940	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	45334	8.538	ng/ul	0.00
73) Anthracene-d10	17.187	188	656784	16.850	ng/ul	0.00
81) Pyrene-d10	19.575	212	886859	14.349	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.610	264	1085307	17.804	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021345.D
Acq On : 03 Aug 2024 15:24
Operator : CG/JU
Sample : P3278-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZQ8

Manual IntegrationsAPPROVED

Quant Time: Aug 04 23:51:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/05/2024
Supervised By :mohammad ahmed 08/05/2024

