

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021348.D
 Acq On : 03 Aug 2024 17:40
 Operator : CG/JU
 Sample : P3278-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	26	29	36	rVB2	17277	28480	0.85%	0.106%
2	3.475	79	83	91	rBV	10718	22160	0.66%	0.083%
3	3.593	101	103	118	rBV	125895	270914	8.05%	1.011%
4	3.881	148	152	156	rVB3	8977	12008	0.36%	0.045%
5	4.470	250	252	258	rVB7	2259	3394	0.10%	0.013%
6	6.864	651	659	673	rBV	116746	381866	11.35%	1.425%
7	6.981	674	679	702	rVB	167711	350738	10.42%	1.309%
8	7.181	707	713	726	rBV	205442	413716	12.30%	1.544%
9	7.622	780	788	806	rBV	509785	975359	28.99%	3.641%
10	7.758	808	811	815	rVB6	3647	5490	0.16%	0.020%
11	8.375	910	916	939	rBV2	168087	529166	15.73%	1.975%
12	8.799	977	988	1011	rBV	186508	431630	12.83%	1.611%
13	9.116	1037	1042	1045	rBV7	6725	9156	0.27%	0.034%
14	9.381	1078	1087	1090	rBV8	7531	15747	0.47%	0.059%
15	9.510	1101	1109	1132	rBV2	145178	347577	10.33%	1.297%
16	9.687	1137	1139	1146	rVB6	2430	3441	0.10%	0.013%
17	10.093	1197	1208	1226	rBV4	100654	473218	14.07%	1.766%
18	10.387	1248	1258	1277	rBV	766189	1385851	41.19%	5.173%
19	10.581	1281	1291	1317	rBV	150422	509447	15.14%	1.902%
20	11.216	1389	1399	1404	rBV4	14260	42426	1.26%	0.158%
21	12.028	1533	1537	1541	rVB7	2381	4544	0.14%	0.017%
22	12.840	1672	1675	1680	rBV6	2097	3632	0.11%	0.014%
23	13.046	1704	1710	1715	rBV10	2901	5517	0.16%	0.021%
24	13.681	1810	1818	1837	rBV	520271	889186	26.43%	3.319%
25	13.951	1855	1864	1876	rBV	622419	1035369	30.77%	3.865%
26	14.263	1910	1917	1940	rVV	1174042	1956672	58.16%	7.303%
27	14.487	1946	1955	1961	rBV4	23181	63736	1.89%	0.238%
28	14.657	1978	1984	1985	rBV	44208	64200	1.91%	0.240%
29	15.034	2044	2048	2049	rBV4	2757	3649	0.11%	0.014%
30	15.063	2049	2053	2058	rVV6	5031	7194	0.21%	0.027%
31	15.122	2058	2063	2069	rVB10	4752	9281	0.28%	0.035%
32	15.287	2082	2091	2107	rBV	690677	1365294	40.58%	5.096%
33	15.481	2118	2124	2139	rBV	137738	309448	9.20%	1.155%
34	16.004	2207	2213	2218	rBV10	4023	8692	0.26%	0.032%
35	16.816	2348	2351	2355	rBV6	4217	7617	0.23%	0.028%
36	16.863	2357	2359	2364	rVB6	6041	9485	0.28%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021348.D
Acq On : 03 Aug 2024 17:40
Operator : CG/JU
Sample : P3278-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	16.986	2376	2380	2386	rVB7	9618	14193	0.42%	0.053%
38	17.075	2388	2395	2407	rBV	1463880	2483412	73.81%	9.269%
39	17.187	2408	2414	2432	rVB2	912208	1519579	45.17%	5.672%
40	17.481	2462	2464	2470	rVB7	5050	7679	0.23%	0.029%
41	17.757	2508	2511	2517	rVB7	10399	16020	0.48%	0.060%
42	18.010	2549	2554	2564	rBV2	117561	235324	6.99%	0.878%
43	19.116	2740	2742	2745	rBV4	12837	13725	0.41%	0.051%
44	19.345	2777	2781	2789	rBV6	42682	72002	2.14%	0.269%
45	19.486	2803	2805	2809	rVB5	18147	16900	0.50%	0.063%
46	19.575	2814	2820	2830	rBV	1269876	2024496	60.17%	7.556%
47	21.180	3089	3093	3099	rVB3	122892	204659	6.08%	0.764%
48	21.527	3147	3152	3166	rBV	1823980	2853519	84.82%	10.651%
49	24.598	3666	3674	3689	rVB	755468	2010572	59.76%	7.504%
50	24.816	3702	3711	3726	rVB2	1049217	3364397	100.00%	12.558%




Sum of corrected areas: 26791777

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021348.D
Acq On : 03 Aug 2024 17:40
Operator : CG/JU
Sample : P3278-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

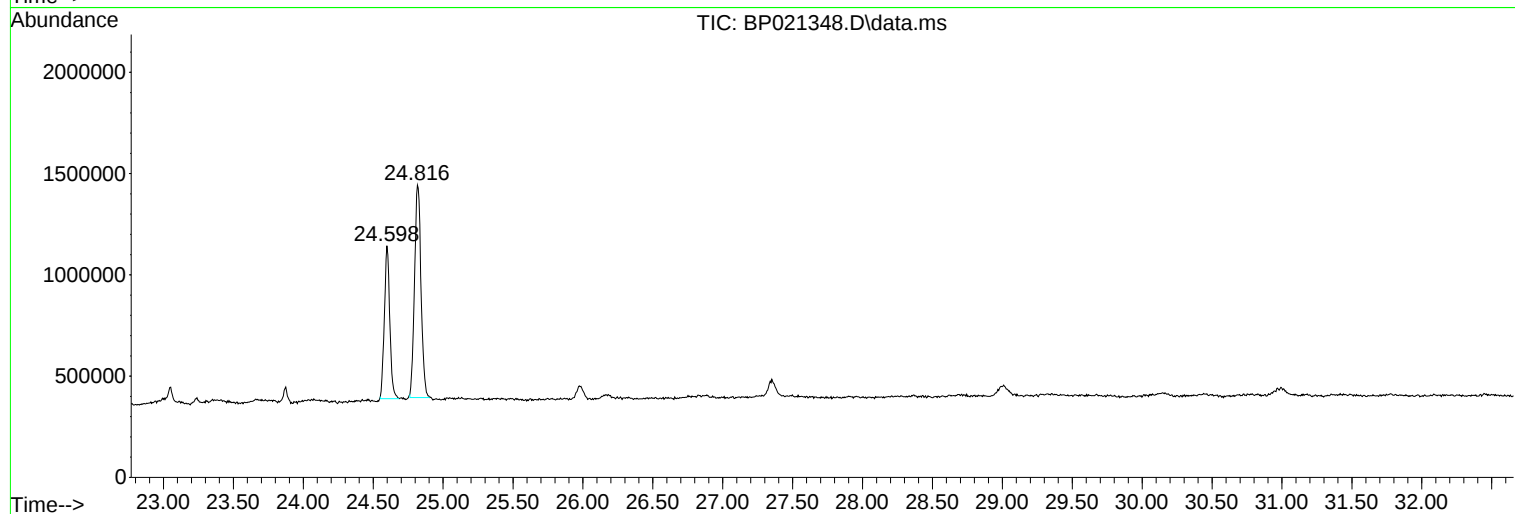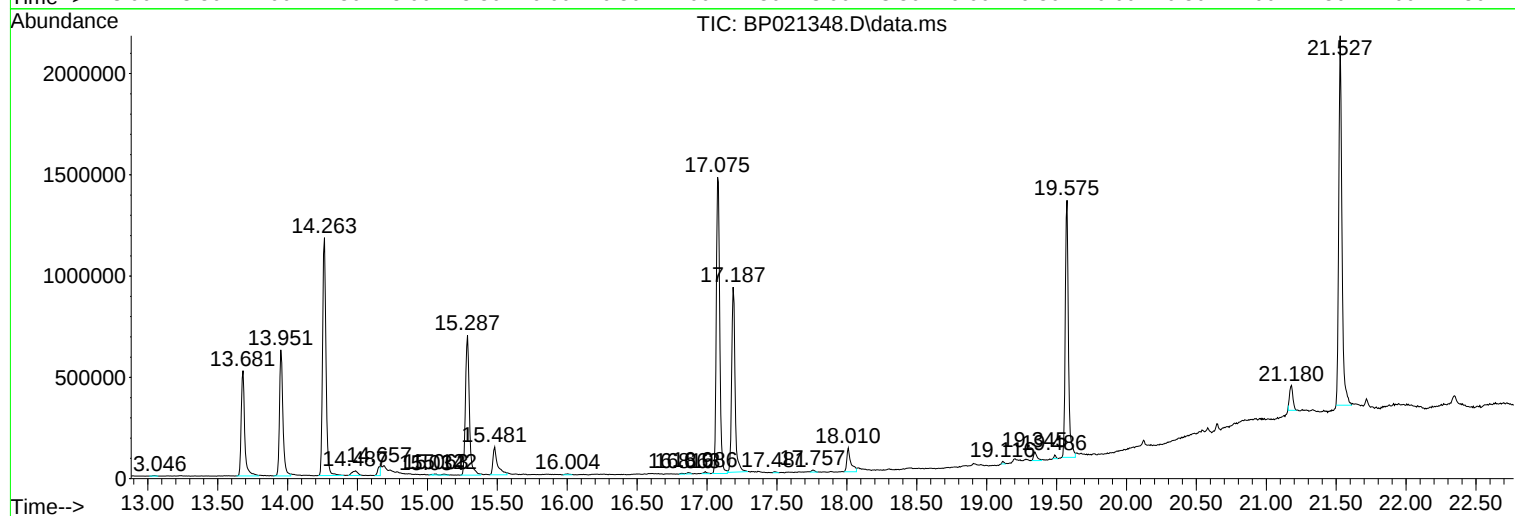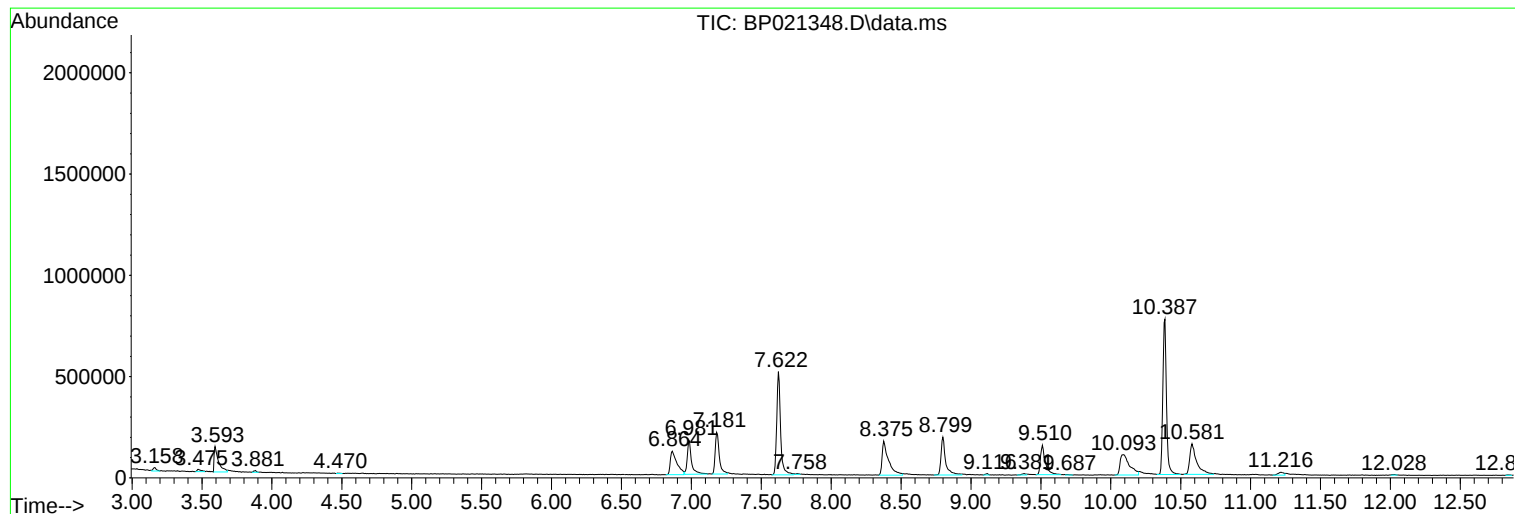

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021348.D
Acq On : 03 Aug 2024 17:40
Operator : CG/JU
Sample : P3278-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021348.D
Acq On : 03 Aug 2024 17:40
Operator : CG/JU
Sample : P3278-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc