

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021362.D
 Acq On : 04 Aug 2024 04:58
 Operator : CG/JU
 Sample : P3278-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	18	23	38	rVB	720798	1261763	36.06%	4.055%
2	3.464	78	81	92	rBV	33650	71893	2.05%	0.231%
3	3.587	99	102	126	rVB	215057	409415	11.70%	1.316%
4	3.875	148	151	157	rVB	12793	21325	0.61%	0.069%
5	6.852	651	657	672	rBV	186939	540274	15.44%	1.736%
6	6.975	672	678	695	rVB	253627	482723	13.80%	1.551%
7	7.181	706	713	729	rBV	330153	610765	17.46%	1.963%
8	7.616	780	787	809	rBV	827890	1438839	41.12%	4.624%
9	7.999	850	852	858	rVB7	2421	3934	0.11%	0.013%
10	8.363	908	914	934	rBV	248830	708674	20.25%	2.278%
11	8.622	957	958	963	rVB5	3173	3927	0.11%	0.013%
12	8.793	979	987	1002	rBV	255383	566182	16.18%	1.820%
13	8.934	1009	1011	1018	rVB8	2554	3662	0.10%	0.012%
14	9.034	1027	1028	1033	rVB5	3353	4021	0.11%	0.013%
15	9.110	1035	1041	1047	rVV9	4210	9933	0.28%	0.032%
16	9.369	1079	1085	1091	rBV3	13557	29023	0.83%	0.093%
17	9.416	1091	1093	1101	rVB9	2678	4291	0.12%	0.014%
18	9.499	1101	1107	1125	rBV	198406	471983	13.49%	1.517%
19	10.069	1197	1204	1224	rBV	204367	670890	19.17%	2.156%
20	10.381	1250	1257	1275	rBV	1023476	2000128	57.17%	6.428%
21	10.563	1281	1288	1318	rBV2	205668	654002	18.69%	2.102%
22	11.193	1388	1395	1406	rBV2	28690	90410	2.58%	0.291%
23	11.787	1490	1496	1500	rBV7	3617	6950	0.20%	0.022%
24	11.999	1527	1532	1539	rVB6	5255	8537	0.24%	0.027%
25	13.051	1706	1711	1716	rBV6	5873	9444	0.27%	0.030%
26	13.675	1810	1817	1834	rBV	564696	1077366	30.79%	3.462%
27	13.957	1854	1865	1878	rBV	732982	1296781	37.06%	4.168%
28	14.081	1884	1886	1891	rVB6	3295	4166	0.12%	0.013%
29	14.140	1891	1896	1904	rVB6	9163	14549	0.42%	0.047%
30	14.263	1909	1917	1933	rBV	1474165	2548357	72.84%	8.190%
31	14.481	1946	1954	1963	rBV3	38748	89489	2.56%	0.288%
32	14.669	1979	1986	1990	rBV4	32540	77310	2.21%	0.248%
33	15.063	2047	2053	2058	rBV9	4322	8992	0.26%	0.029%
34	15.116	2058	2062	2070	rVB7	5686	10248	0.29%	0.033%
35	15.281	2083	2090	2108	rBV	830156	1541221	44.05%	4.953%
36	15.487	2119	2125	2131	rBV2	62320	163473	4.67%	0.525%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
 Data File : BP021362.D
 Acq On : 04 Aug 2024 04:58
 Operator : CG/JU
 Sample : P3278-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E1ZS2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	15.857	2185	2188	2196	rBV10	3206	7560	0.22%	0.024%
38	15.992	2207	2211	2222	rVV7	11528	29325	0.84%	0.094%
39	16.498	2294	2297	2300	rBV5	2853	3636	0.10%	0.012%
40	16.810	2347	2350	2353	rBV3	5401	5540	0.16%	0.018%
41	16.998	2379	2382	2386	rBV5	7777	10349	0.30%	0.033%
42	17.081	2390	2396	2407	rBV	1682108	2563776	73.28%	8.239%
43	17.187	2407	2414	2437	rVB2	786758	1472133	42.08%	4.731%
44	17.481	2462	2464	2474	rVB2	4715	9564	0.27%	0.031%
45	17.581	2478	2481	2485	rVB5	5796	7592	0.22%	0.024%
46	17.775	2510	2514	2519	rVB4	11721	18017	0.51%	0.058%
47	18.016	2549	2555	2564	rBV2	80584	171888	4.91%	0.552%
48	19.222	2753	2760	2761	rBV3	16729	38830	1.11%	0.125%
49	19.339	2778	2780	2788	rVB7	23305	36459	1.04%	0.117%
50	19.486	2803	2805	2809	rVB4	16060	16782	0.48%	0.054%
51	19.575	2814	2820	2832	rBV	1004925	1631672	46.64%	5.244%
52	21.527	3146	3152	3162	rBV2	1538131	2781548	79.50%	8.939%
53	24.592	3666	3673	3685	rVB	698717	1897882	54.24%	6.099%
54	24.810	3702	3710	3727	rVB	1094898	3498784	100.00%	11.244%




Sum of corrected areas: 31116277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021362.D
Acq On : 04 Aug 2024 04:58
Operator : CG/JU
Sample : P3278-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZS2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

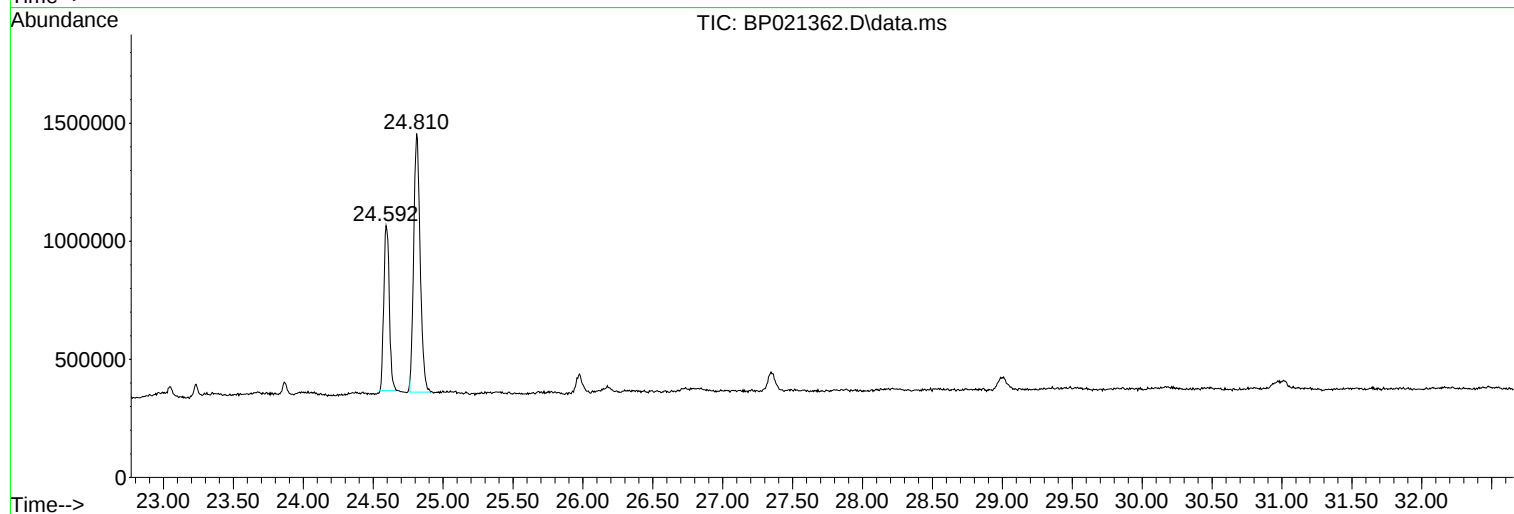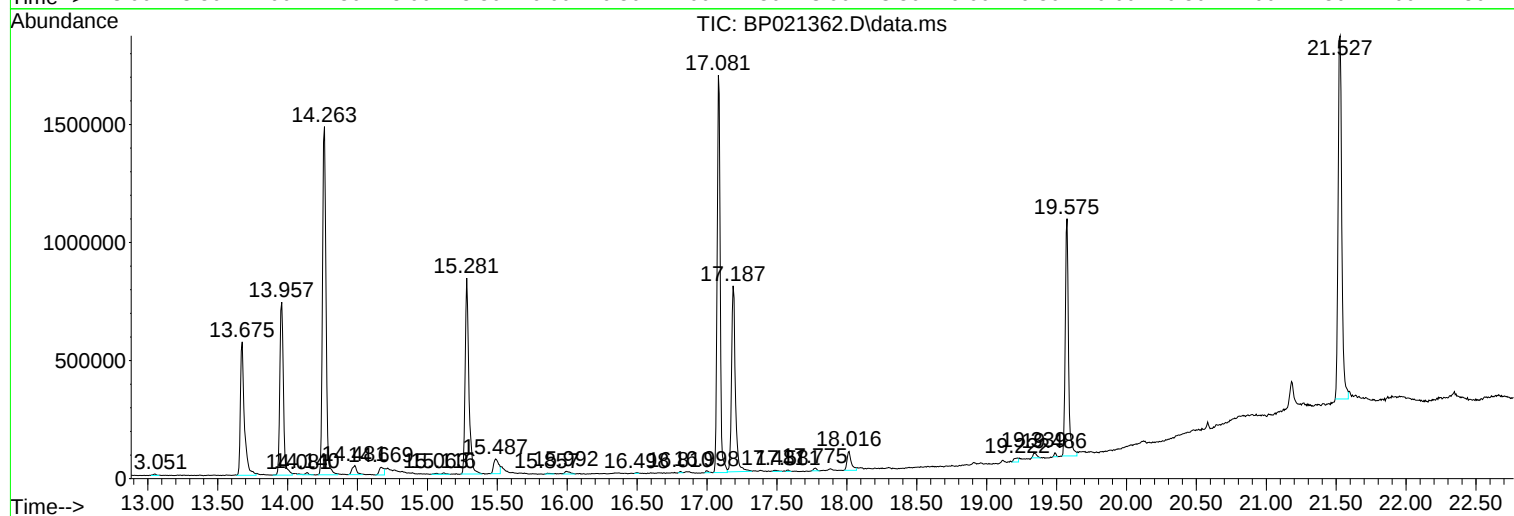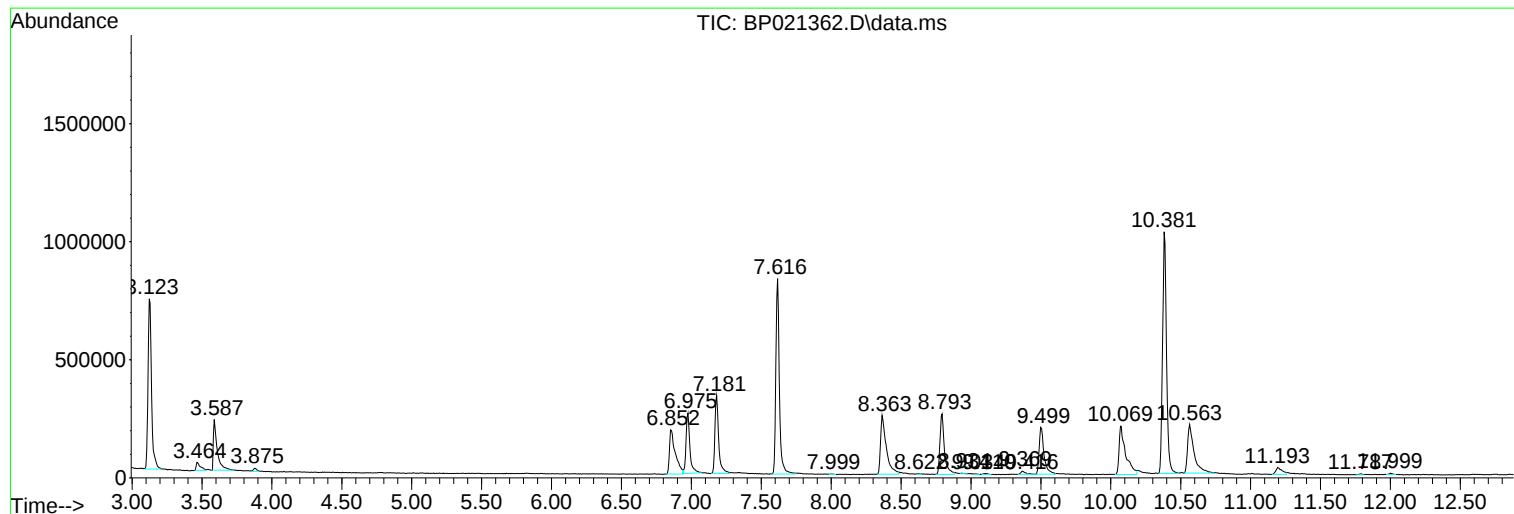

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021362.D
Acq On : 04 Aug 2024 04:58
Operator : CG/JU
Sample : P3278-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZS2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080324\
Data File : BP021362.D
Acq On : 04 Aug 2024 04:58
Operator : CG/JU
Sample : P3278-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E1ZS2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc