
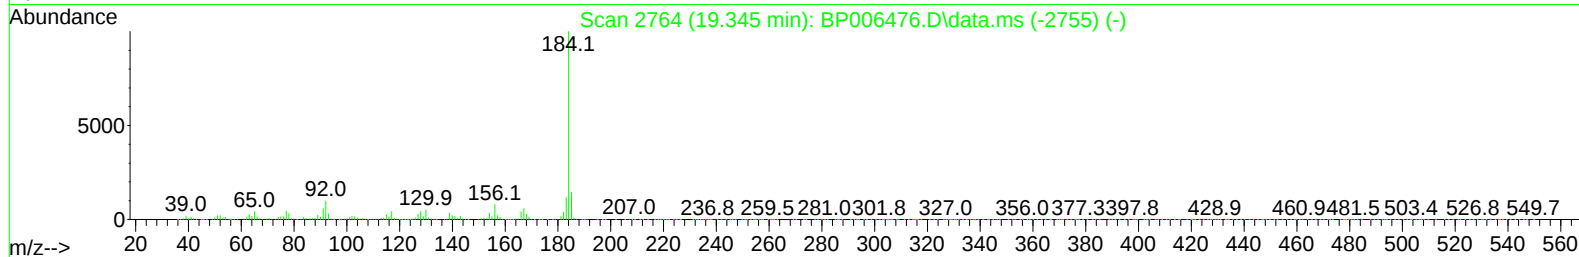
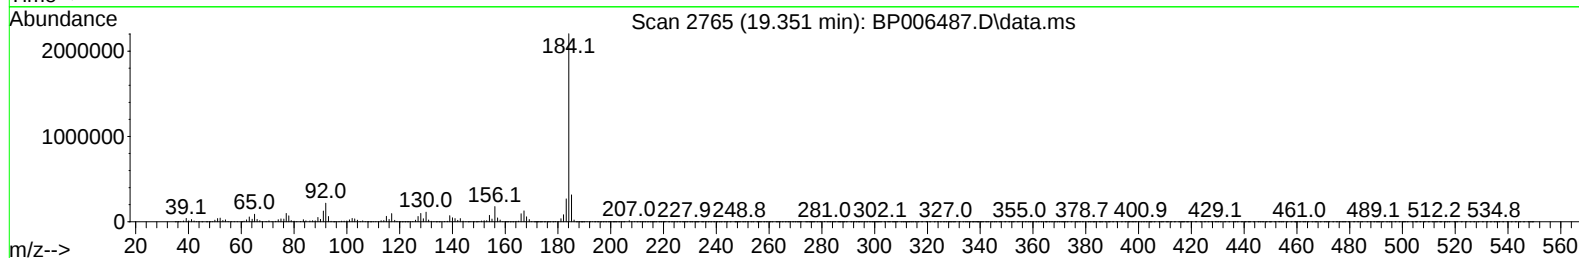


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080421\
 Data File : BP006487.D
 Acq On : 04 Aug 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 11:34:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

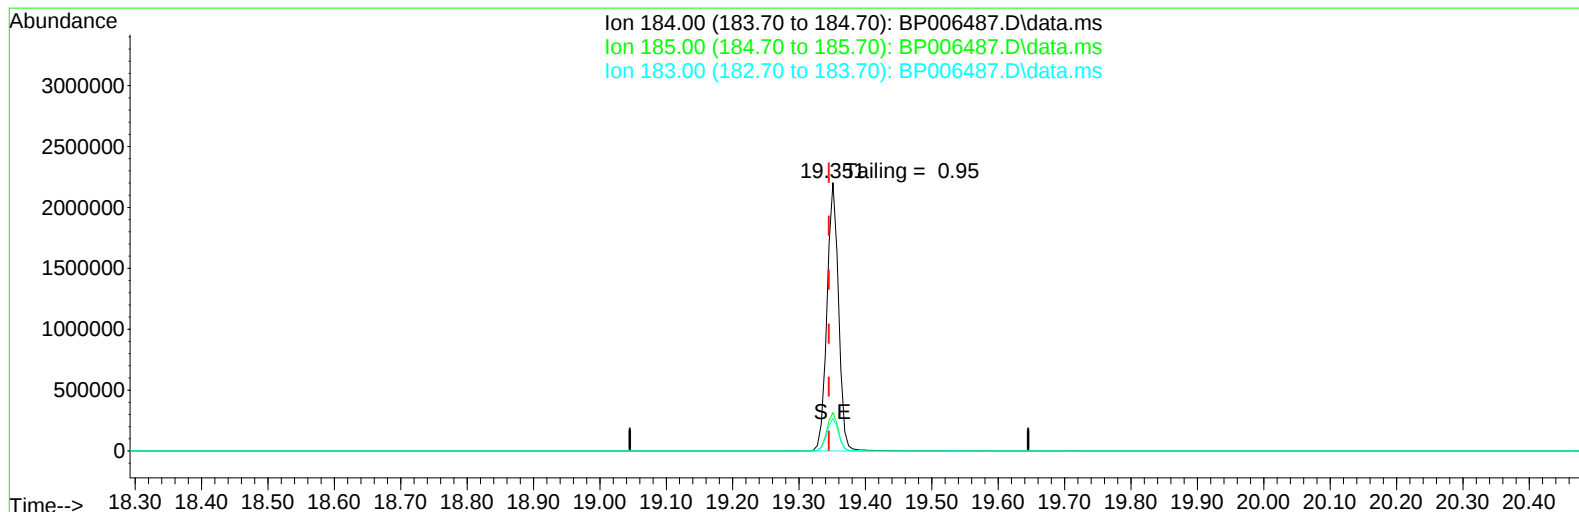

TIC: BP006487.D\data.ms

(77) Benzidine




19.351min (+ 0.006) 2030.05 ng

response 2671196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.33
183.00	11.90	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080421\
 Data File : BP006487.D
 Acq On : 04 Aug 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 11:34:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

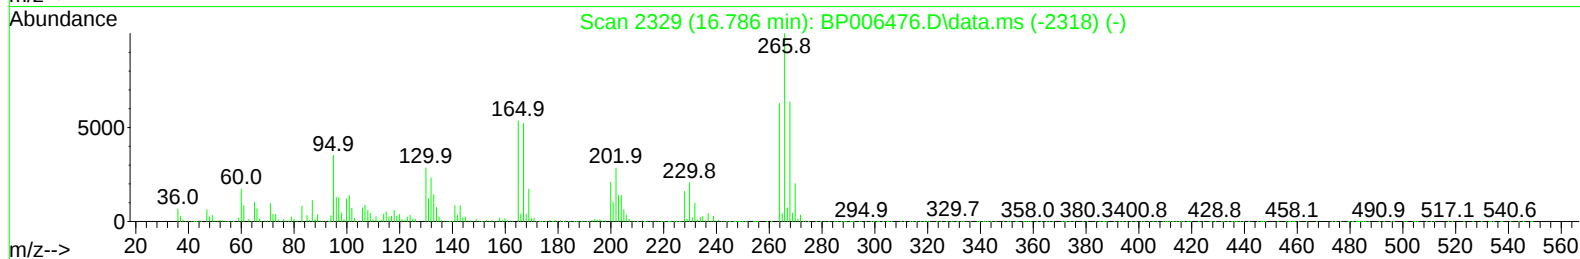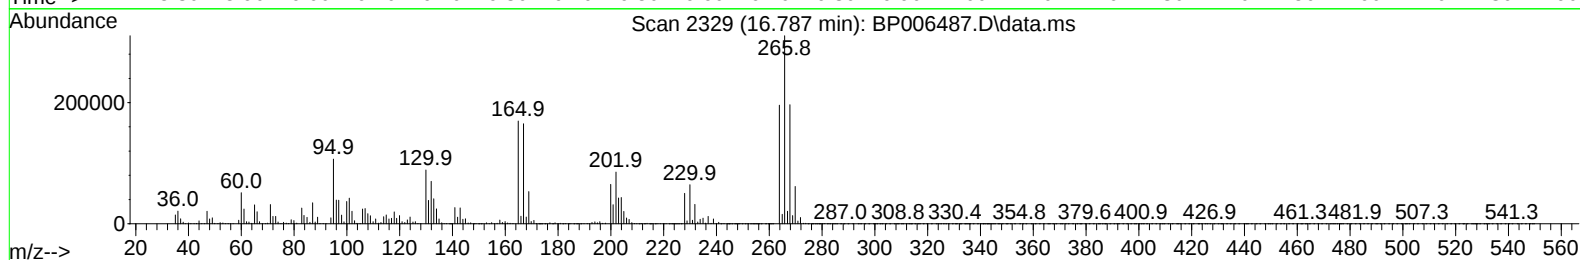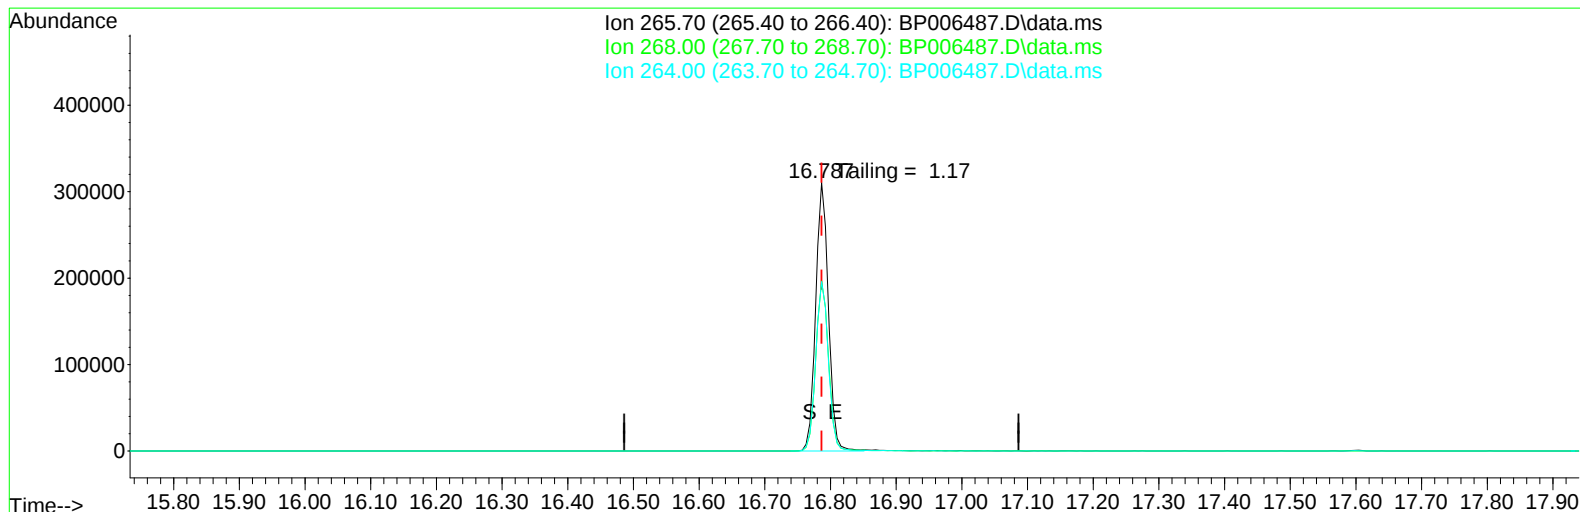

TIC: BP006487.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.000) 122681.06 ng

response 421553

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.35
264.00	62.90	63.08
0.00	0.00	0.00