
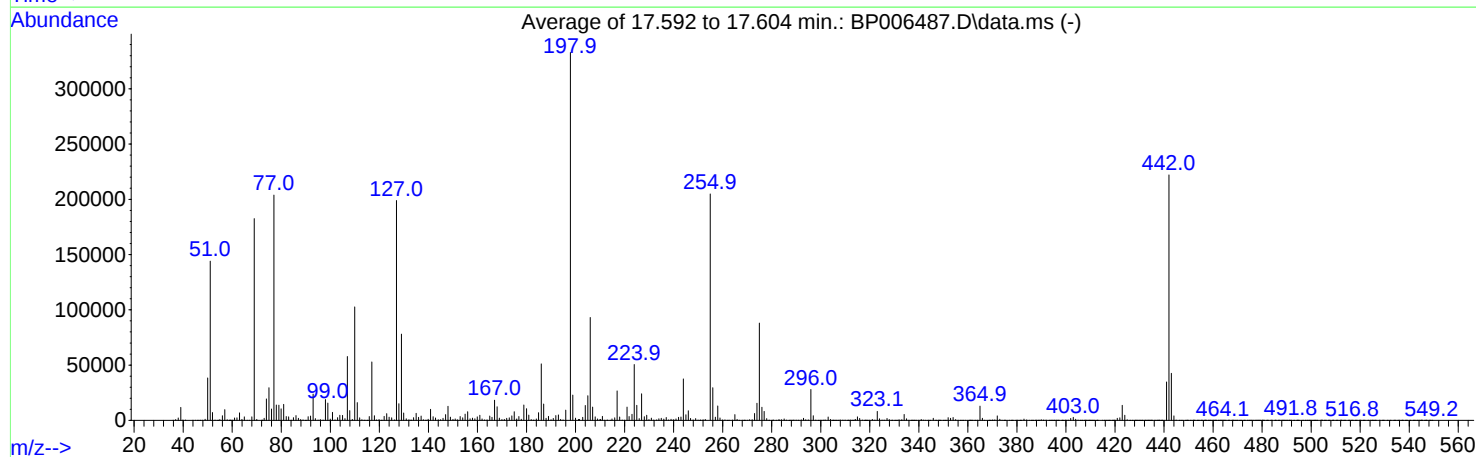


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080421\
 Data File : BP006487.D
 Acq On : 04 Aug 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:41:30 2021

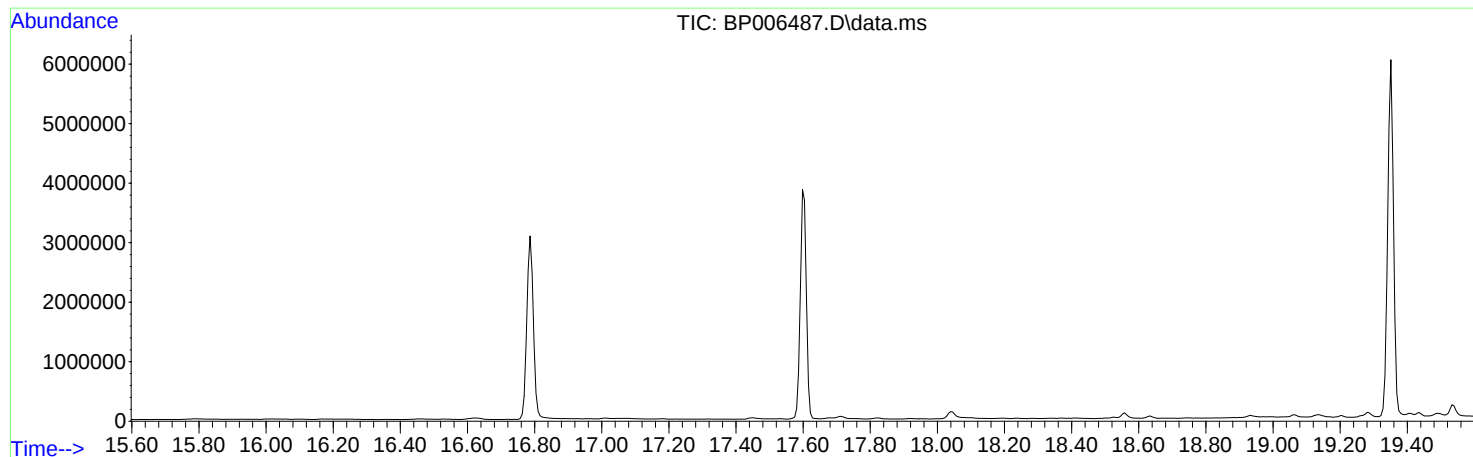




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	143998	PASS
68	69	0.00	2	1.8	3196	PASS
69	198	0.00	100	54.8	182504	PASS
70	69	0.00	2	0.5	857	PASS
127	198	10	80	59.7	198868	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	332838	PASS
199	198	5	9	6.9	22832	PASS
275	198	10	60	26.4	87998	PASS
365	198	1	100	3.9	12936	PASS
441	198	0.01	100	10.4	34769	PASS
442	442	100	100	100.0	222120	PASS
443	442	15	24	19.2	42637	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080421\
Data File : BP006487.D
Acq On : 04 Aug 2021 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 04 11:34:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

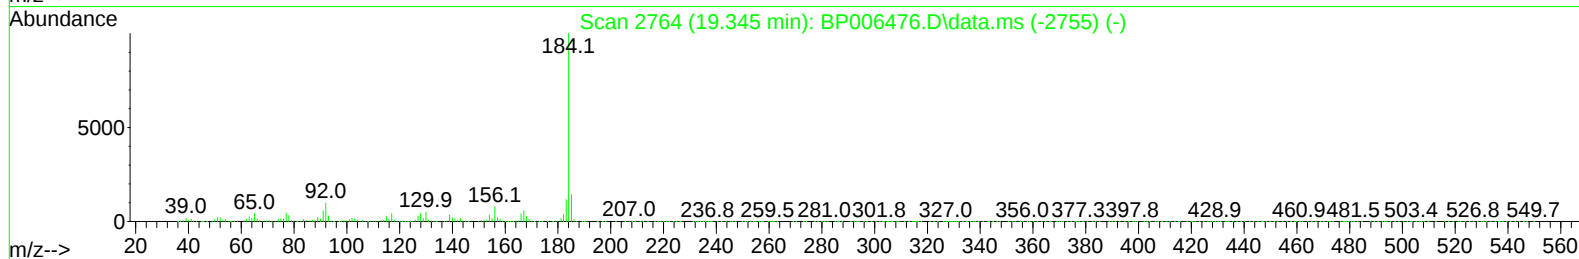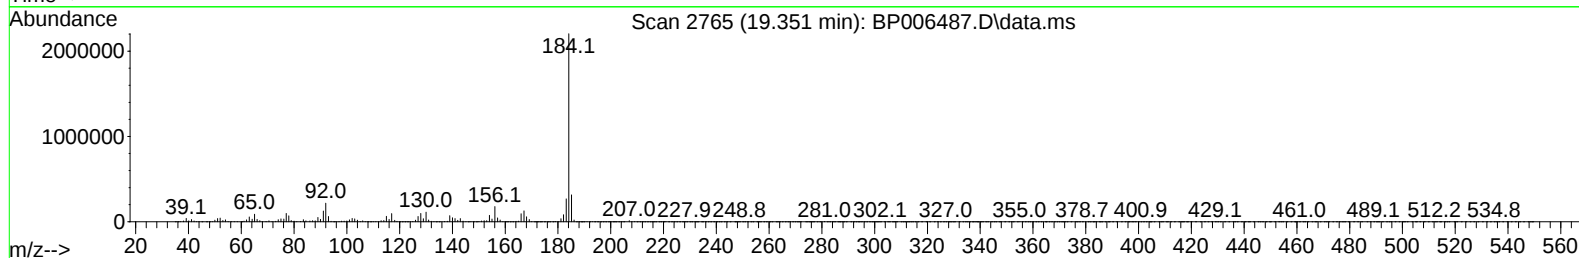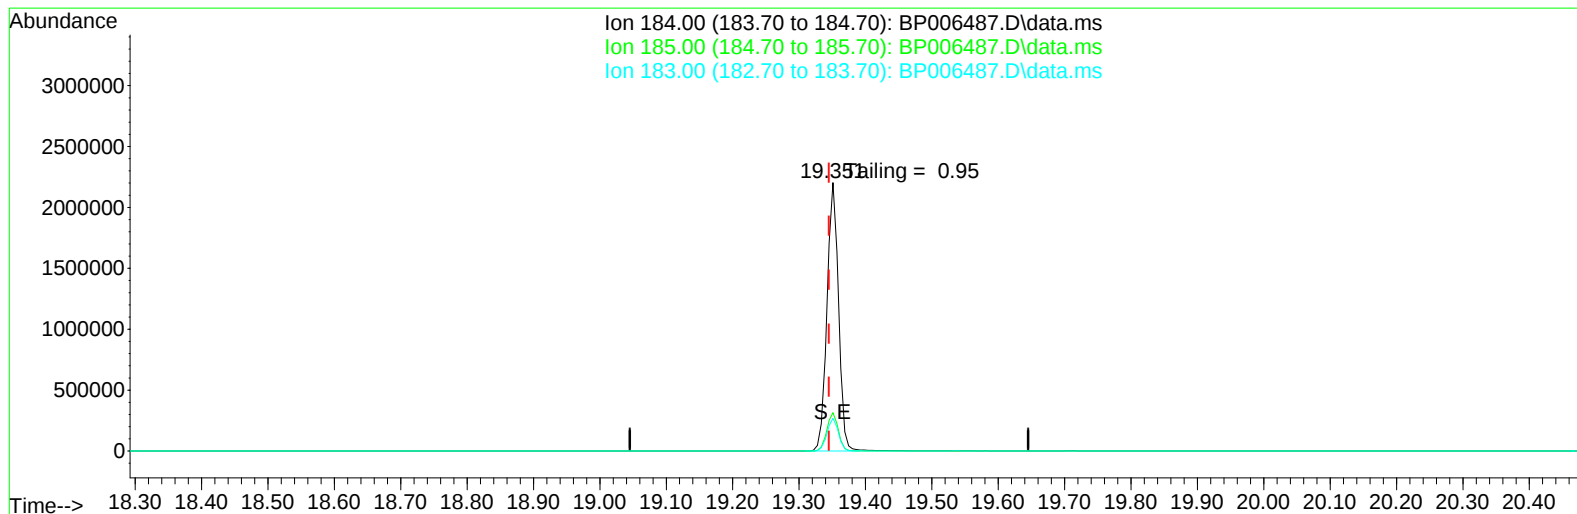

TIC: BP006487.D\data.ms

(77) Benzidine

19.351min (+ 0.006) 2030.05 ng




response 2671196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.33
183.00	11.90	12.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080421\
 Data File : BP006487.D
 Acq On : 04 Aug 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 04 11:34:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

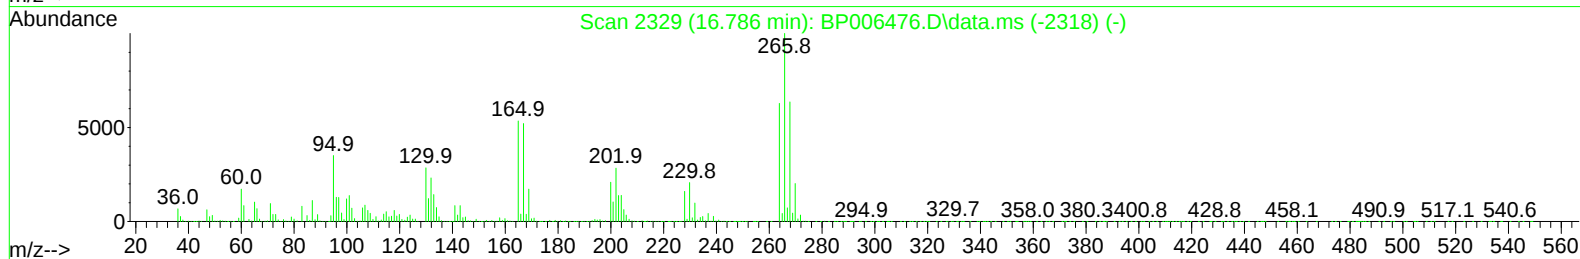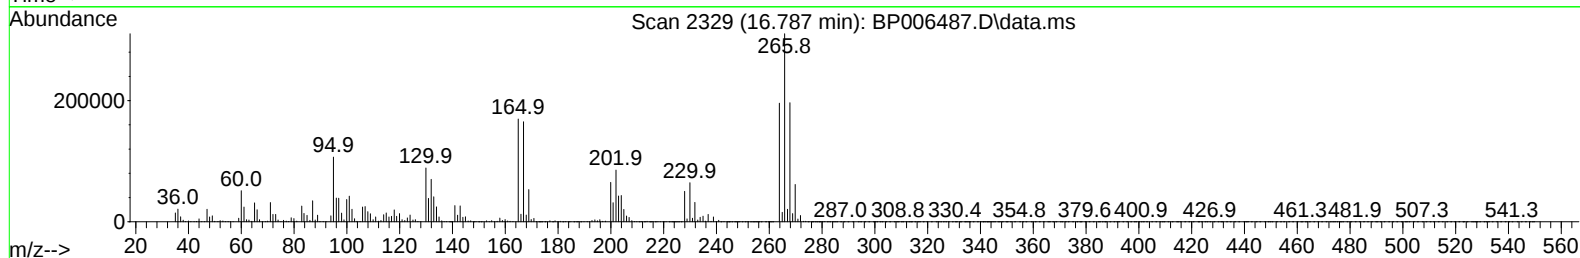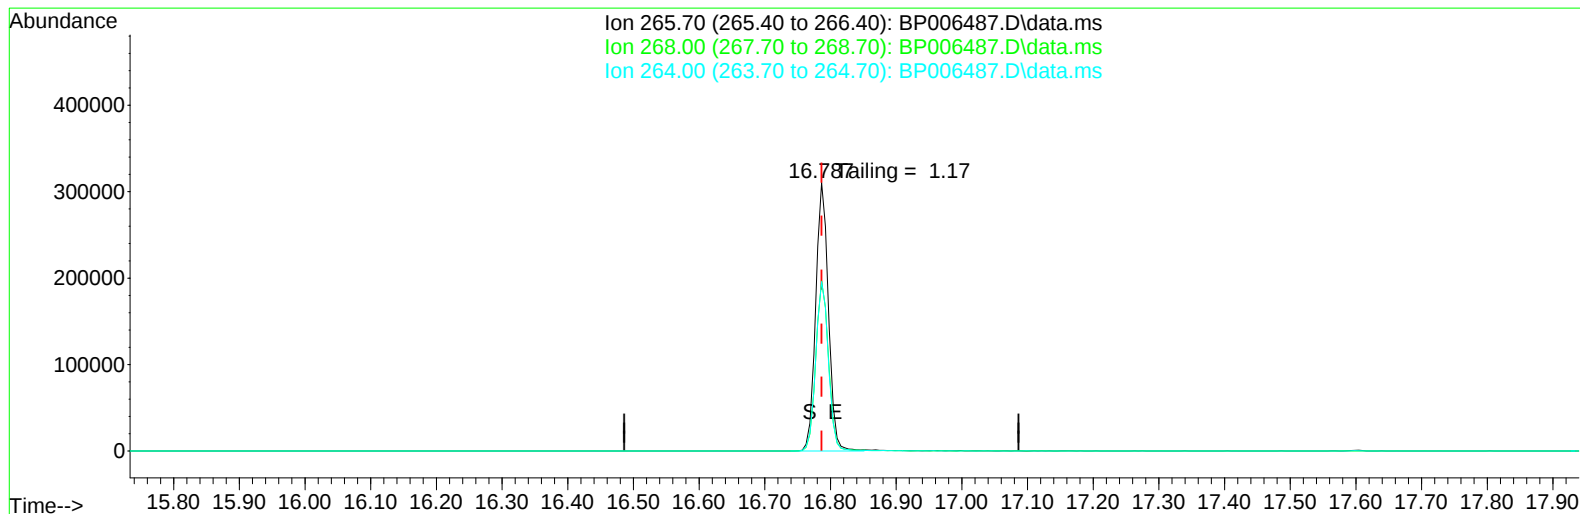

TIC: BP006487.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.000) 122681.06 ng

response 421553

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.35
264.00	62.90	63.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/4/2021	BNA_P	<u>BP006487.D</u>
Compound Name	Response	Retention Time
DDT	1256452	20.55
DDD	7305	20.12
DDE	2174	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9479	1265931	0.75

Instrument :
BNA_P
ClientSampleId :
DFTPP