

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011259.D
 Acq On : 04 Aug 2022 12:02
 Operator : CG/JU
 Sample : N3956-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF00

Quant Time: Aug 04 22:53:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.604	152	185746	20.000	ng/u1	0.00
20) Naphthalene-d8	10.398	136	941741	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	467032	20.000	ng/u1	# 0.00
64) Phenanthrene-d10	17.045	188	948503	20.000	ng/u1	0.00
79) Chrysene-d12	21.174	240	892707	20.000	ng/u1	0.00
88) Perylene-d12	23.492	264	955318	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	5623	2.448	ng/uL	0.00
4) Pyridine-d5	3.505	84	48196	7.778	ng/u1	0.00
7) Phenol-d5	6.787	99	51560	3.331	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	279852	25.055	ng/u1	0.00
11) 2-Chlorophenol-d4	7.134	132	188627	14.950	ng/u1	0.00
15) 4-Methylphenol-d8	8.328	113	132499	10.403	ng/u1	0.00
21) Nitrobenzene-d5	8.769	128	163542	24.144	ng/u1	0.00
24) 2-Nitrophenol-d4	9.487	143	100932	15.896	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	308049	25.442	ng/u1	0.00
31) 4-Chloroaniline-d4	10.551	131	426258	22.756	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	1008976	31.543	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1188593	29.534	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	5464	1.005	ng/u1	0.02
60) Fluorene-d10	15.281	176	913462	33.562	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	10920	2.479	ng/u1	0.00
73) Anthracene-d10	17.145	188	1428547	34.269	ng/u1	0.00
81) Pyrene-d10	19.410	212	1573683	34.866	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.345	264	1640076	34.452	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.434	105	27544	1.334	ng/u1	94
59) Diethylphthalate	15.122	149	166008	4.985	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011259.D
Acq On : 04 Aug 2022 12:02
Operator : CG/JU
Sample : N3956-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF00

Quant Time: Aug 04 22:53:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration




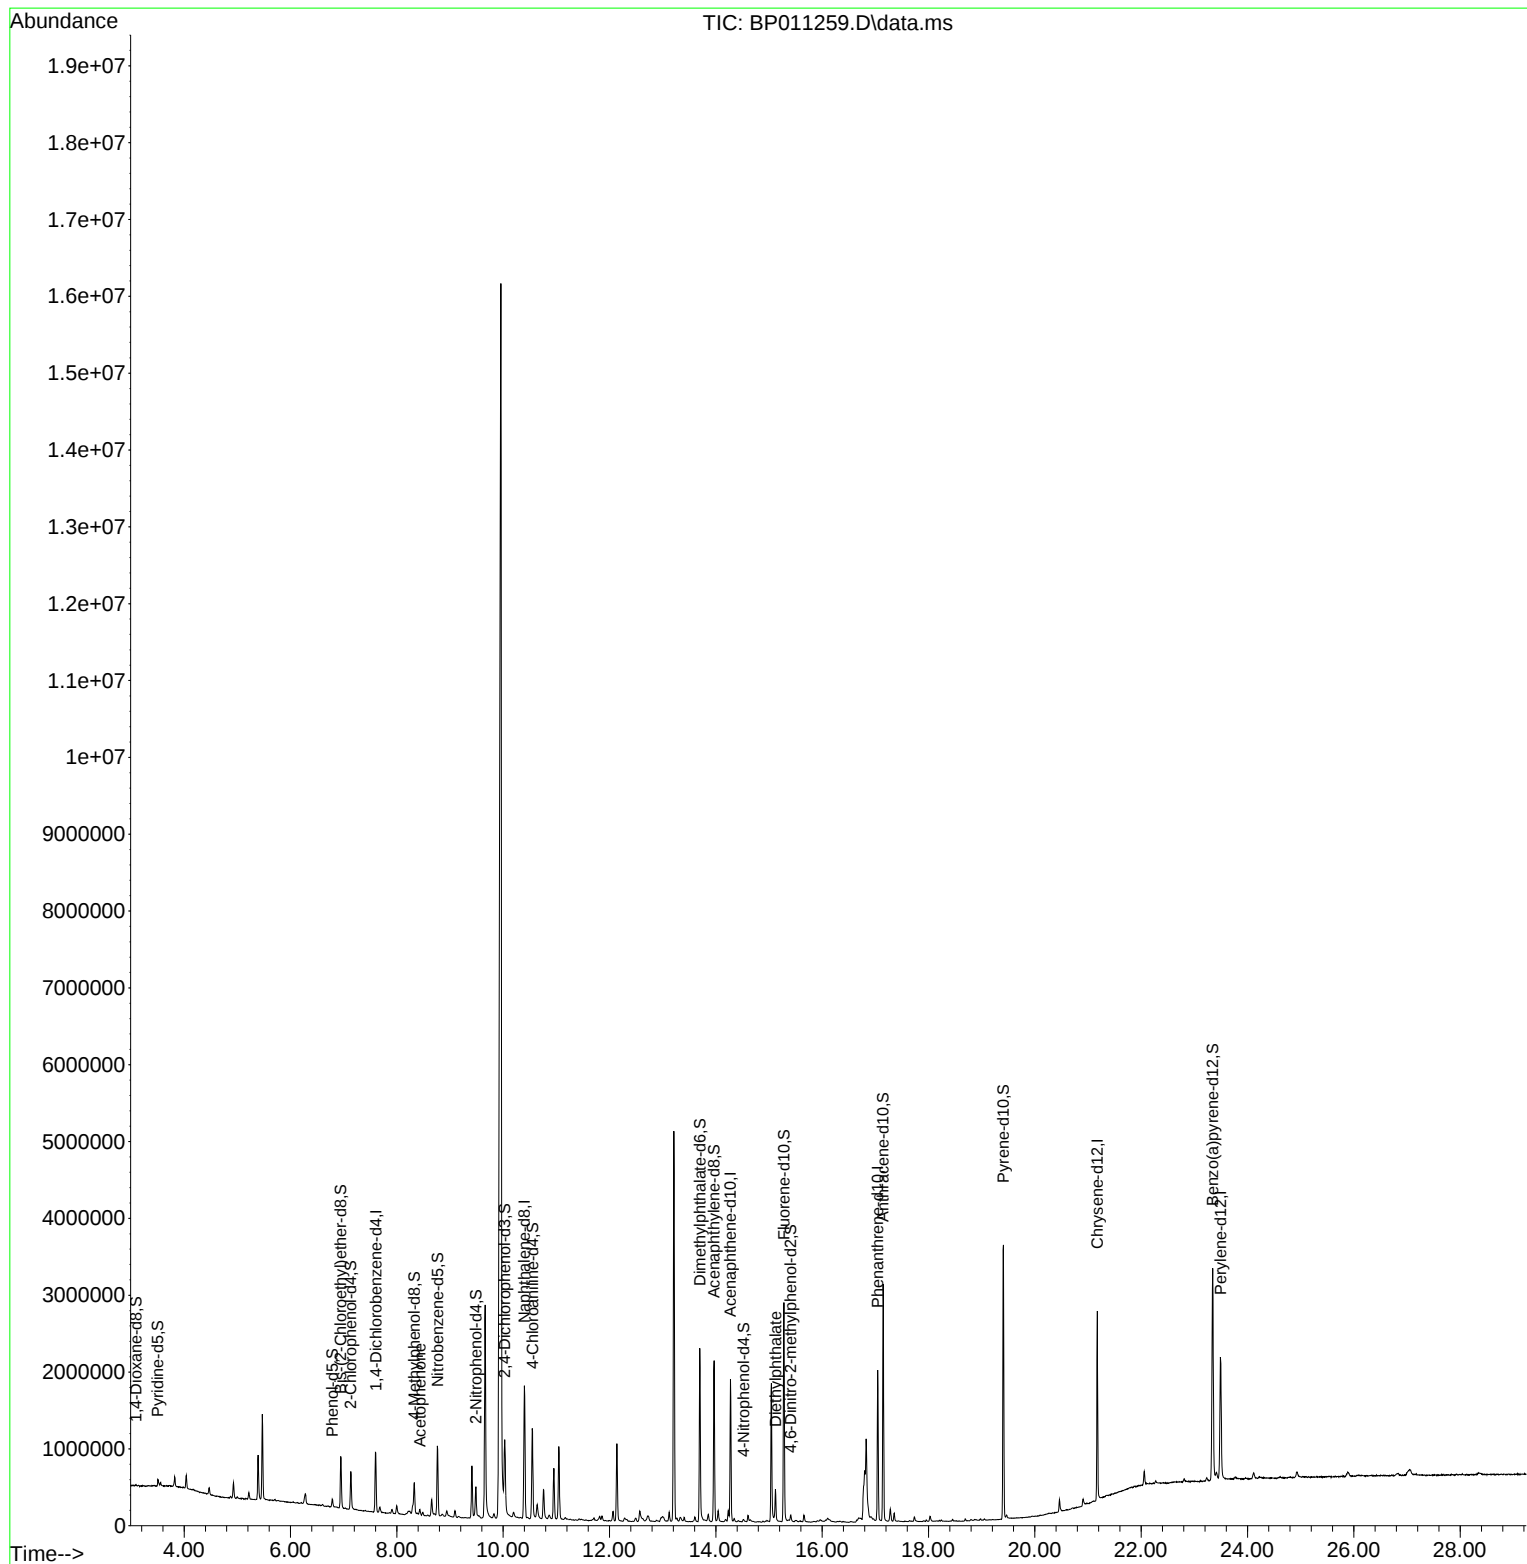


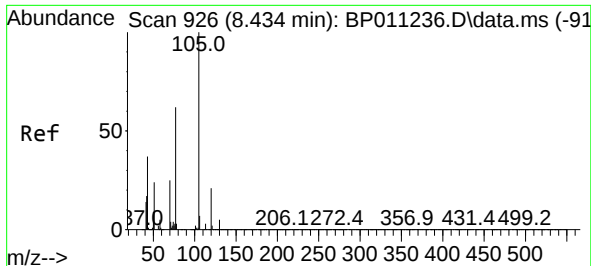

#16
Acetophenone
Concen: 1.334 ng/ul
RT: 8.434 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP011259.D
Acq: 04 Aug 2022 12:02

Instrument :
BNA_P
ClientSampleId :
EXF00

Tgt Ion:	105	Resp:	27544
Ion	Ratio	Lower	Upper
105	100		
77	85.6	65.4	98.0
51	37.9	26.5	39.7

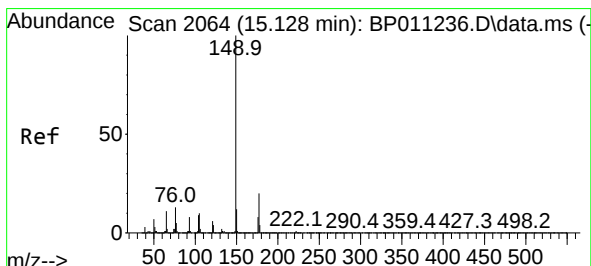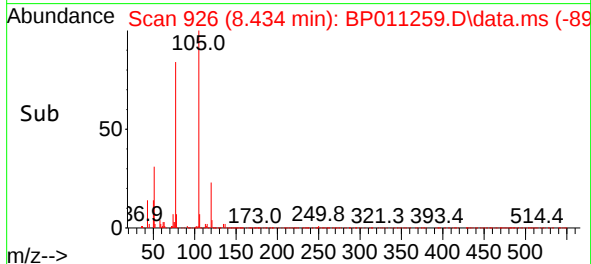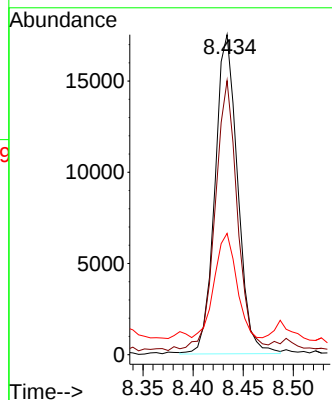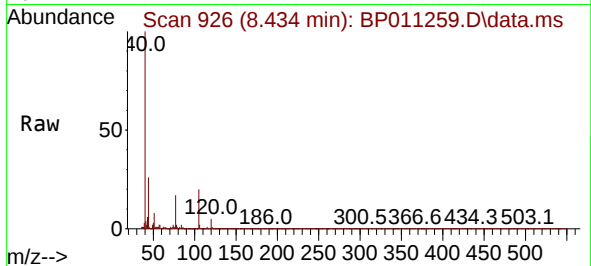

#59
Diethylphthalate
Concen: 4.985 ng/ul
RT: 15.122 min Scan# 2063
Delta R.T. -0.006 min
Lab File: BP011259.D
Acq: 04 Aug 2022 12:02

Tgt Ion:	149	Resp:	166008
Ion	Ratio	Lower	Upper
149	100		
177	19.9	16.1	24.1
150	13.0	9.4	14.0

