

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011264.D
 Acq On : 04 Aug 2022 14:55
 Operator : CG/JU
 Sample : N3956-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 04 22:54:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	235033	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	1039732	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	530568	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	1059819	20.000	ng/u1	0.00
79) Chrysene-d12	21.175	240	976400	20.000	ng/u1	0.00
88) Perylene-d12	23.492	264	991865	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	6968	2.397	ng/uL	0.00
4) Pyridine-d5	3.511	84	49028	6.253	ng/u1	0.00
7) Phenol-d5	6.799	99	122027	6.230	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	6.952	67	438555	31.029	ng/u1	0.00
11) 2-Chlorophenol-d4	7.140	132	366811	22.976	ng/u1	0.00
15) 4-Methylphenol-d8	8.328	113	262875	16.311	ng/u1	0.00
21) Nitrobenzene-d5	8.769	128	252940	33.822	ng/u1	0.00
24) 2-Nitrophenol-d4	9.499	143	197555	28.182	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.028	165	391042	29.253	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	458133	22.153	ng/u1	0.02
46) Dimethylphthalate-d6	13.698	166	1357423	37.355	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1682534	36.801	ng/u1	0.00
54) 4-Nitrophenol-d4	14.522	143	17339	2.806	ng/u1	0.02
60) Fluorene-d10	15.275	176	1187904	38.418	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	128634	26.139	ng/u1	0.00
73) Anthracene-d10	17.145	188	1718792	36.901	ng/u1	0.00
81) Pyrene-d10	19.410	212	1893766	38.361	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.345	264	1822948	36.882	ng/u1	0.00
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.034	93	65465	3.799	ng/u1	87
34) Caprolactam	11.369	113	84095	20.323	ng/u1#	3


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011264.D
Acq On : 04 Aug 2022 14:55
Operator : CG/JU
Sample : N3956-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Aug 04 22:54:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration




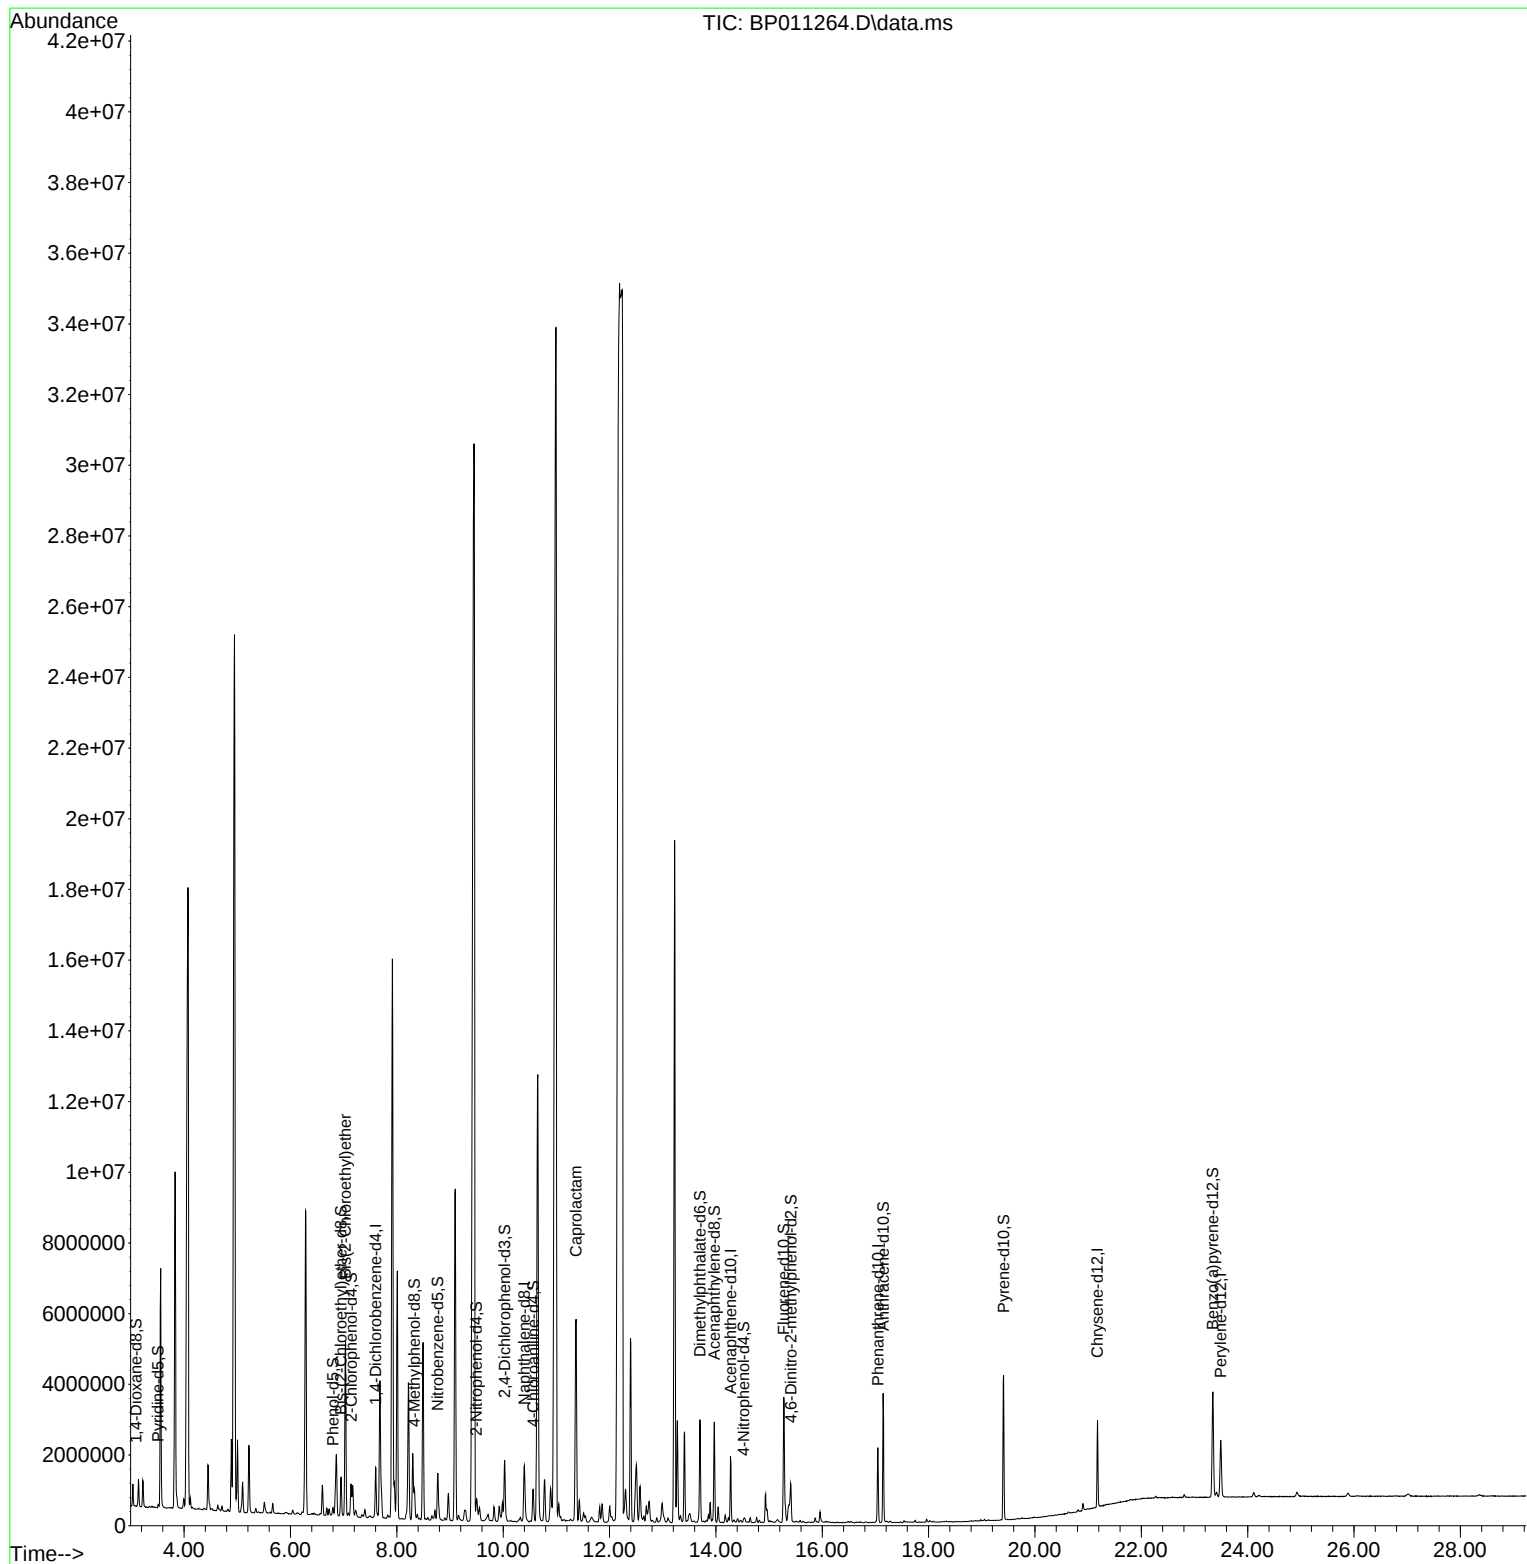


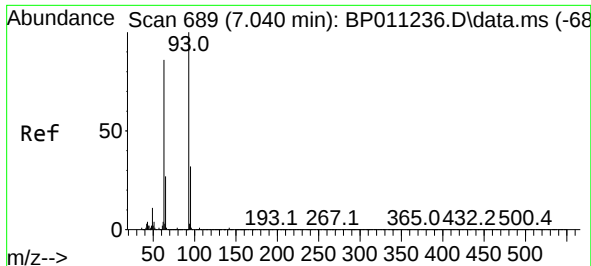

#10
 Bis(2-Chloroethyl)ether
 Concen: 3.799 ng/ul
 RT: 7.034 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BP011264.D
 Acq: 04 Aug 2022 14:55

Instrument :
 BNA_P
 ClientSampleId :

Tgt Ion: 93 Resp: 65465
 Ion Ratio Lower Upper
 93 100
 63 104.5 71.0 106.6
 95 31.7 26.0 39.0

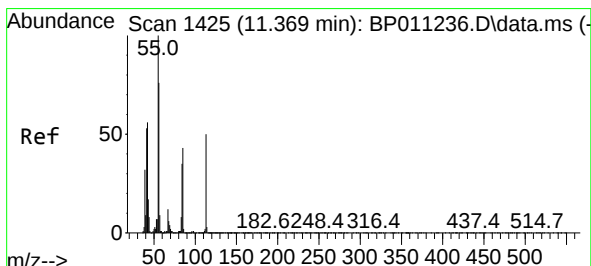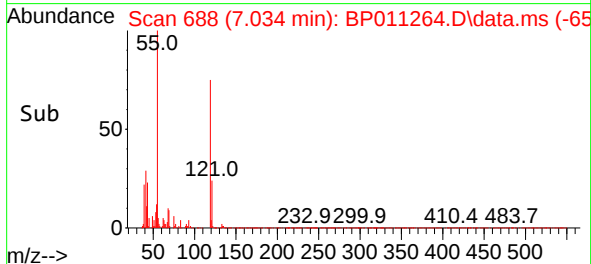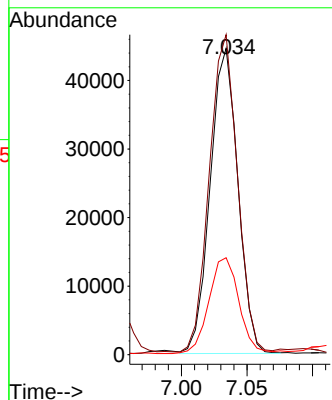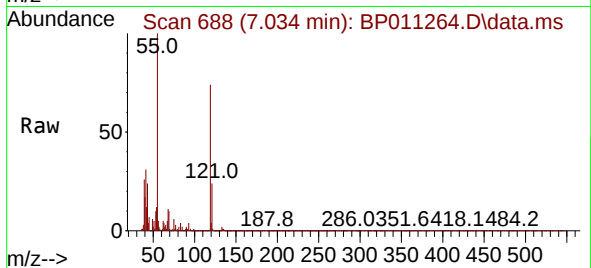

#34
 Caprolactam
 Concen: 20.323 ng/ul
 RT: 11.369 min Scan# 1425
 Delta R.T. 0.000 min
 Lab File: BP011264.D
 Acq: 04 Aug 2022 14:55

Tgt Ion: 113 Resp: 84095
 Ion Ratio Lower Upper
 113 100
 55 43.7 164.2 246.4#
 56 44.6 127.0 190.6#

