

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011265.D
 Acq On : 04 Aug 2022 15:30
 Operator : CG/JU
 Sample : N3956-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF03

Quant Time: Aug 04 22:54:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	206044	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	938430	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	511952	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	1052218	20.000	ng/u1	0.00
79) Chrysene-d12	21.174	240	1065955	20.000	ng/u1	0.00
88) Perylene-d12	23.498	264	1119600	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	6219	2.440	ng/uL	0.00
4) Pyridine-d5	3.511	84	41592	6.051	ng/u1	0.00
7) Phenol-d5	6.787	99	119245	6.945	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	355801	28.716	ng/u1	0.00
11) 2-Chlorophenol-d4	7.134	132	312467	22.326	ng/u1	0.00
15) 4-Methylphenol-d8	8.328	113	234913	16.627	ng/u1	0.00
21) Nitrobenzene-d5	8.763	128	204657	30.320	ng/u1	0.00
24) 2-Nitrophenol-d4	9.487	143	166940	26.385	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	329179	27.283	ng/u1	0.00
31) 4-Chloroaniline-d4	10.546	131	369813	19.812	ng/u1	0.00
46) Dimethylphthalate-d6	13.698	166	1226460	34.978	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	1472029	33.367	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	15247	2.557	ng/u1	0.01
60) Fluorene-d10	15.281	176	1051743	35.252	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	101807	20.837	ng/u1	0.00
73) Anthracene-d10	17.145	188	1647255	35.621	ng/u1	0.00
81) Pyrene-d10	19.410	212	1933707	35.879	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.345	264	1997012	35.794	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.123	88	9999	4.254	ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011265.D
Acq On : 04 Aug 2022 15:30
Operator : CG/JU
Sample : N3956-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF03

Quant Time: Aug 04 22:54:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

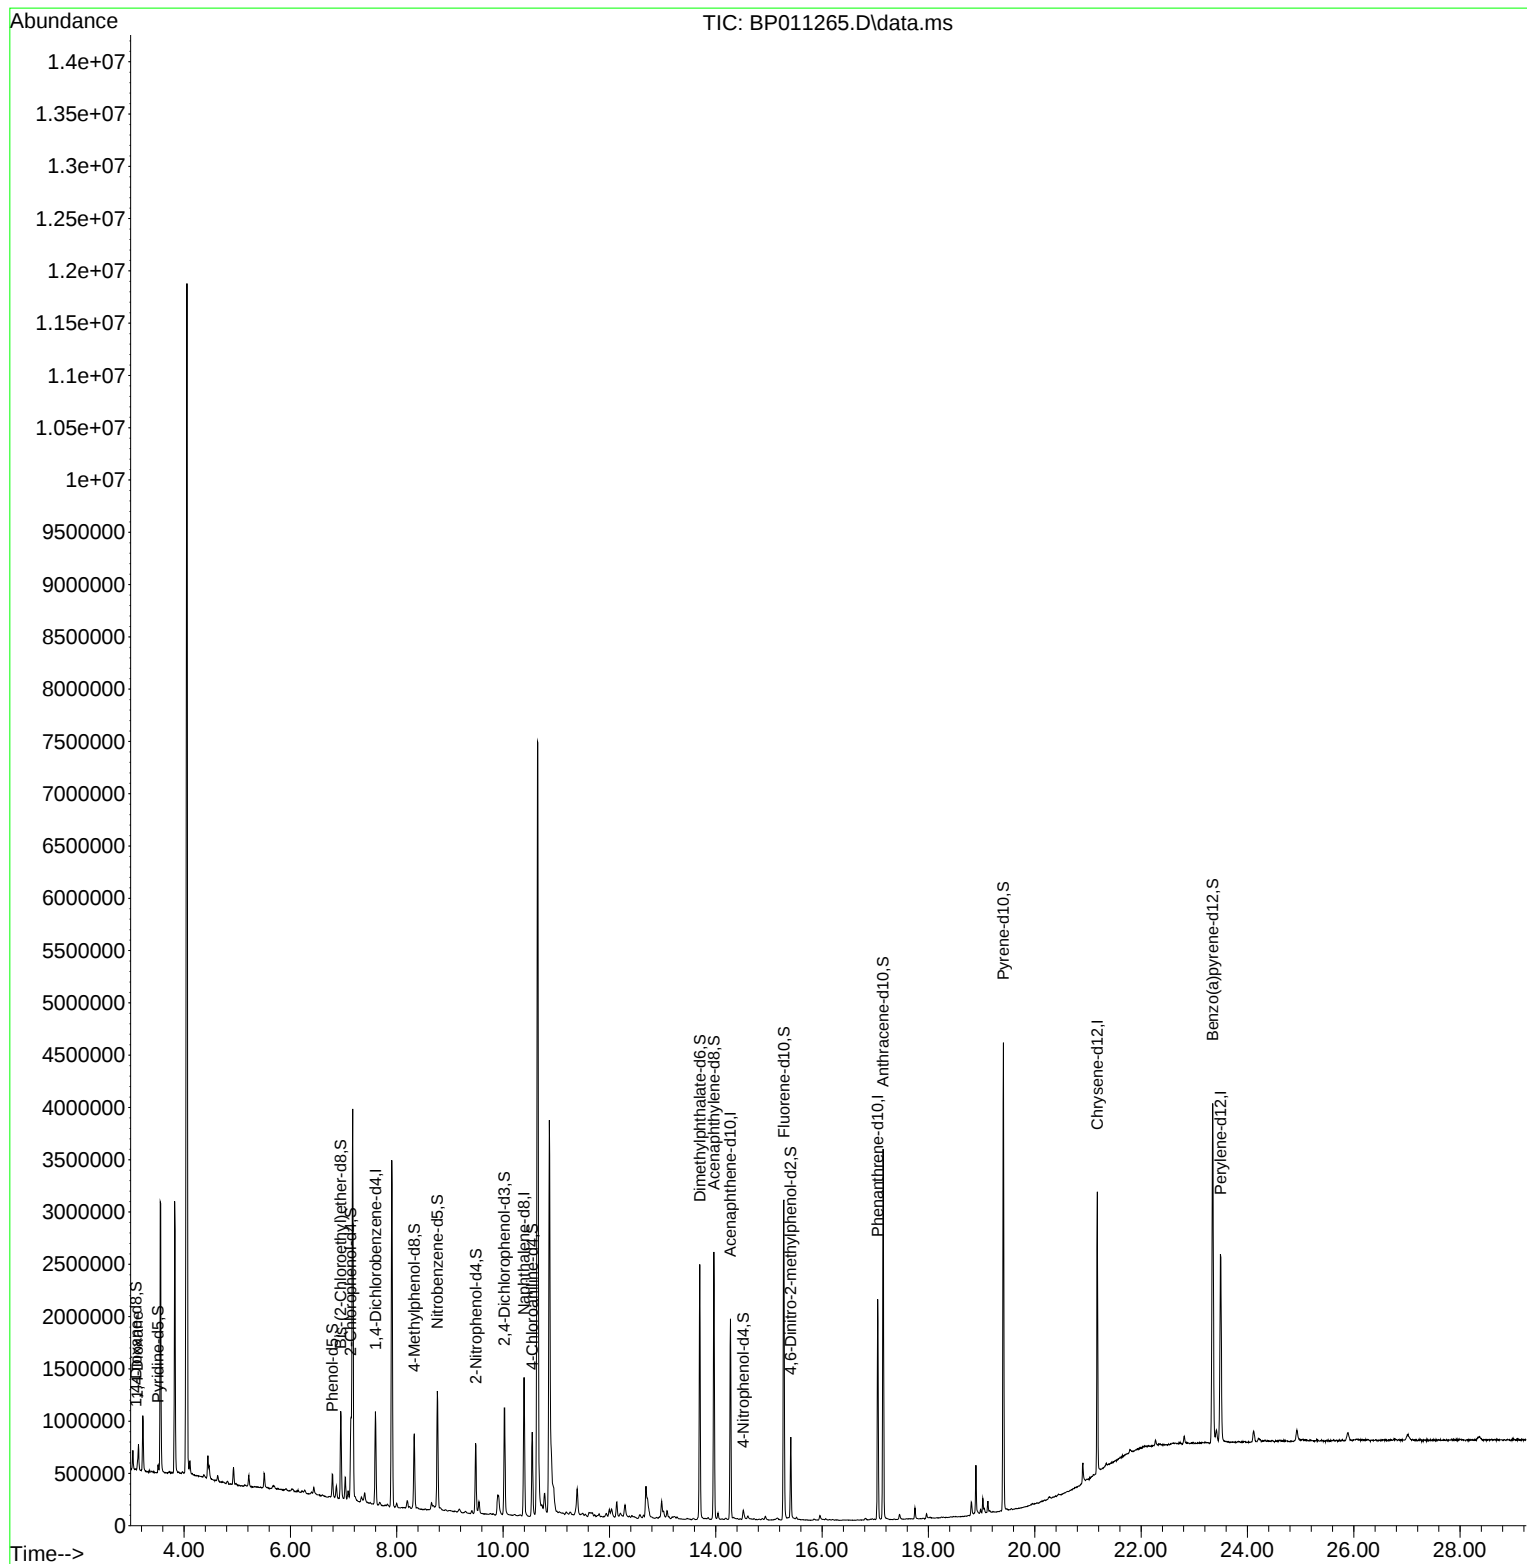

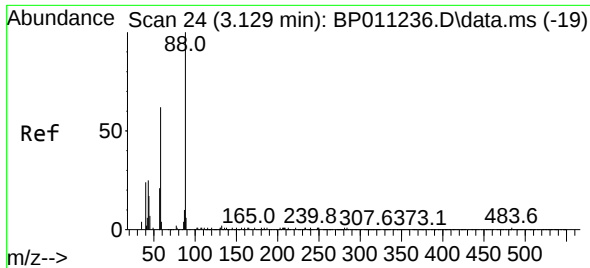

#2
 1,4-Dioxane
 Concen: 4.254 ng/uL
 RT: 3.123 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP011265.D
 Acq: 04 Aug 2022 15:30

Instrument :
 BNA_P
 ClientSampleId :
 EXF03

Tgt Ion: 88 Resp: 9999
 Ion Ratio Lower Upper
 88 100
 43 297.1 29.6 44.4#
 58 78.4 49.1 73.7#

