

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011263.D
 Acq On : 04 Aug 2022 14:20
 Operator : CG/JU
 Sample : N3956-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF05

Quant Time: Aug 04 22:54:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 02 23:52:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.605	152	223673	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	1110985	20.000	ng/u1	# 0.01
38) Acenaphthene-d10	14.281	164	604461	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	1191366	20.000	ng/u1	0.00
79) Chrysene-d12	21.175	240	1083541	20.000	ng/u1	0.00
88) Perylene-d12	23.492	264	1087295	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	6548	2.367	ng/uL	0.00
4) Pyridine-d5	3.511	84	46931	6.289	ng/u1	0.00
7) Phenol-d5	6.846	99	872284	46.796	ng/u1	0.06
9) Bis-(2-Chloroethyl)eth...	6.958	67	420962	31.297	ng/u1	0.00
11) 2-Chlorophenol-d4	7.152	132	402315	26.480	ng/u1	0.01
15) 4-Methylphenol-d8	8.358	113	298261	19.446	ng/u1	0.03
21) Nitrobenzene-d5	8.769	128	259659	32.494	ng/u1	0.00
24) 2-Nitrophenol-d4	9.493	143	252001	33.643	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.110	165	22164206	1551.697	ng/u1	0.09
31) 4-Chloroaniline-d4	10.593	131	329124	14.894	ng/u1	0.05
46) Dimethylphthalate-d6	13.722	166	1377562	33.275	ng/u1	0.02
49) Acenaphthylene-d8	13.969	160	1890986	36.304	ng/u1	0.00
54) 4-Nitrophenol-d4	14.540	143	57289	8.138	ng/u1	0.04
60) Fluorene-d10	15.281	176	1279141	36.312	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	205707	37.185	ng/u1	0.00
73) Anthracene-d10	17.151	188	1908861	36.457	ng/u1	0.00
81) Pyrene-d10	19.410	212	2077813	37.927	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.339	264	1967022	36.304	ng/u1	0.00
Target Compounds						
					Qvalue	
13) 2-Methylphenol	8.069	108	24191	1.600	ng/u1	95
18) 4-Methylphenol	8.422	108	61780	3.809	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011263.D
Acq On : 04 Aug 2022 14:20
Operator : CG/JU
Sample : N3956-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF05

Quant Time: Aug 04 22:54:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 02 23:52:37 2022
Response via : Initial Calibration

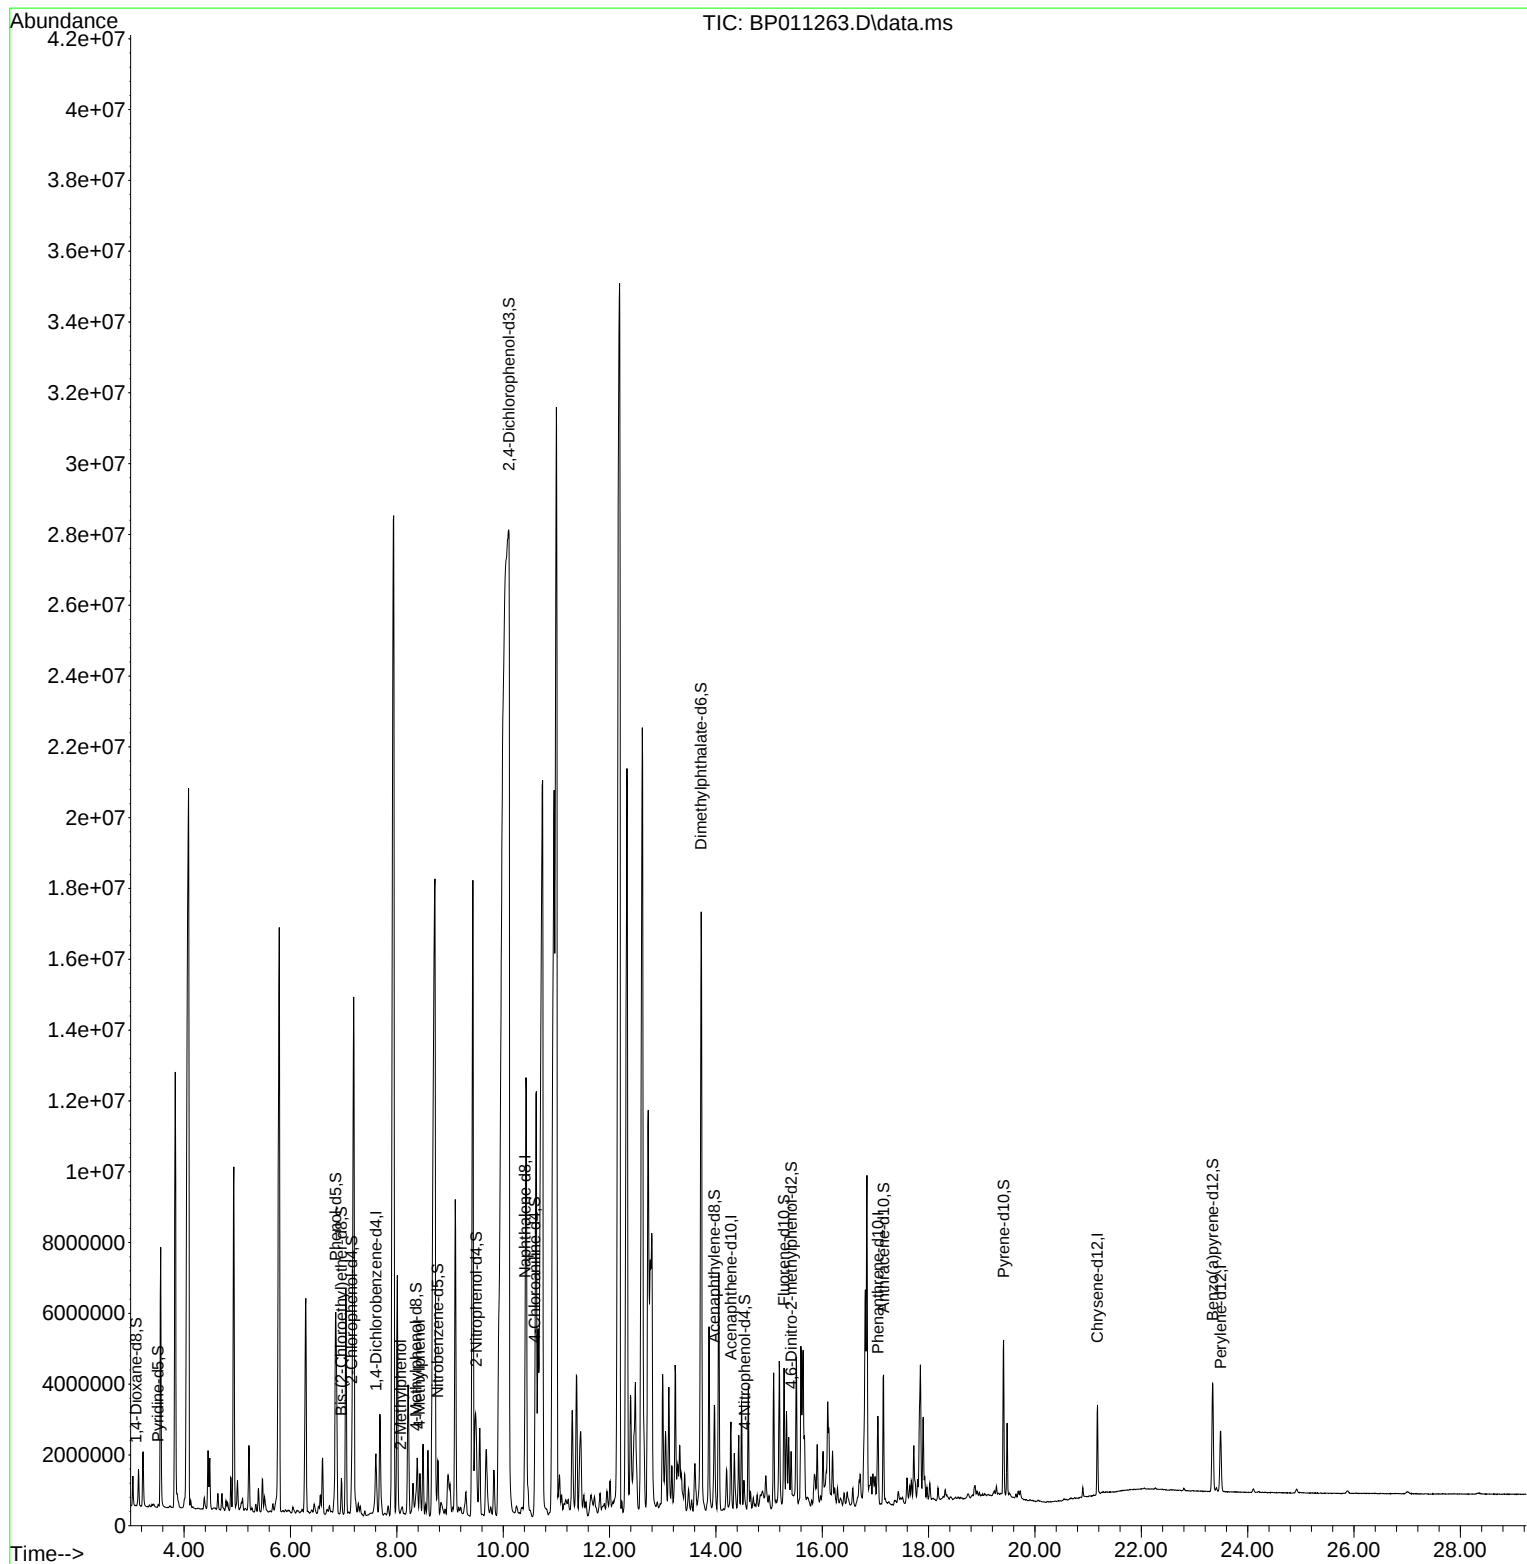

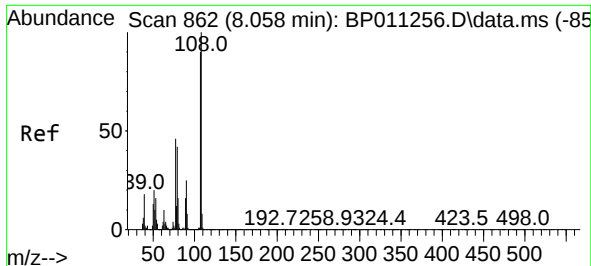

#13

2-Methylphenol

Concen: 1.600 ng/ul

RT: 8.069 min Scan# 80

Delta R.T. 0.012 min

Lab File: BP011263.D

Acq: 04 Aug 2022 14:20

Instrument :

BNA_P

ClientSampleId :





EXF05

Tgt Ion:108 Resp: 24191

Ion Ratio Lower Upper

108 100

107 85.4 71.8 107.6

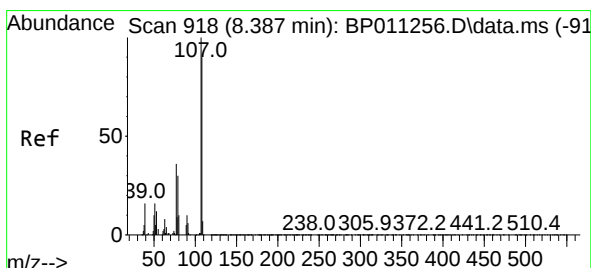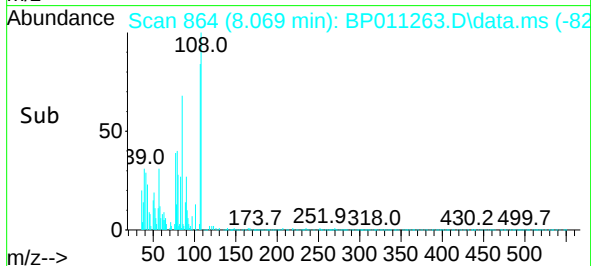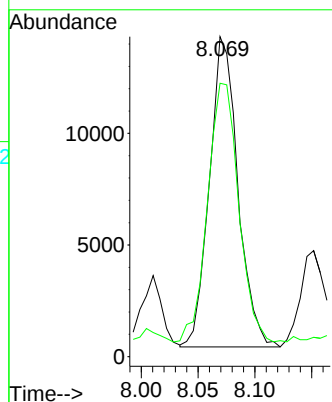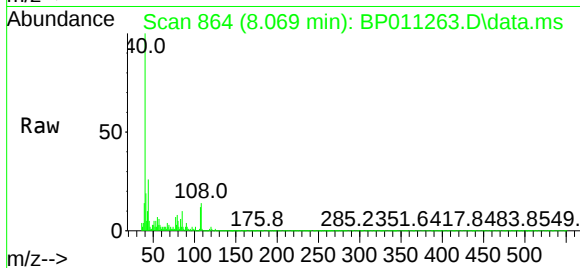

#18

4-Methylphenol

Concen: 3.809 ng/ul

RT: 8.422 min Scan# 924

Delta R.T. 0.029 min

Lab File: BP011263.D

Acq: 04 Aug 2022 14:20

Tgt Ion:108 Resp: 61780

Ion Ratio Lower Upper

108 100

107 116.4 88.2 132.4

