

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011257.D
 Acq On : 04 Aug 2022 10:50
 Operator : CG/JU
 Sample : PB146567BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK567

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	84	88	98	rBV	279789	418333	8.76%	0.795%
2	6.781	640	645	658	rVB	1024298	1550005	32.45%	2.945%
3	6.946	668	673	683	rVB	990347	1436670	30.08%	2.730%
4	7.134	699	705	716	rVB	1086765	1600469	33.51%	3.041%
5	7.599	778	784	791	rVB	994086	1493314	31.26%	2.838%
6	8.322	901	907	920	rBV	1253019	1854568	38.83%	3.524%
7	8.763	976	982	993	rVB	1210945	1834700	38.41%	3.486%
8	9.481	1098	1104	1113	rBV	668238	1072731	22.46%	2.038%
9	10.022	1189	1196	1218	rVB	1112933	1763239	36.91%	3.350%
10	10.393	1252	1259	1269	rVB	1444660	2254066	47.19%	4.283%
11	10.546	1278	1285	1302	rBV	1077458	1774422	37.15%	3.372%
12	13.698	1815	1821	1834	rBV	1995828	2463526	51.57%	4.681%
13	13.963	1859	1866	1880	rBV	2496514	3227823	67.58%	6.133%
14	14.275	1912	1919	1930	rBV	2107091	2762986	57.84%	5.250%
15	14.504	1951	1958	1980	rBV	368088	776211	16.25%	1.475%
16	15.275	2082	2089	2105	rBV	2903078	3844766	80.49%	7.306%
17	15.410	2106	2112	2127	rVV	547777	784870	16.43%	1.491%
18	15.516	2127	2130	2137	rVB4	17981	29523	0.62%	0.056%
19	16.069	2221	2224	2230	rVB5	4615	6671	0.14%	0.013%
20	16.828	2350	2353	2361	rVB9	3203	5902	0.12%	0.011%
21	17.045	2380	2390	2400	rBV	2068442	2526124	52.89%	4.800%
22	17.145	2401	2407	2430	rVV	3061329	3983812	83.40%	7.570%
23	17.286	2430	2431	2438	rVB6	3800	7410	0.16%	0.014%
24	18.033	2550	2558	2561	rBV8	2273	5239	0.11%	0.010%
25	18.980	2715	2719	2724	rBV5	20073	29770	0.62%	0.057%
26	19.051	2727	2731	2735	rVV2	14918	23162	0.48%	0.044%
27	19.404	2786	2791	2800	rBV	3469067	4189363	87.71%	7.960%
28	21.175	3087	3092	3100	rBV	2418255	2952661	61.81%	5.611%
29	23.339	3454	3460	3469	rBV2	2540863	4776616	100.00%	9.076%
30	23.492	3480	3486	3498	rVB2	1665907	3178019	66.53%	6.039%




Sum of corrected areas: 52626971

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011257.D
Acq On : 04 Aug 2022 10:50
Operator : CG/JU
Sample : PB146567BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

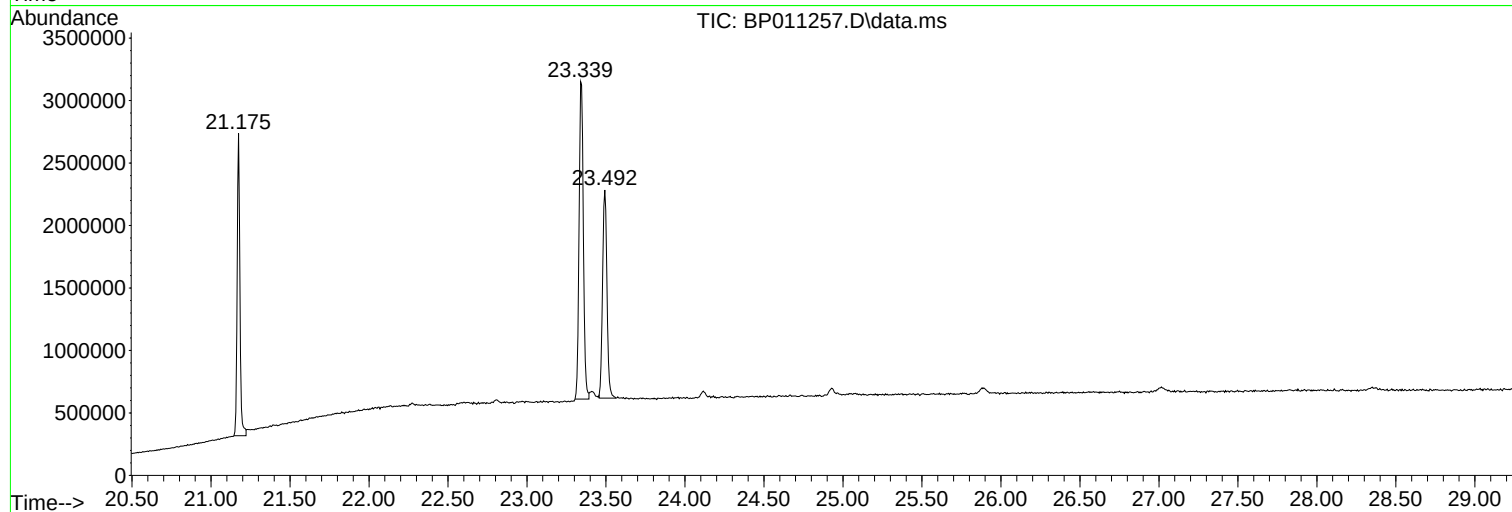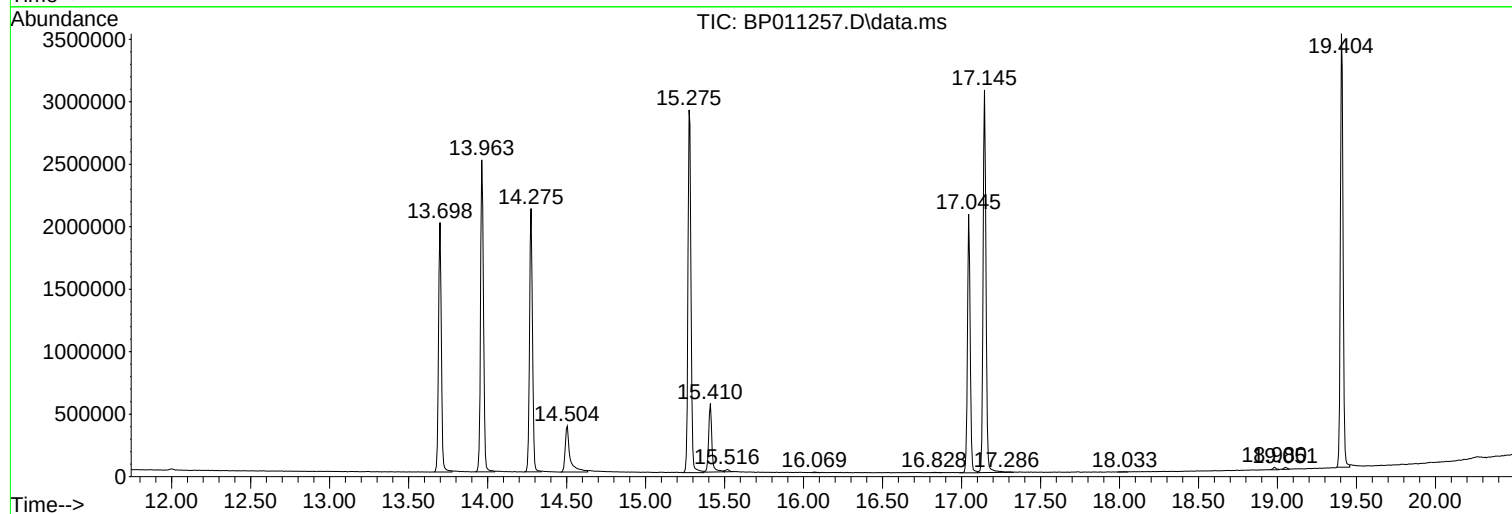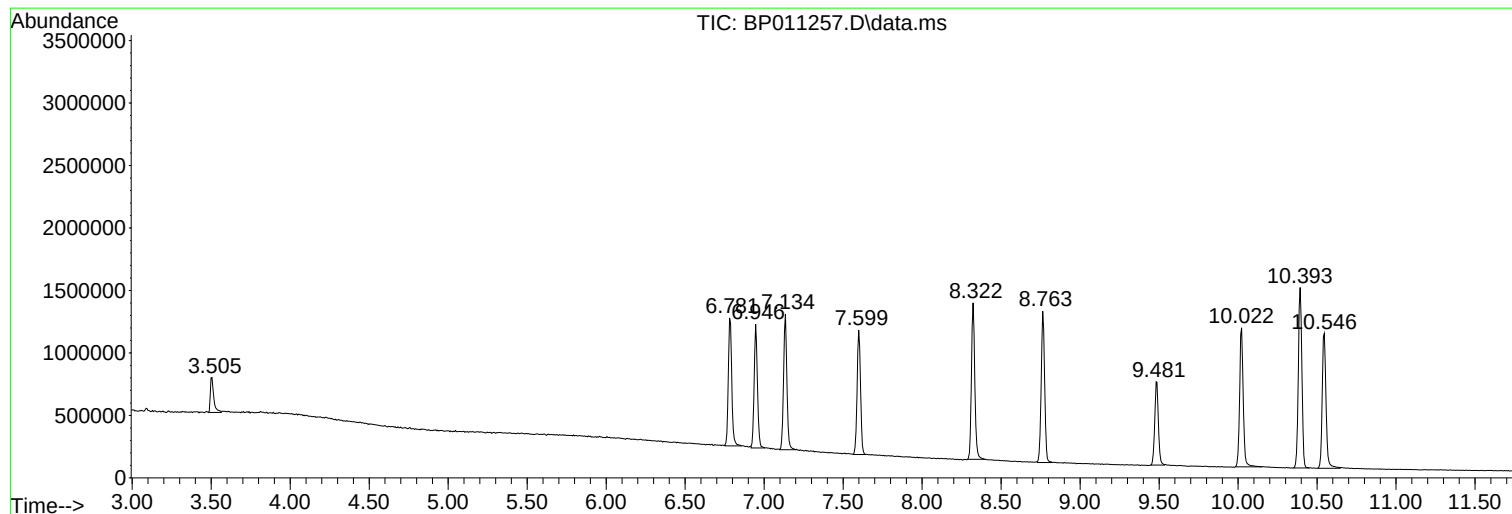

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011257.D
Acq On : 04 Aug 2022 10:50
Operator : CG/JU
Sample : PB146567BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011257.D
Acq On : 04 Aug 2022 10:50
Operator : CG/JU
Sample : PB146567BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK567

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc