

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
 Data File : BP011258.D
 Acq On : 04 Aug 2022 11:25
 Operator : CG/JU
 Sample : PB146590BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.505	85	88	96	rBV	217421	312116	5.52%	0.634%
2	6.781	640	645	658	rVB	729440	1124927	19.91%	2.286%
3	6.946	668	673	685	rVB	717223	1095038	19.38%	2.225%
4	7.134	700	705	716	rVB	751017	1129603	19.99%	2.296%
5	7.599	779	784	796	rVB	718107	1109509	19.64%	2.255%
6	8.322	901	907	919	rBV	906714	1331054	23.56%	2.705%
7	8.763	976	982	990	rVB	893527	1363656	24.13%	2.771%
8	9.481	1098	1104	1113	rBV	461273	750144	13.28%	1.524%
9	10.022	1189	1196	1213	rBV	793939	1280171	22.66%	2.602%
10	10.393	1253	1259	1267	rVB	1073663	1610729	28.51%	3.273%
11	10.546	1278	1285	1297	rBV	853606	1341589	23.74%	2.726%
12	13.698	1813	1821	1833	rBV	1756874	2181441	38.61%	4.433%
13	13.963	1860	1866	1879	rBV	2130023	2681876	47.47%	5.450%
14	14.275	1912	1919	1931	rBV	1813289	2312705	40.93%	4.700%
15	14.504	1950	1958	1978	rBV	470921	908259	16.07%	1.846%
16	15.275	2083	2089	2106	rBV	2786485	3578215	63.33%	7.272%
17	15.410	2106	2112	2127	rVV	667042	895526	15.85%	1.820%
18	15.516	2127	2130	2135	rVB3	14890	23492	0.42%	0.048%
19	17.045	2383	2390	2401	rBV	2038175	2473568	43.78%	5.027%
20	17.145	2401	2407	2432	rVB	3360581	4300260	76.11%	8.739%
21	18.980	2715	2719	2724	rBV3	17057	22531	0.40%	0.046%
22	19.051	2727	2731	2738	rVV	15677	23578	0.42%	0.048%
23	19.404	2786	2791	2808	rBV	3974170	4986618	88.26%	10.134%
24	21.175	3087	3092	3099	rBV	2794530	3255988	57.63%	6.617%
25	23.345	3454	3461	3469	rBV2	2993785	5650213	100.00%	11.482%
26	23.492	3480	3486	3497	rVB2	1892448	3464738	61.32%	7.041%




Sum of corrected areas: 49207544

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011258.D
Acq On : 04 Aug 2022 11:25
Operator : CG/JU
Sample : PB146590BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

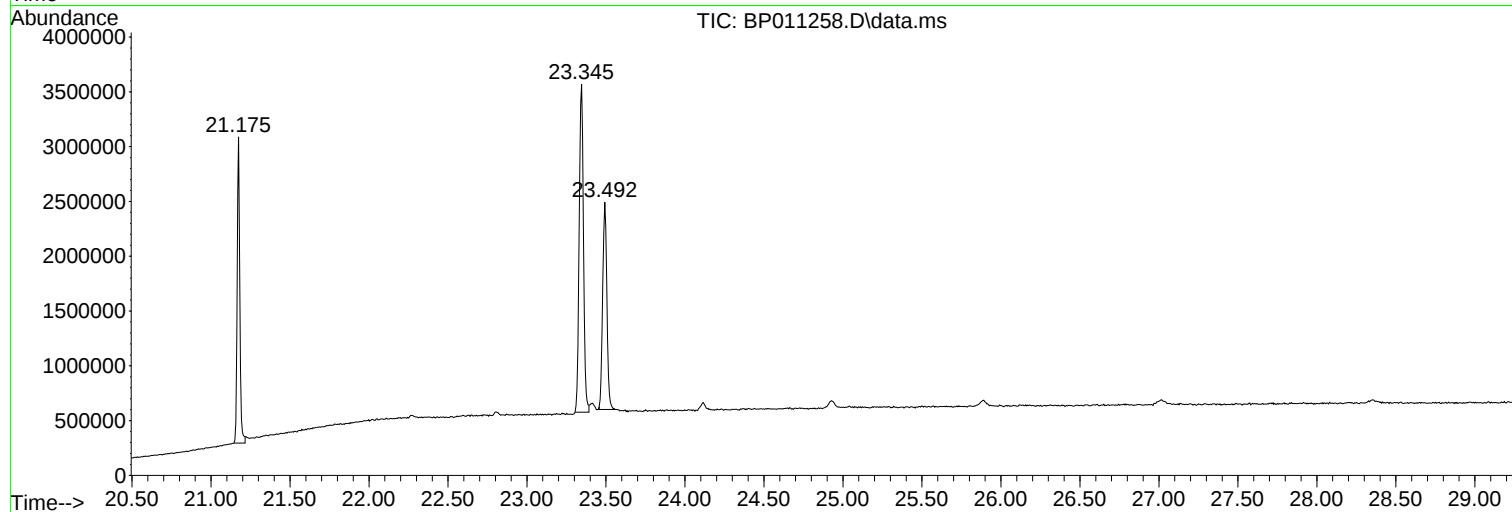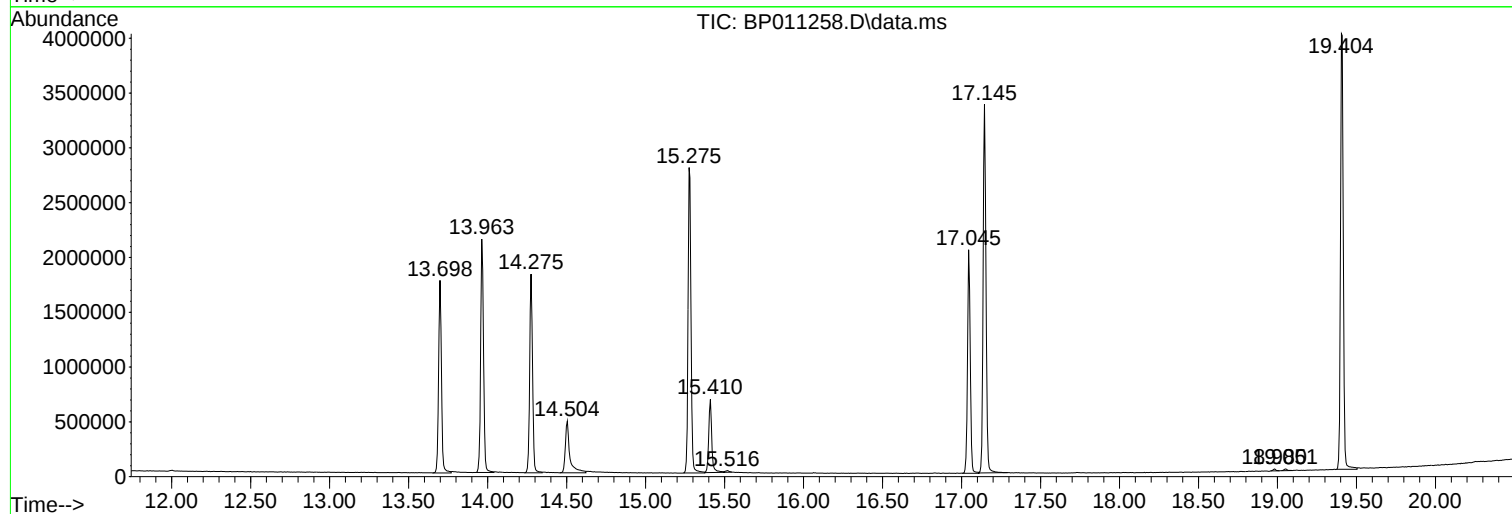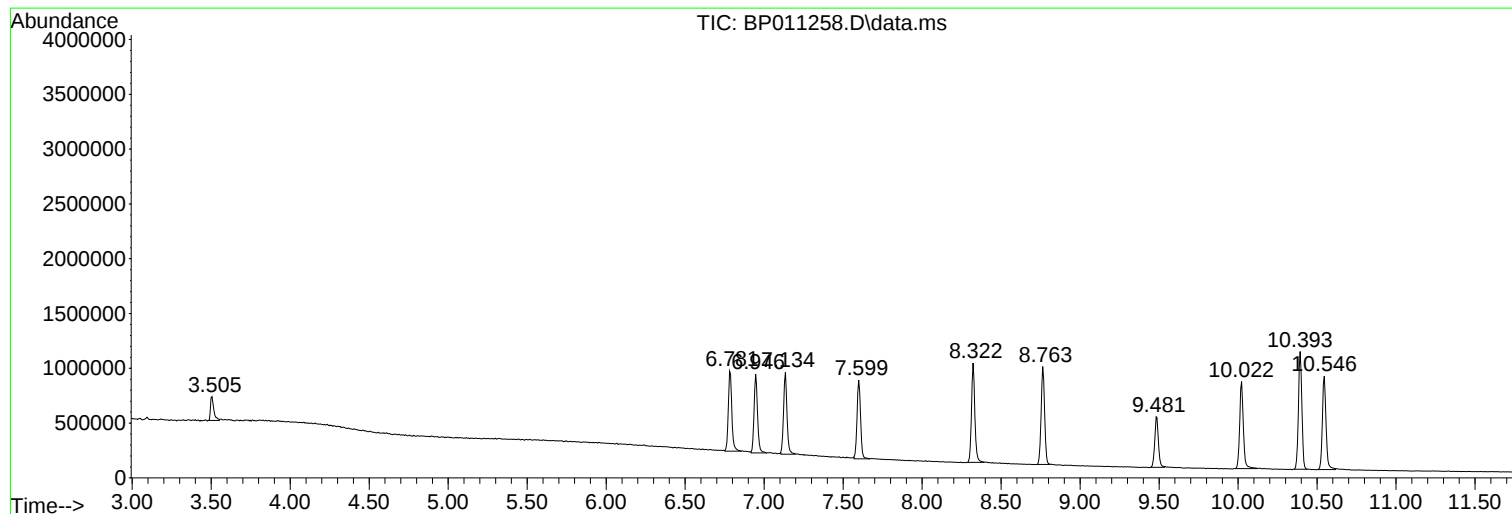

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011258.D
Acq On : 04 Aug 2022 11:25
Operator : CG/JU
Sample : PB146590BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080422\
Data File : BP011258.D
Acq On : 04 Aug 2022 11:25
Operator : CG/JU
Sample : PB146590BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc