
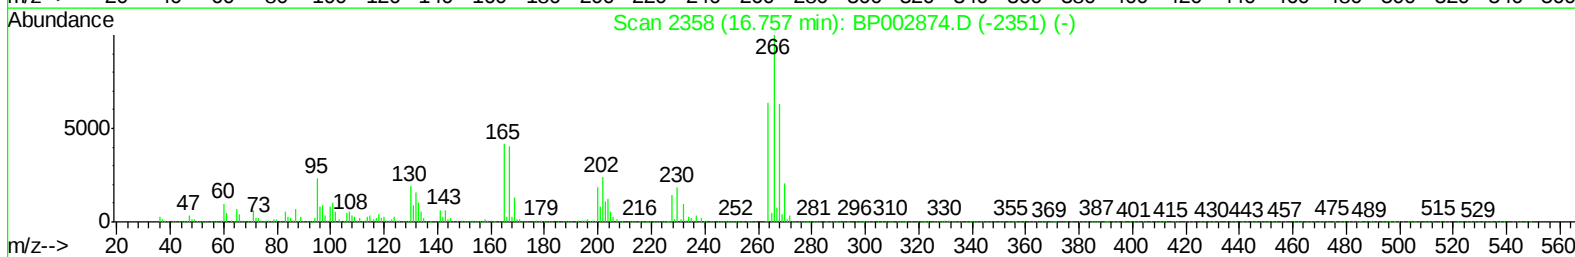
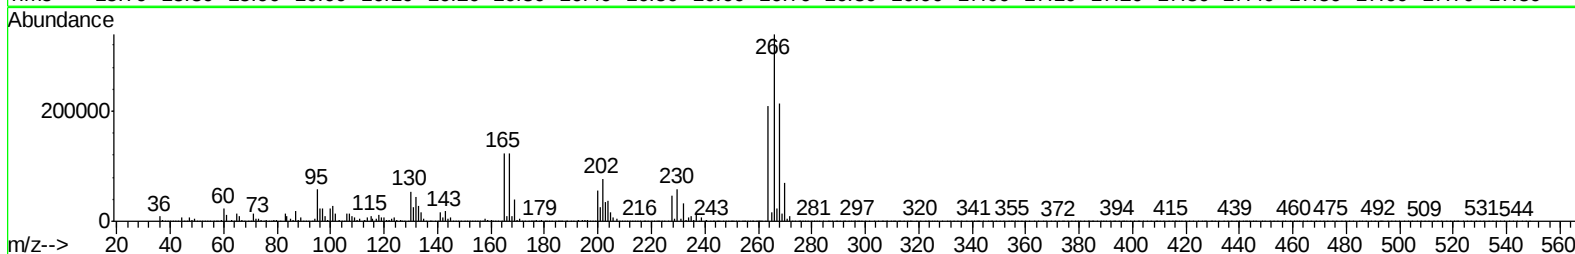


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP080520\
 Data File : BP002904.D
 Acq On : 05 Aug 2020 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 07:31:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

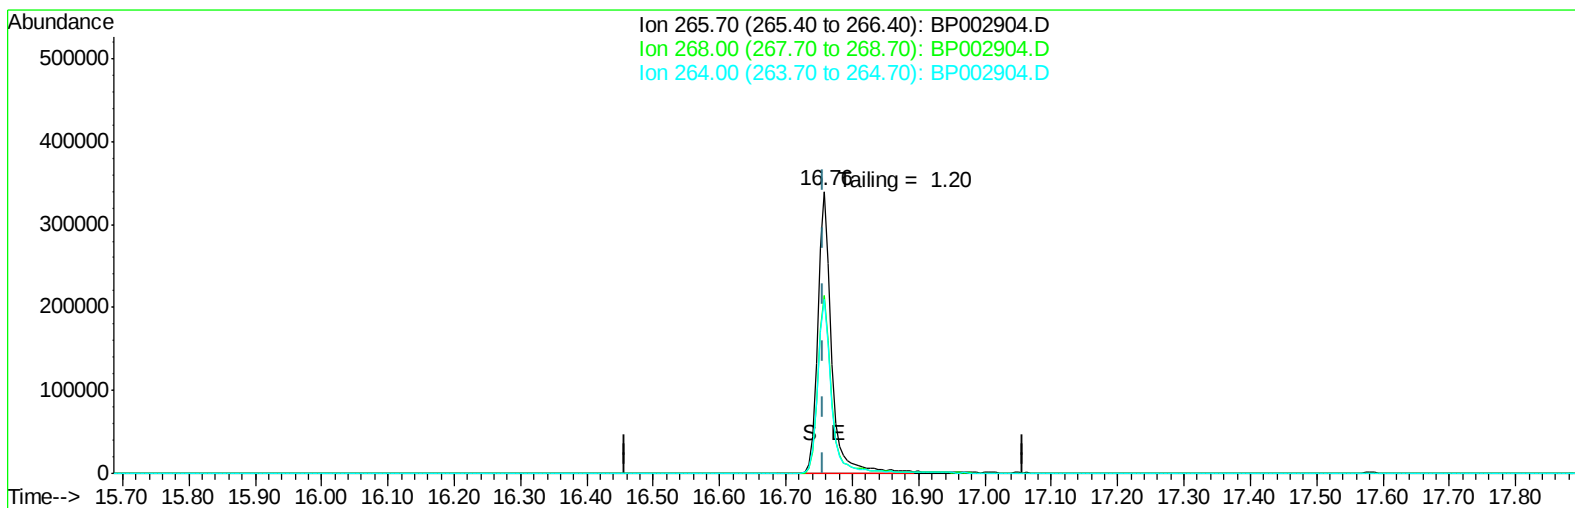

TIC: BP002904.D

(70) Pentachlorophenol (C)




16.757min (+0.000) 80344.38ng

response 496579

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	63.34
264.00	63.60	61.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP080520\
 Data File : BP002904.D
 Acq On : 05 Aug 2020 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 07:31:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

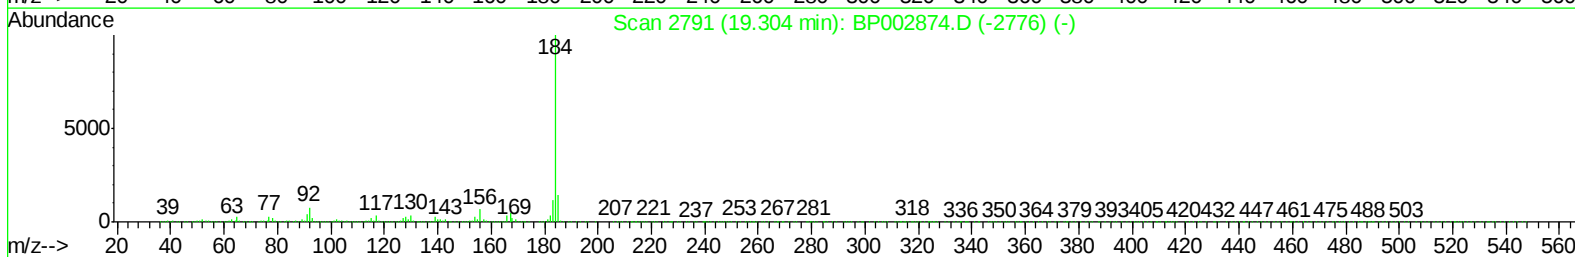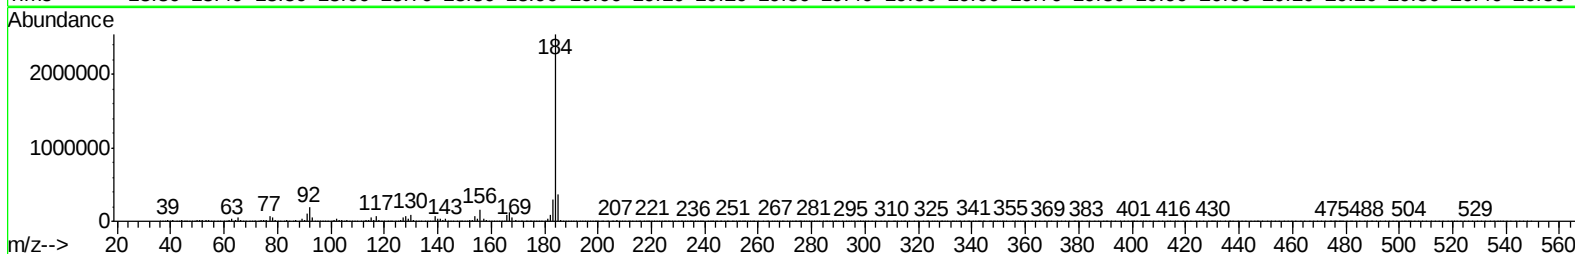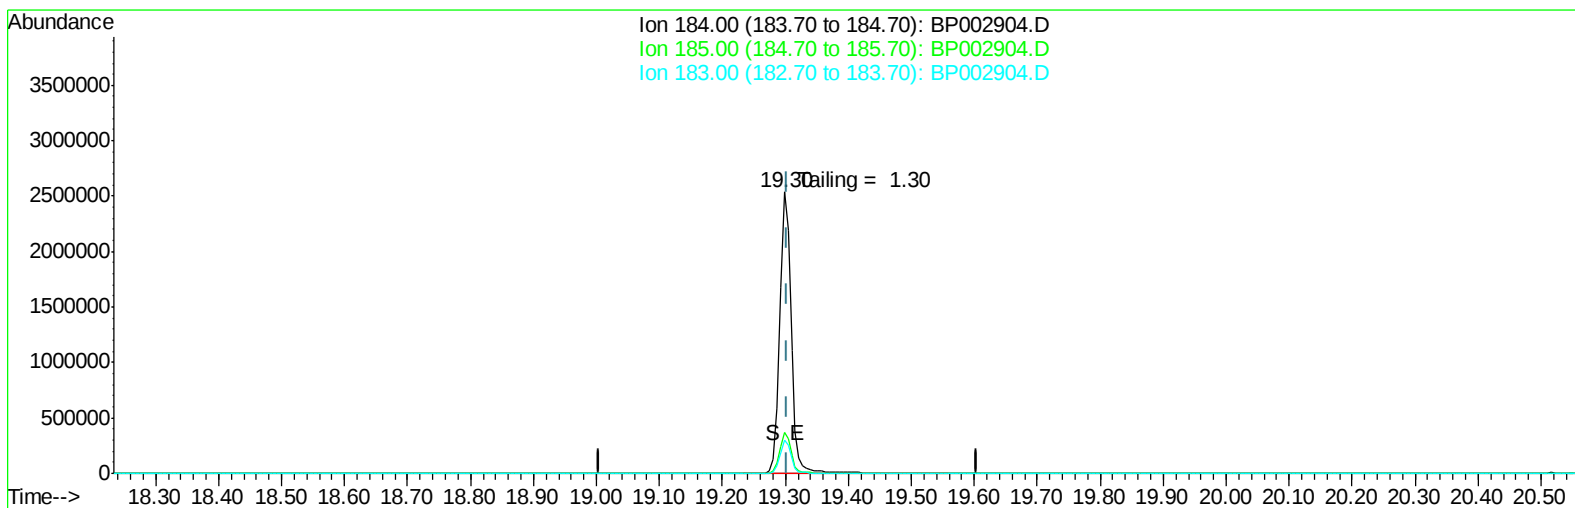

TIC: BP002904.D

(77) Benzidine

19.298min (-0.006) 72856.47ng

response 3245832

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.68
183.00	11.60	11.97
0.00	0.00	0.00