


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP080520\
 Data File : BP002904.D
 Acq On : 05 Aug 2020 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 15:30:34 2020

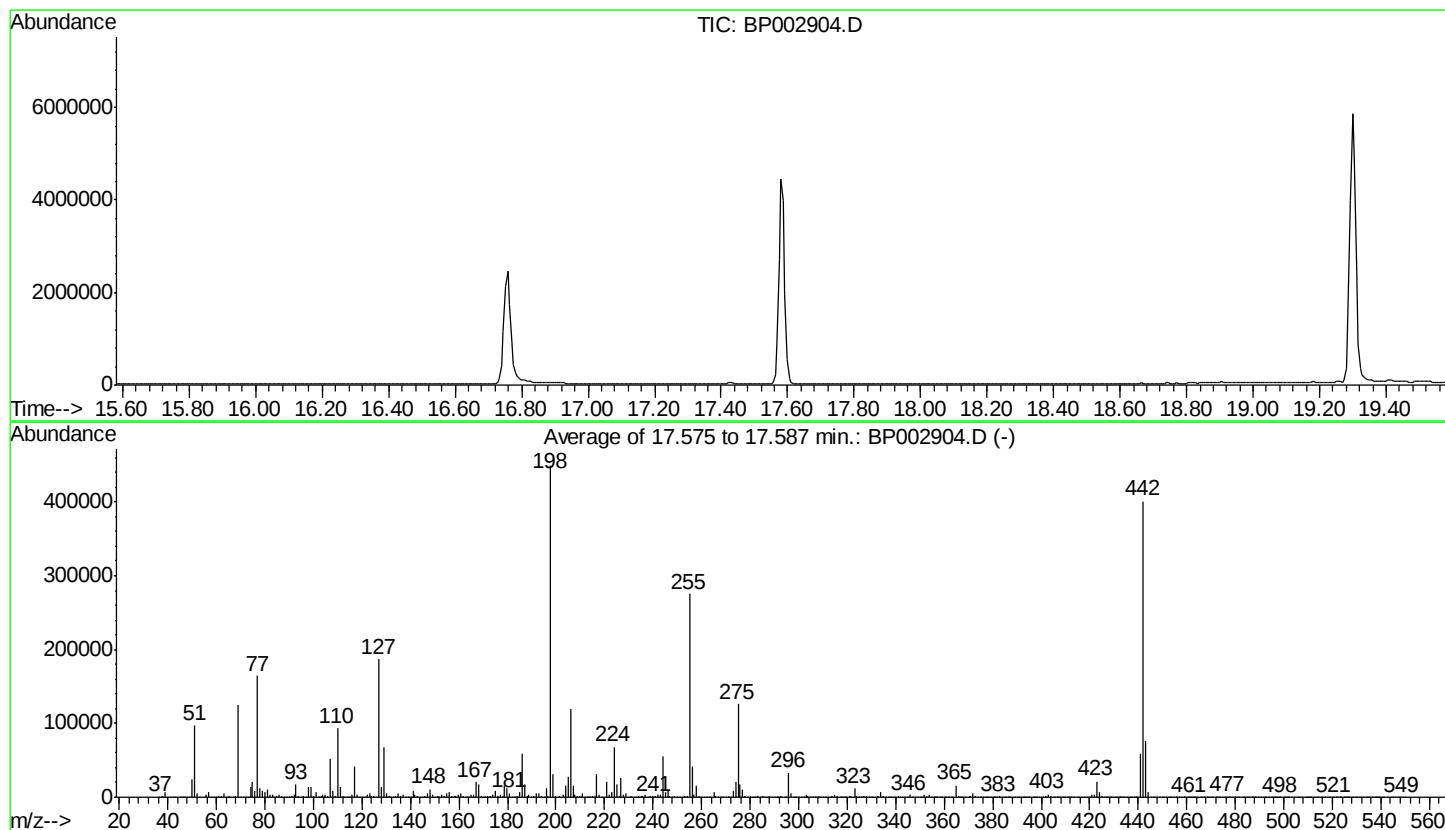

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	96574	PASS
68	69	0.00	2	1.8	2183	PASS
69	198	0.00	100	27.8	124634	PASS
70	69	0.00	2	0.4	515	PASS
127	198	10	80	41.5	186474	PASS
197	198	0.00	2	0.5	2339	PASS
198	198	100	100	100.0	449109	PASS
199	198	5	9	6.8	30759	PASS
275	198	10	60	28.0	125826	PASS
365	198	1	100	3.6	16093	PASS
441	198	0.01	100	13.2	59222	PASS
442	198	50	100	89.4	401301	PASS
443	442	15	24	19.2	76957	PASS