

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006505.D
 Acq On : 05 Aug 2021 13:59
 Operator : CG/JU
 Sample : M3276-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PRE-MAEC-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.905	304	309	319	rVB	1418239	1931834	17.94%	2.884%
2	5.358	379	386	395	rBV	4393694	6096882	56.62%	9.102%
3	5.969	484	490	498	rBV	271389	391392	3.63%	0.584%
4	6.934	644	654	667	rBV	4110792	6346547	58.94%	9.475%
5	7.757	786	794	803	rBV	927723	1456895	13.53%	2.175%
6	8.910	983	990	1000	rBV	2457214	4072156	37.82%	6.080%
7	10.328	1223	1231	1239	rBV	299899	478658	4.45%	0.715%
8	10.540	1259	1267	1273	rBV	1197841	2011039	18.68%	3.002%
9	13.010	1678	1687	1697	rBV	5444667	7885174	73.23%	11.772%
10	14.387	1911	1921	1928	rBV	1616936	2389907	22.20%	3.568%
11	15.222	2058	2063	2066	rBV	100386	145225	1.35%	0.217%
12	15.875	2168	2174	2184	rBV	4010796	5737912	53.29%	8.566%
13	17.139	2382	2389	2394	rBV	1863749	2725452	25.31%	4.069%
14	18.045	2538	2543	2551	rBV	863914	1191913	11.07%	1.779%
15	18.110	2552	2554	2560	rVB	89793	125538	1.17%	0.187%
16	18.304	2583	2587	2599	rVB2	149495	264385	2.46%	0.395%
17	18.510	2618	2622	2627	rBV	324372	402313	3.74%	0.601%
18	18.910	2687	2690	2694	rBV	201455	224524	2.09%	0.335%
19	19.157	2726	2732	2738	rBV2	145505	329313	3.06%	0.492%
20	19.216	2739	2742	2749	rVB	94003	125845	1.17%	0.188%
21	19.280	2749	2753	2769	rBV	614585	1020371	9.48%	1.523%
22	19.504	2788	2791	2795	rVB	112799	124237	1.15%	0.185%
23	19.716	2821	2827	2837	rVB	8418923	10767694	100.00%	16.076%
24	19.916	2857	2861	2866	rVB	319714	348838	3.24%	0.521%
25	20.716	2994	2997	3002	rVB2	309046	357488	3.32%	0.534%
26	20.963	3035	3039	3048	rBV	660633	934711	8.68%	1.395%
27	21.045	3049	3053	3059	rVB5	217881	370560	3.44%	0.553%
28	21.233	3080	3085	3089	rBV	2452906	3193885	29.66%	4.768%
29	21.639	3151	3154	3160	rVB	507328	664816	6.17%	0.993%
30	21.710	3163	3166	3172	rVB2	478004	614288	5.70%	0.917%
31	22.304	3263	3267	3271	rBV3	304506	461745	4.29%	0.689%
32	22.768	3343	3346	3353	rVB3	442413	676253	6.28%	1.010%
33	23.563	3475	3481	3489	rVB2	1564424	3113290	28.91%	4.648%




Sum of corrected areas: 66981080

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006505.D
Acq On : 05 Aug 2021 13:59
Operator : CG/JU
Sample : M3276-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

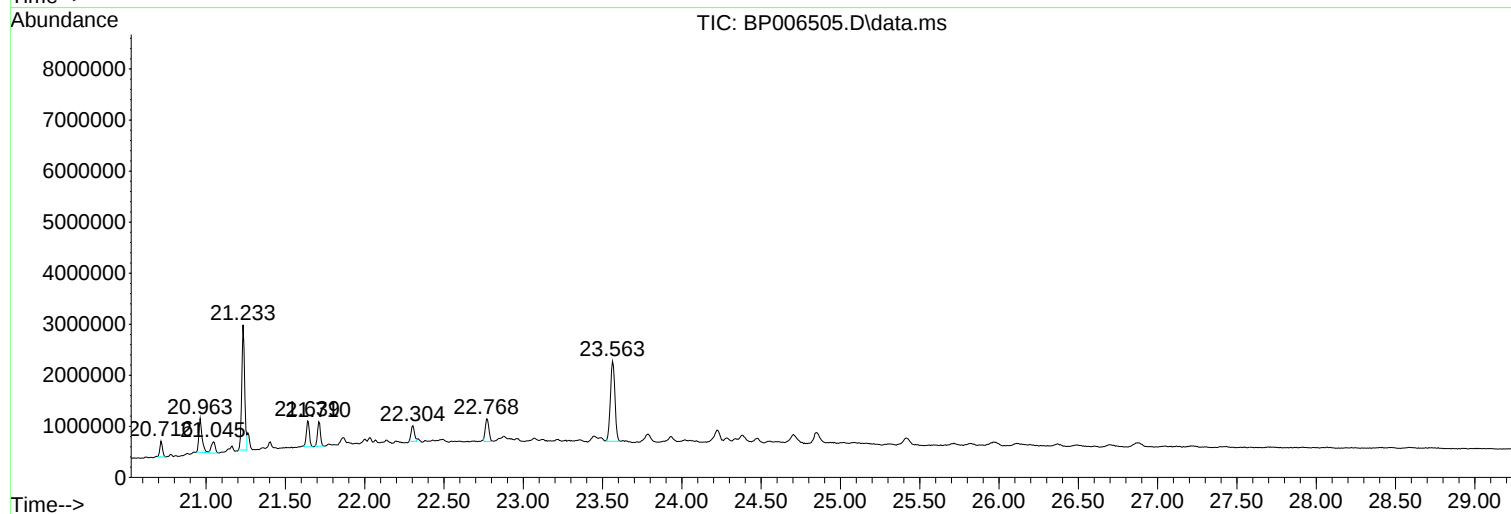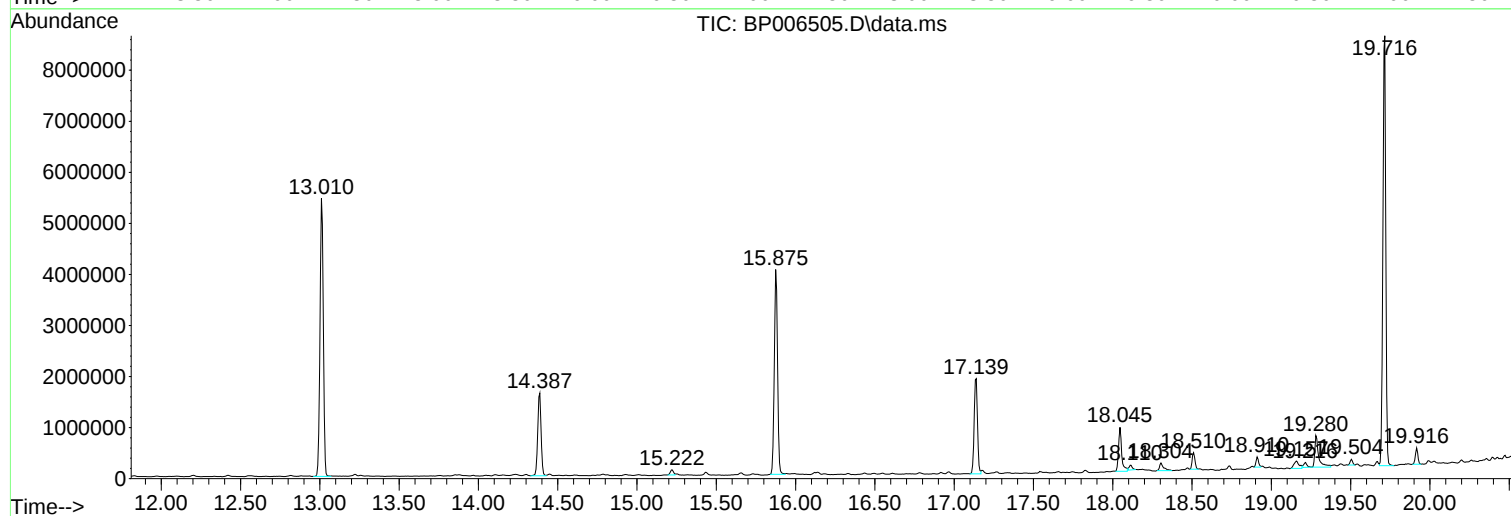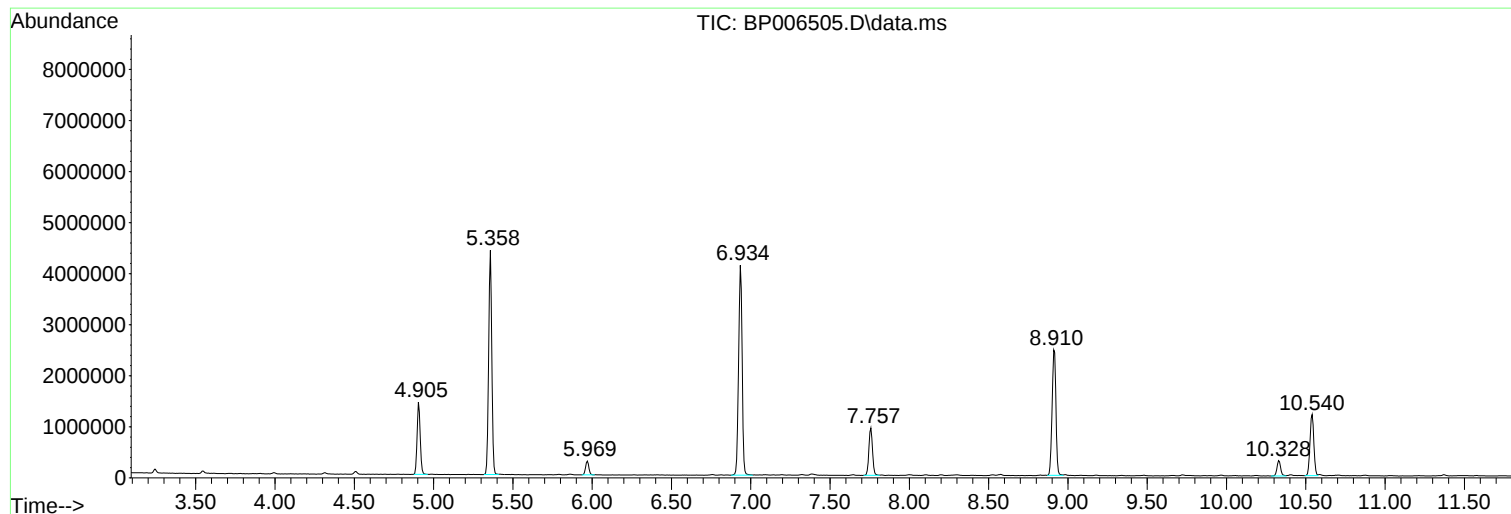

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006505.D
Acq On : 05 Aug 2021 13:59
Operator : CG/JU
Sample : M3276-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006505.D
Acq On : 05 Aug 2021 13:59
Operator : CG/JU
Sample : M3276-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------