

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006506.D
 Acq On : 05 Aug 2021 14:33
 Operator : CG/JU
 Sample : M3276-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PRE-MAEC-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	32	rVB	93620	131741	1.24%	0.095%
2	4.905	304	309	318	rBV	1387241	1954995	18.41%	1.407%
3	5.358	379	386	393	rBV	4474691	6225843	58.62%	4.480%
4	5.970	484	490	495	rBV	283817	393388	3.70%	0.283%
5	6.934	644	654	661	rBV	4133766	6565697	61.82%	4.725%
6	7.387	726	731	732	rBV	87516	110523	1.04%	0.080%
7	7.758	784	794	802	rBV	1100914	1730690	16.30%	1.245%
8	8.911	984	990	998	rVV	2567156	4136746	38.95%	2.977%
9	10.328	1225	1231	1240	rBV	313049	506052	4.76%	0.364%
10	10.540	1259	1267	1273	rBV	1446450	2443536	23.01%	1.758%
11	10.693	1288	1293	1300	rVB3	52079	109484	1.03%	0.079%
12	11.369	1398	1408	1417	rBV	156424	288728	2.72%	0.208%
13	11.969	1504	1510	1520	rVB5	54097	108396	1.02%	0.078%
14	13.010	1678	1687	1697	rBV	5567827	8351640	78.64%	6.010%
15	13.222	1715	1723	1728	rVB4	75477	137922	1.30%	0.099%
16	13.881	1829	1835	1839	rVB4	84197	139552	1.31%	0.100%
17	14.299	1902	1906	1910	rVB	94765	116793	1.10%	0.084%
18	14.387	1911	1921	1927	rVV	1989909	2989126	28.14%	2.151%
19	14.446	1927	1931	1940	rVB	206235	308887	2.91%	0.222%
20	14.787	1984	1989	1993	rBV	107553	187013	1.76%	0.135%
21	15.175	2051	2055	2059	rBV	71238	112838	1.06%	0.081%
22	15.251	2066	2068	2072	rVB	92835	108620	1.02%	0.078%
23	15.434	2095	2099	2105	rVB	244835	320226	3.02%	0.230%
24	15.657	2133	2137	2144	rVB2	133866	233829	2.20%	0.168%
25	15.734	2145	2150	2159	rVV7	126745	263833	2.48%	0.190%
26	15.875	2168	2174	2183	rVB	4210324	6074801	57.20%	4.371%
27	16.122	2211	2216	2218	rBV	249463	408783	3.85%	0.294%
28	16.493	2276	2279	2283	rVB2	105313	140637	1.32%	0.101%
29	16.916	2348	2351	2354	rVV2	106071	117958	1.11%	0.085%
30	16.963	2355	2359	2367	rVB2	237175	432338	4.07%	0.311%
31	17.140	2383	2389	2392	rBV	2124915	3166124	29.81%	2.278%
32	17.181	2392	2396	2403	rVV	1743436	2437098	22.95%	1.754%
33	17.269	2407	2411	2417	rVB	470068	661115	6.22%	0.476%
34	17.545	2456	2458	2462	rVB	128453	129213	1.22%	0.093%
35	18.051	2539	2544	2553	rBV2	2879398	3996402	37.63%	2.876%
36	18.310	2584	2588	2599	rVB	1234989	1893283	17.83%	1.362%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006506.D
 Acq On : 05 Aug 2021 14:33
 Operator : CG/JU
 Sample : M3276-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PRE-MAEC-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.516	2618	2623	2628	rVB	2345773	2968067	27.95%	2.136%
38	18.734	2657	2660	2664	rVB	470554	595697	5.61%	0.429%
39	18.881	2683	2685	2687	rBV	248361	223309	2.10%	0.161%
40	18.916	2687	2691	2695	rVB	1547758	1824373	17.18%	1.313%
41	19.157	2727	2732	2736	rBV	2656116	3943252	37.13%	2.837%
42	19.292	2751	2755	2763	rBV2	2534454	3674658	34.60%	2.644%
43	19.481	2784	2787	2788	rBV	444245	468543	4.41%	0.337%
44	19.510	2788	2792	2796	rVB	1891431	2458823	23.15%	1.769%
45	19.669	2816	2819	2822	rBV2	585162	787010	7.41%	0.566%
46	19.716	2822	2827	2836	rVB	8278291	10620746	100.00%	7.642%
47	19.922	2858	2862	2866	rBV	1807956	2194470	20.66%	1.579%
48	19.998	2872	2875	2878	rVB2	436807	480747	4.53%	0.346%
49	20.722	2994	2998	3003	rVB2	1749449	2141551	20.16%	1.541%
50	20.969	3036	3040	3048	rVB	2480513	3957455	37.26%	2.848%
51	21.051	3050	3054	3059	rVB3	1340054	2126824	20.03%	1.530%
52	21.239	3080	3086	3089	rBV2	3022623	5327138	50.16%	3.833%
53	21.269	3089	3091	3098	rVB2	2747529	3157286	29.73%	2.272%
54	21.645	3151	3155	3161	rVB	3246802	4182977	39.38%	3.010%
55	21.716	3163	3167	3174	rVB	3145141	4023479	37.88%	2.895%
56	22.310	3263	3268	3272	rBV2	2164202	3178087	29.92%	2.287%
57	22.780	3343	3348	3355	rVB	2674773	4265611	40.16%	3.069%
58	23.574	3478	3483	3489	rVB2	1698151	3095753	29.15%	2.228%
59	23.798	3517	3521	3532	rVB	1575141	3034802	28.57%	2.184%
60	24.239	3591	3596	3608	rVB	2114978	4520786	42.57%	3.253%
61	24.398	3619	3623	3633	rVB	1336939	2914523	27.44%	2.097%
62	24.874	3698	3704	3713	rVB	2315433	5370058	50.56%	3.864%




Sum of corrected areas: 138969875

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006506.D
Acq On : 05 Aug 2021 14:33
Operator : CG/JU
Sample : M3276-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

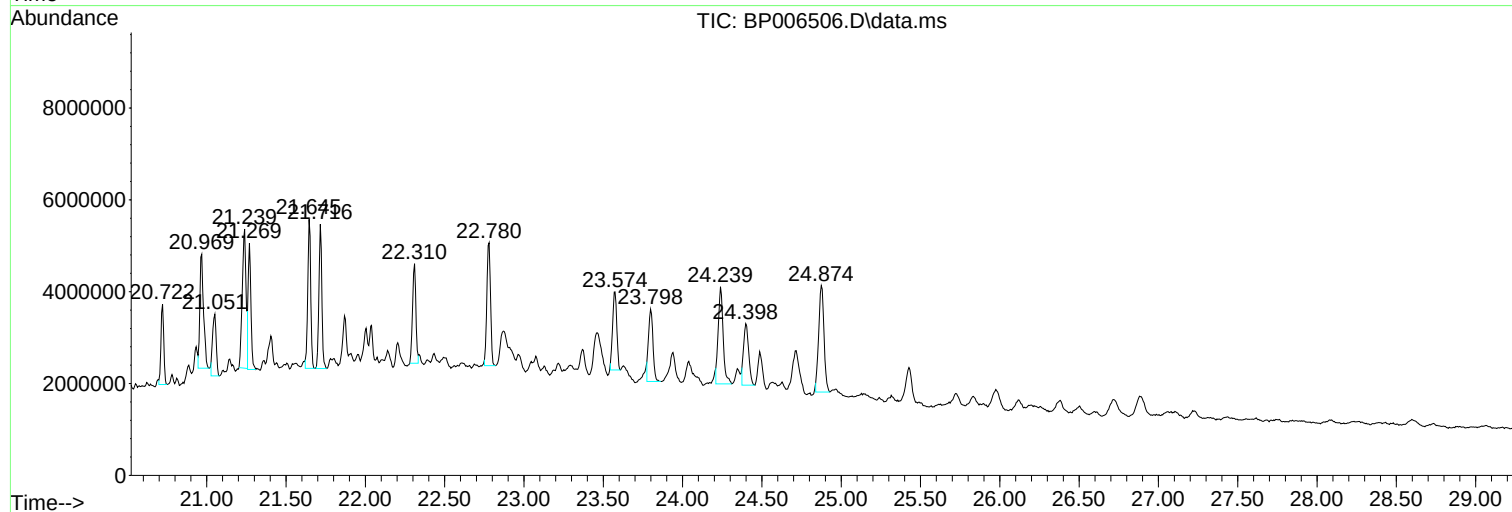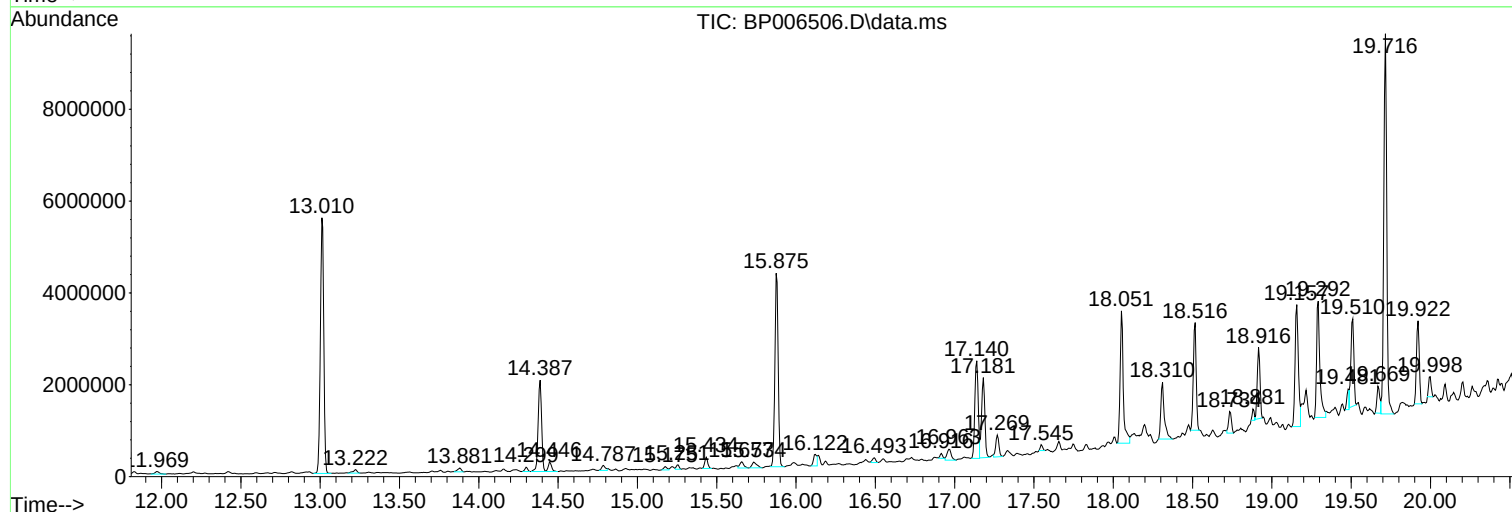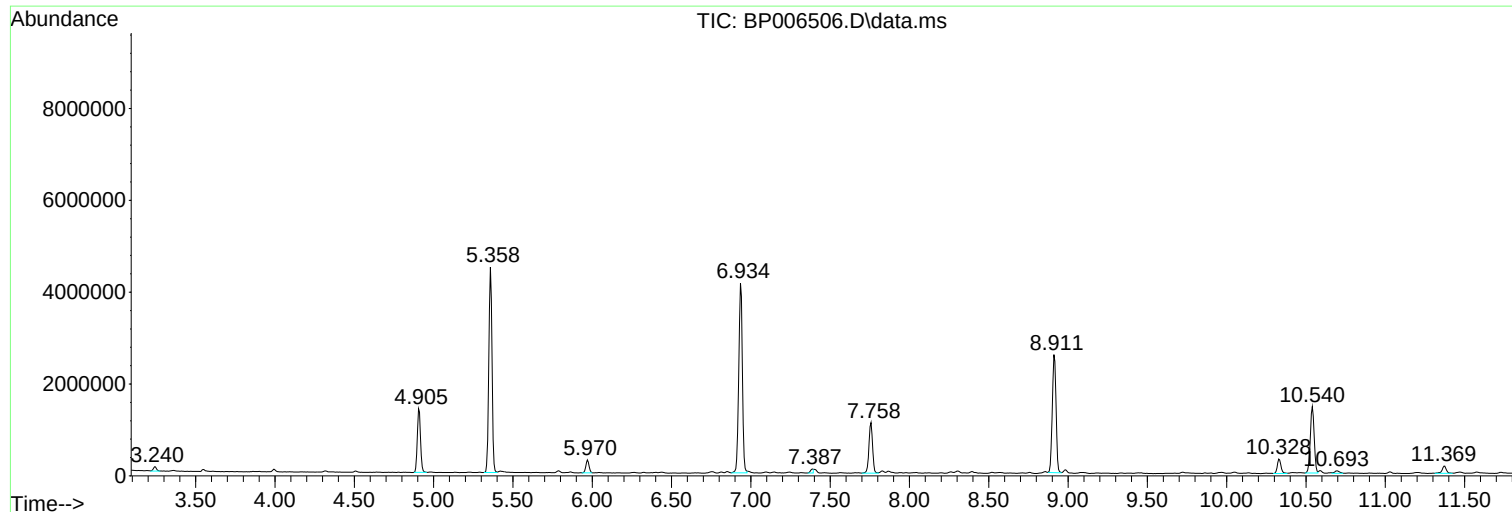

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006506.D
Acq On : 05 Aug 2021 14:33
Operator : CG/JU
Sample : M3276-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006506.D
Acq On : 05 Aug 2021 14:33
Operator : CG/JU
Sample : M3276-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PRE-MAEC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------