
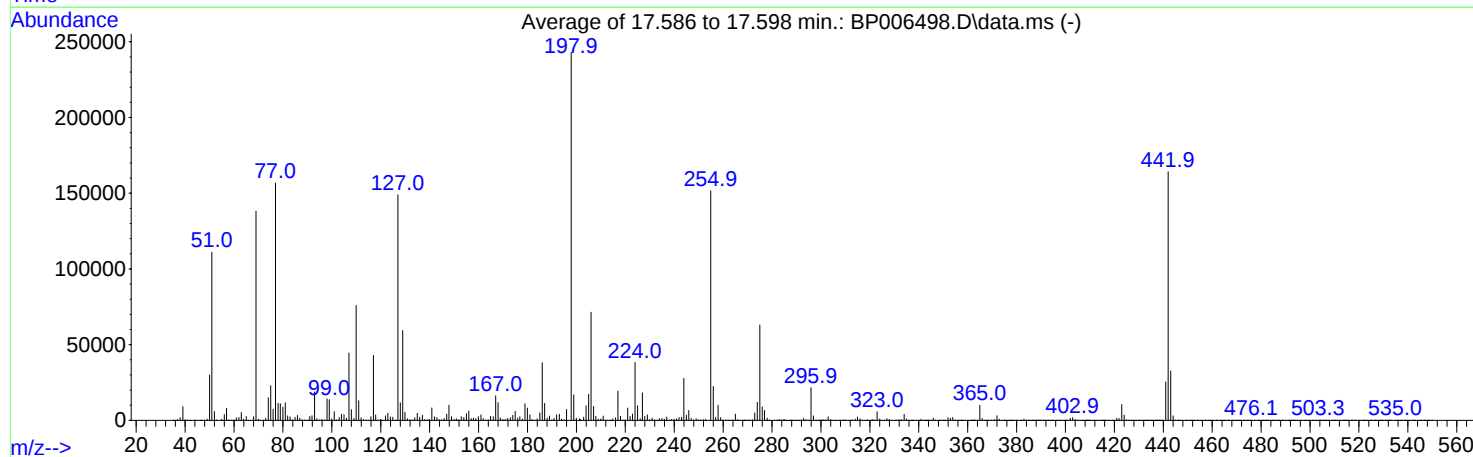


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006498.D
 Acq On : 05 Aug 2021 09:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:41:30 2021

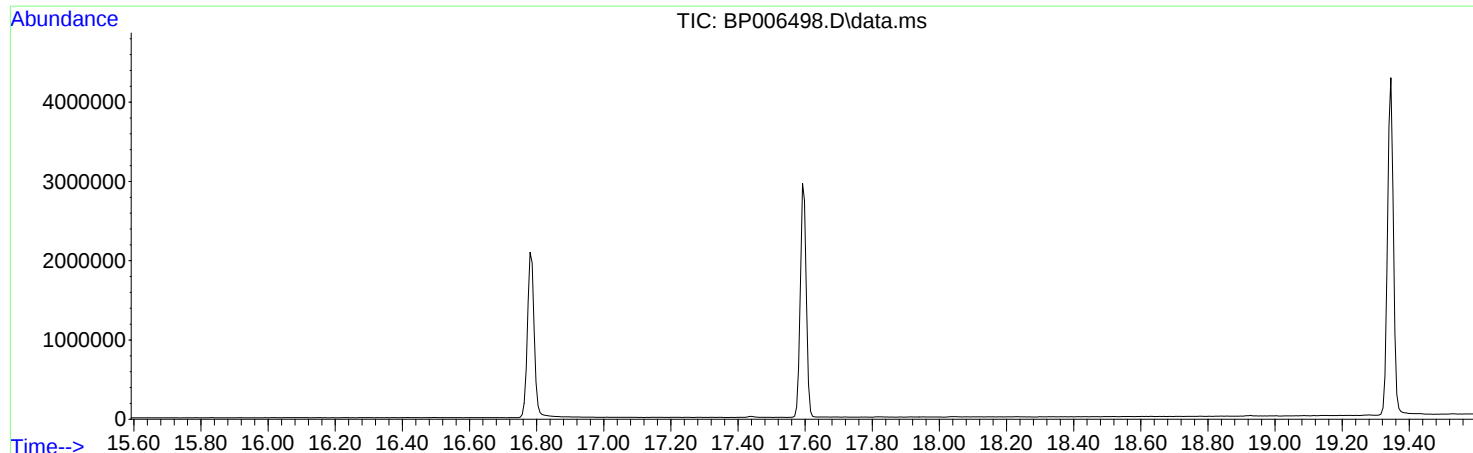




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	111012	PASS
68	69	0.00	2	1.7	2415	PASS
69	198	0.00	100	56.9	138161	PASS
70	69	0.00	2	0.5	727	PASS
127	198	10	80	61.3	148986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	242915	PASS
199	198	5	9	6.9	16760	PASS
275	198	10	60	25.9	63024	PASS
365	198	1	100	4.1	9966	PASS
441	198	0.01	100	10.4	25374	PASS
442	442	100	100	100.0	164158	PASS
443	442	15	24	19.9	32672	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006498.D
 Acq On : 05 Aug 2021 09:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 05 11:43:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

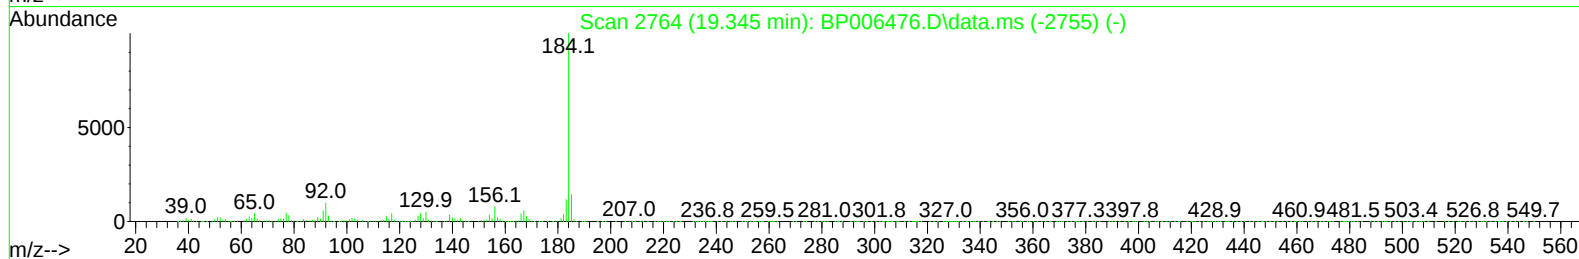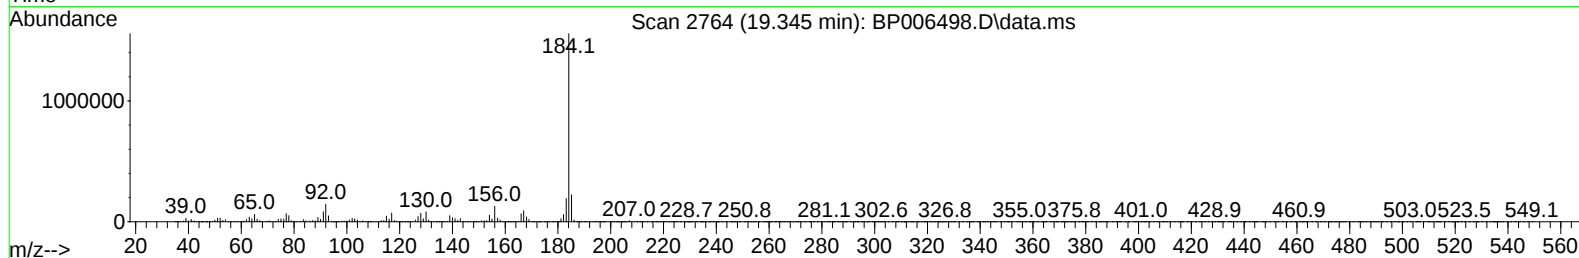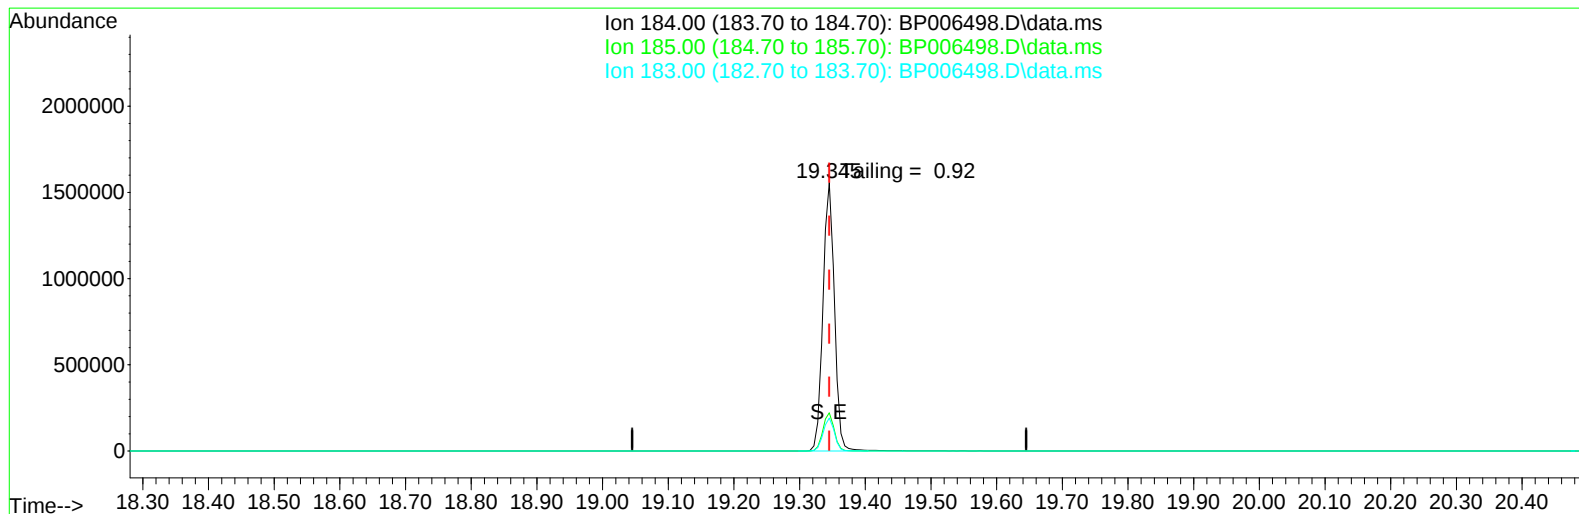

TIC: BP006498.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 85048.08 ng




response 1889829

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.28
183.00	11.90	12.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006498.D
Acq On : 05 Aug 2021 09:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 05 11:43:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

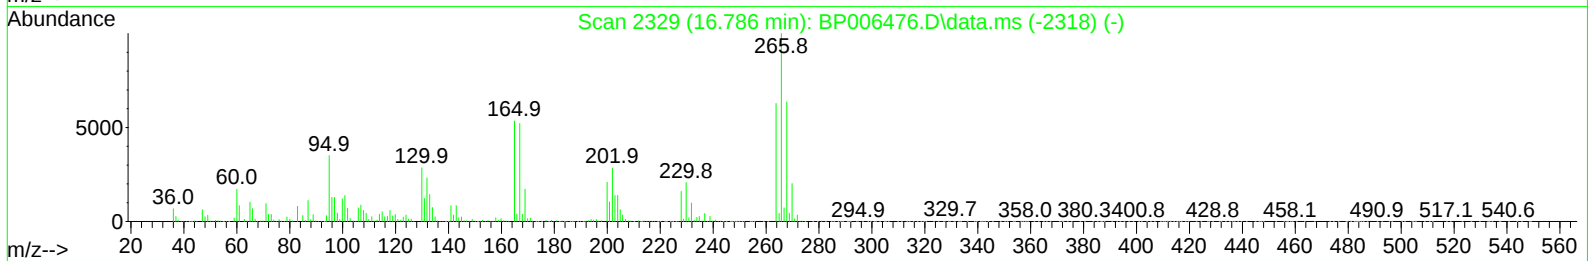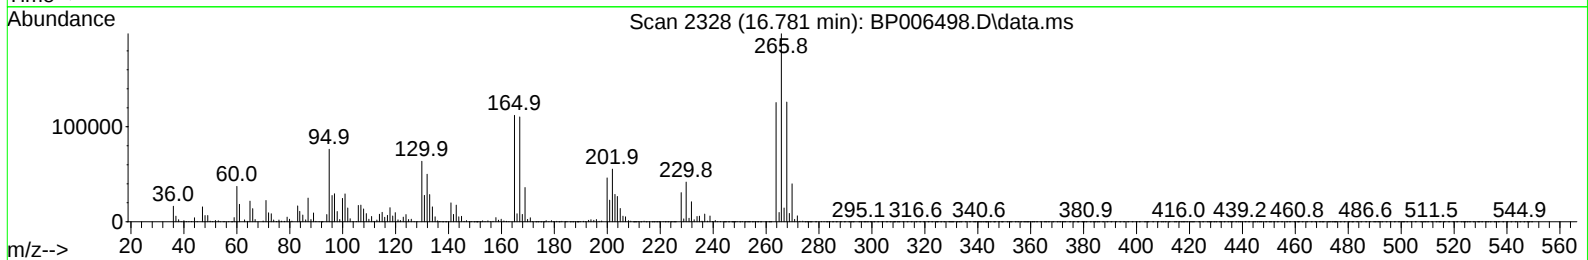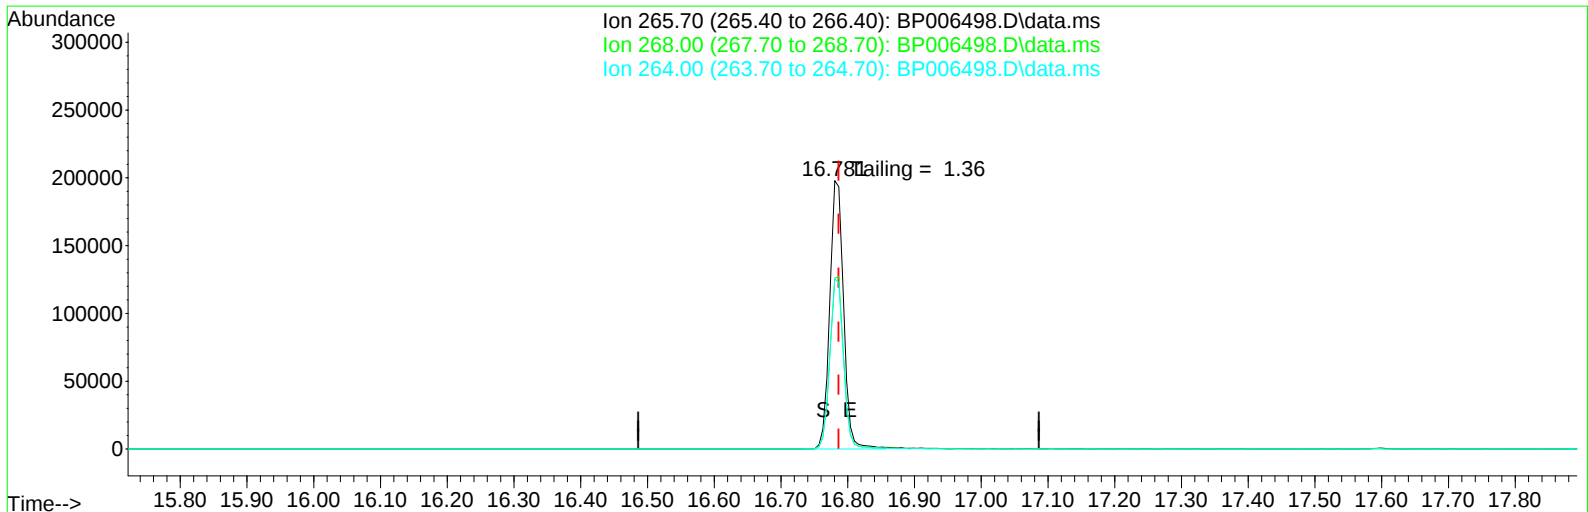

TIC: BP006498.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.006) 411086.67 ng

response 287639

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.65
264.00	62.90	63.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2021	BNA_P	BP006498.D
Compound Name	Response	Retention Time
DDT	894586	20.55
DDD	6119	20.11
DDE	1842	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7961	902547	0.88