
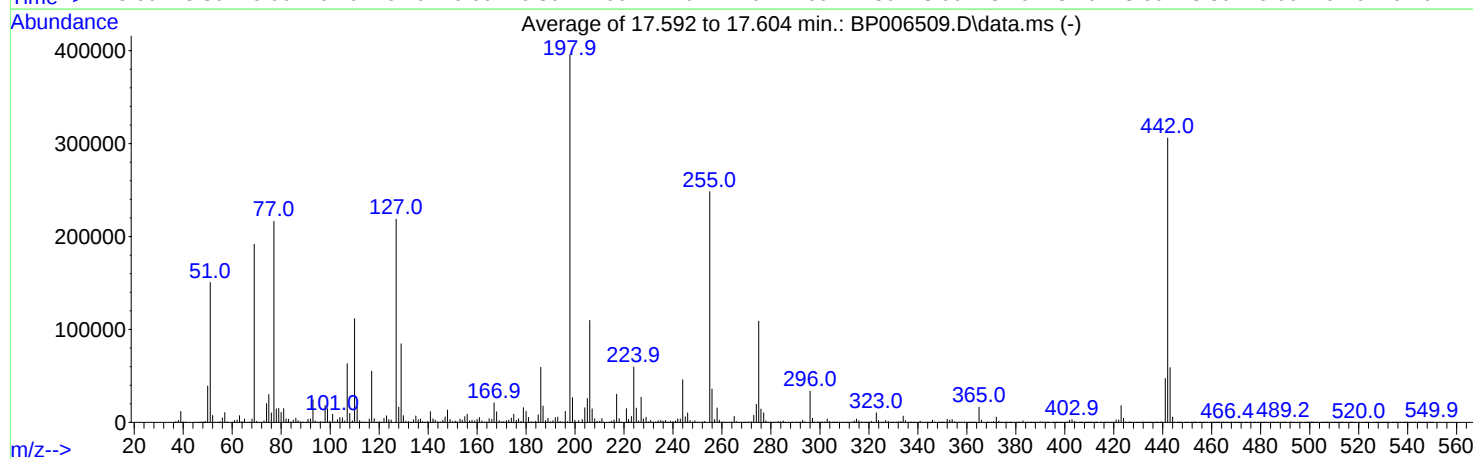


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006509.D
 Acq On : 05 Aug 2021 16:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:41:30 2021

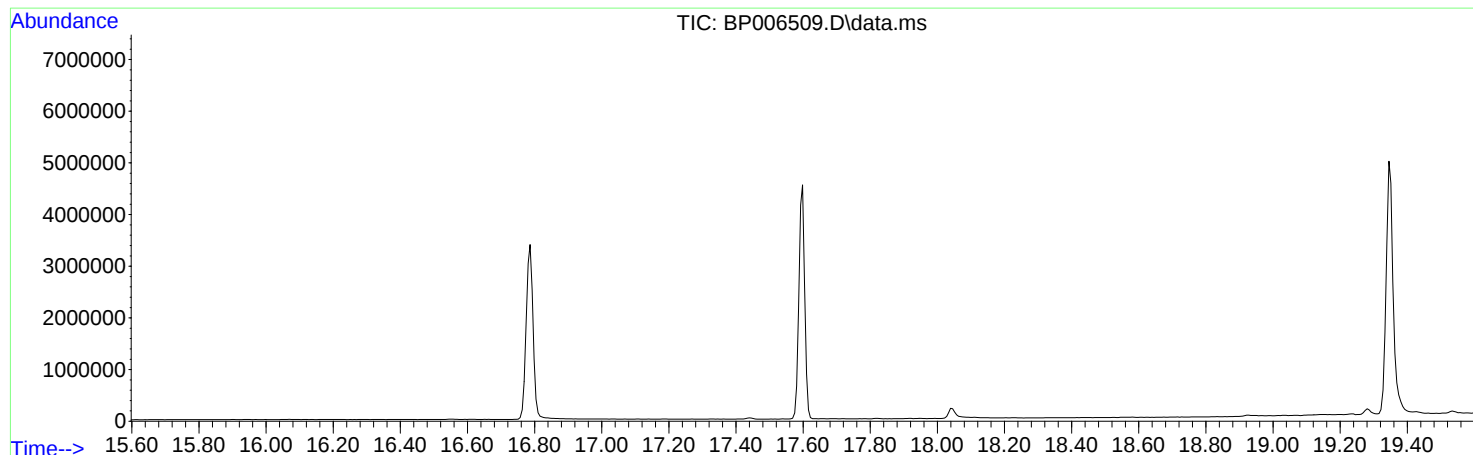




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	150489	PASS
68	69	0.00	2	1.9	3649	PASS
69	198	0.00	100	48.4	191643	PASS
70	69	0.00	2	0.6	1066	PASS
127	198	10	80	55.2	218705	PASS
197	198	0.00	2	0.2	638	PASS
198	198	100	100	100.0	395870	PASS
199	198	5	9	6.8	26740	PASS
275	198	10	60	27.5	108852	PASS
365	198	1	100	4.1	16363	PASS
441	198	0.01	100	11.9	47192	PASS
442	442	100	100	100.0	305984	PASS
443	442	15	24	19.3	58923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
Data File : BP006509.D
Acq On : 05 Aug 2021 16:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 05 18:00:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

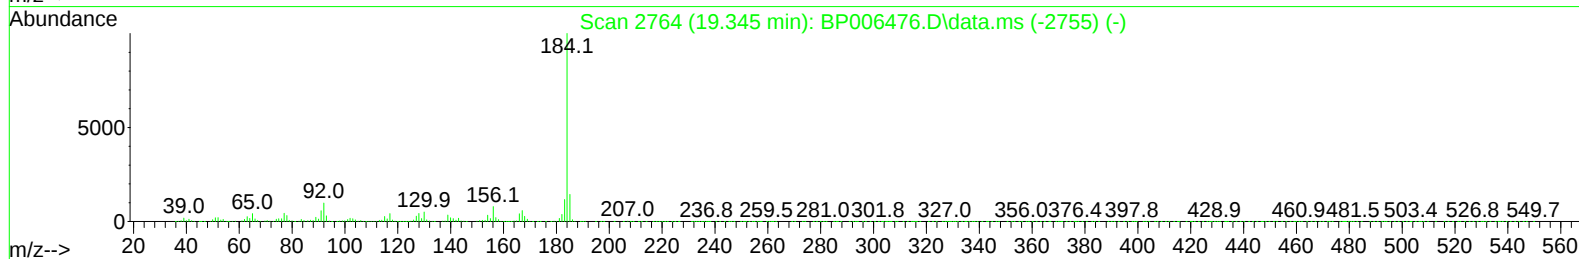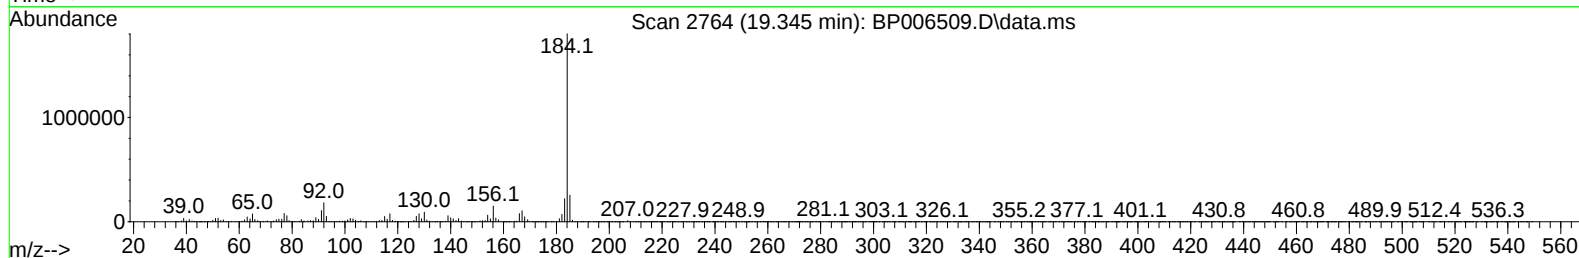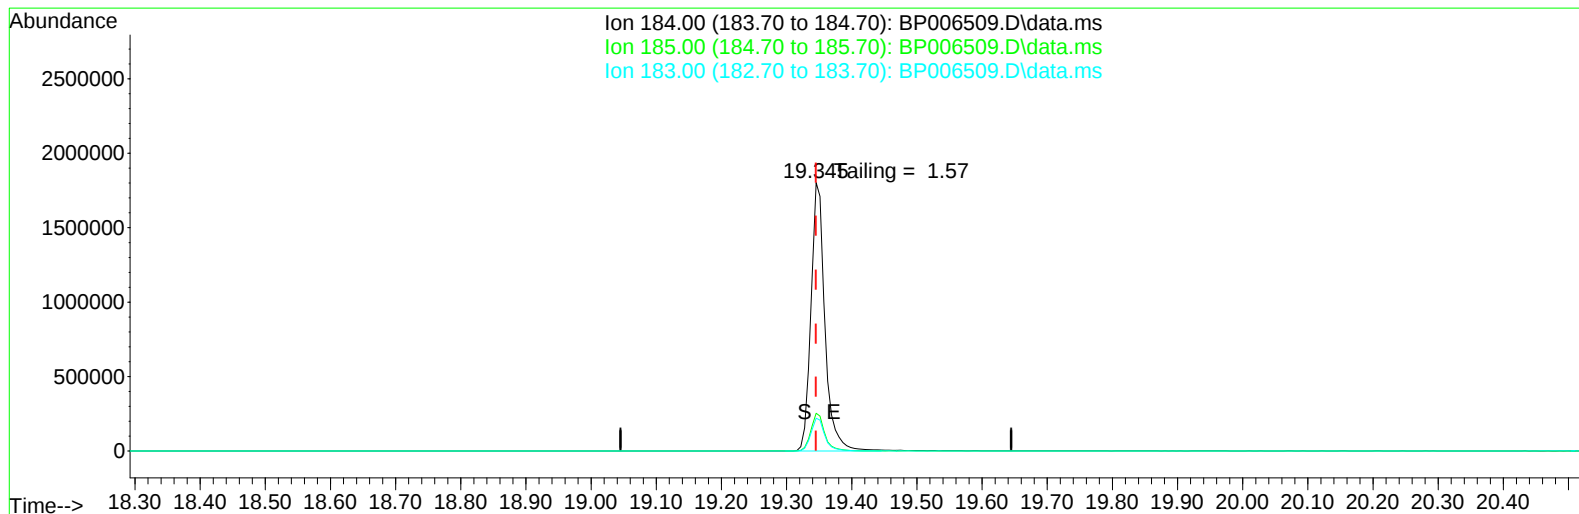

TIC: BP006509.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 44471.39 ng




response 2700819

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.11
183.00	11.90	12.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080521\
 Data File : BP006509.D
 Acq On : 05 Aug 2021 16:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 05 18:00:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

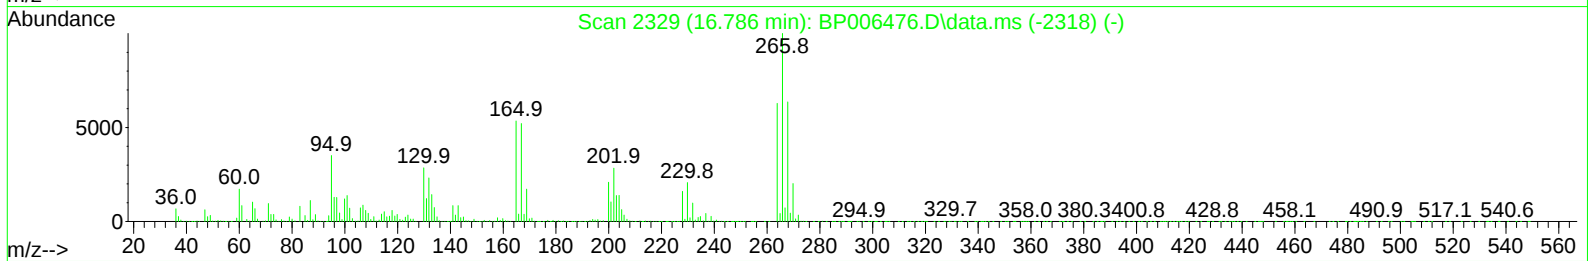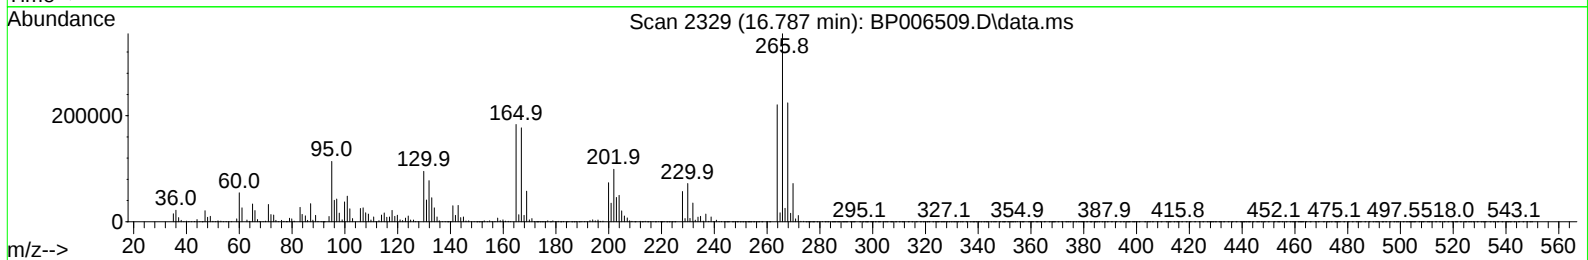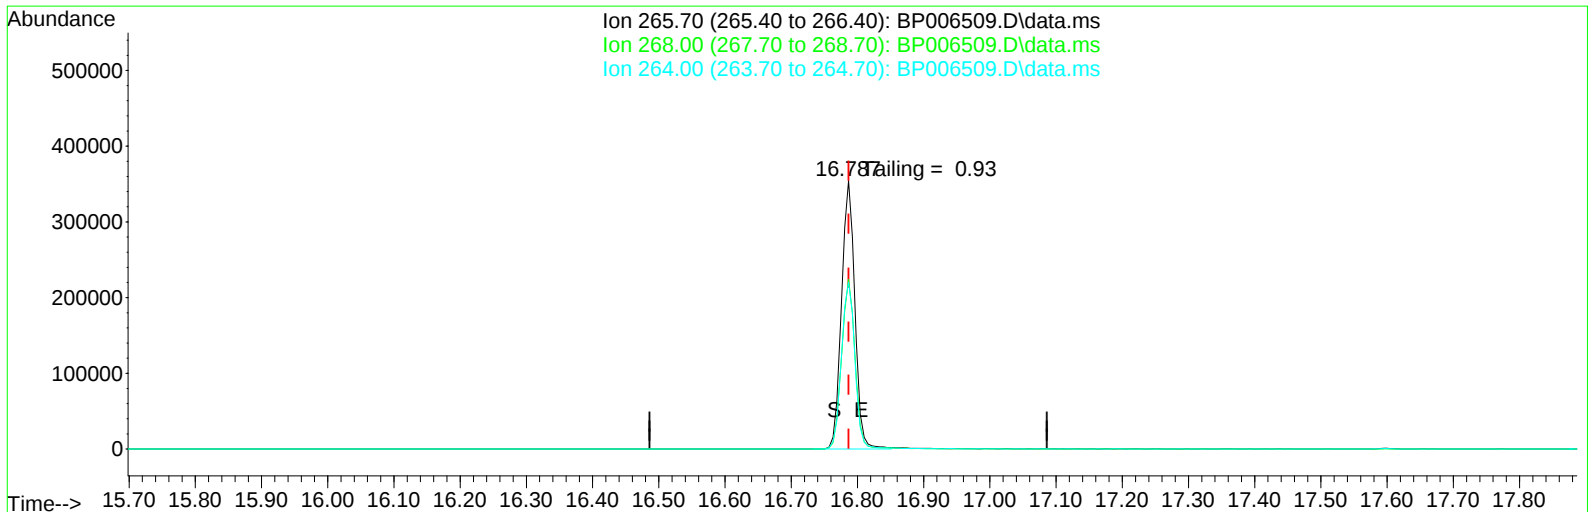

TIC: BP006509.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.000) 89885.31 ng

response 498786

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.24
264.00	62.90	62.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2021	BNA_P	BP006509.D
Compound Name	Response	Retention Time
DDT	1423692	20.55
DDD	23902	20.11
DDE	2732	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26634	1450326	1.84