


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP080620\
 Data File : BP002912.D
 Acq On : 06 Aug 2020 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 15:30:34 2020

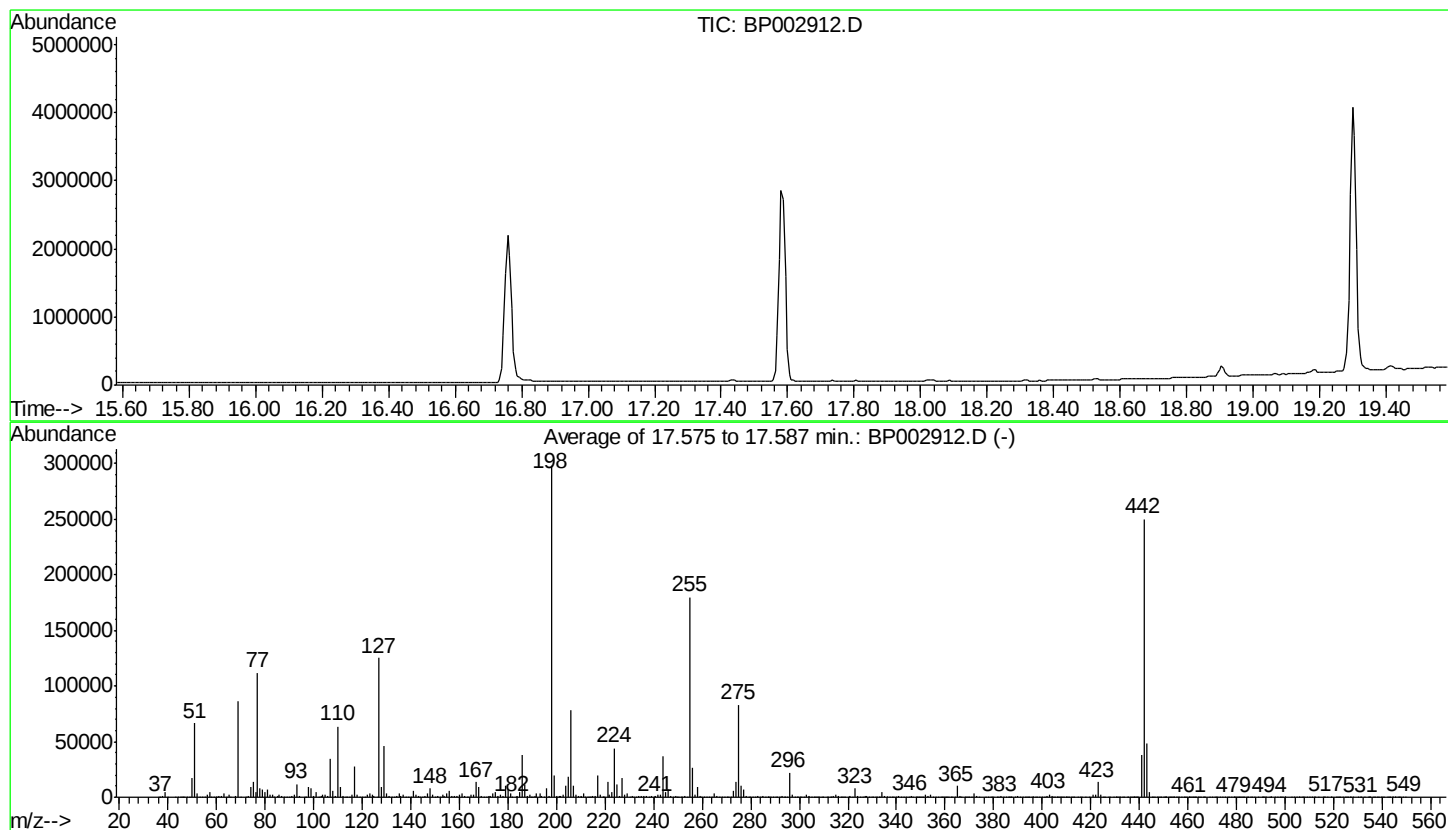

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.3	66587	PASS
68	69	0.00	2	1.6	1419	PASS
69	198	0.00	100	29.0	86389	PASS
70	69	0.00	2	0.3	274	PASS
127	198	10	80	41.9	124997	PASS
197	198	0.00	2	0.5	1478	PASS
198	198	100	100	100.0	298218	PASS
199	198	5	9	6.7	20103	PASS
275	198	10	60	27.8	82901	PASS
365	198	1	100	3.3	9874	PASS
441	198	0.01	100	12.7	37799	PASS
442	198	50	100	83.9	250346	PASS
443	442	15	24	19.4	48645	PASS