

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006545.D
 Acq On : 06 Aug 2021 18:47
 Operator : CG/JU
 Sample : M3279-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20210532-COM-5

Quant Time: Aug 07 05:38:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.752	152	182152	20.000	ng	0.00
21) Naphthalene-d8	10.534	136	722537	20.000	ng	#-0.01
39) Acenaphthene-d10	14.381	164	372373	20.000	ng	-0.01
64) Phenanthrene-d10	17.134	188	705155	20.000	ng	# 0.00
76) Chrysene-d12	21.233	240	699011	20.000	ng	# 0.00
86) Perylene-d12	23.557	264	797254	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.358	112	1511484	127.451	ng	0.00
7) Phenol-d6	6.934	99	1901198	112.855	ng	0.00
23) Nitrobenzene-d5	8.911	82	1268726	81.049	ng	0.00
42) 2,4,6-Tribromophenol	15.875	330	470521	120.903	ng	0.00
45) 2-Fluorobiphenyl	13.010	172	1884673	75.723	ng	0.00
79) Terphenyl-d14	19.710	244	2415782	69.251	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006545.D
Acq On : 06 Aug 2021 18:47
Operator : CG/JU
Sample : M3279-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20210532-COM-5

Quant Time: Aug 07 05:38:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration




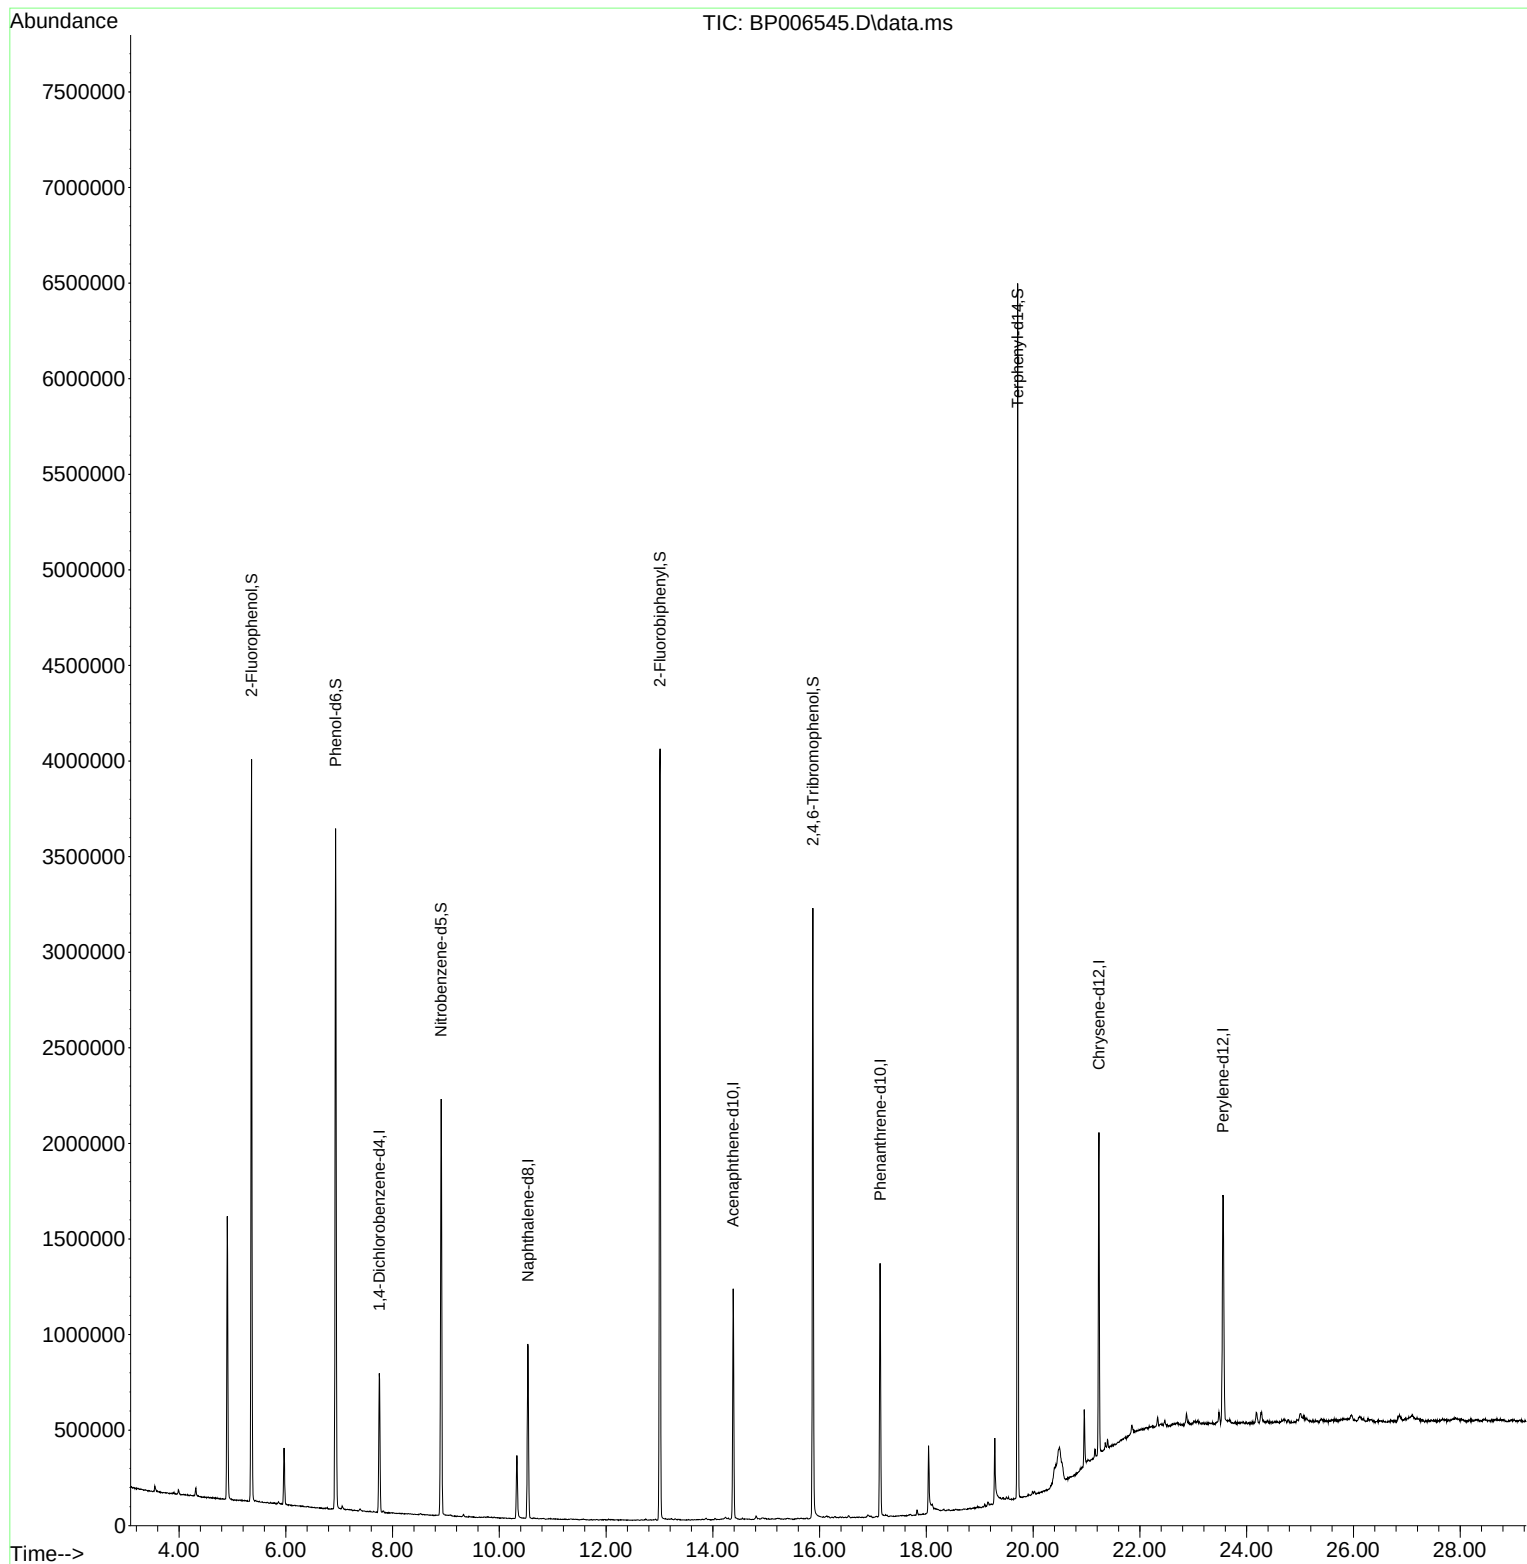


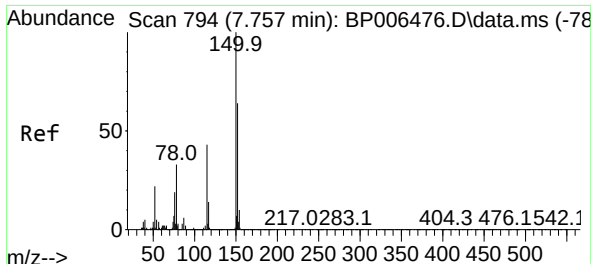

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.752 min Scan# 793
Delta R.T. -0.005 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47




Instrument :
BNA_P
ClientSampleId :
20210532-COM-5


Tgt Ion:152 Resp: 182152
Ion Ratio Lower Upper
152 100
150 159.1 125.6 188.4
115 67.9 48.5 72.7

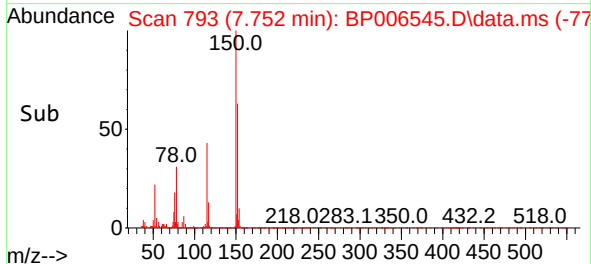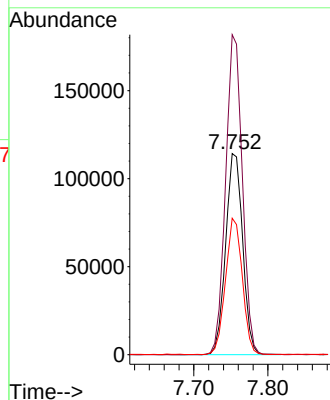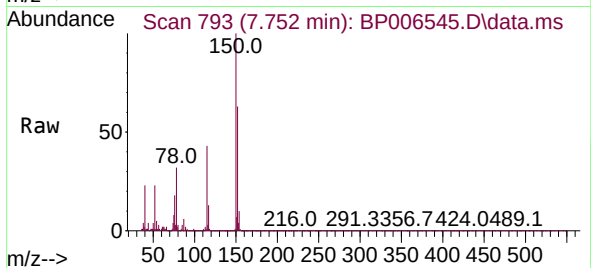

#5
2-Fluorophenol
Concen: 127.451 ng
RT: 5.358 min Scan# 386
Delta R.T. 0.000 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47

Tgt Ion:112 Resp: 1511484
Ion Ratio Lower Upper
112 100
64 61.7 41.4 62.2
63 31.5 23.8 35.8


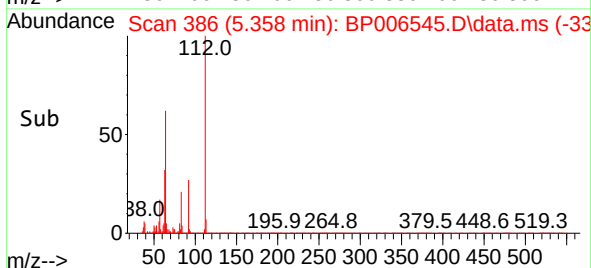
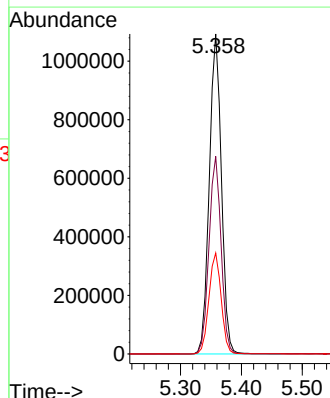
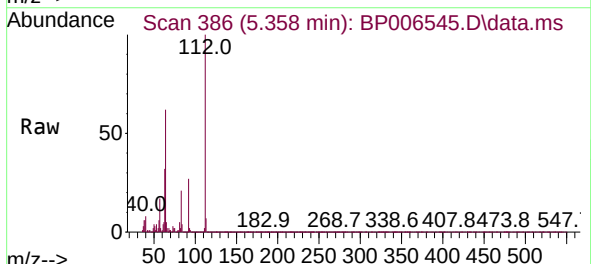




#7
Phenol-d6
Concen: 112.855 ng
RT: 6.934 min Scan# 654
Delta R.T. 0.000 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47




Instrument :
BNA_P
ClientSampleId :
20210532-COM-5


Tgt Ion:	99	Resp:	1901198
Ion	Ratio	Lower	Upper
99	100		
42	17.2	13.4	20.0
71	36.9	30.6	46.0

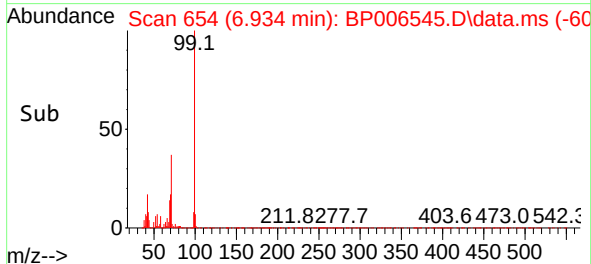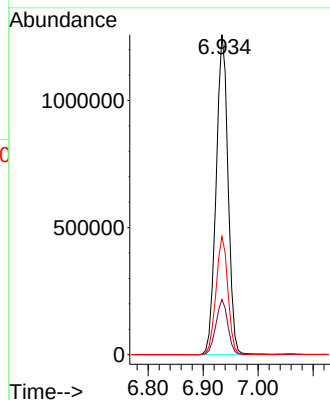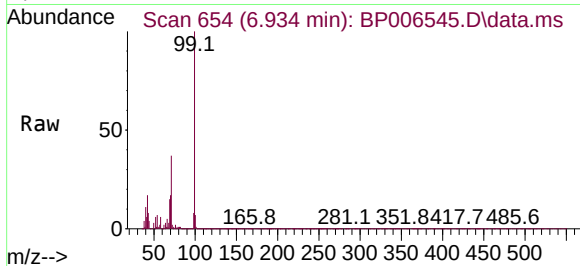

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.534 min Scan# 1266
Delta R.T. -0.012 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47

Tgt Ion:	136	Resp:	722537
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	12.8
54	8.2	4.6	6.8#
68	7.4	3.6	5.4#

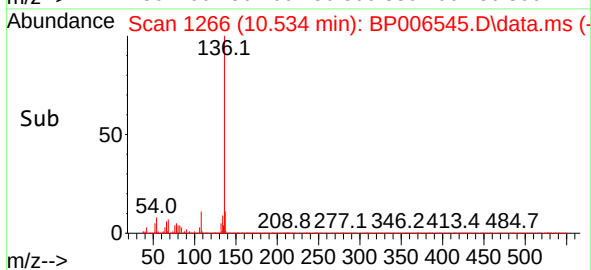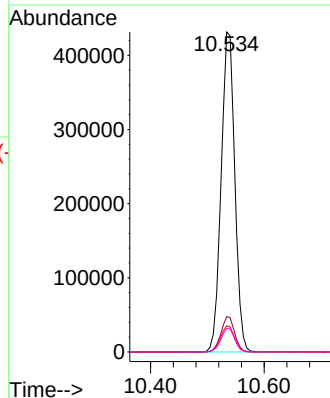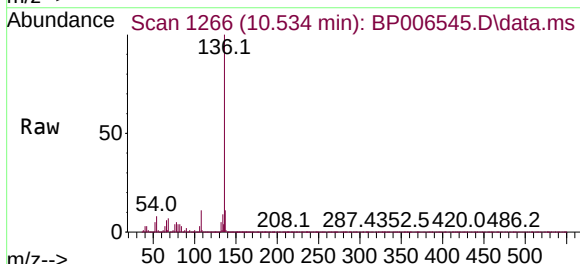

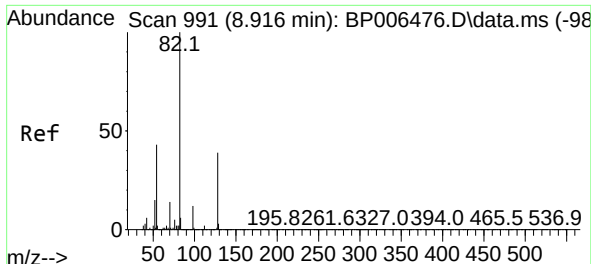

#23

Nitrobenzene-d5

Concen: 81.049 ng

RT: 8.911 min Scan# 990

Delta R.T. -0.006 min

Lab File: BP006545.D

Acq: 06 Aug 2021 18:47

Instrument :





BNA_P

ClientSampleId :

20210532-COM-5

Tgt Ion: 82 Resp: 1268726

Ion	Ratio	Lower	Upper
82	100		
128	38.7	35.7	53.5
54	43.0	35.0	52.4

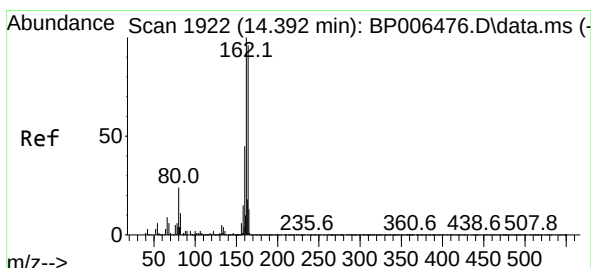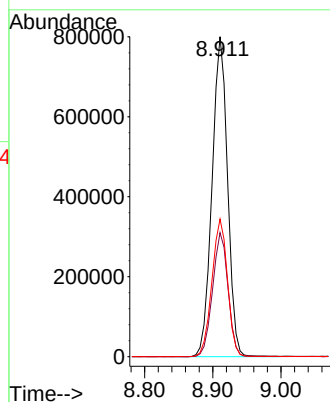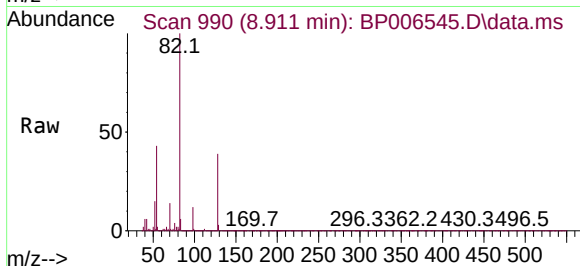

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.381 min Scan# 1920




Delta R.T. -0.012 min


Lab File: BP006545.D

Acq: 06 Aug 2021 18:47

Tgt Ion: 164 Resp: 372373

Ion	Ratio	Lower	Upper
164	100		
162	101.0	80.2	120.2
160	46.8	34.5	51.7


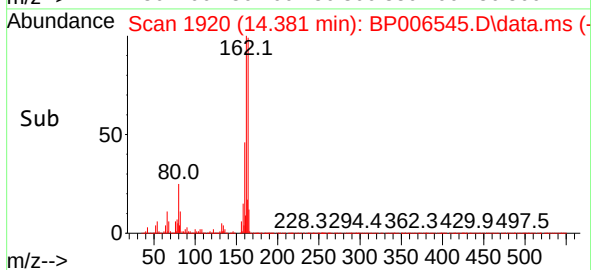
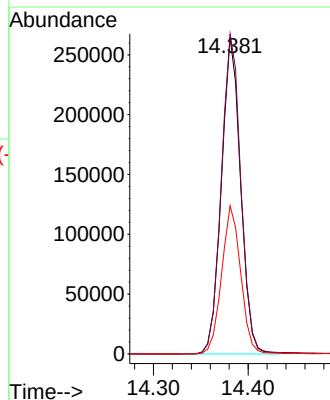
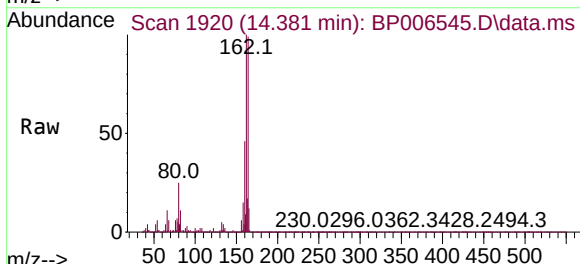




#42
2,4,6-Tribromophenol
Concen: 120.903 ng
RT: 15.875 min Scan# 2174
Delta R.T. -0.006 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47




Instrument :
BNA_P
ClientSampleId :
20210532-COM-5


Tgt Ion:330 Resp: 470521
Ion Ratio Lower Upper
330 100
332 97.3 77.8 116.8
141 48.7 25.4 38.2#

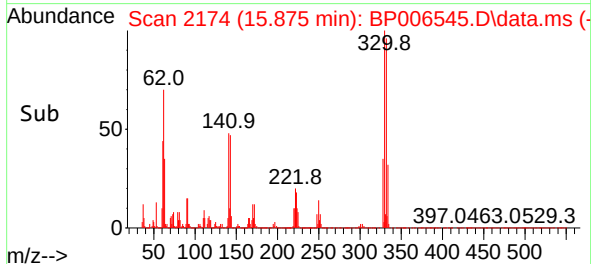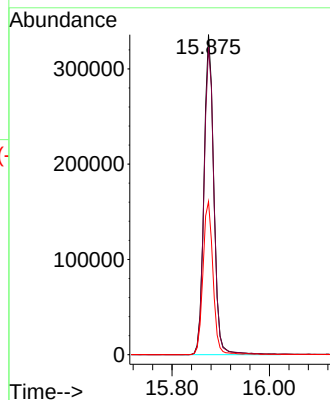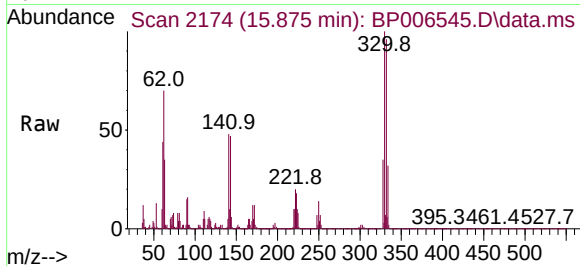

#45
2-Fluorobiphenyl
Concen: 75.723 ng
RT: 13.010 min Scan# 1687
Delta R.T. -0.006 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47

Tgt Ion:172 Resp: 1884673
Ion Ratio Lower Upper
172 100
171 35.6 27.9 41.9
170 23.2 18.6 27.8


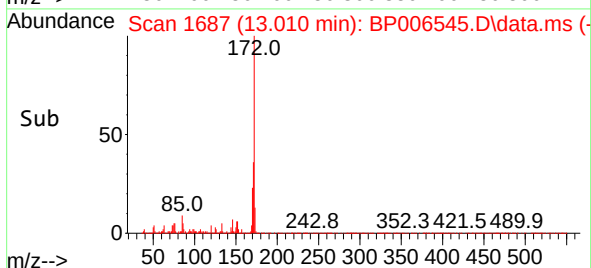
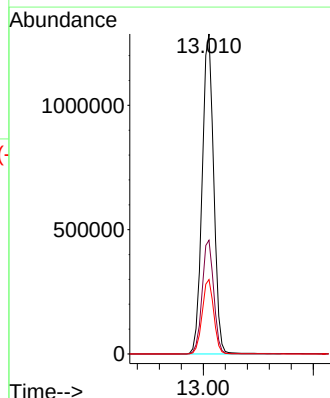
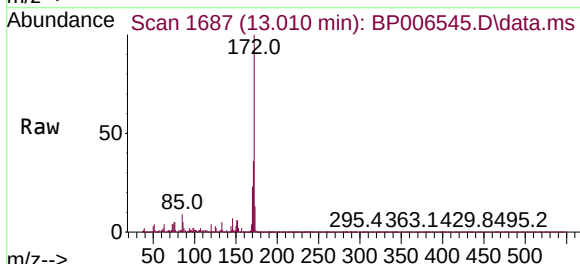




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.134 min Scan# 2388
Delta R.T. -0.006 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47




Instrument :
BNA_P
ClientSampleId :
20210532-COM-5


Tgt Ion:188 Resp: 705155
Ion Ratio Lower Upper
188 100
94 12.6 5.6 8.4#
80 14.4 6.3 9.5#

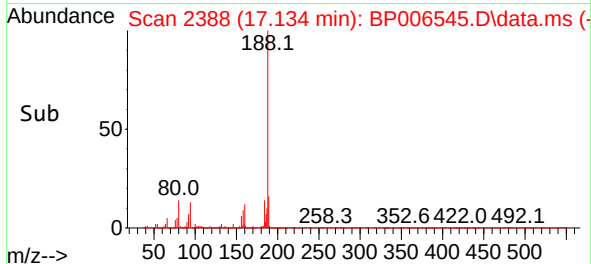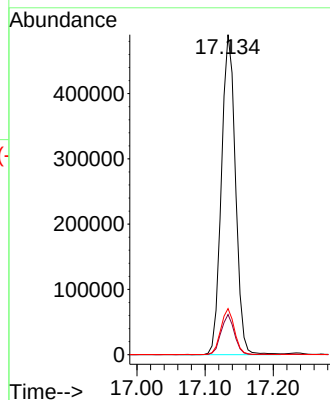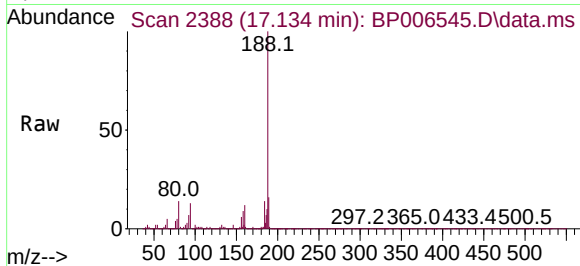

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.233 min Scan# 3085
Delta R.T. -0.006 min
Lab File: BP006545.D
Acq: 06 Aug 2021 18:47

Tgt Ion:240 Resp: 699011
Ion Ratio Lower Upper
240 100
120 13.7 6.5 9.7#
236 25.4 20.6 31.0


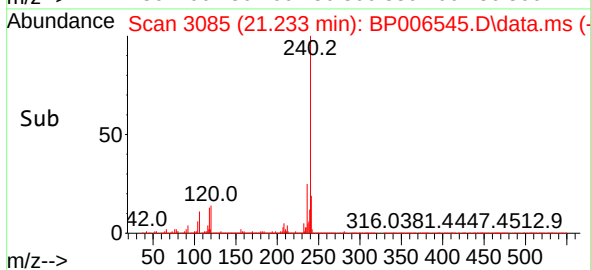
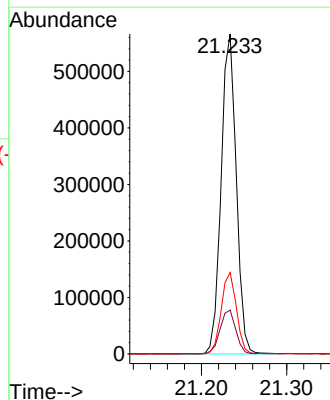
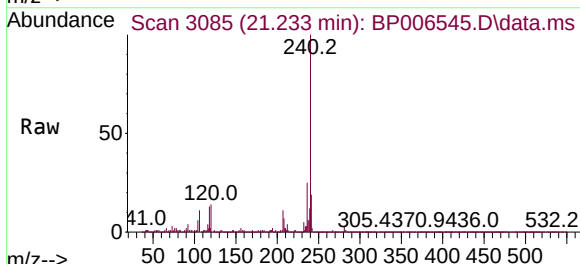




#79
 Terphenyl-d14
 Concen: 69.251 ng
 RT: 19.710 min Scan# 2826
 Delta R.T. -0.006 min
 Lab File: BP006545.D
 Acq: 06 Aug 2021 18:47

Instrument :
 BNA_P
 ClientSampleId :
 20210532-COM-5

Tgt Ion:244 Resp: 2415782
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.0 9.0
 122 13.8 7.1 10.7#

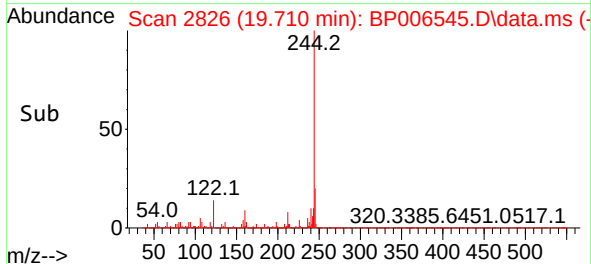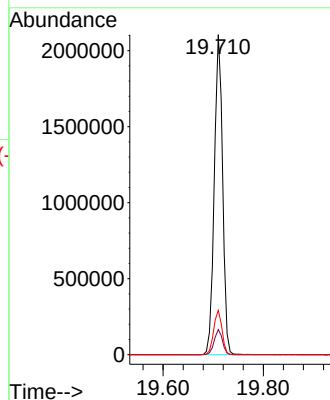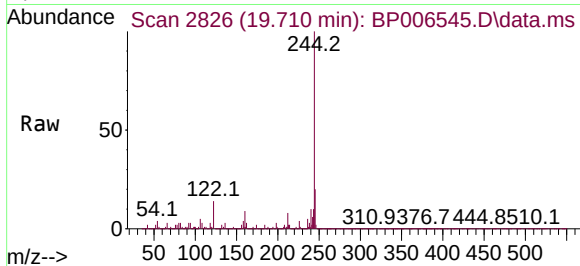

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.557 min Scan# 3480
 Delta R.T. -0.012 min
 Lab File: BP006545.D
 Acq: 06 Aug 2021 18:47

Tgt Ion:264 Resp: 797254
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.6 28.0
 265 22.4 17.6 26.4

