
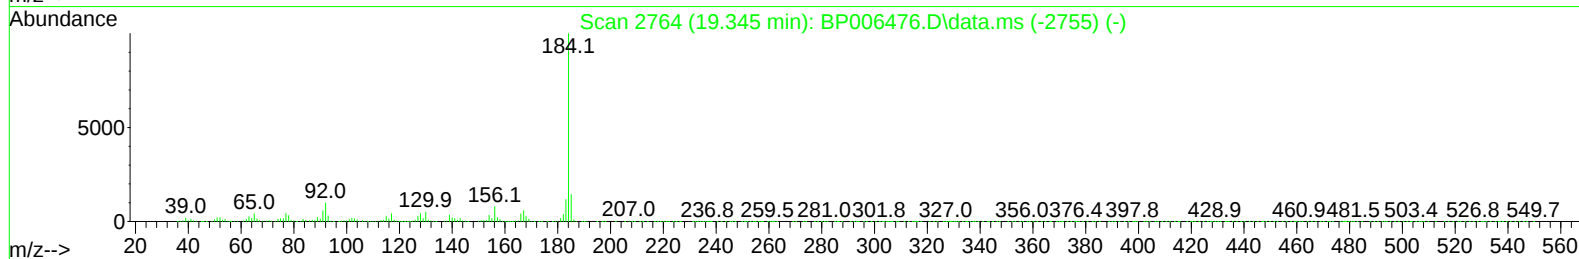
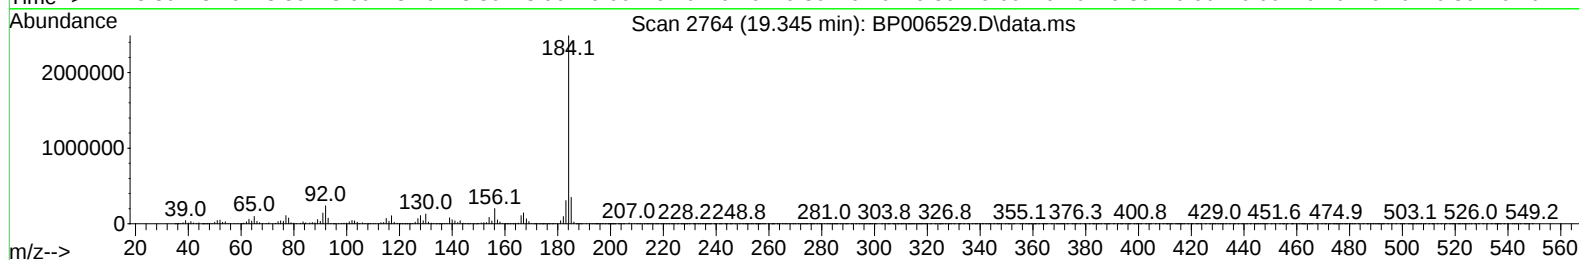


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006529.D
Acq On : 06 Aug 2021 07:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 16:44:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

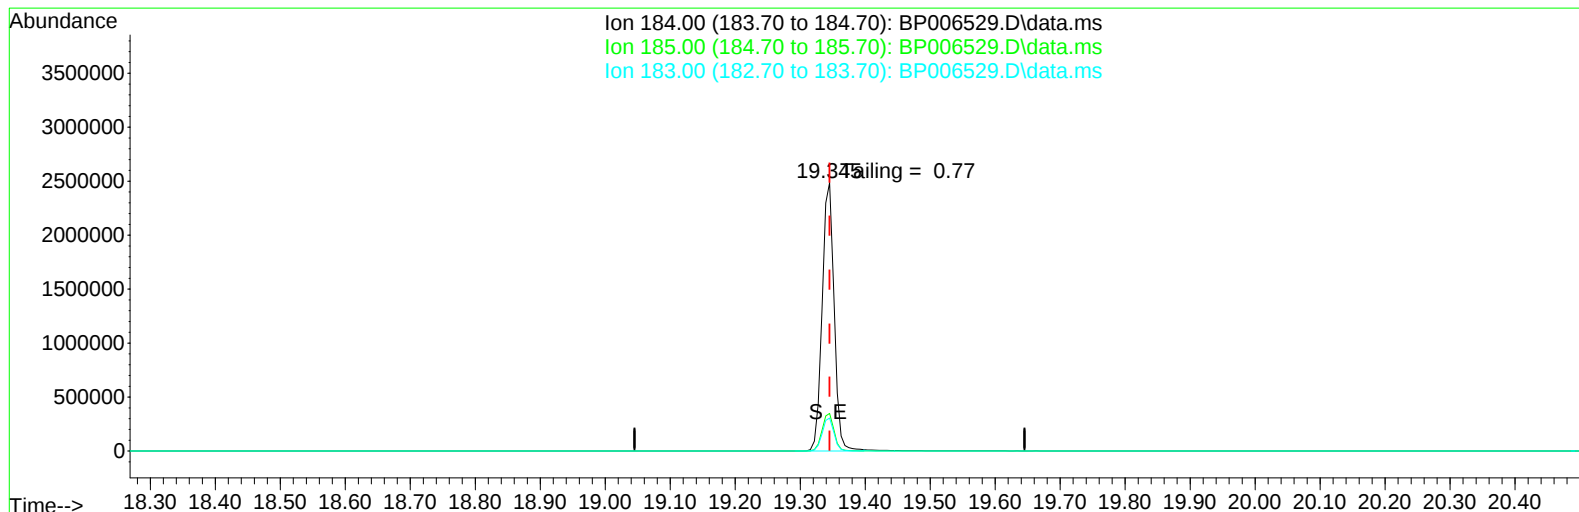

TIC: BP006529.D\data.ms

(77) Benzidine




19.345min (+ 0.000) 1543798.18 ng

response 3206370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.04
183.00	11.90	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006529.D
Acq On : 06 Aug 2021 07:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 16:44:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

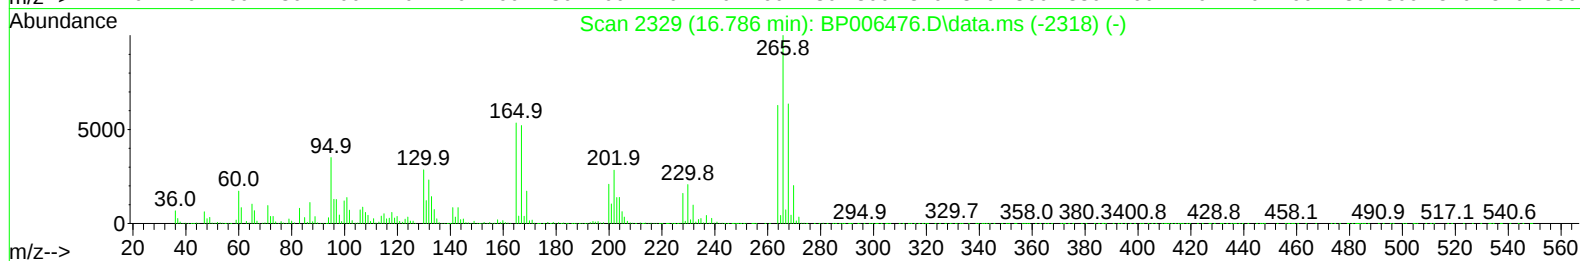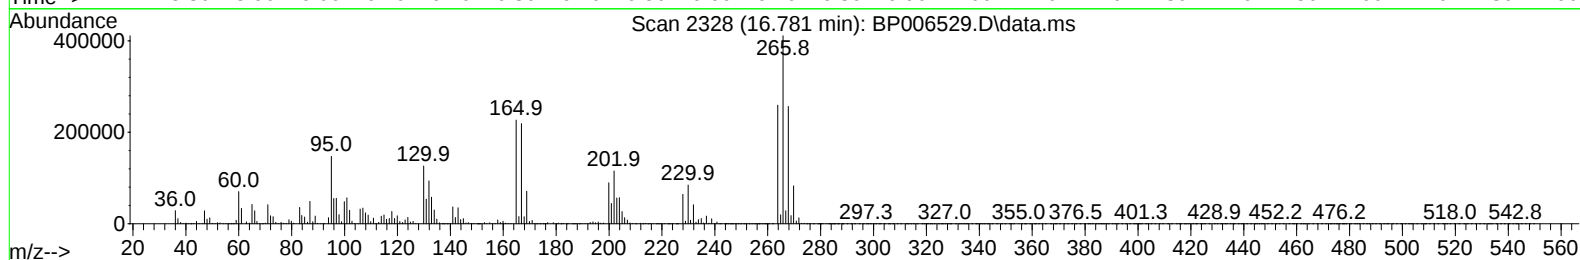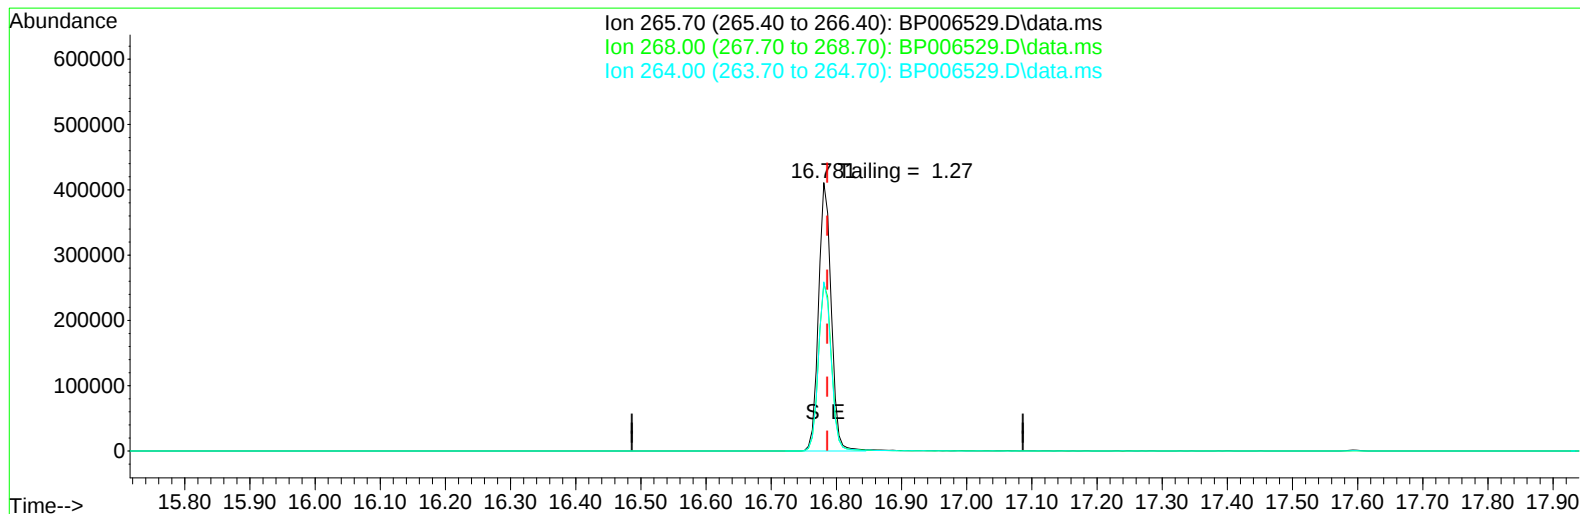

TIC: BP006529.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.006) 1975466.19 ng

response 561108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.36
264.00	62.90	63.05
0.00	0.00	0.00