

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006541.D
 Acq On : 06 Aug 2021 16:27
 Operator : CG/JU
 Sample : PB138238BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB138238BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.358	380	386	398	rVB	4670999	6477135	51.95%	11.164%
2	6.934	647	654	668	rVB	4136599	6577063	52.75%	11.336%
3	7.752	787	793	803	rVB	820064	1288833	10.34%	2.221%
4	8.911	982	990	1003	rBV	2641233	4245480	34.05%	7.317%
5	10.534	1259	1266	1274	rBV	1095786	1826030	14.65%	3.147%
6	13.010	1679	1687	1699	rBV	6032757	8459732	67.85%	14.581%
7	14.381	1911	1920	1930	rBV	1500354	2241523	17.98%	3.863%
8	15.875	2167	2174	2199	rBV	4233931	6203708	49.76%	10.693%
9	17.139	2382	2389	2399	rBV	1870611	2595934	20.82%	4.474%
10	19.716	2821	2827	2832	rBV	10290121	12468287	100.00%	21.490%
11	21.233	3080	3085	3092	rBV	2188766	2806815	22.51%	4.838%
12	23.563	3475	3481	3492	rVB2	1424999	2828402	22.68%	4.875%




Sum of corrected areas: 58018942

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006541.D
Acq On : 06 Aug 2021 16:27
Operator : CG/JU
Sample : PB138238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

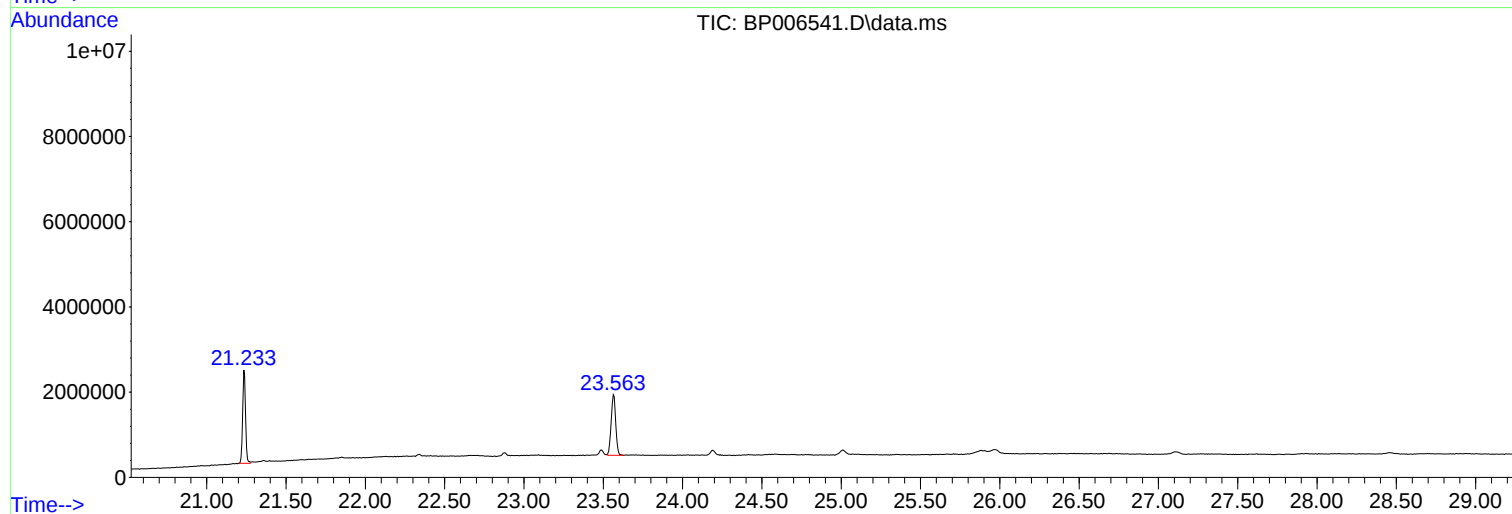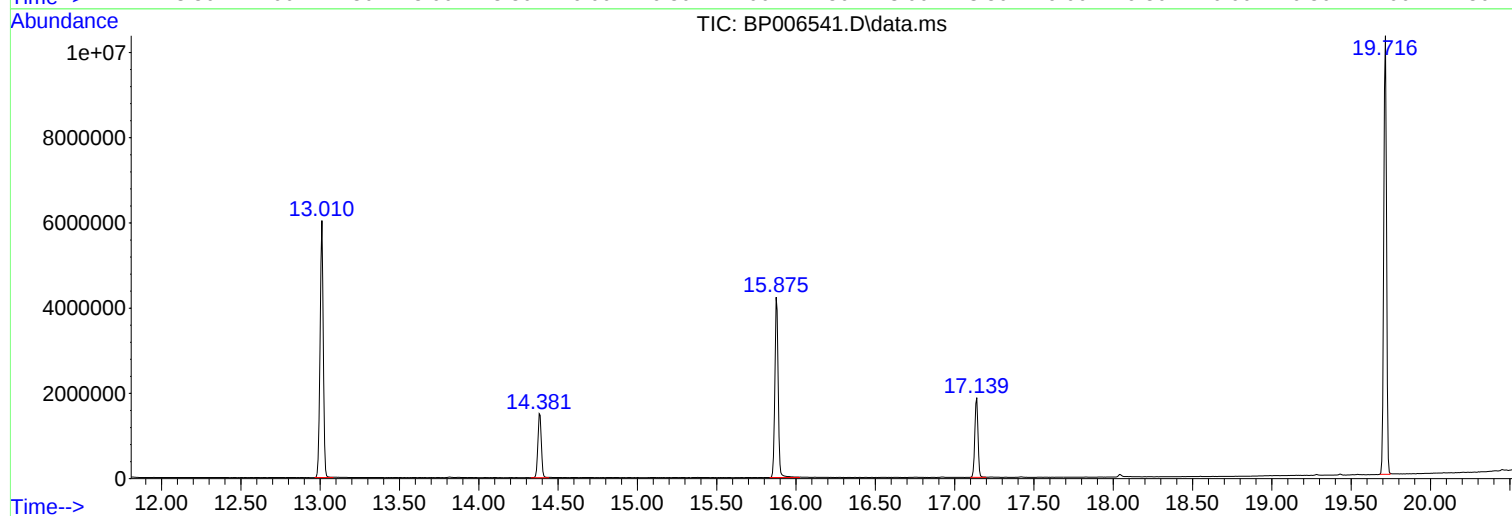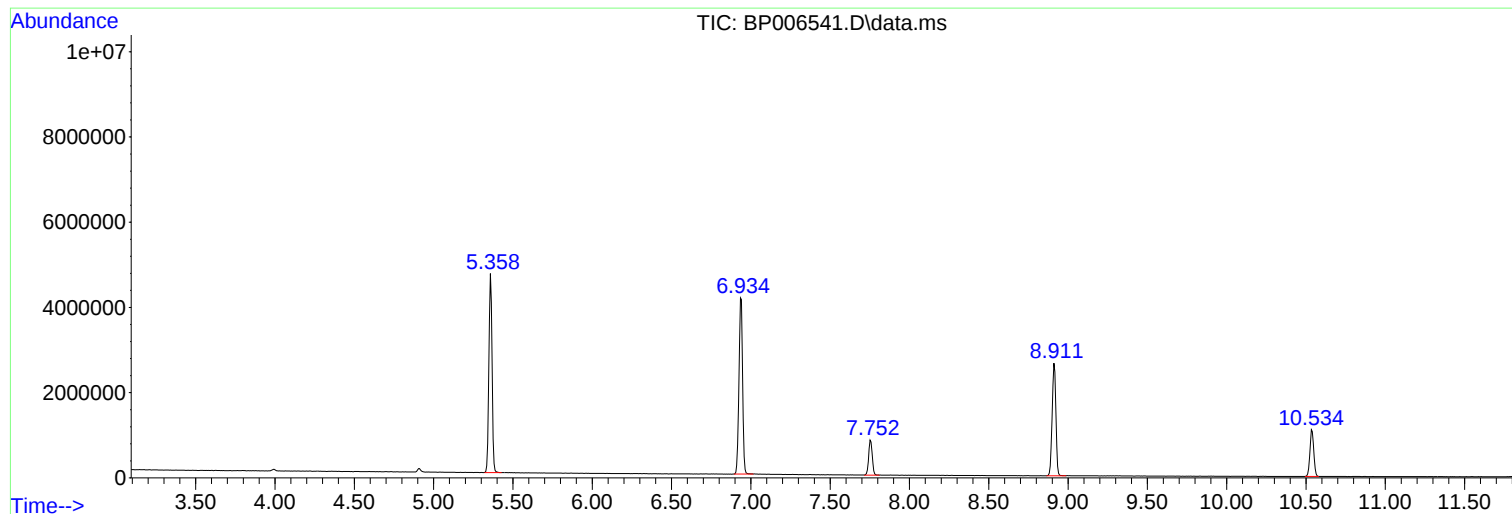

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006541.D
Acq On : 06 Aug 2021 16:27
Operator : CG/JU
Sample : PB138238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006541.D
Acq On : 06 Aug 2021 16:27
Operator : CG/JU
Sample : PB138238BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB138238BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------