
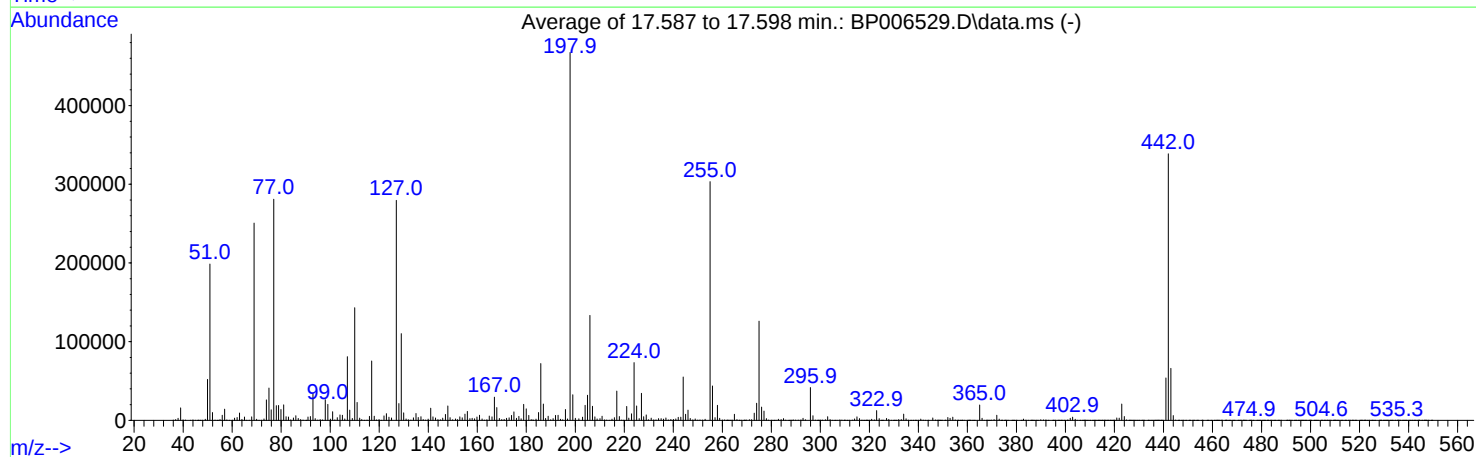


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006529.D
 Acq On : 06 Aug 2021 07:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:41:30 2021

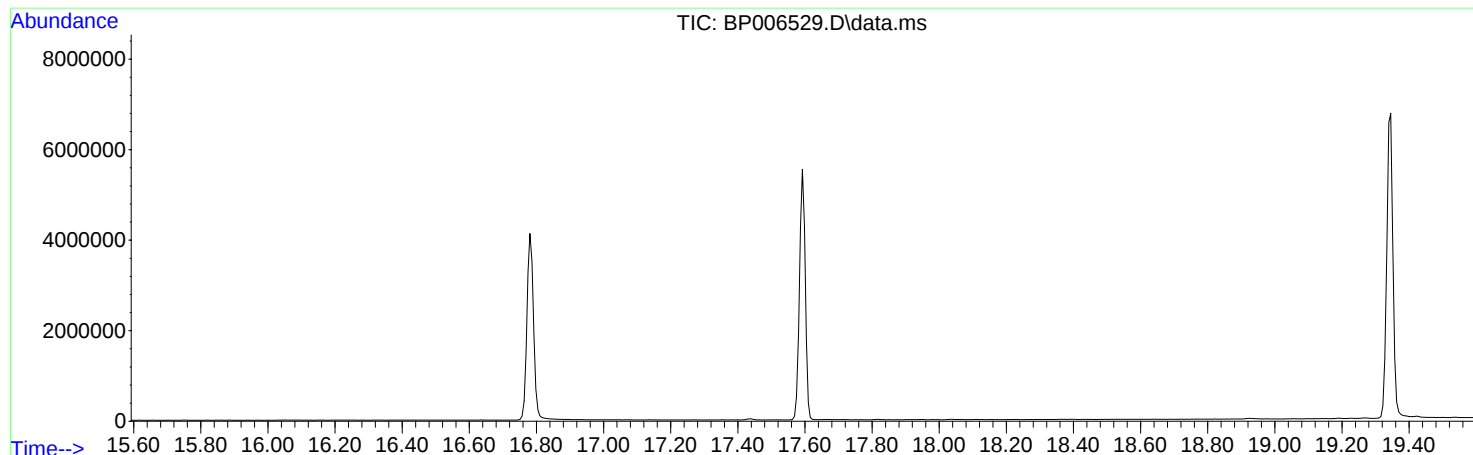




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	198578	PASS
68	69	0.00	2	1.8	4391	PASS
69	198	0.00	100	53.6	250717	PASS
70	69	0.00	2	0.6	1430	PASS
127	198	10	80	59.8	279663	PASS
197	198	0.00	2	0.4	1923	PASS
198	198	100	100	100.0	467423	PASS
199	198	5	9	6.9	32456	PASS
275	198	10	60	27.0	125997	PASS
365	198	1	100	4.2	19501	PASS
441	198	0.01	100	11.5	53851	PASS
442	442	100	100	100.0	338731	PASS
443	442	15	24	19.5	66093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006529.D
 Acq On : 06 Aug 2021 07:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 06 16:44:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

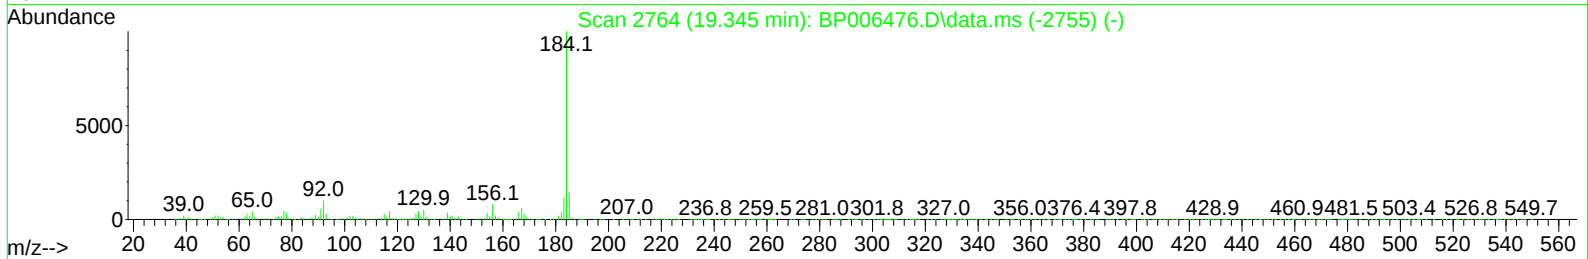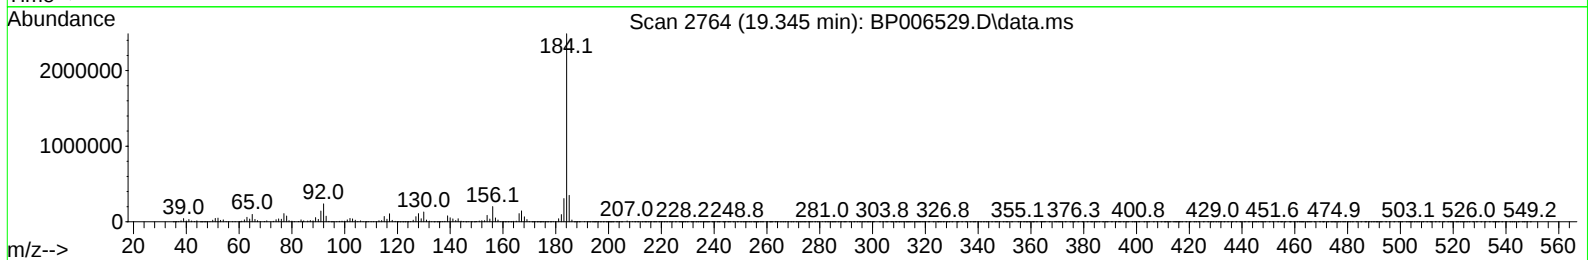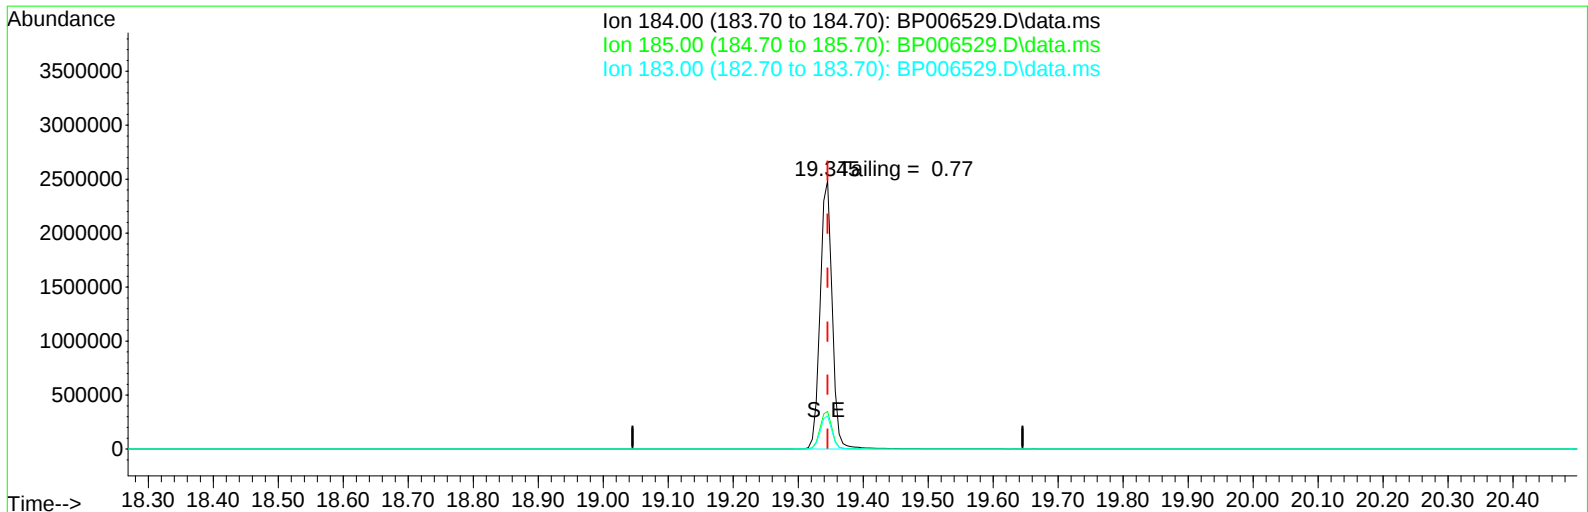

TIC: BP006529.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 1543798.18 ng




response 3206370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.04
183.00	11.90	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
Data File : BP006529.D
Acq On : 06 Aug 2021 07:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 06 16:44:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:41:30 2021
Response via : Initial Calibration

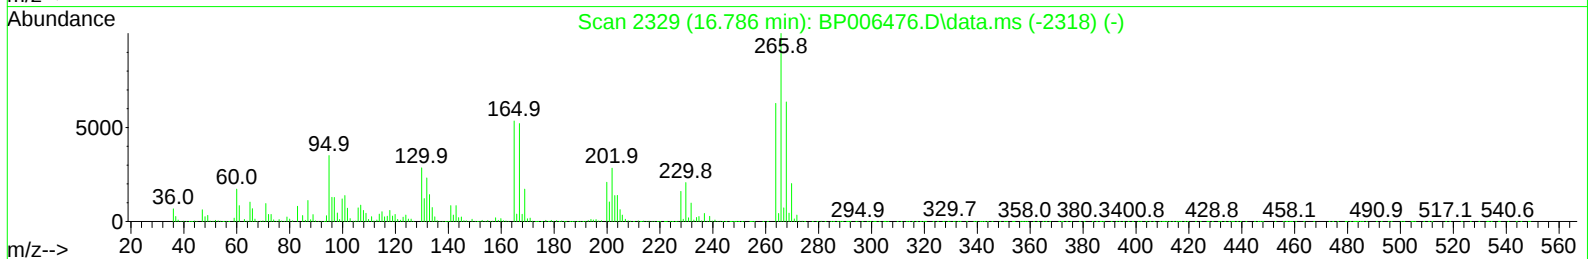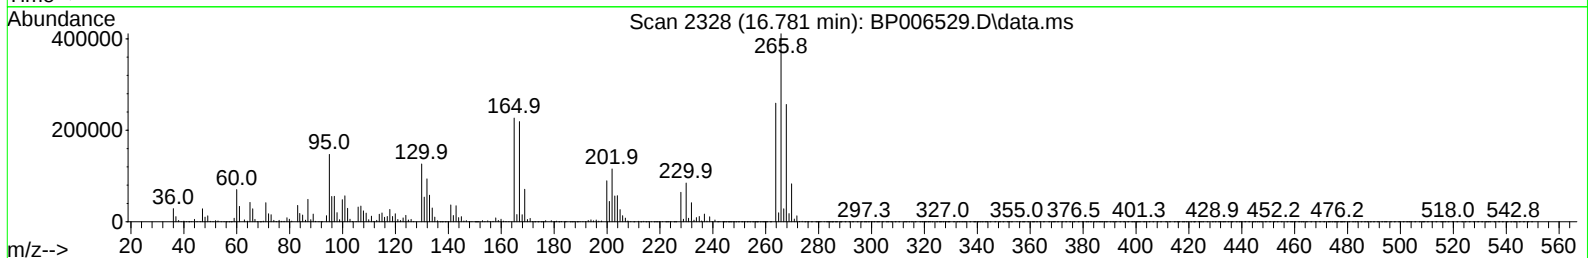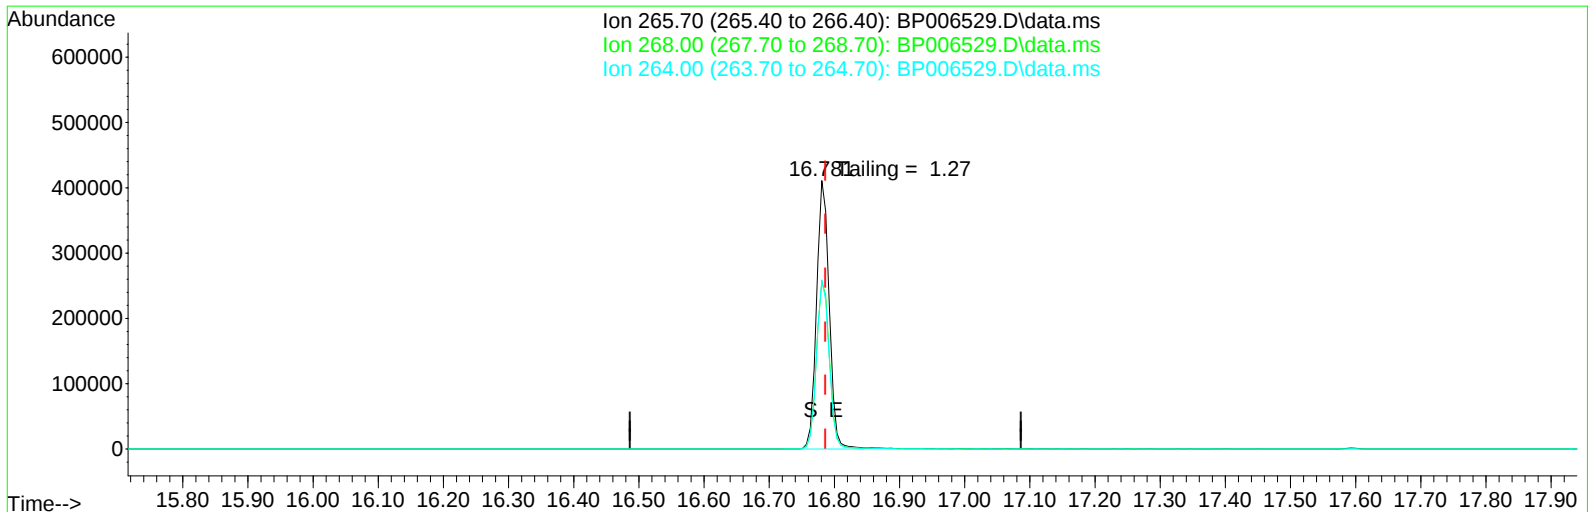

TIC: BP006529.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.006) 1975466.19 ng

response 561108

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.36
264.00	62.90	63.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/6/2021	BNA_P	<u>BP006529.D</u>
Compound Name	Response	Retention Time
DDT	1546069	20.54
DDD	55636	20.11
DDE	3764	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
59400	1605469	3.70