
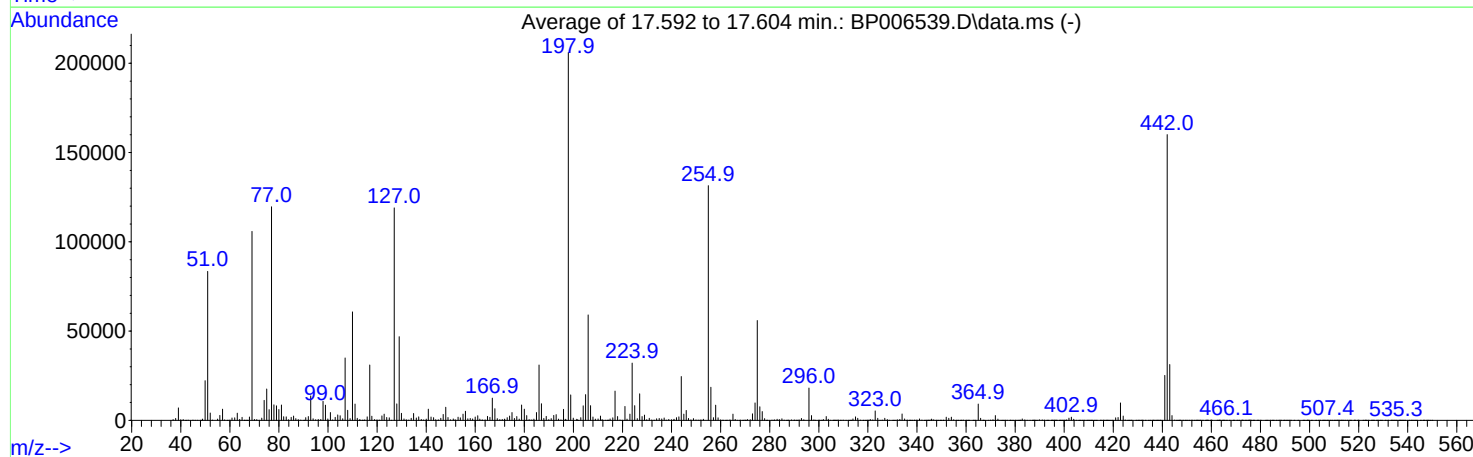


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006539.D
 Acq On : 06 Aug 2021 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:41:30 2021

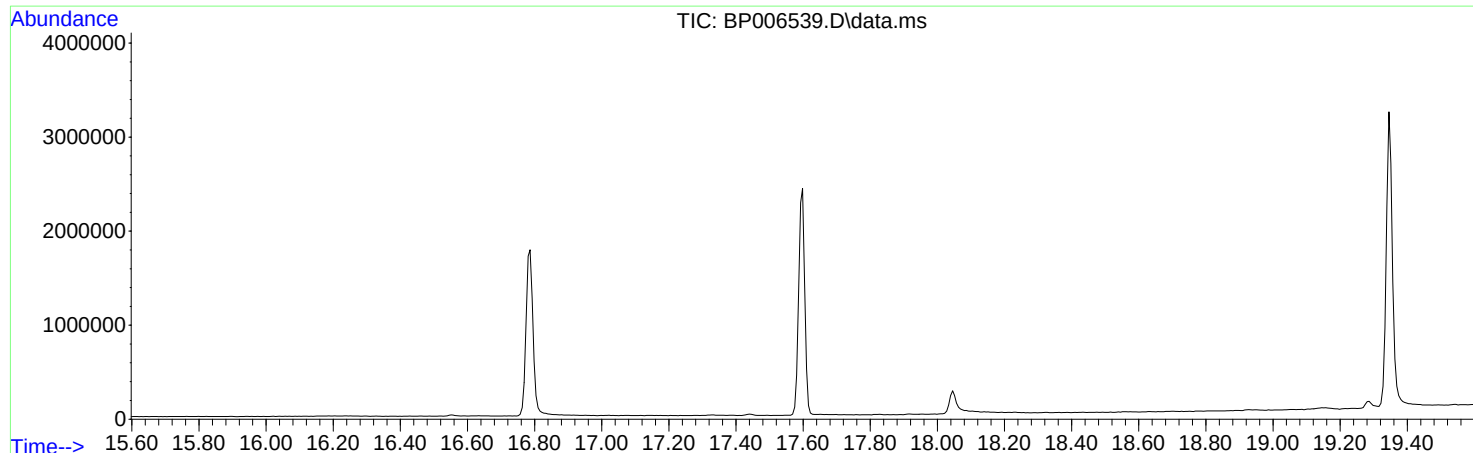




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	83465	PASS
68	69	0.00	2	1.8	1914	PASS
69	198	0.00	100	51.4	105823	PASS
70	69	0.00	2	0.5	541	PASS
127	198	10	80	57.8	119055	PASS
197	198	0.00	2	0.3	620	PASS
198	198	100	100	100.0	206036	PASS
199	198	5	9	6.9	14258	PASS
275	198	10	60	27.1	55936	PASS
365	198	1	100	4.4	9126	PASS
441	198	0.01	100	12.2	25216	PASS
442	442	100	100	100.0	160043	PASS
443	442	15	24	19.5	31278	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006539.D
 Acq On : 06 Aug 2021 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 06 16:38:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

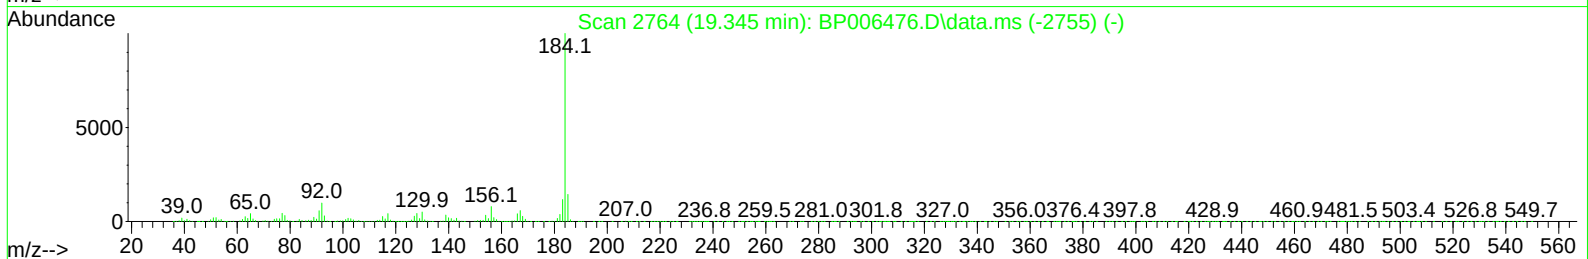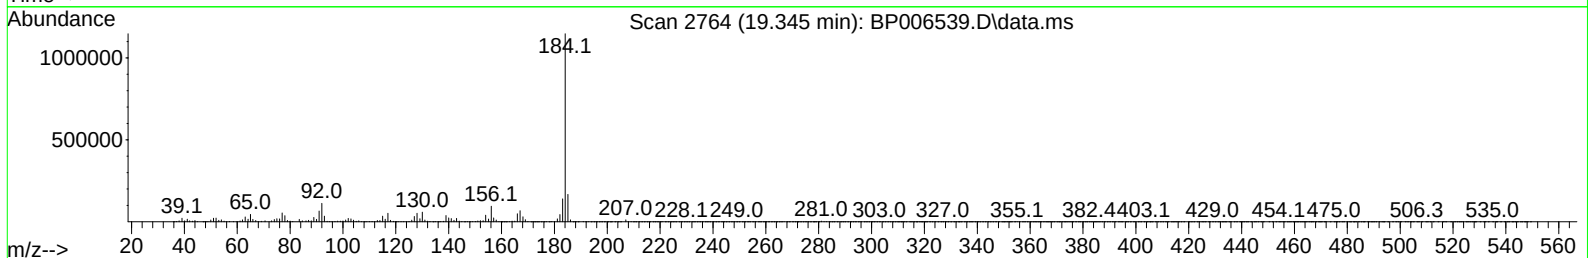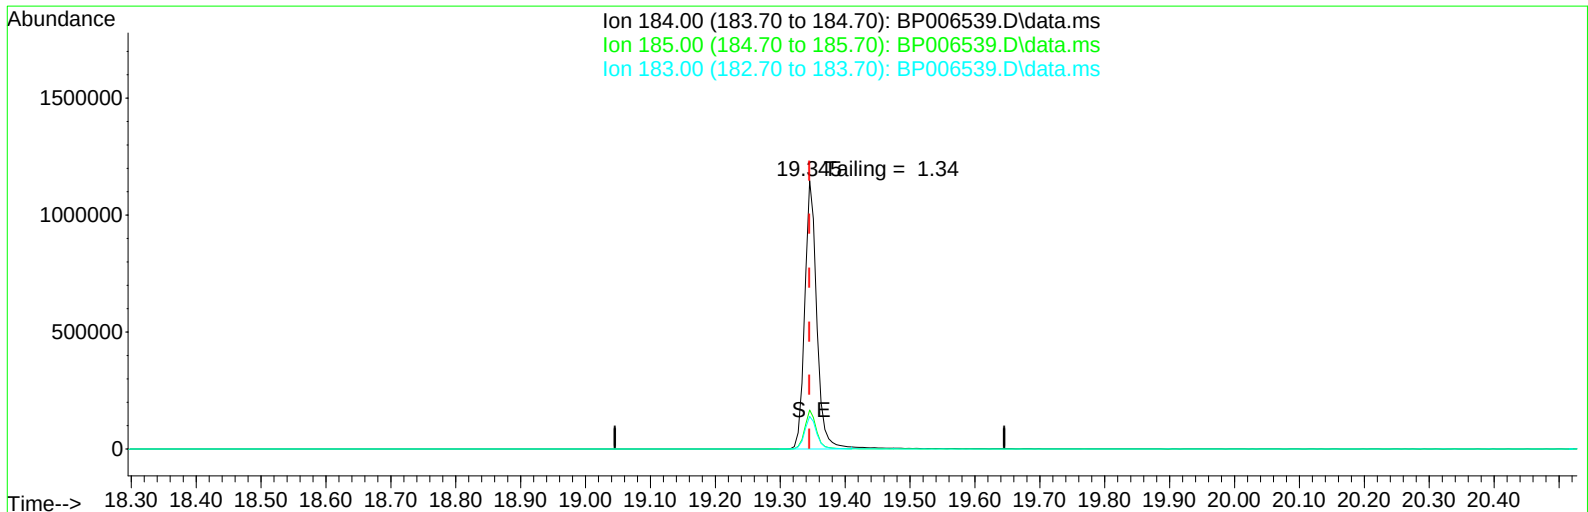

TIC: BP006539.D\data.ms

(77) Benzidine

19.345min (+ 0.000) 175895.89 ng




response 1505313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.57
183.00	11.90	12.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080621\
 Data File : BP006539.D
 Acq On : 06 Aug 2021 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Aug 06 16:38:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:41:30 2021
 Response via : Initial Calibration

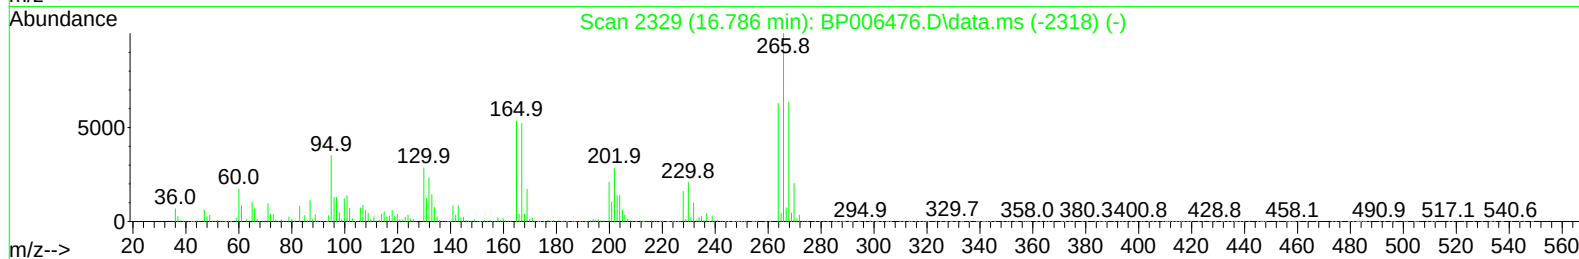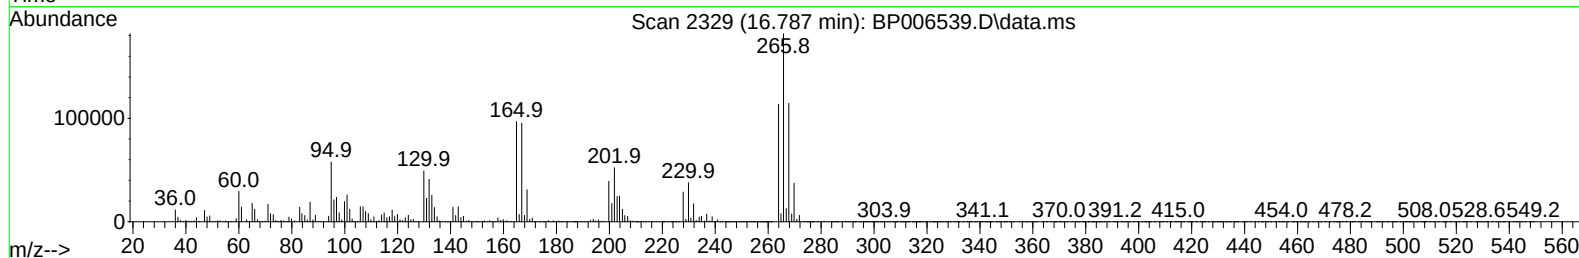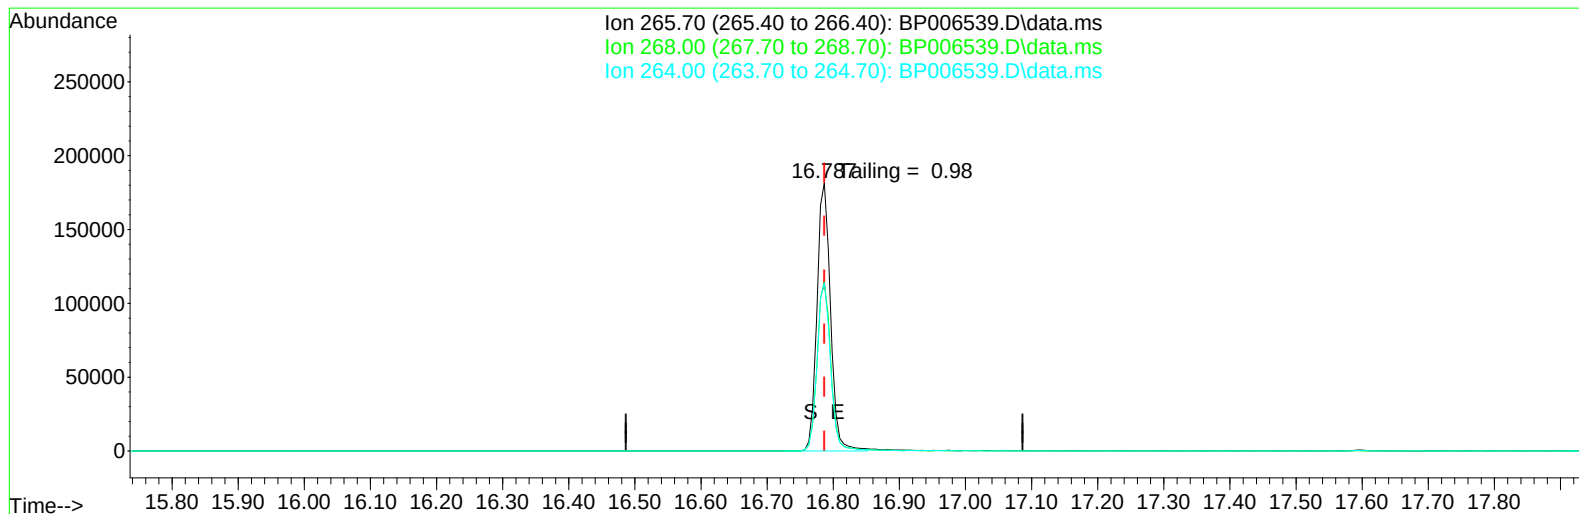

TIC: BP006539.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.000) 1715285.50 ng

response 261428

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.99
264.00	62.90	62.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/6/2021	BNA_P	<u>BP006539.D</u>
Compound Name	Response	Retention Time
DDT	752195	20.55
DDD	17532	20.12
DDE	2008	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19540	771735	2.53