




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021395.D
Acq On : 06 Aug 2024 17:44
Operator : CG/JU
Sample : P3456-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Manual IntegrationsAPPROVED

Quant Time: Aug 06 18:38:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/09/2024

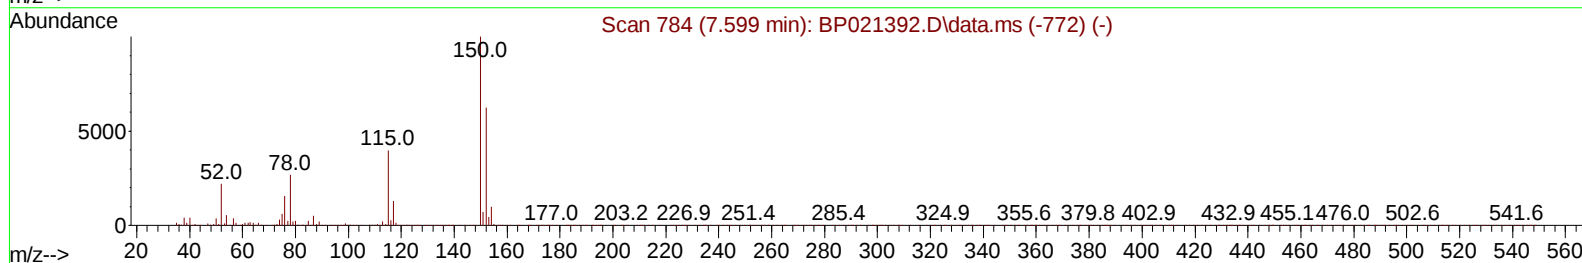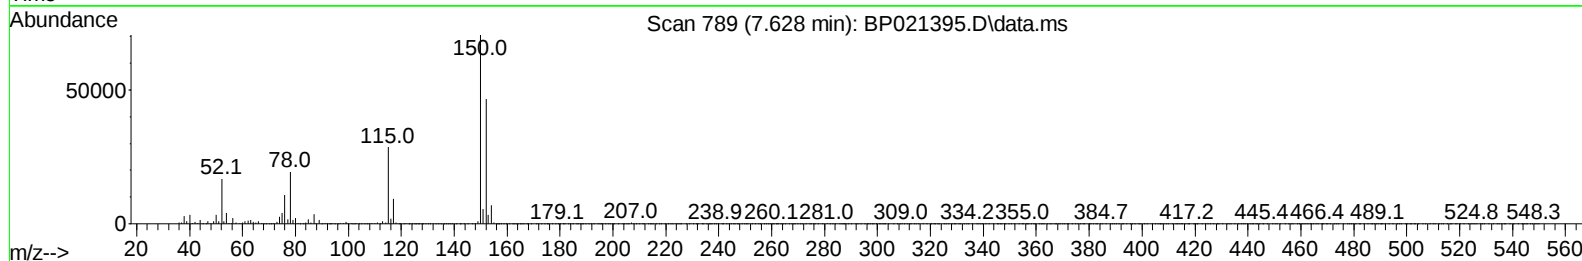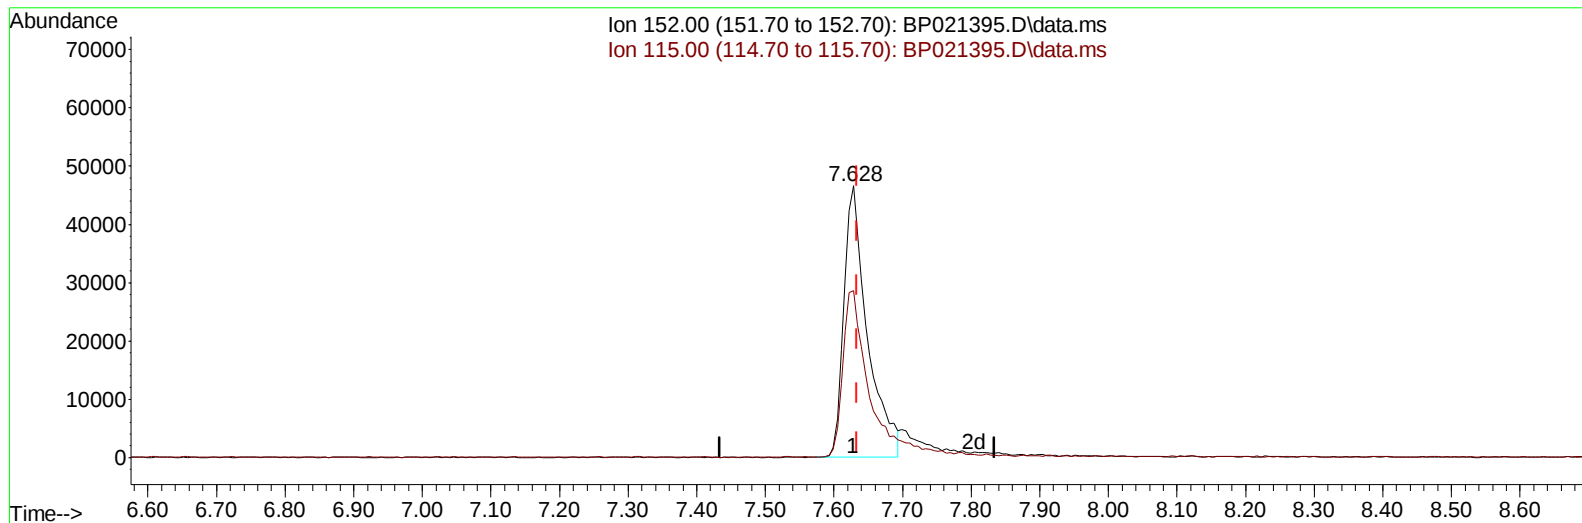

TIC: BP021395.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.628min (-0.006) 20.00 ng/u1

response 111168

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	62.30	61.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021395.D
Acq On : 06 Aug 2024 17:44
Operator : CG/JU
Sample : P3456-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Manual IntegrationsAPPROVED

Quant Time: Aug 06 18:38:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/09/2024

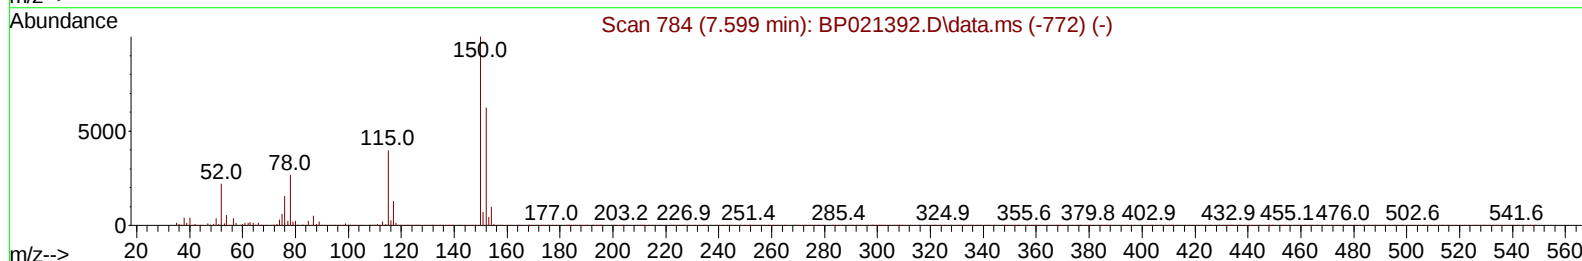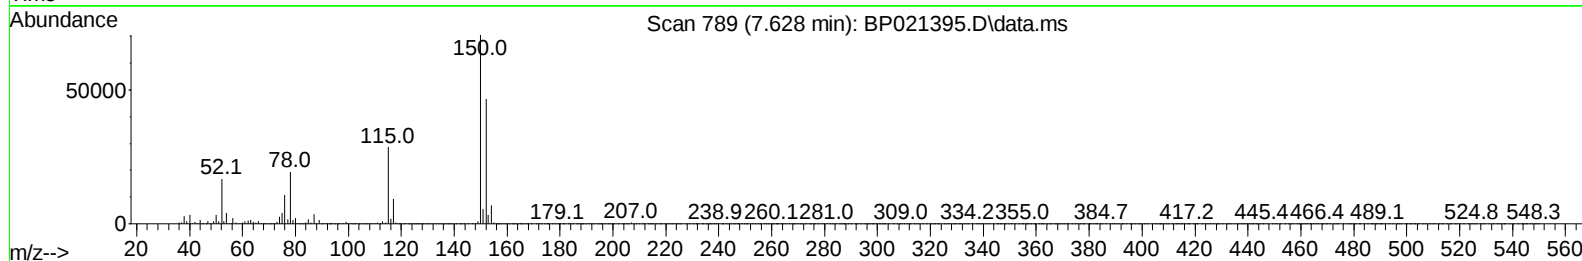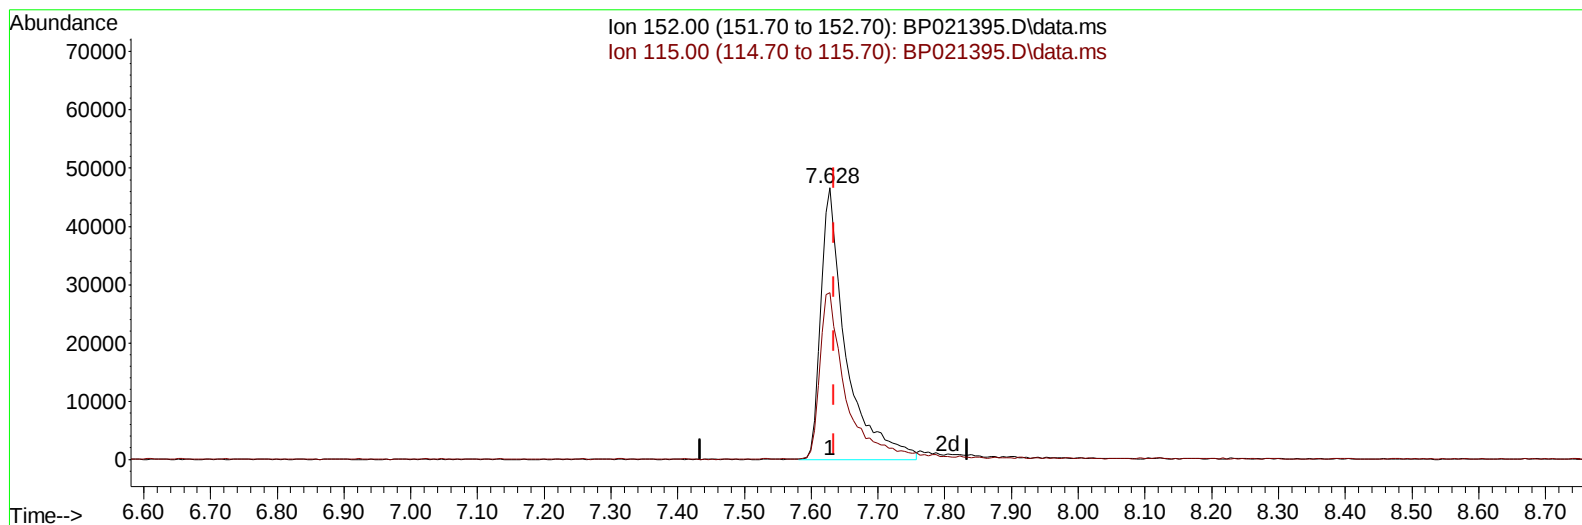

TIC: BP021395.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.628min (-0.006) 20.00 ng/u1 m

response 121966

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	62.30	61.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021395.D
 Acq On : 06 Aug 2024 17:44
 Operator : CG/JU
 Sample : P3456-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/07/2024
 Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 06 23:36:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	121966m	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	471397	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	322014	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	718946	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	796598	20.000	ng/ul	0.00
88) Perylene-d12	24.816	264	939967	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021395.D
Acq On : 06 Aug 2024 17:44
Operator : CG/JU
Sample : P3456-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 06 23:36:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

