




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:43:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

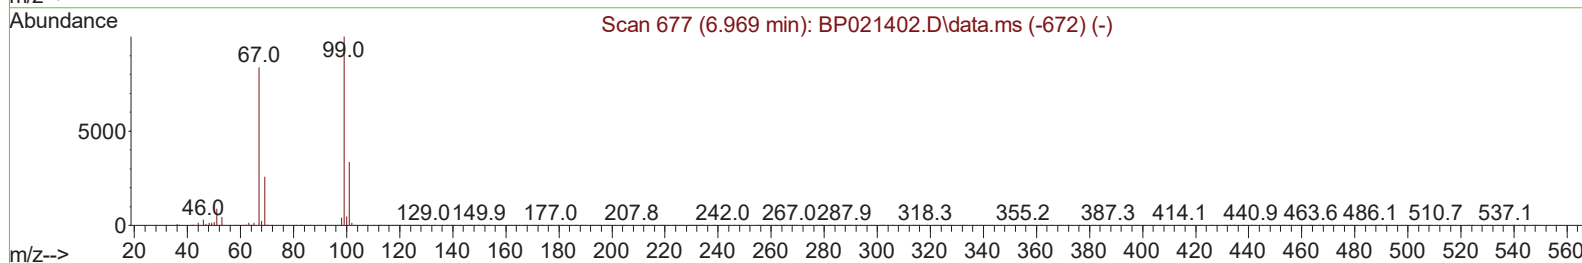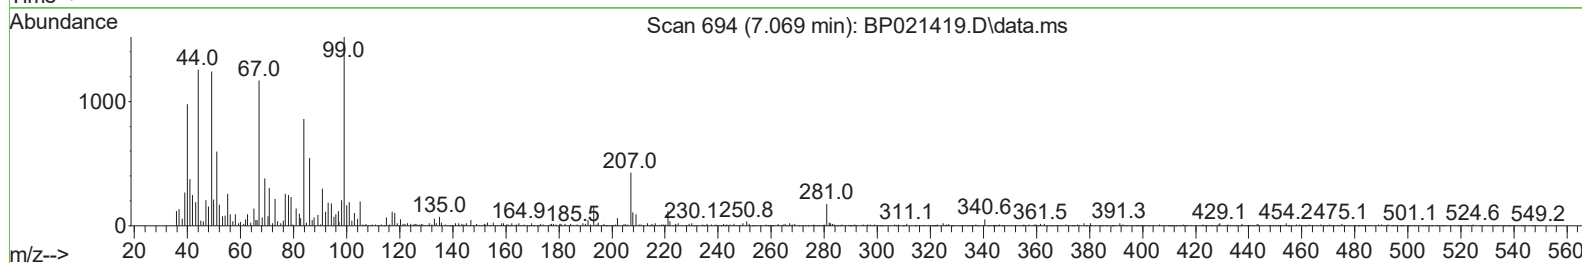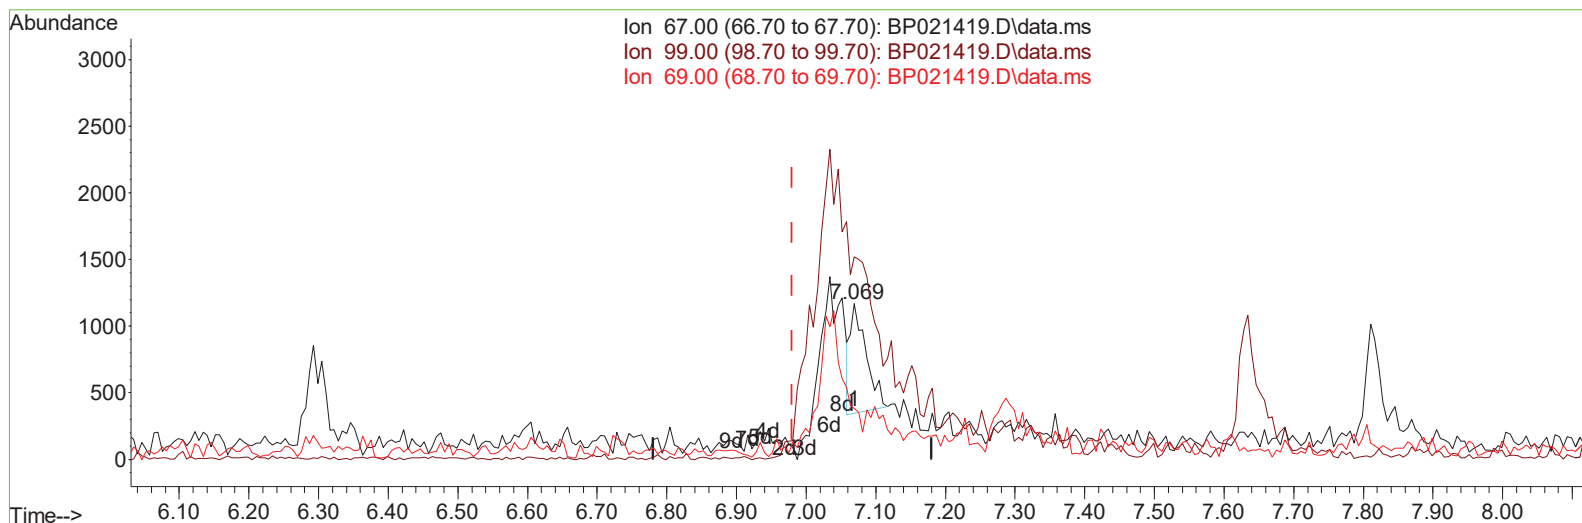

TIC: BP021419.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.069min (+ 0.089) 0.18 ng/u1

response 1310

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	122.50	129.97
69.00	30.60	32.71
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021419.D
 Acq On : 07 Aug 2024 14:03
 Operator : CG/JU
 Sample : P3329-17DL2 30X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:43:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

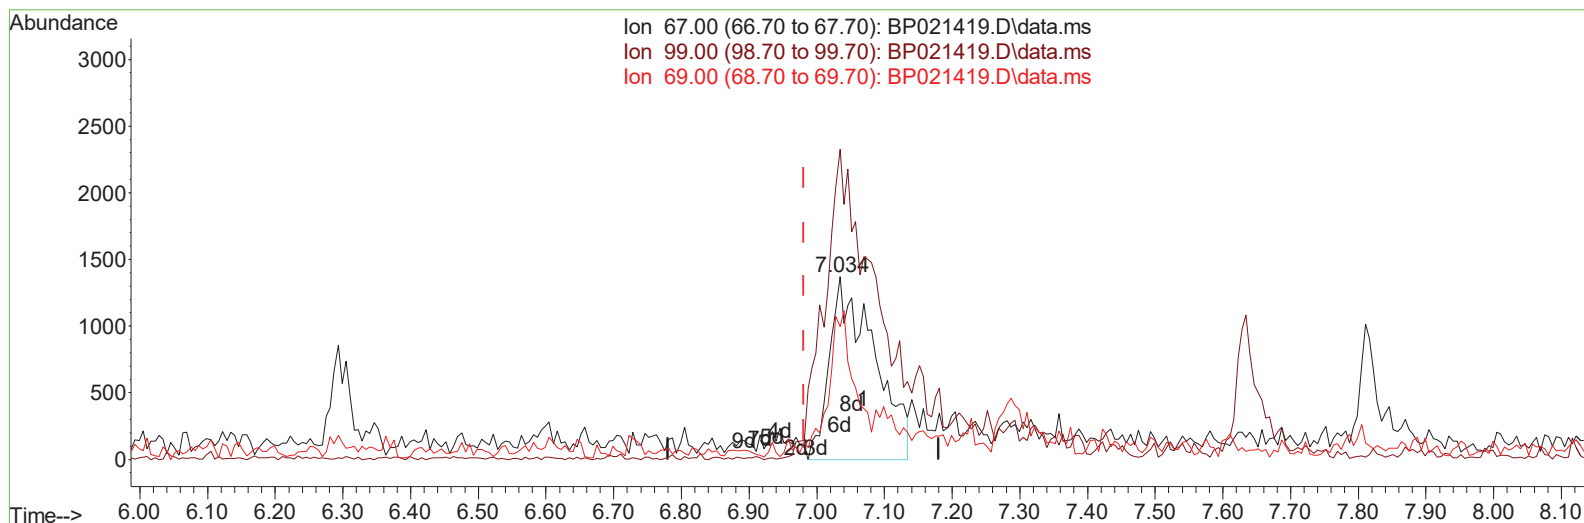




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:43:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

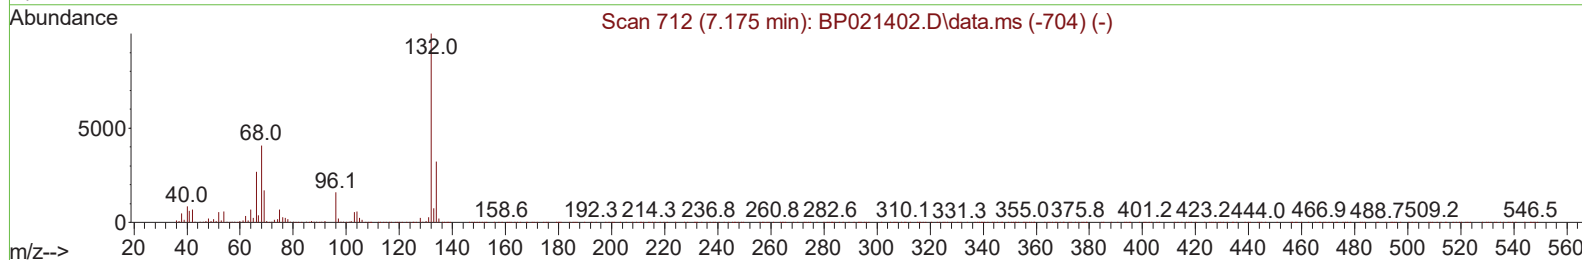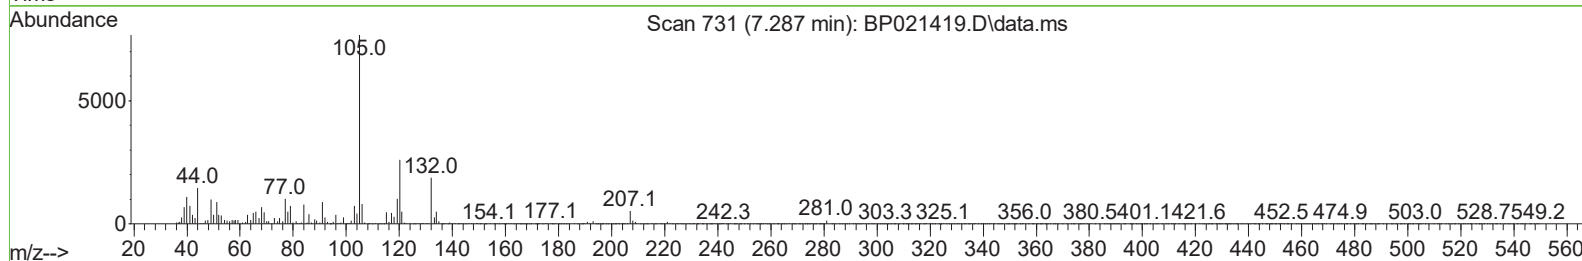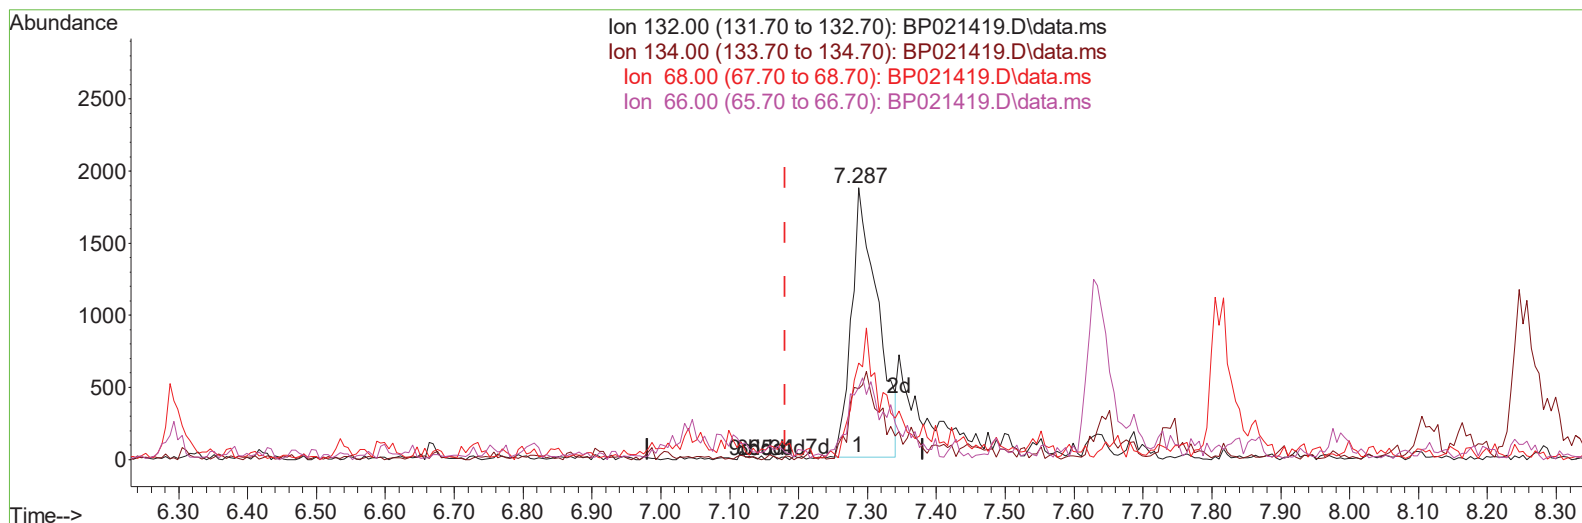

TIC: BP021419.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.287min (+ 0.106) 0.49 ng/u1

response 4888

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.30	26.02
68.00	39.60	35.48
66.00	27.60	26.66




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:43:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

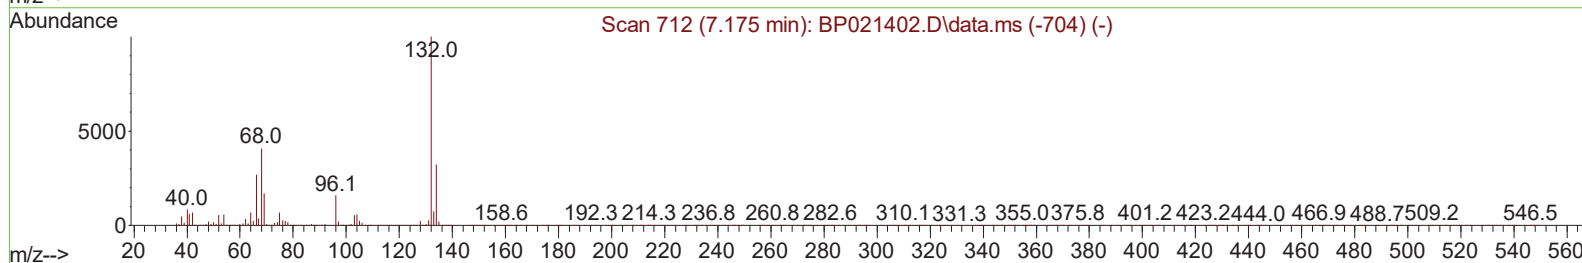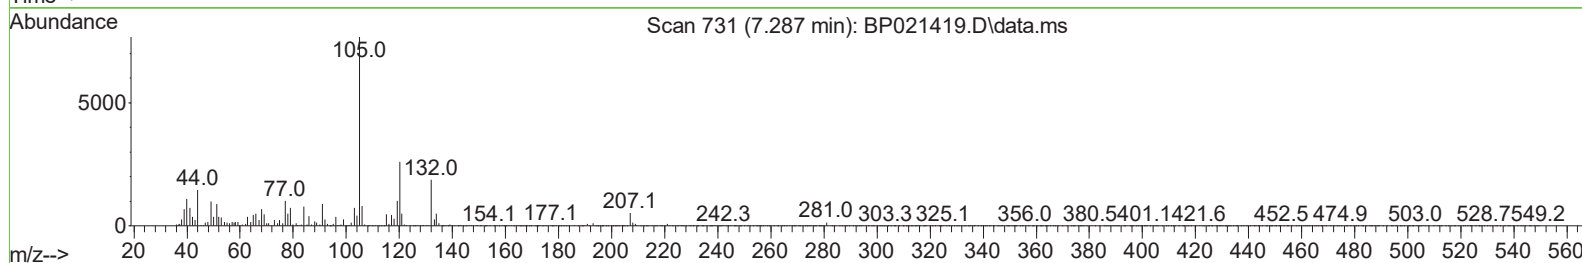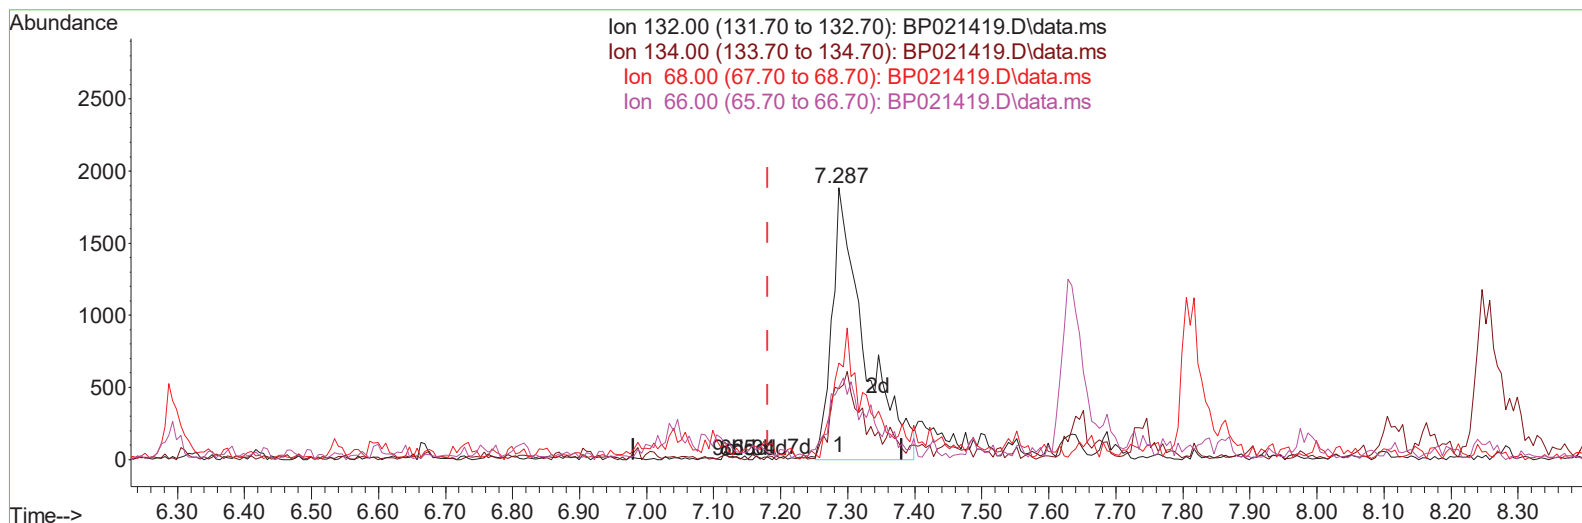

TIC: BP021419.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.287min (+ 0.106) 0.63 ng/ul m

response 6289

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.30	26.02
68.00	39.60	35.48
66.00	27.60	26.66




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:15:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

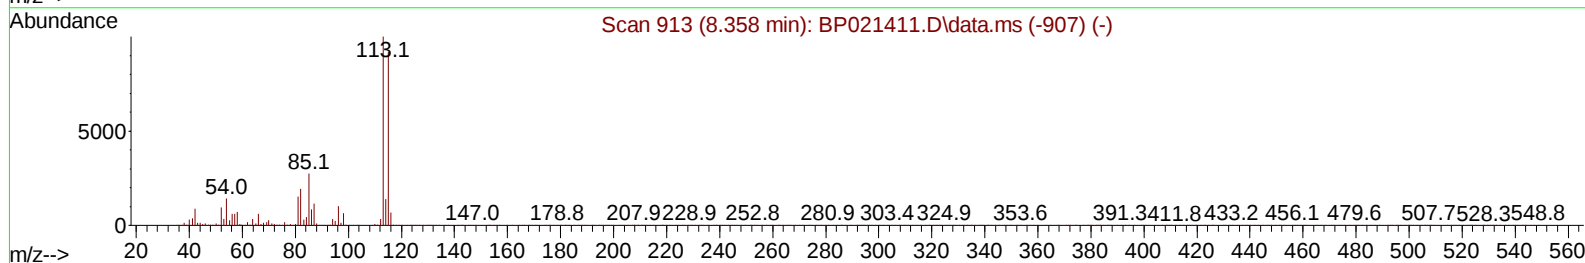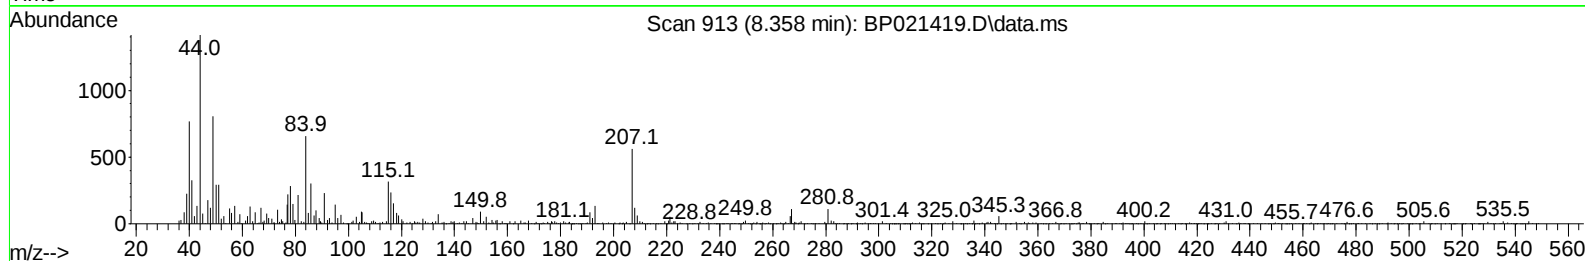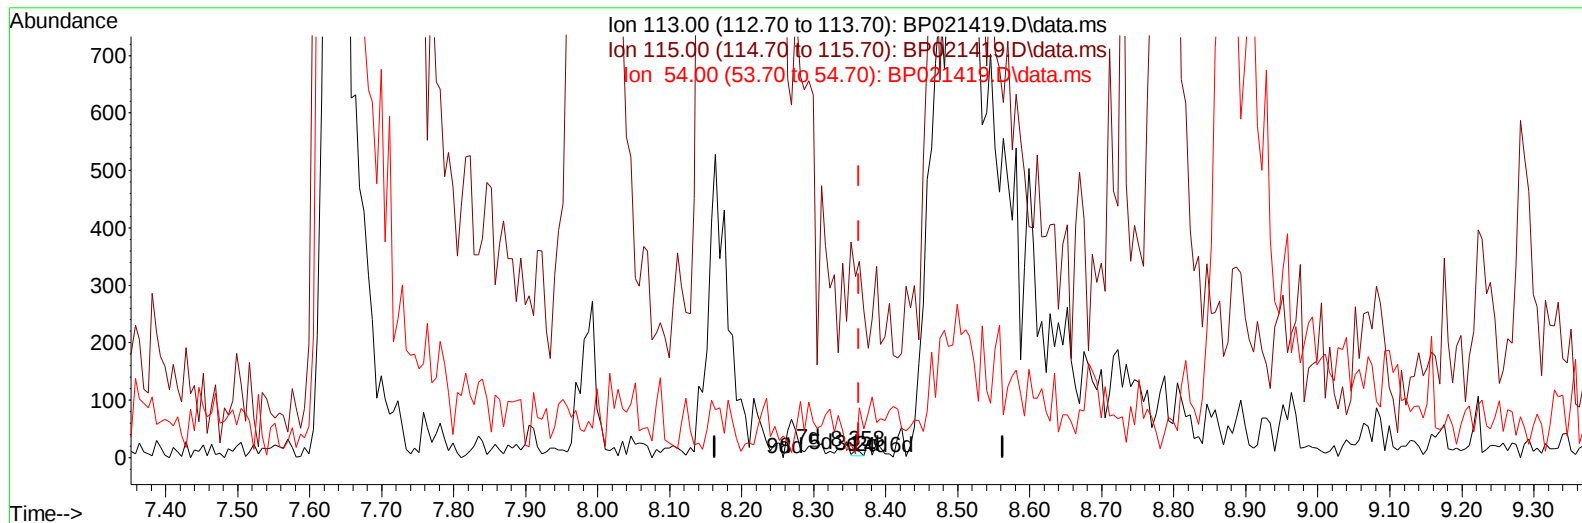

TIC: BP021419.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.358min (-0.005) 0.00 ng/u1

response 6

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	2423.08#
54.00	13.70	46.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:47:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

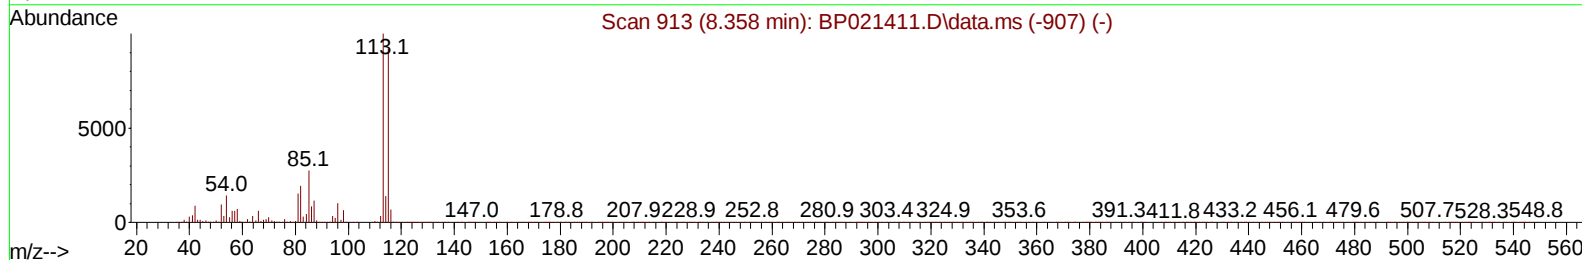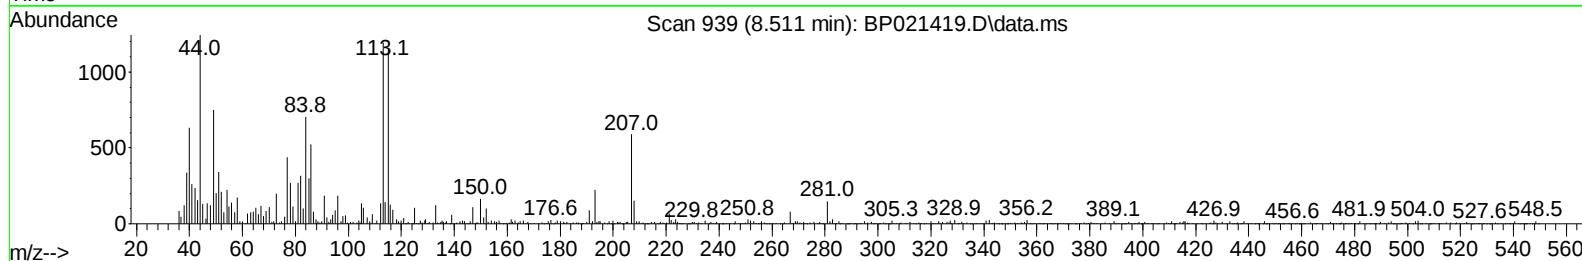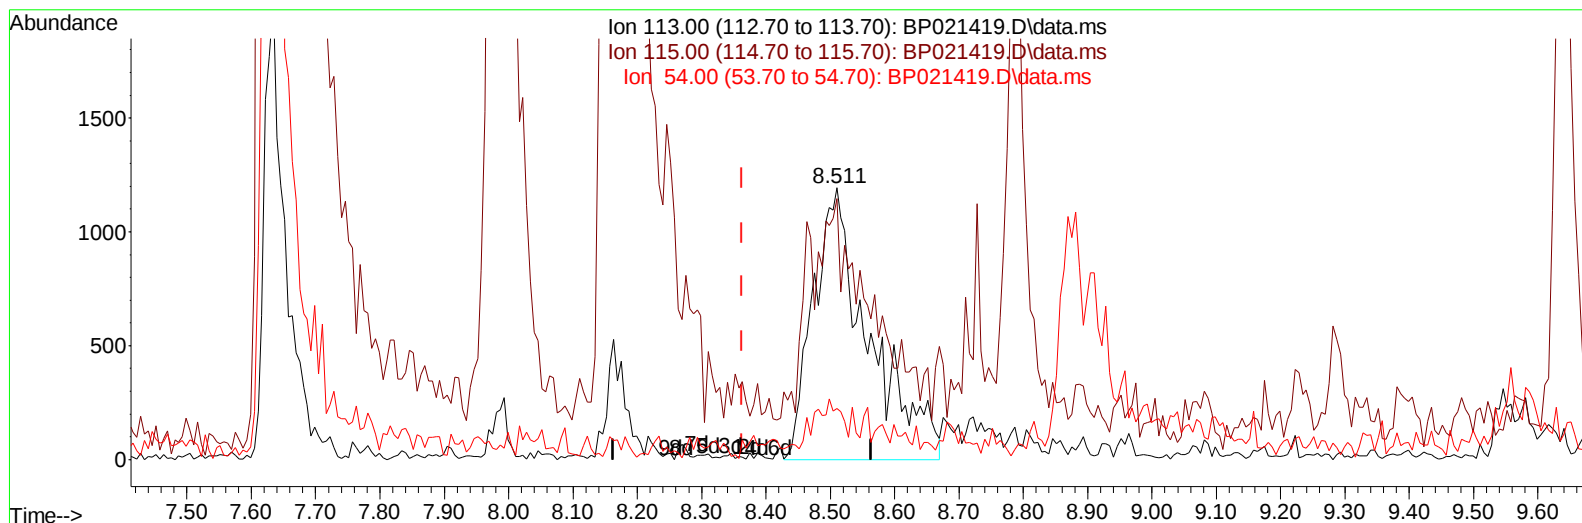

TIC: BP021419.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.511min (+ 0.148) 0.71 ng/ul m

response 7134

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	96.14
54.00	13.70	18.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:15:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

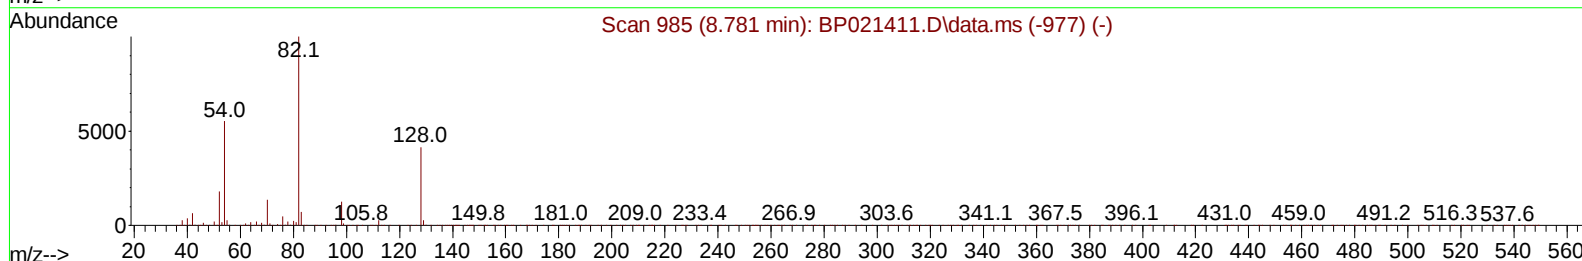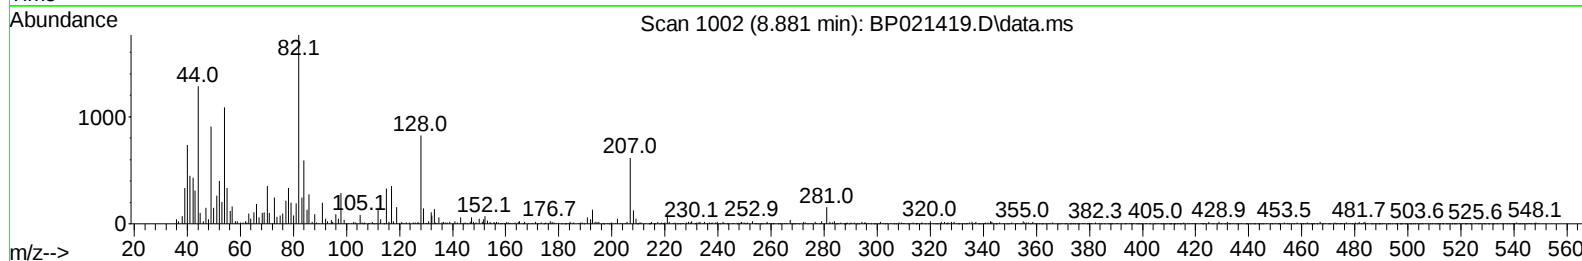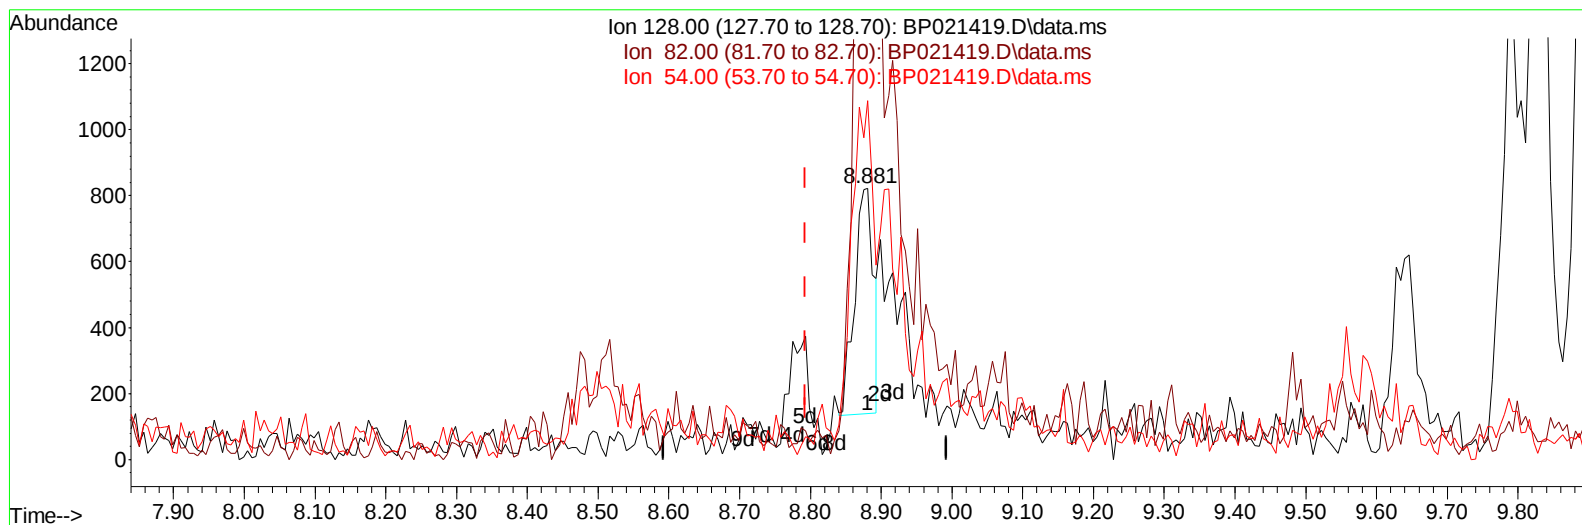

TIC: BP021419.D\data.ms

(21) Nitrobenzene-d5 (S)

8.881min (+ 0.089) 0.25 ng/u1

response 1269

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	214.34
54.00	125.70	132.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:47:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

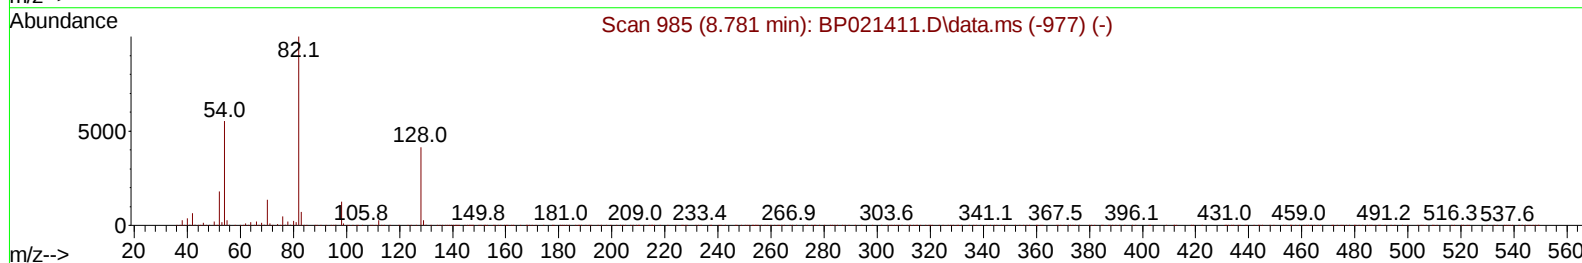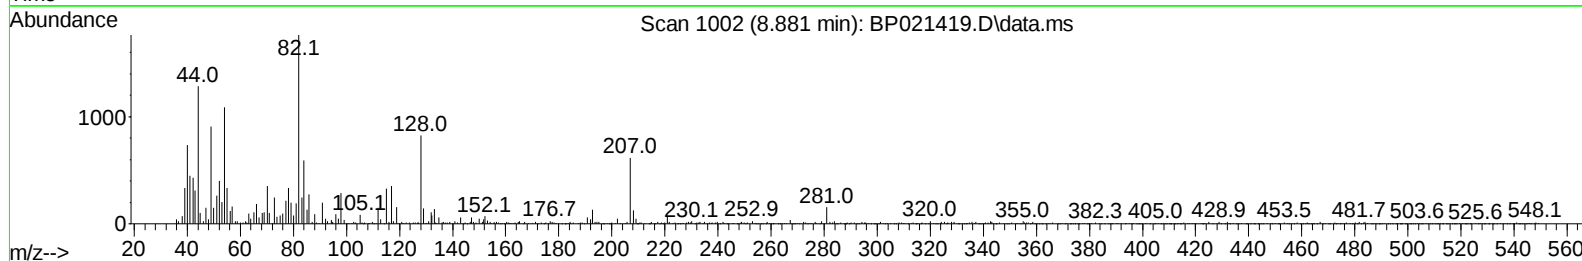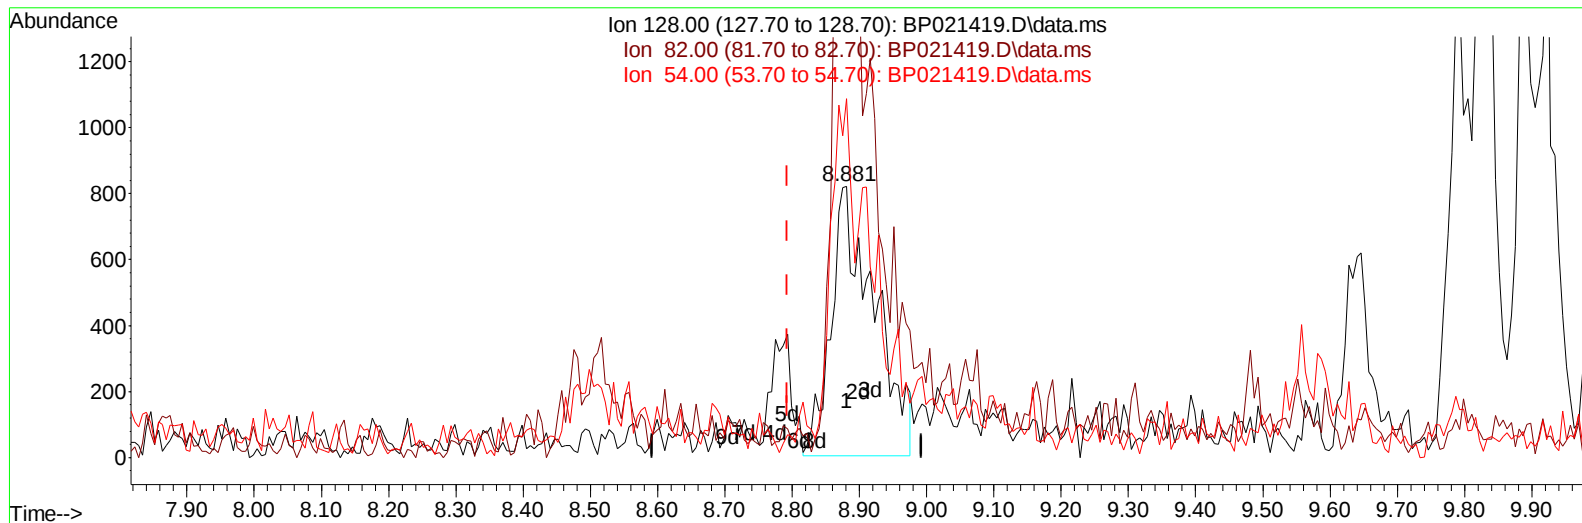

TIC: BP021419.D\data.ms

(21) Nitrobenzene-d5 (S)

8.881min (+ 0.089) 0.71 ng/ul m

response 3636

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	214.34
54.00	125.70	132.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:15:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

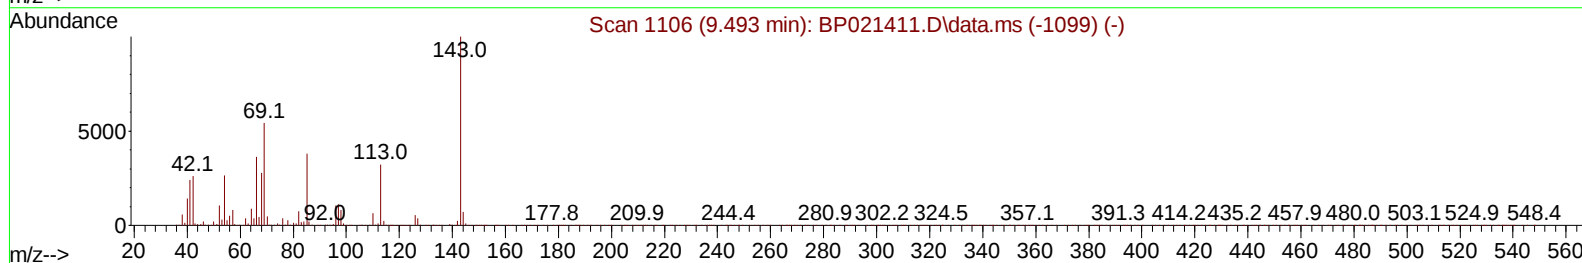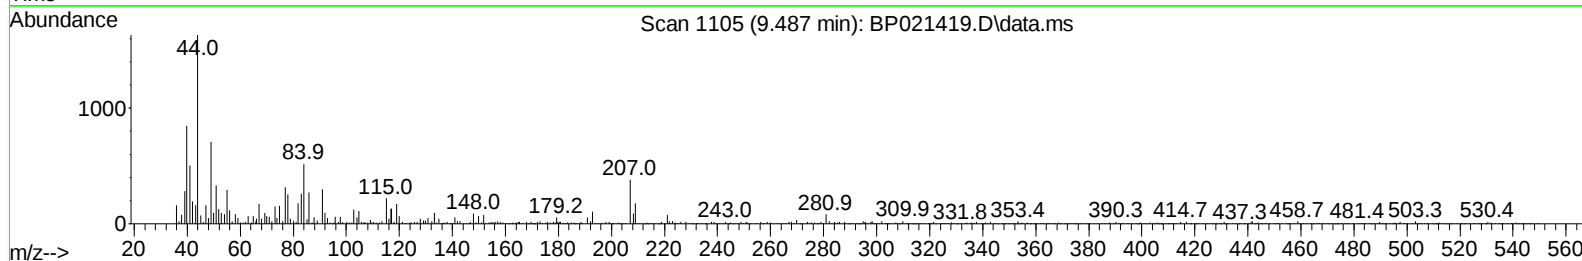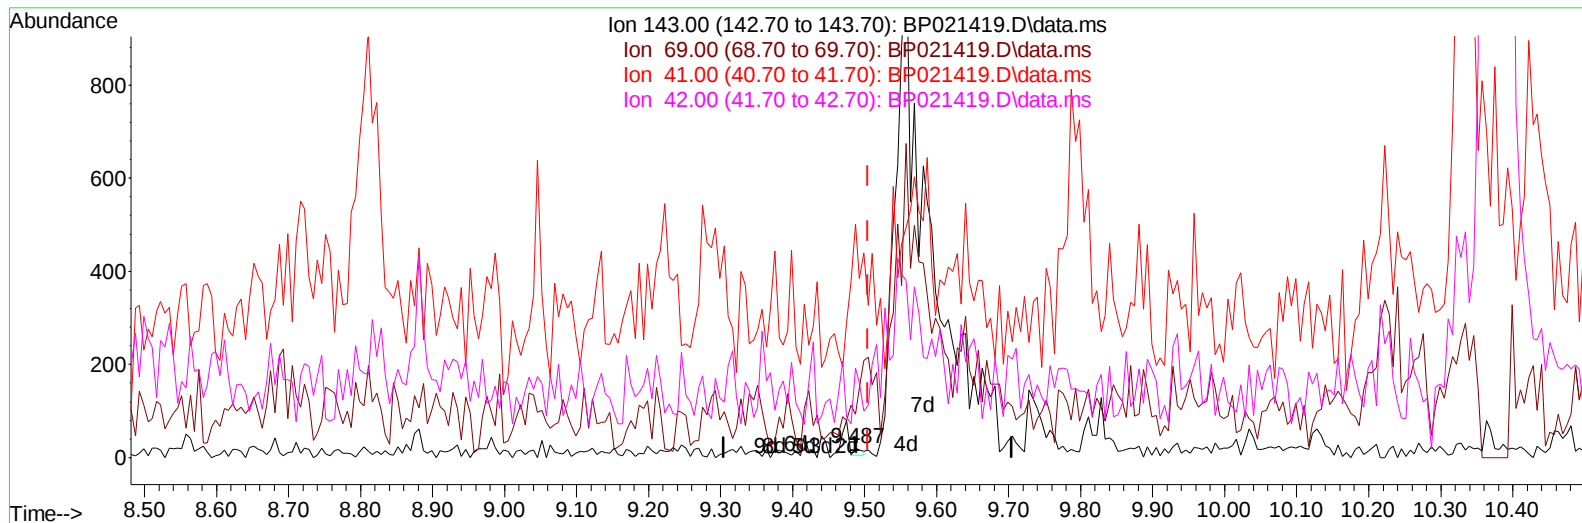

TIC: BP021419.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.487min (-0.017) 0.00 ng/u1

response 13

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	442.86#
41.00	22.70	2385.71#
42.00	22.10	914.29#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:47:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

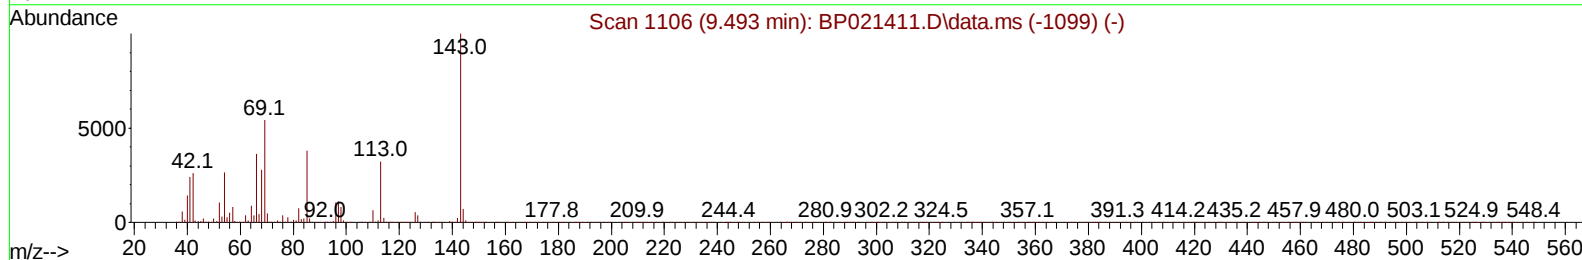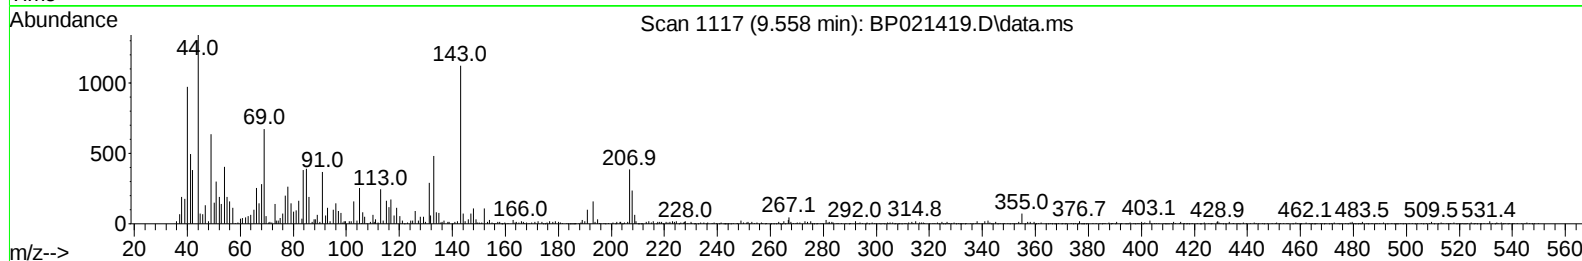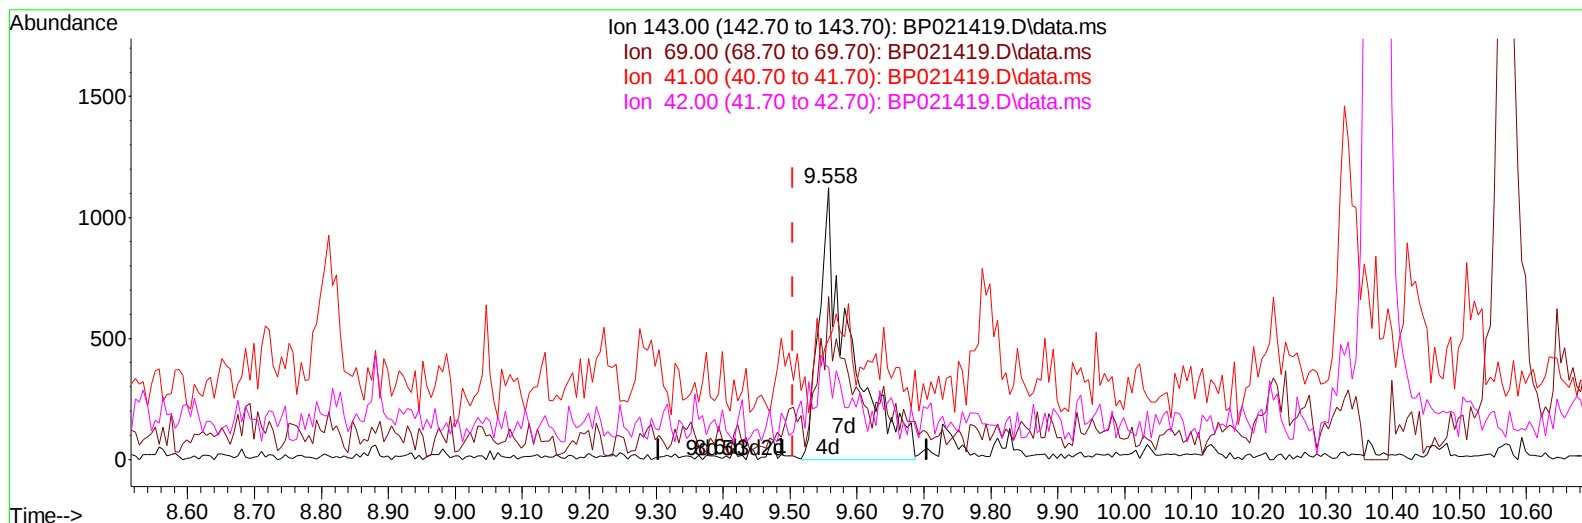

TIC: BP021419.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.558min (+ 0.053) 0.62 ng/ul m

response 3620

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	60.07
41.00	22.70	44.12#
42.00	22.10	33.96#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:15:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

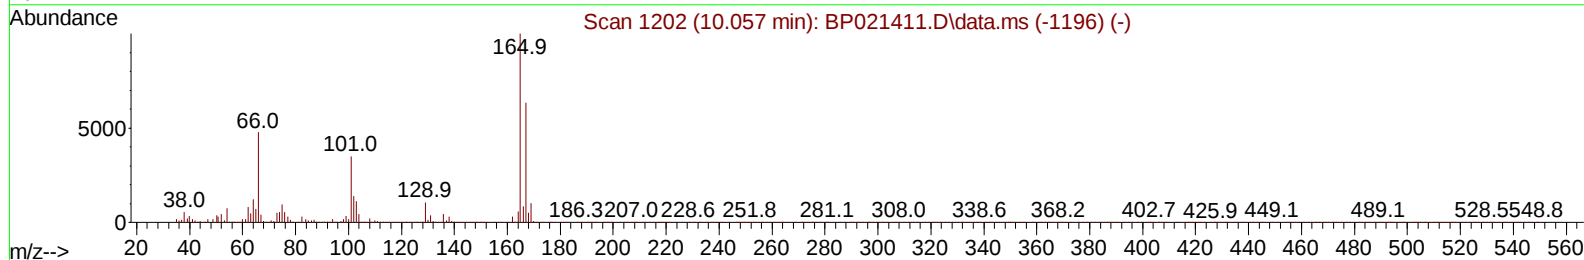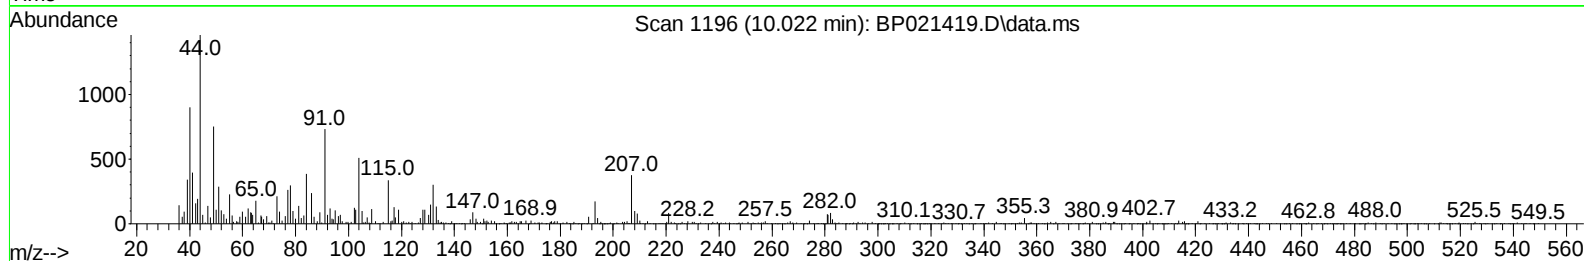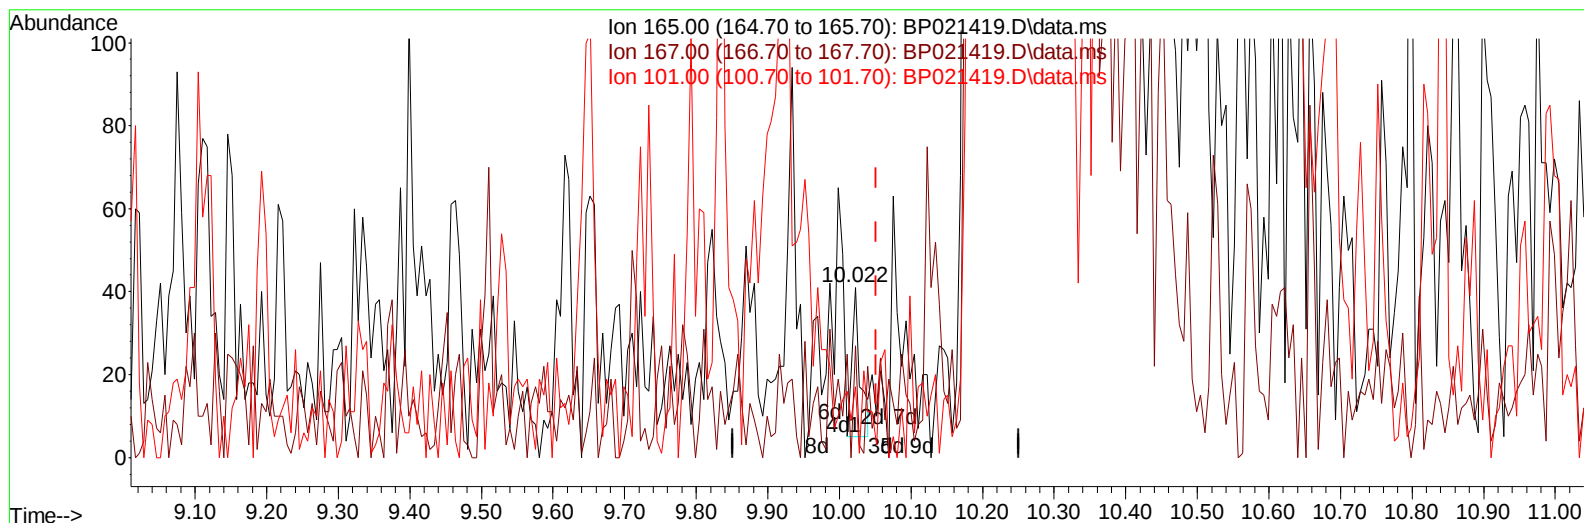

TIC: BP021419.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.022min (-0.029) 0.00 ng/u1

response 29

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	65.85
101.00	35.50	41.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:47:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

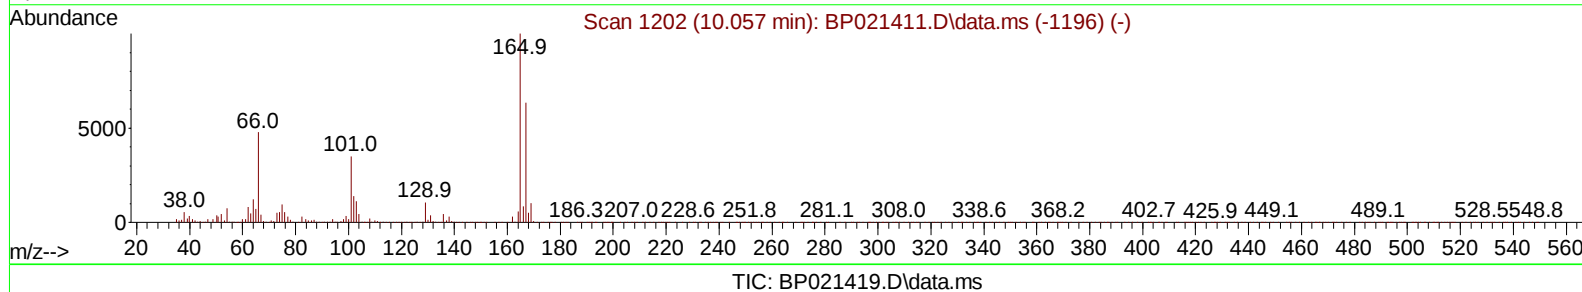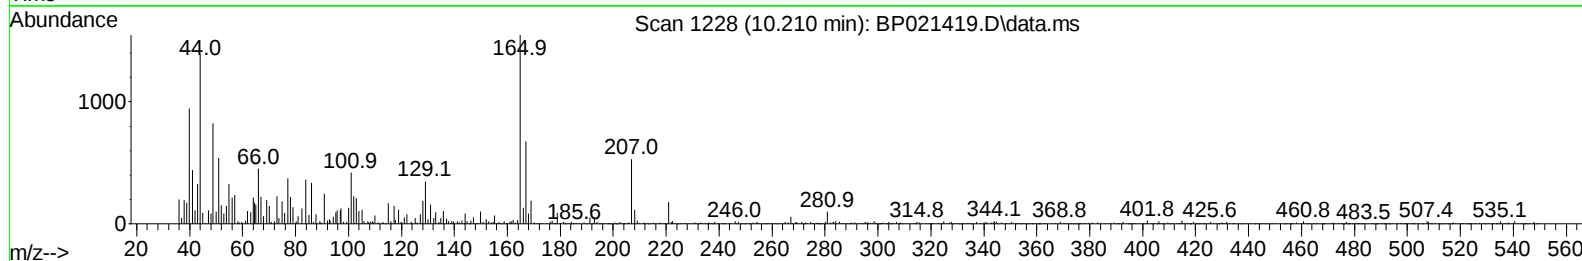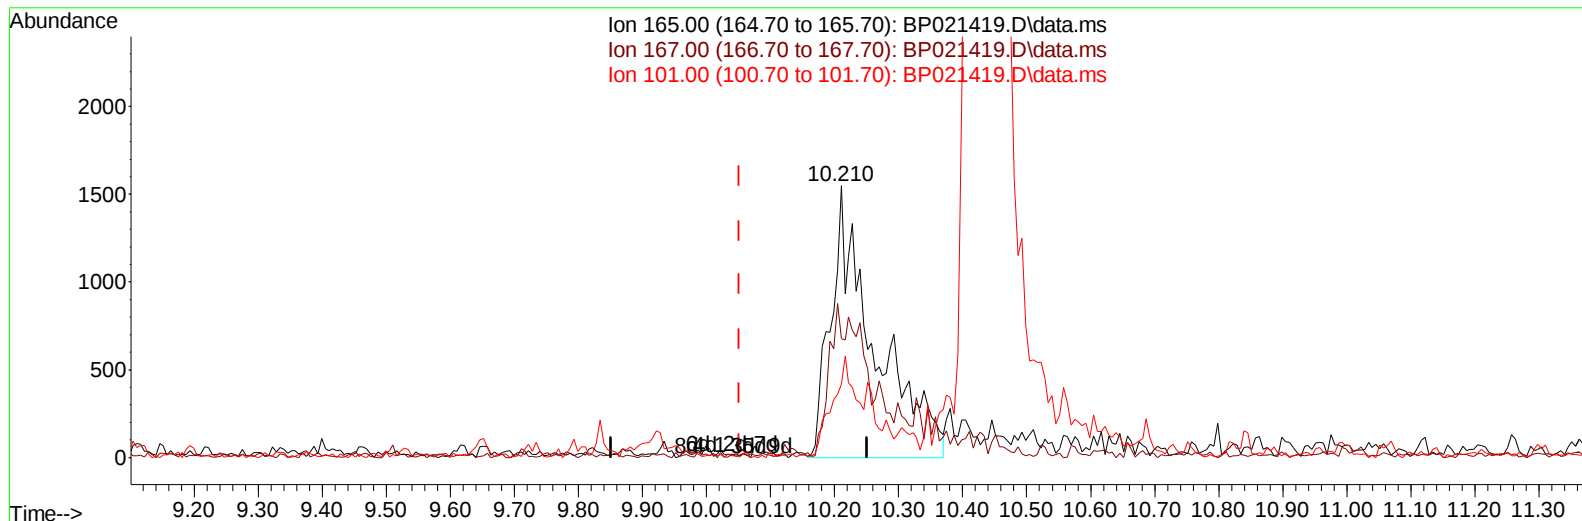

(28) 2,4-Dichlorophenol-d3 (S)

10.210min (+ 0.159) 0.69 ng/ul m

response 7224

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	43.67#
101.00	35.50	27.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 08 03:45:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

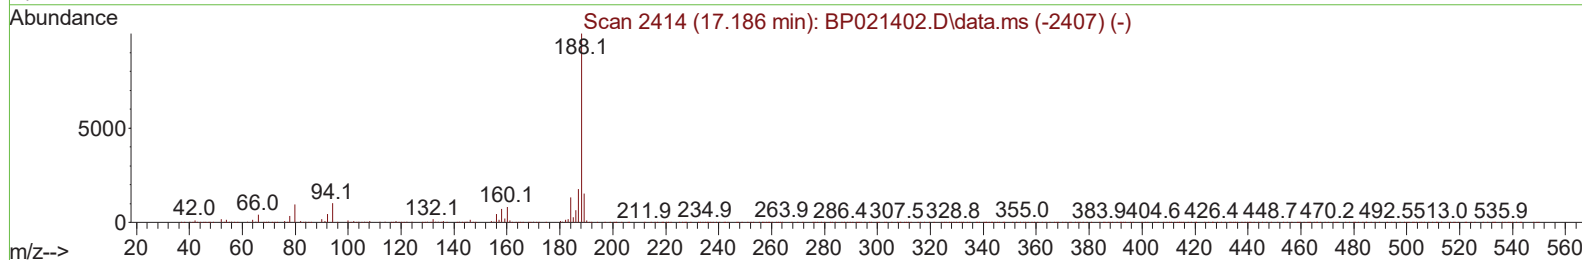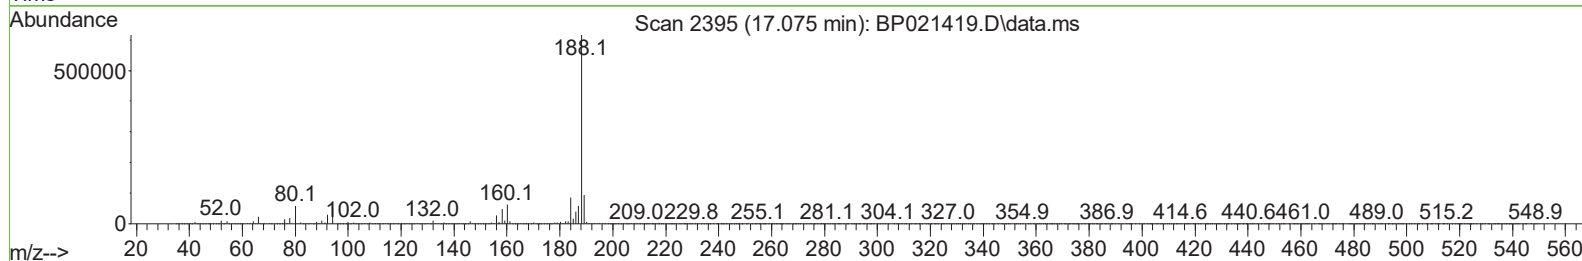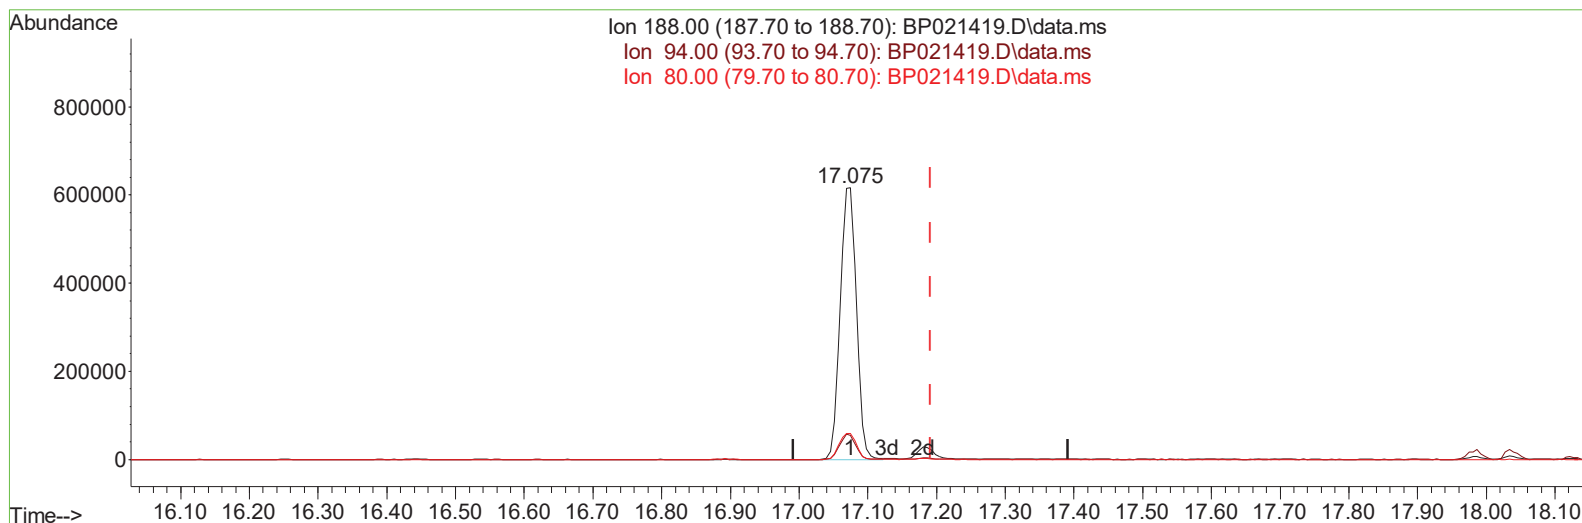

TIC: BP021419.D\data.ms

(73) Anthracene-d10 (S)

17.075min (-0.117) 22.51 ng/u1

response 1009123

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	8.76
80.00	9.20	9.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:45:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

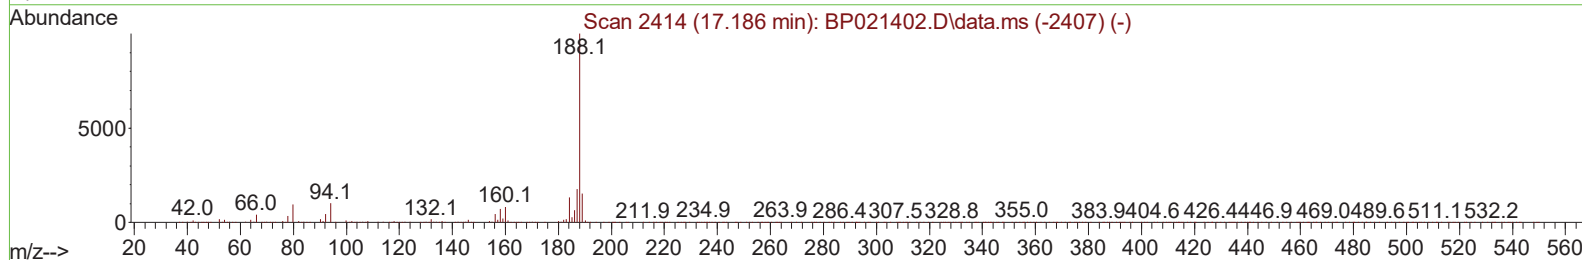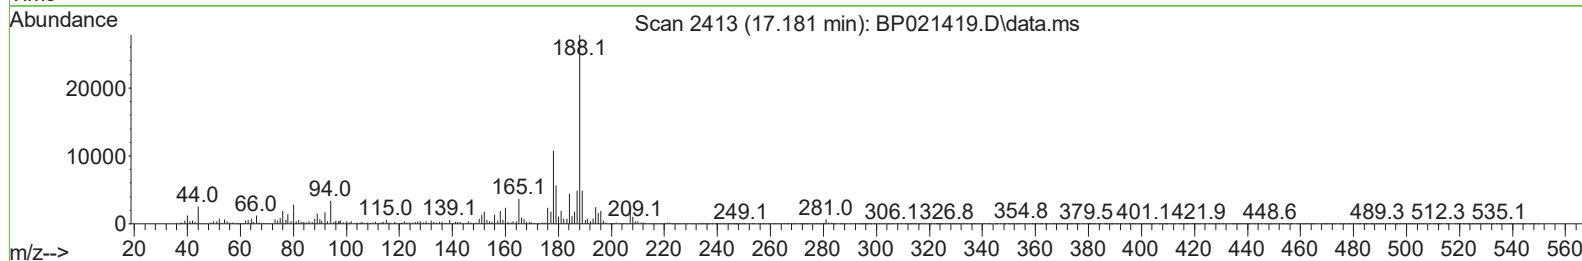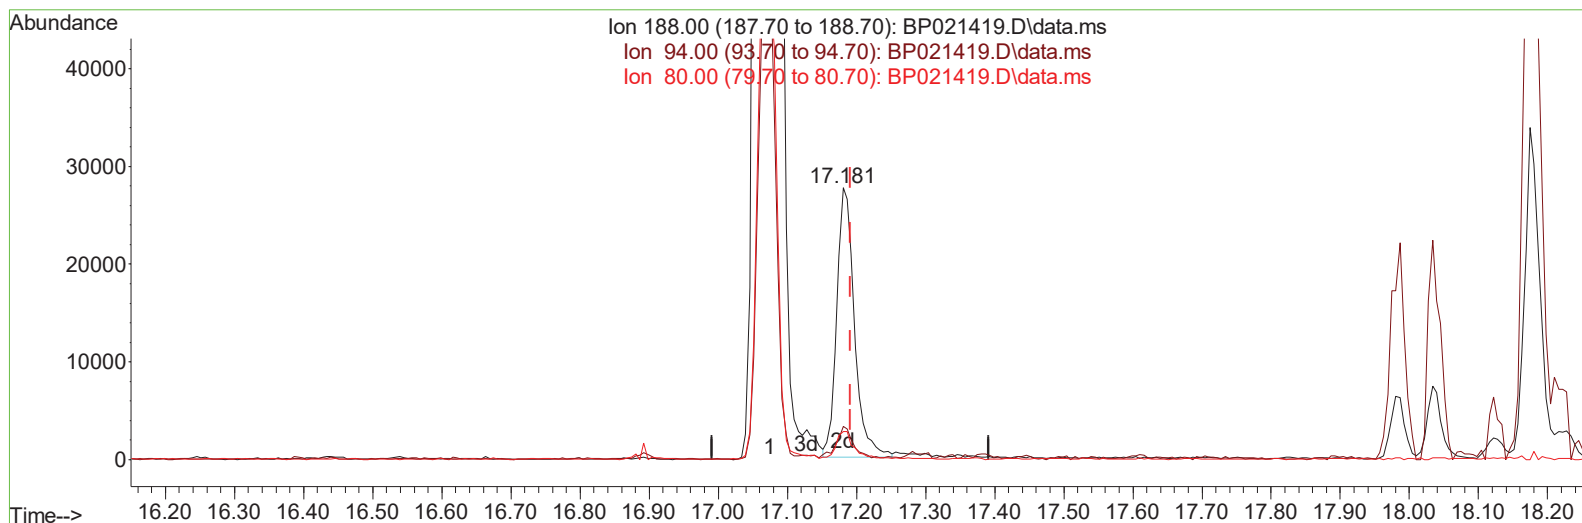

TIC: BP021419.D\data.ms

(73) Anthracene-d10 (S)

17.181min (-0.011) 1.10 ng/ul m

response 49188

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	12.27#
80.00	9.20	10.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:45:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

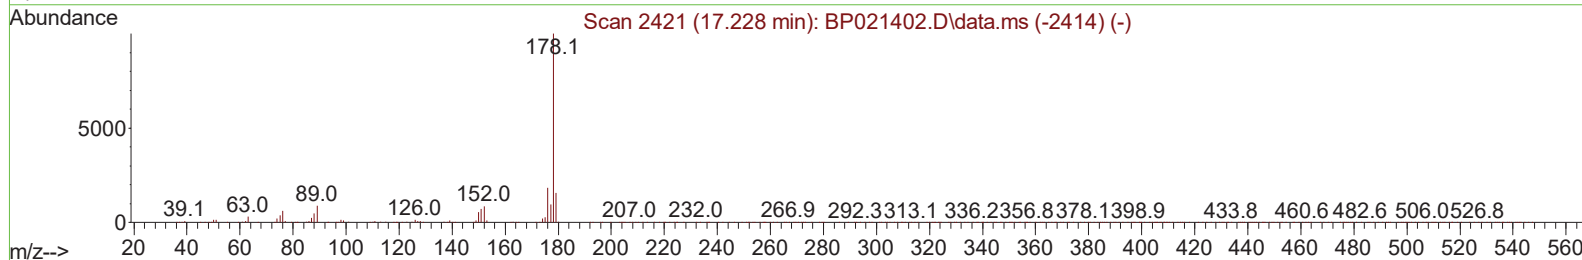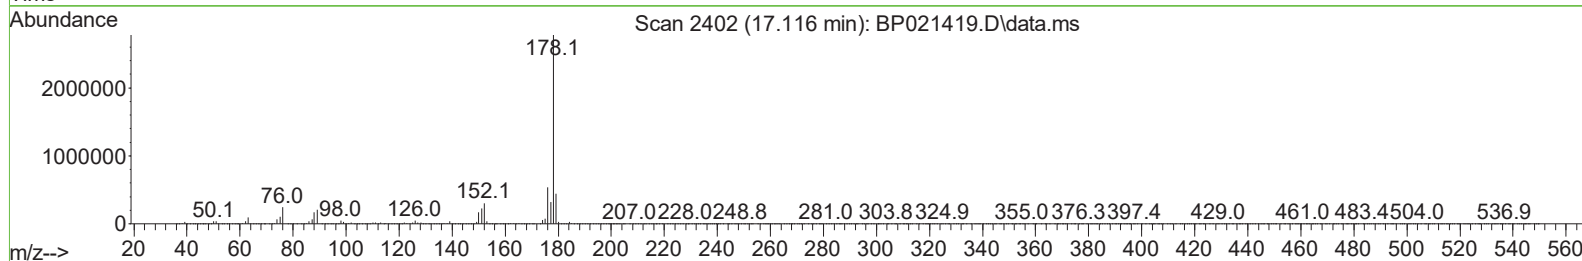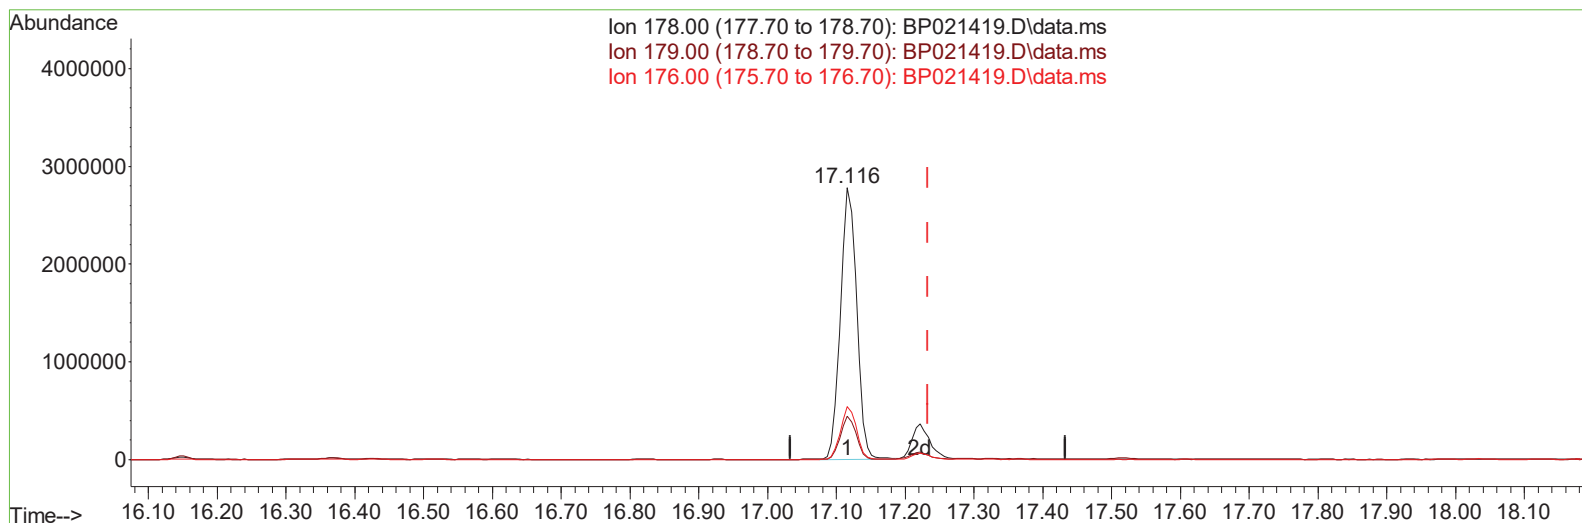

TIC: BP021419.D\data.ms

(74) Anthracene

17.116min (-0.117) 86.16 ng/u1

response 4598195

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.60	15.98
176.00	18.50	19.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:45:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

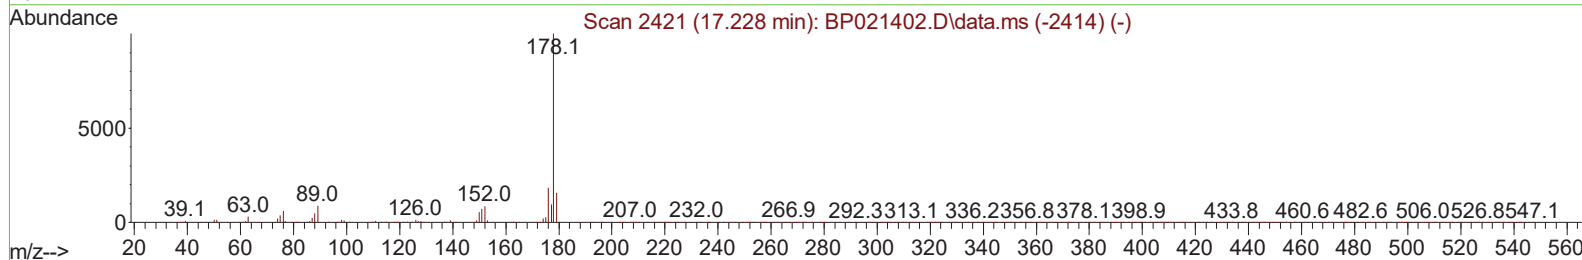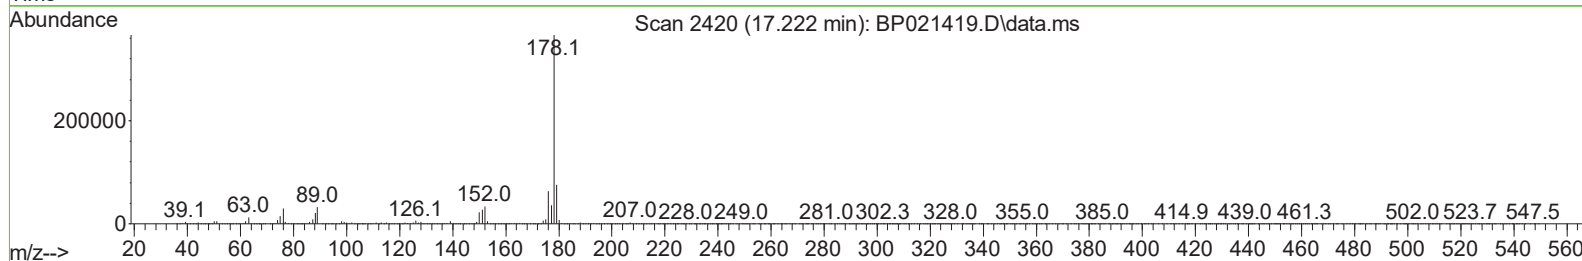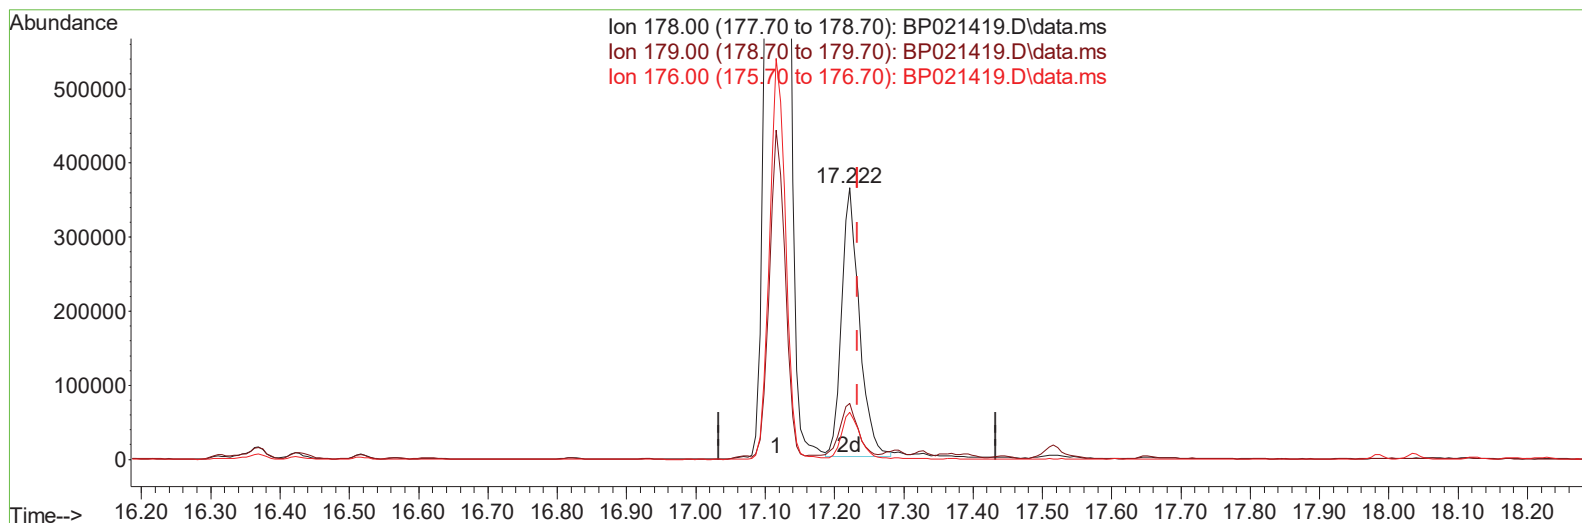

TIC: BP021419.D\data.ms

(74) Anthracene

17.222min (-0.011) 12.07 ng/u1 m

response 644192

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.60	20.73#
176.00	18.50	17.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021419.D
 Acq On : 07 Aug 2024 14:03
 Operator : CG/JU
 Sample : P3329-17DL2 30X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E25DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 08 03:47:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	148973	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	656012	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.257	164	444207	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.075	188	1009123	20.000	ng/ul	-0.02
79) Chrysene-d12	21.516	240	1107425	20.000	ng/ul	-0.02
88) Perylene-d12	24.810	264	1299748	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	7.034	67	6278m	0.853	ng/ul	0.05
11) 2-Chlorophenol-d4	7.287	132	6289m	0.628	ng/ul	0.11
15) 4-Methylphenol-d8	8.511	113	7134m	0.707	ng/ul	0.15
21) Nitrobenzene-d5	8.881	128	3636m	0.714	ng/ul	0.09
24) 2-Nitrophenol-d4	9.558	143	3620m	0.621	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.210	165	7224m	0.685	ng/ul	0.16
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	13.681	166	30594	0.947	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	31304	0.863	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.281	176	28589	1.079	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.181	188	49188m	1.097	ng/ul	-0.01
81) Pyrene-d10	19.563	212	54642	0.798	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.598	264	41283	0.644	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.434	128	3710558	107.531	ng/ul	100
36) 2-Methylnaphthalene	12.052	142	763807	32.246	ng/ul	99
37) 1-Methylnaphthalene	12.275	142	345456	14.181	ng/ul	98
43) 1,1'-Biphenyl	13.093	154	193883	5.972	ng/ul	99
50) Acenaphthylene	13.987	152	50713	1.235	ng/ul#	92
52) Acenaphthene	14.328	153	882143	32.375	ng/ul	98
56) Dibenzofuran	14.675	168	961366	25.765	ng/ul	98
61) Fluorene	15.334	166	1023006	33.598	ng/ul	100
72) Phenanthrene	17.116	178	4592187	87.722	ng/ul	98
74) Anthracene	17.222	178	644192m	12.071	ng/ul	
77) Carbazole	17.528	167	278198	6.377	ng/ul	98
80) Fluoranthene	19.216	202	3045667	36.836	ng/ul	100
82) Pyrene	19.592	202	1685078	20.028	ng/ul	99
85) Benzo(a)anthracene	21.498	228	768607	9.908	ng/ul	98
87) Chrysene	21.569	228	577830	8.016	ng/ul	99
90) Benzo(b)fluoranthene	23.780	252	497223	6.304	ng/ul	98
91) Benzo(k)fluoranthene	23.845	252	179449	2.280	ng/ul	96
93) Benzo(a)pyrene	24.668	252	156984	2.106	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021419.D
Acq On : 07 Aug 2024 14:03
Operator : CG/JU
Sample : P3329-17DL2 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E25DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:47:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

