




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:35:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

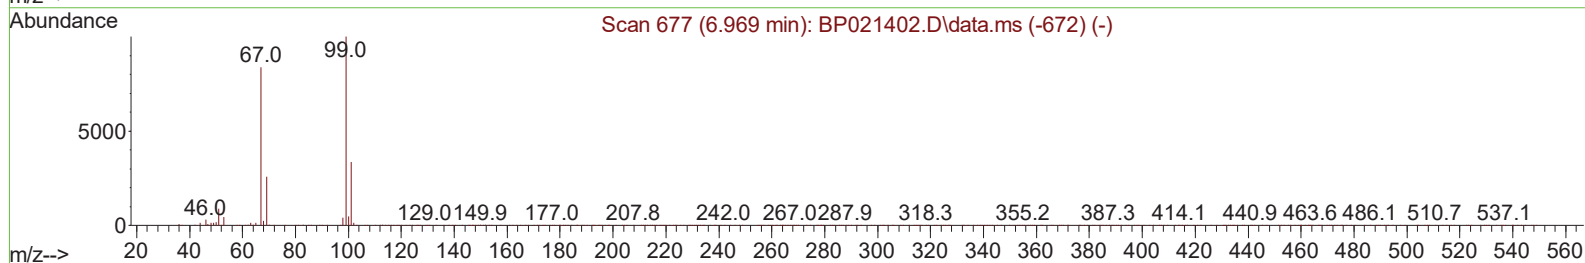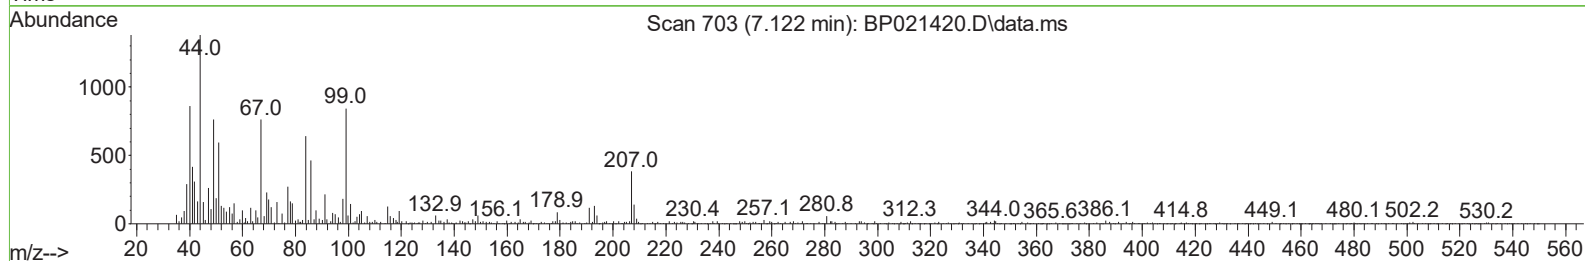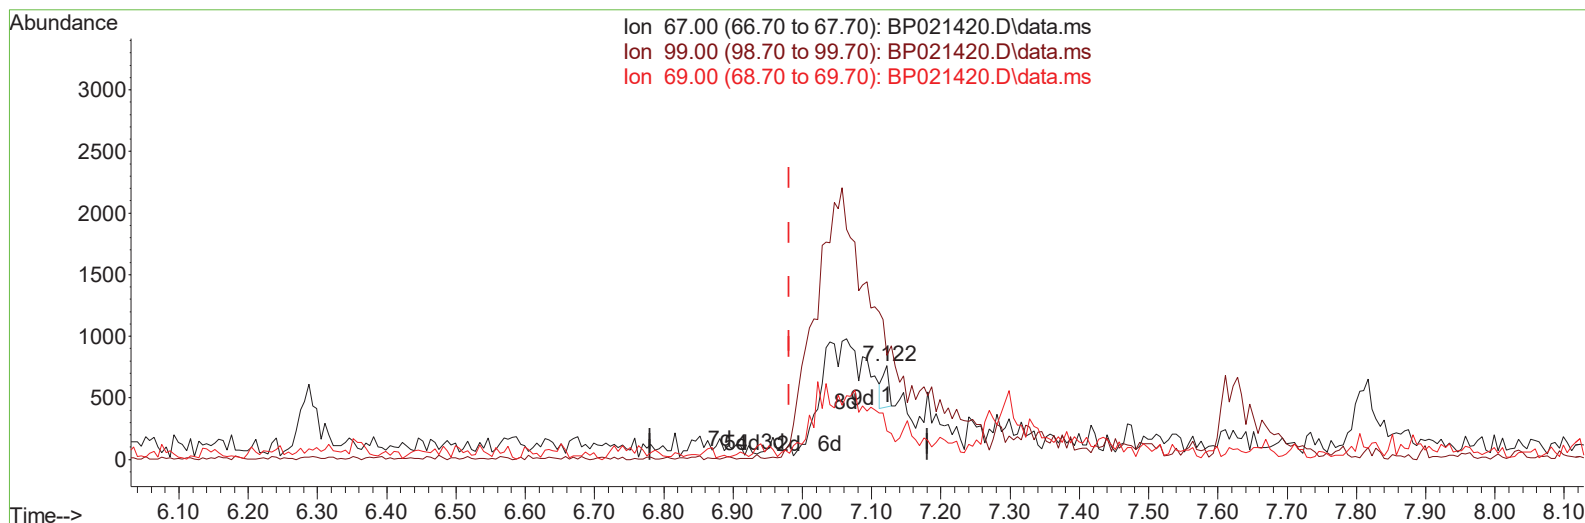

TIC: BP021420.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.122min (+ 0.142) 0.03 ng/u1

response 211

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	122.50	110.48
69.00	30.60	30.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021420.D
 Acq On : 07 Aug 2024 14:50
 Operator : CG/JU
 Sample : P3329-02DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:35:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

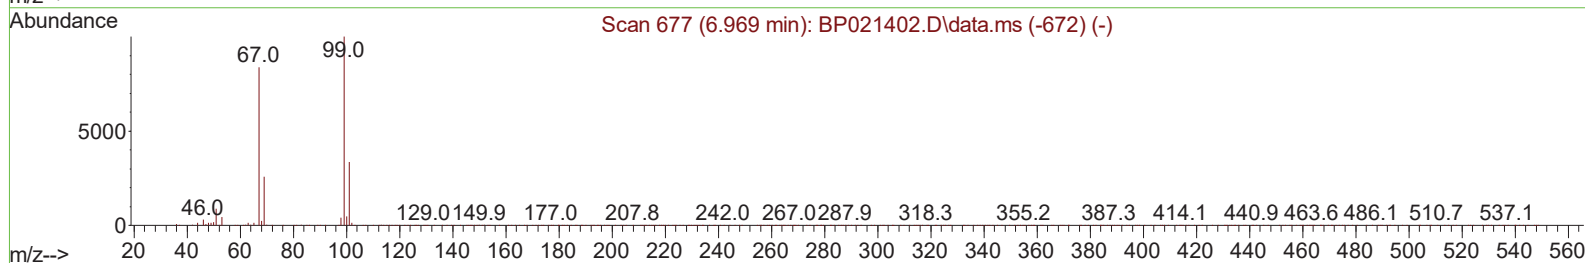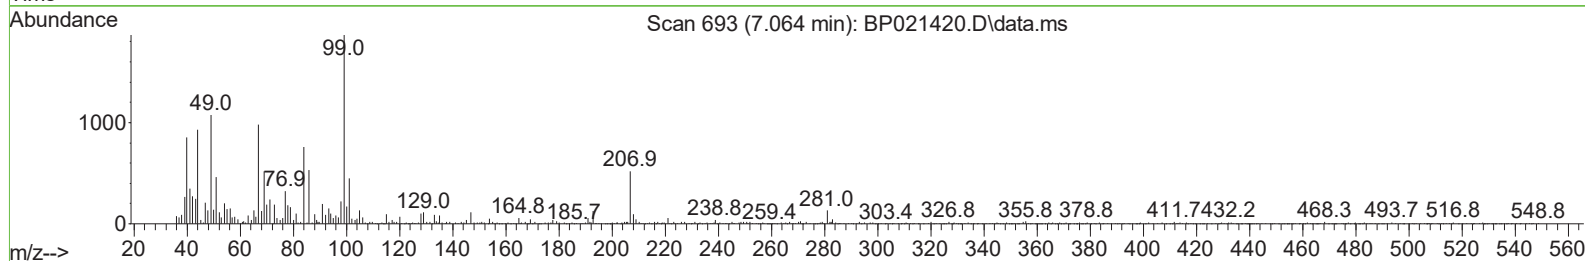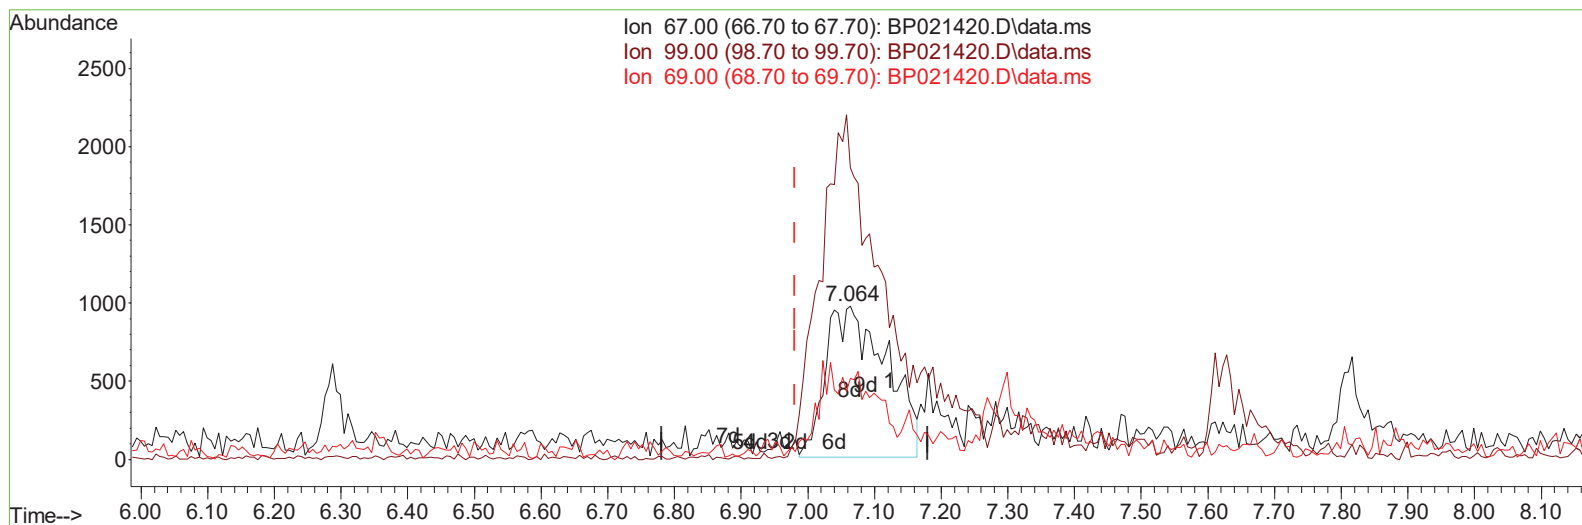

TIC: BP021420.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.064min (+ 0.083) 0.98 ng/u1 m

response 6106

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	122.50	190.21#
69.00	30.60	52.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:17:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

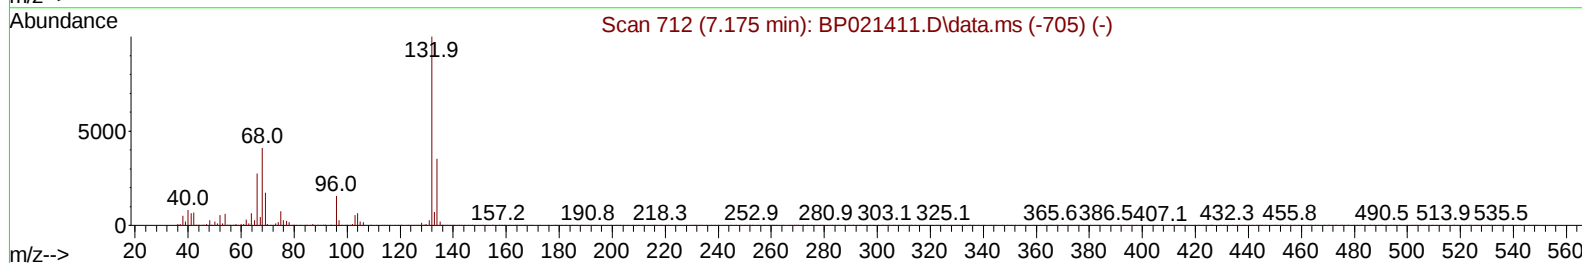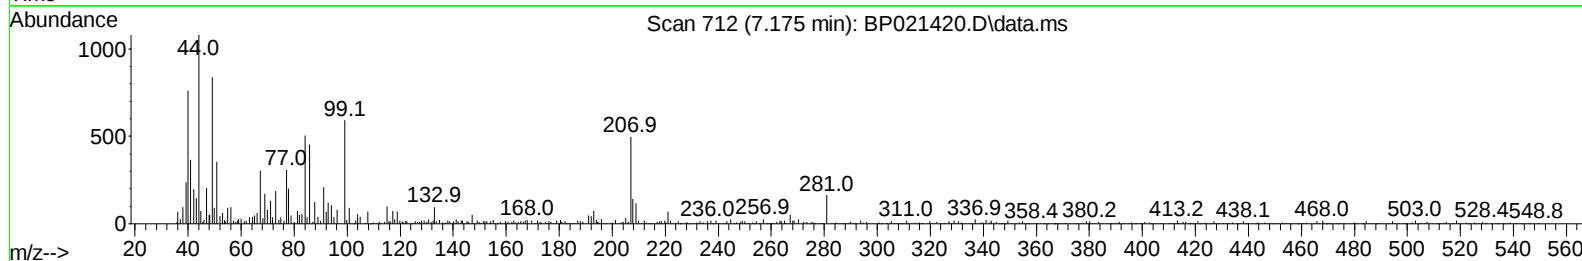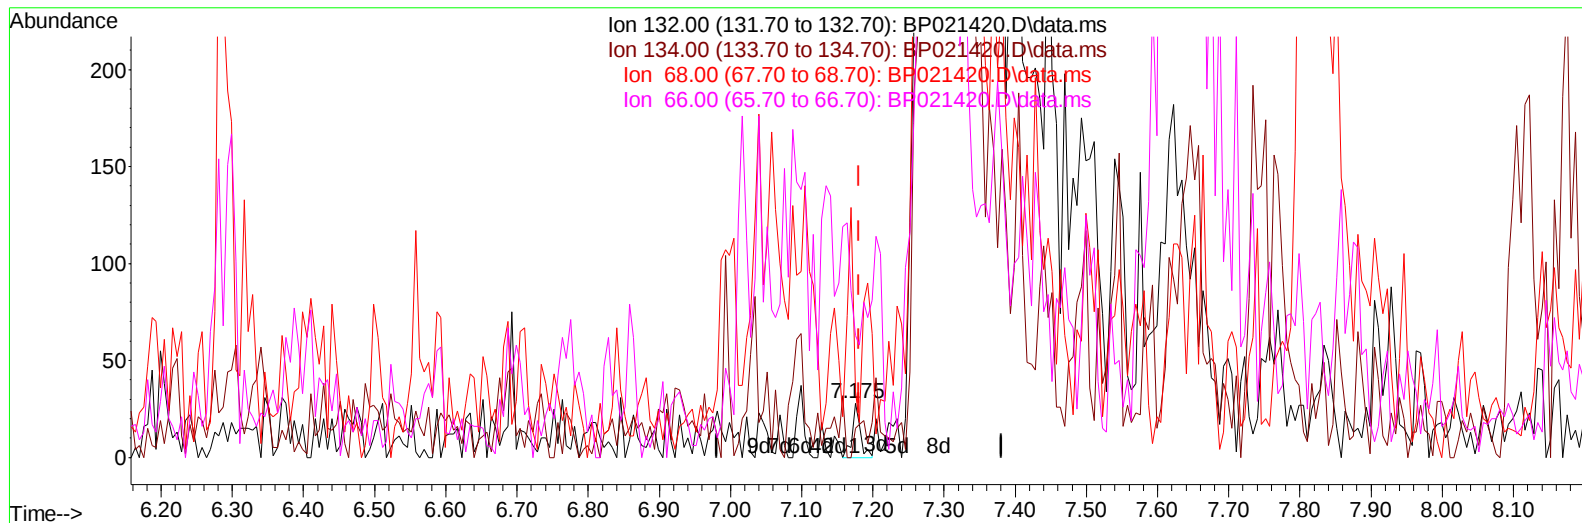

TIC: BP021420.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.175min (-0.005) 0.00 ng/u1

response 22

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.30	53.57#
68.00	39.60	121.43#
66.00	27.60	225.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:17:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

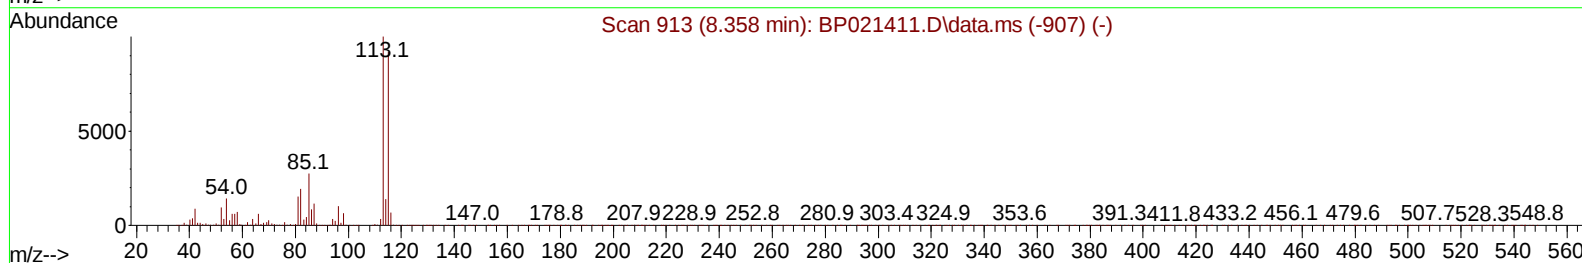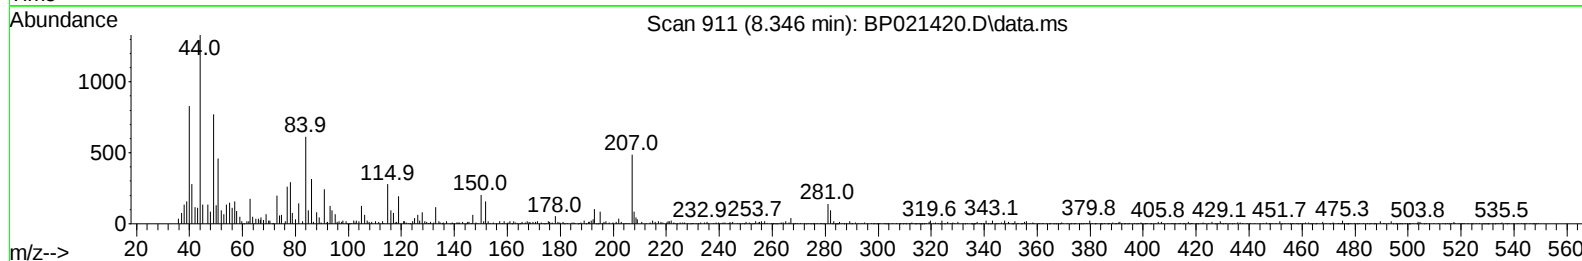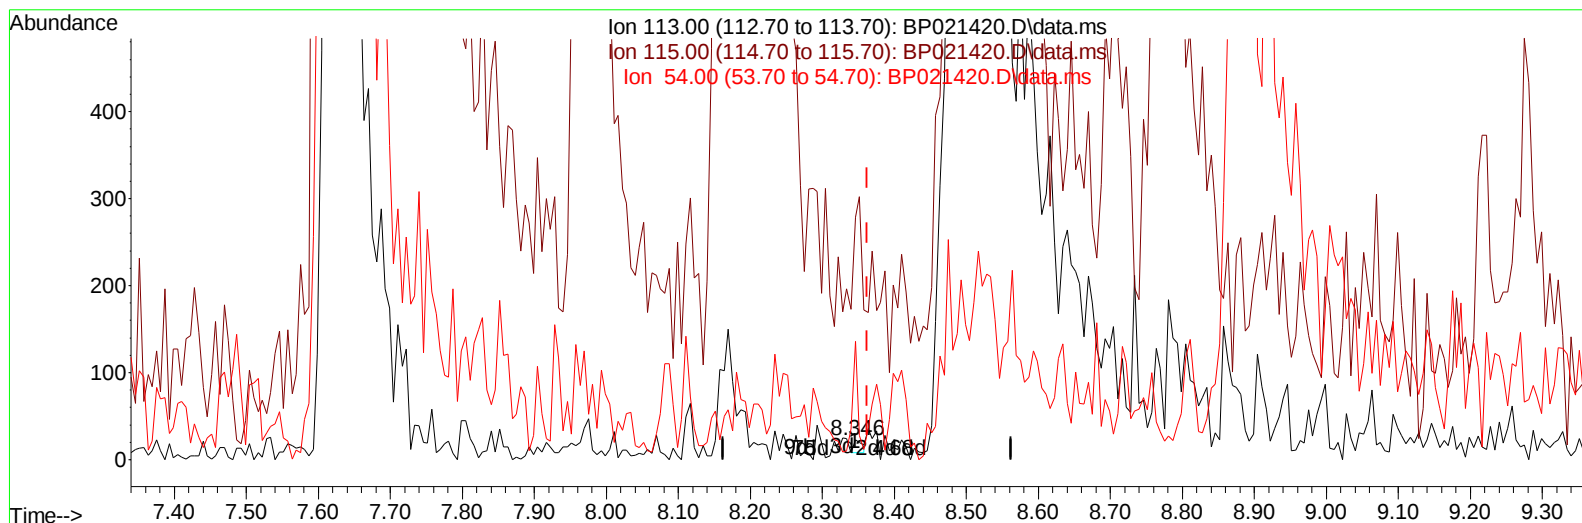

TIC: BP021420.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.346min (-0.017) 0.00 ng/u1

response 13

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	1213.04#
54.00	13.70	591.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:53:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

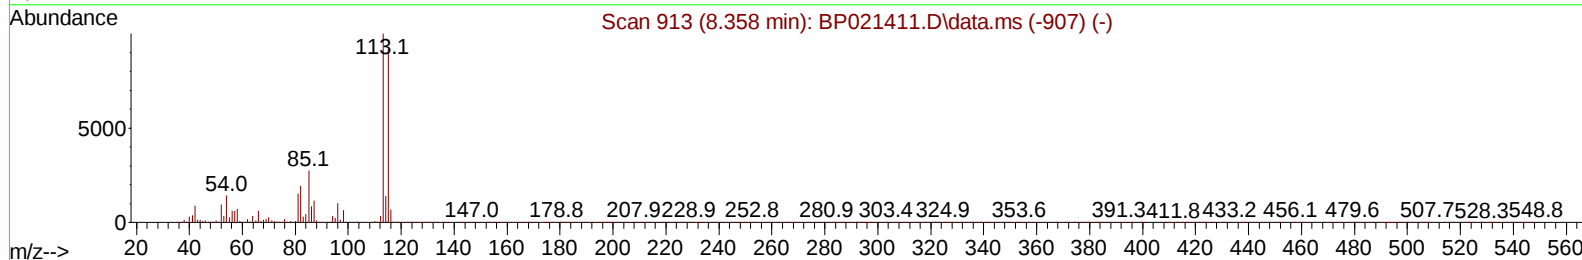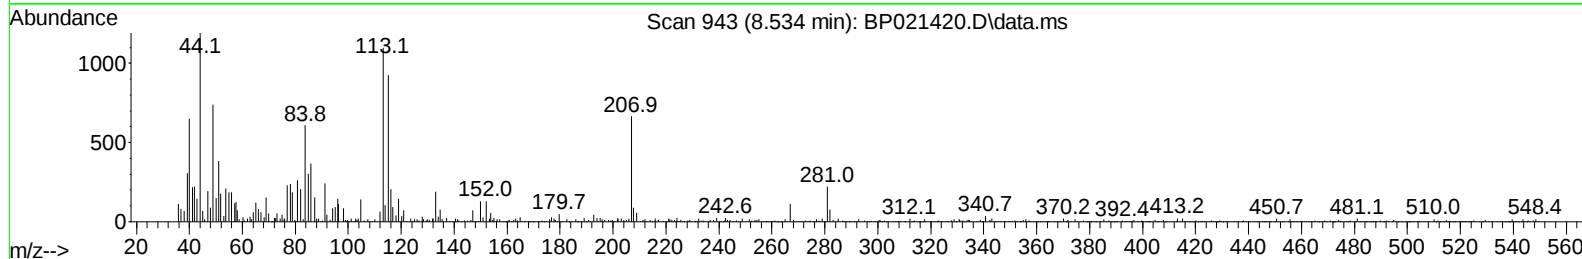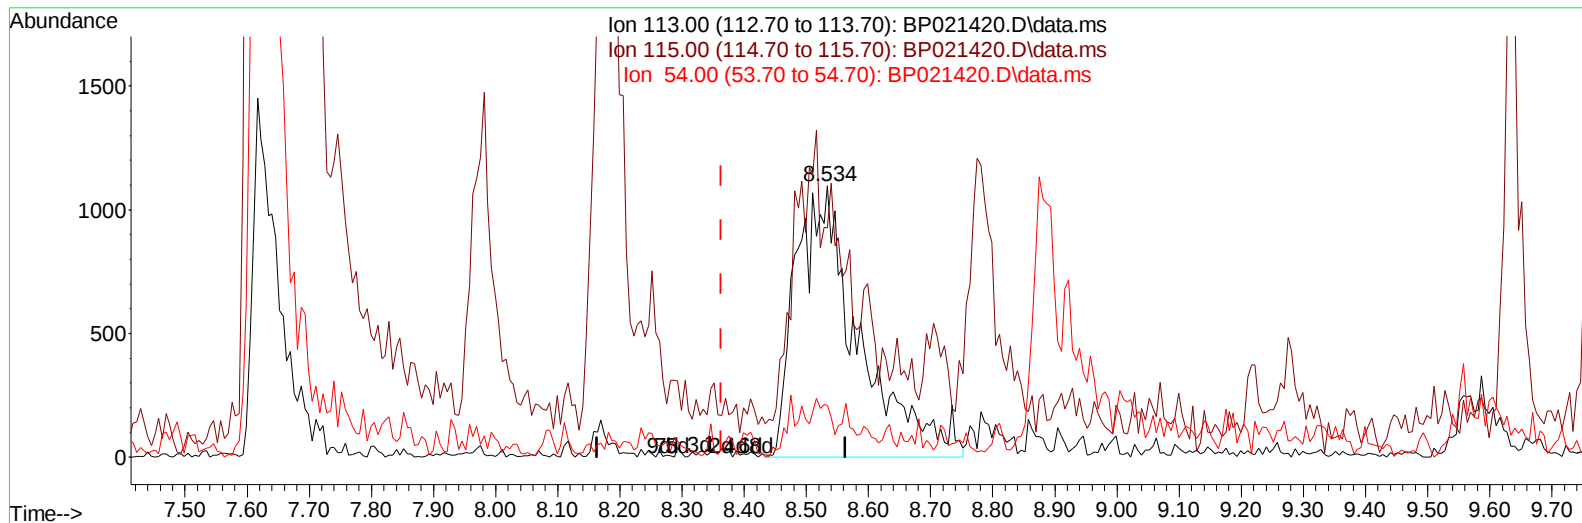

TIC: BP021420.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.534min (+ 0.171) 0.90 ng/ul m

response 7698

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	84.41
54.00	13.70	19.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:50:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

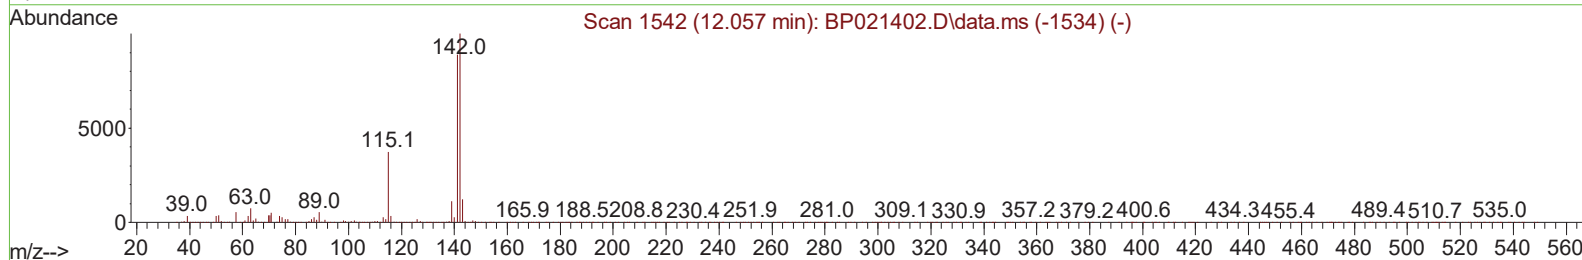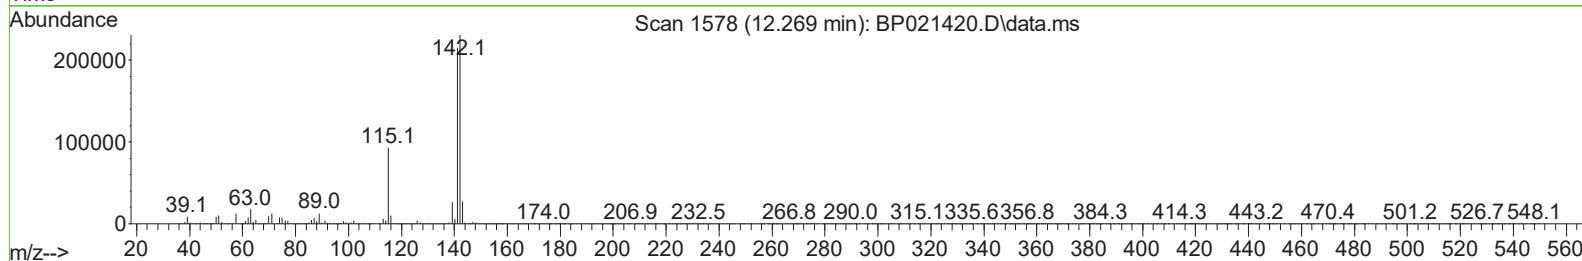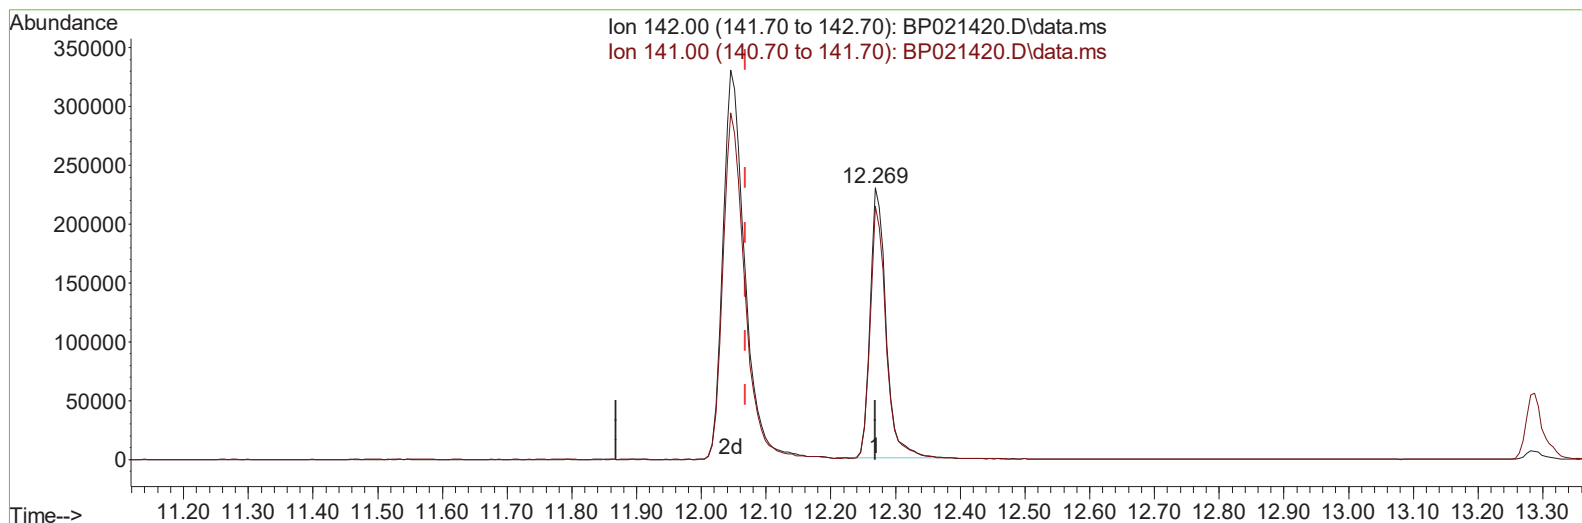

TIC: BP021420.D\data.ms

(36) 2-Methylnaphthalene

12.269min (+ 0.200) 23.29 ng/ul

response 401271

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.70	93.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021420.D
 Acq On : 07 Aug 2024 14:50
 Operator : CG/JU
 Sample : P3329-02DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:50:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

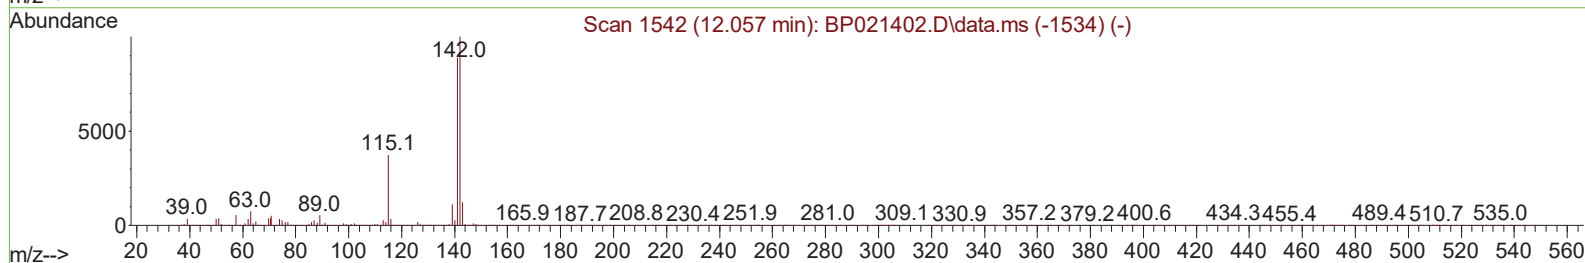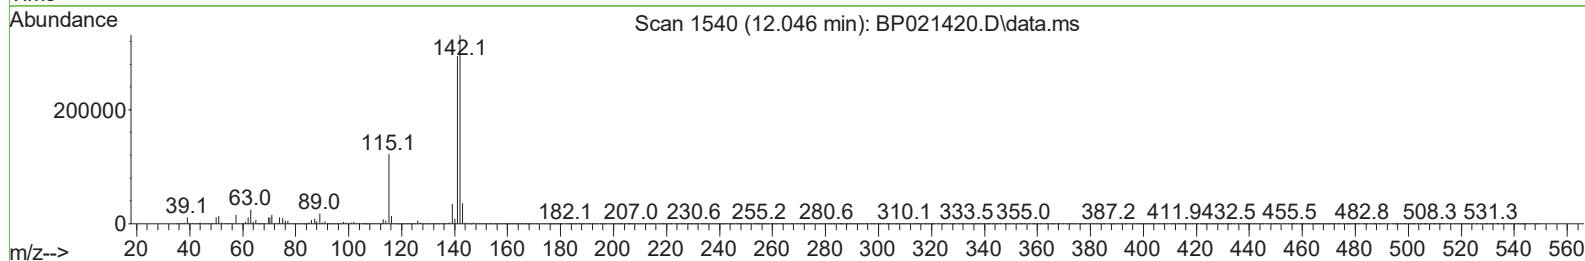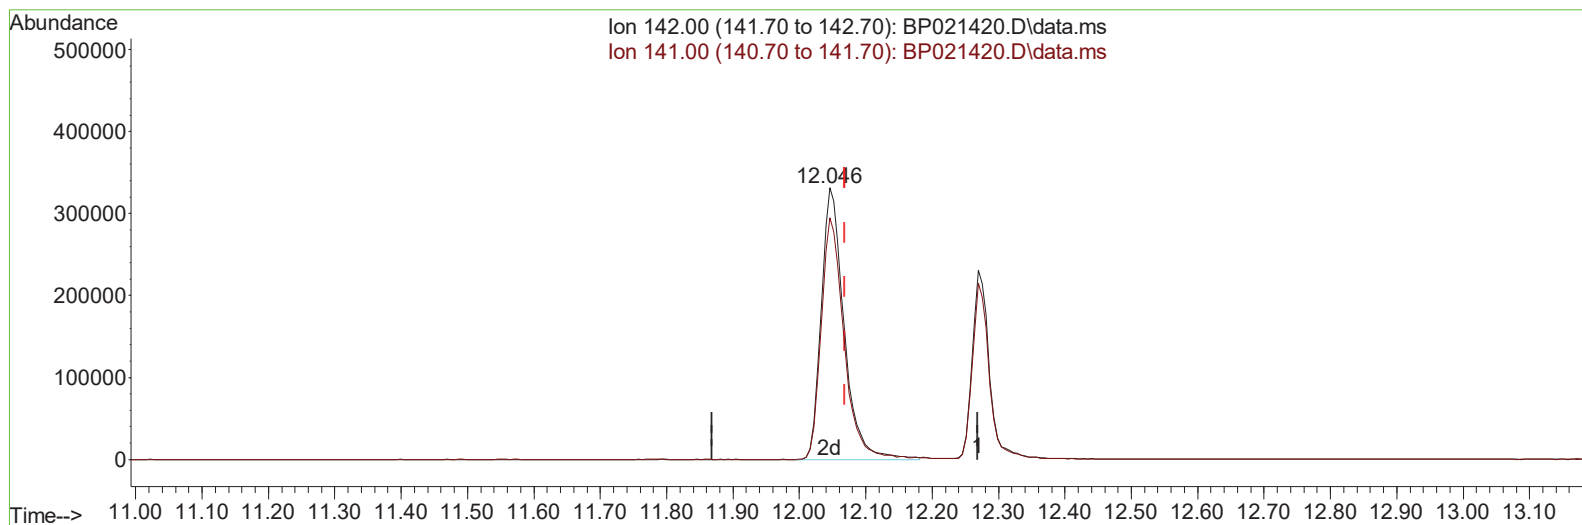

TIC: BP021420.D\data.ms

(36) 2-Methylnaphthalene

12.046min (-0.023) 45.98 ng/ul m

response 792156

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.70	88.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:17:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

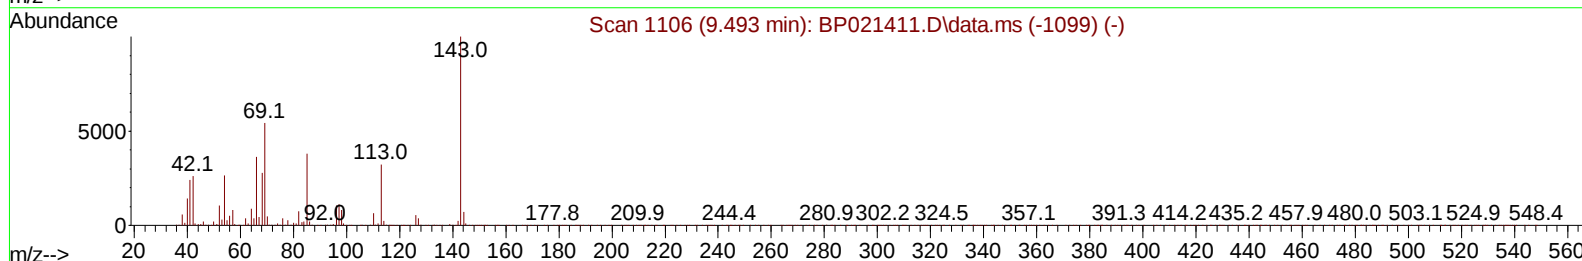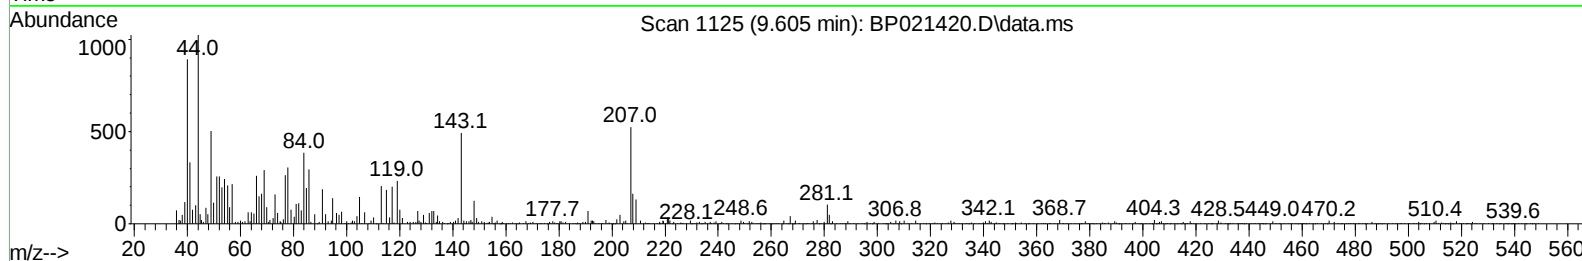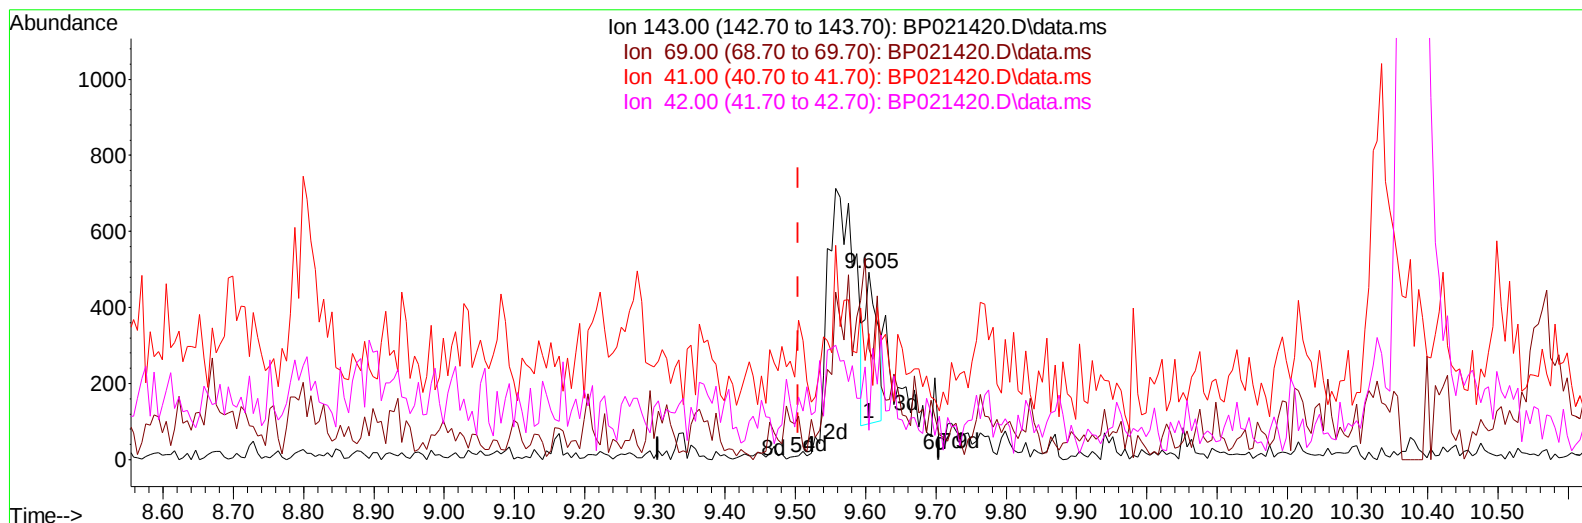

TIC: BP021420.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.605min (+ 0.101) 39.02 ng/u1

response 520

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	59.15
41.00	22.70	67.48#
42.00	22.10	15.65#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:53:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

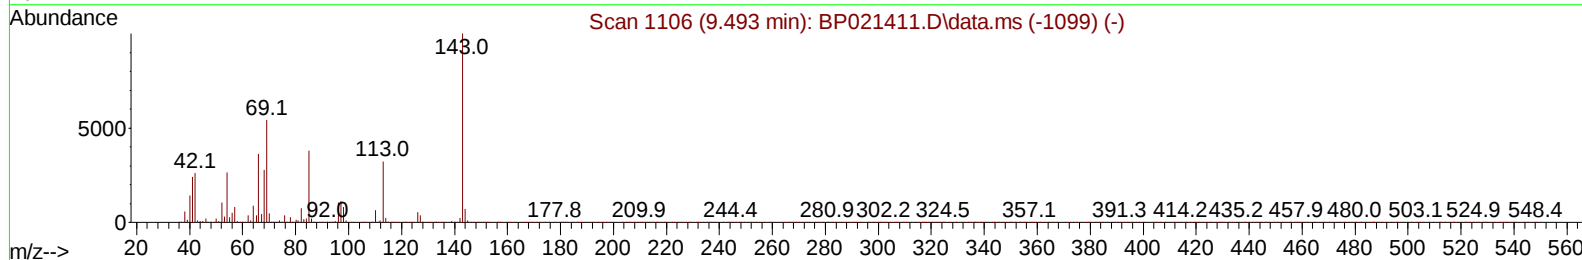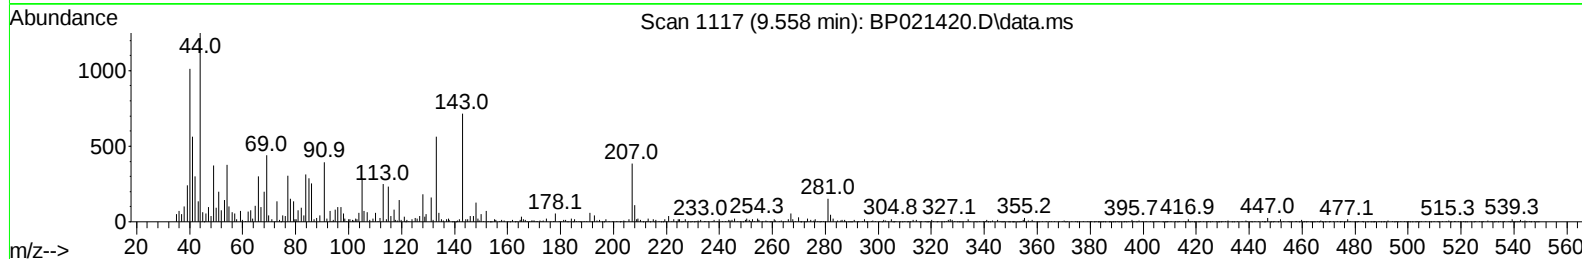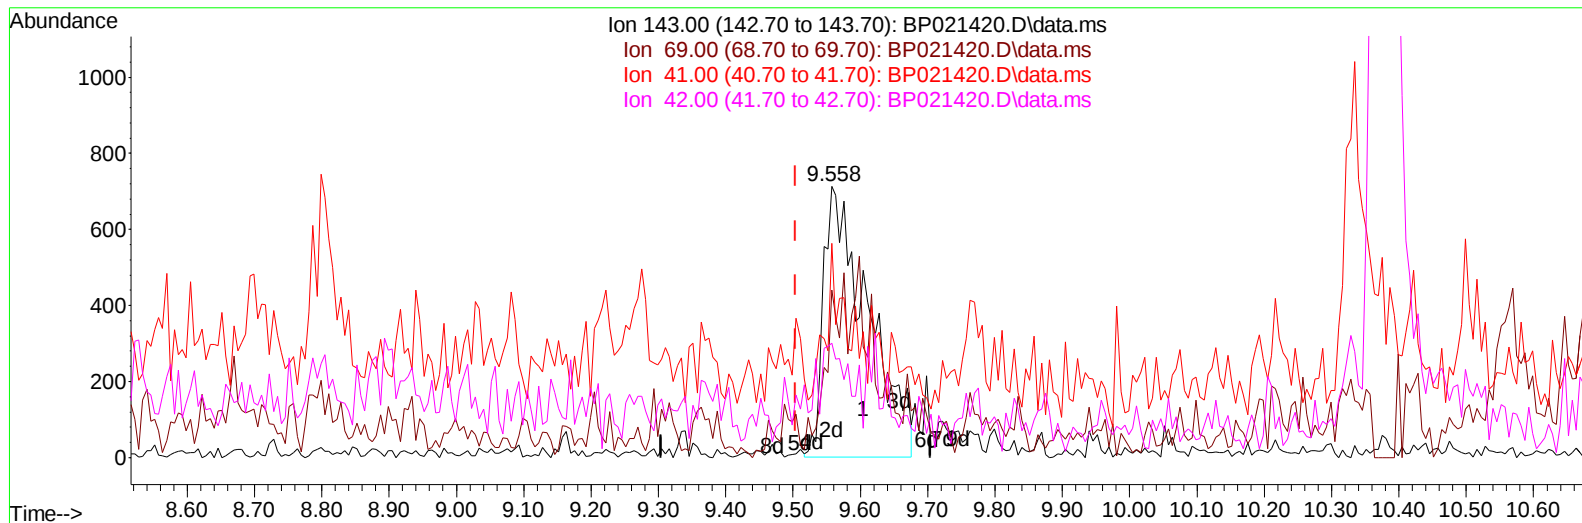

TIC: BP021420.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.558min (+ 0.053) 0.76 ng/ul m

response 3226

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	61.62#
41.00	22.70	78.85#
42.00	22.10	42.16#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 07:17:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

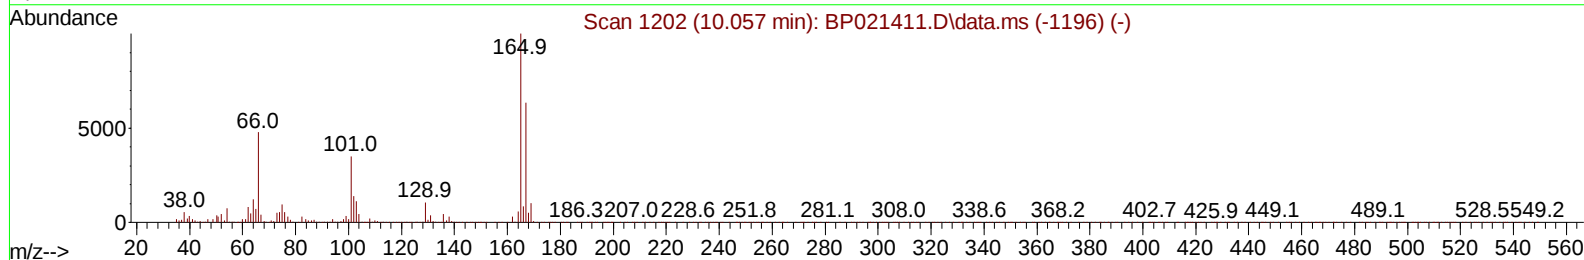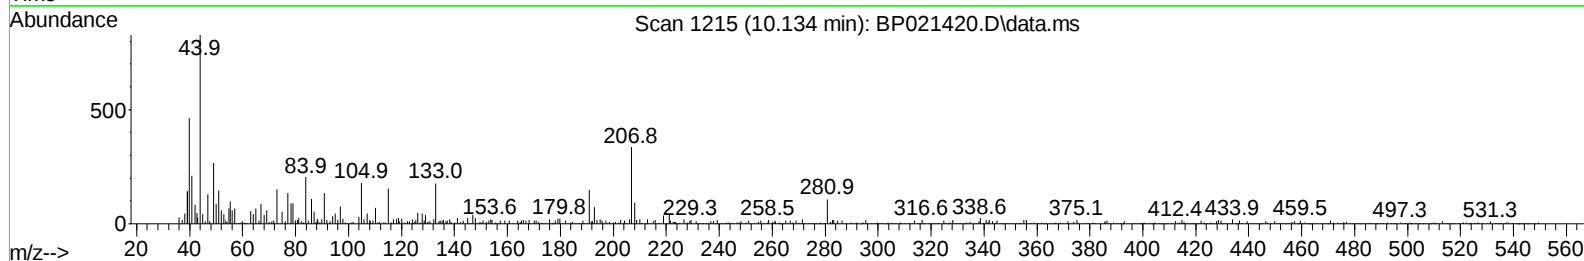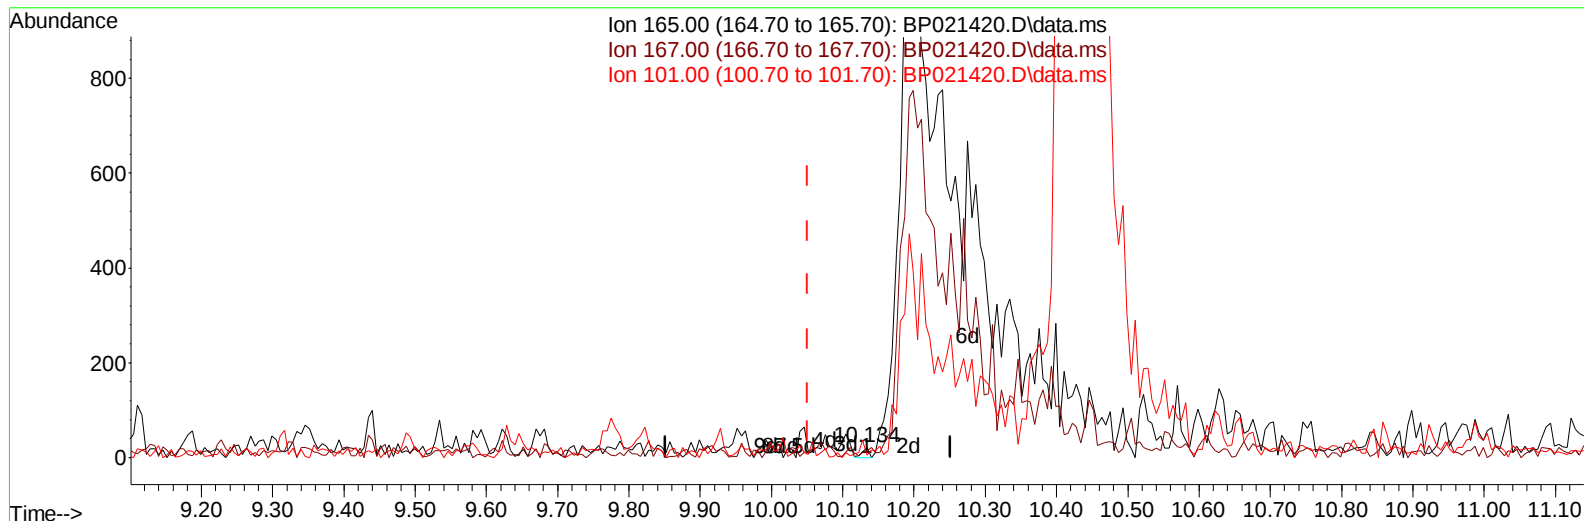

TIC: BP021420.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.134min (+ 0.083) 0.54 ng/u1

response 13

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	63.64
101.00	35.50	63.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021420.D
 Acq On : 07 Aug 2024 14:50
 Operator : CG/JU
 Sample : P3329-02DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:53:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

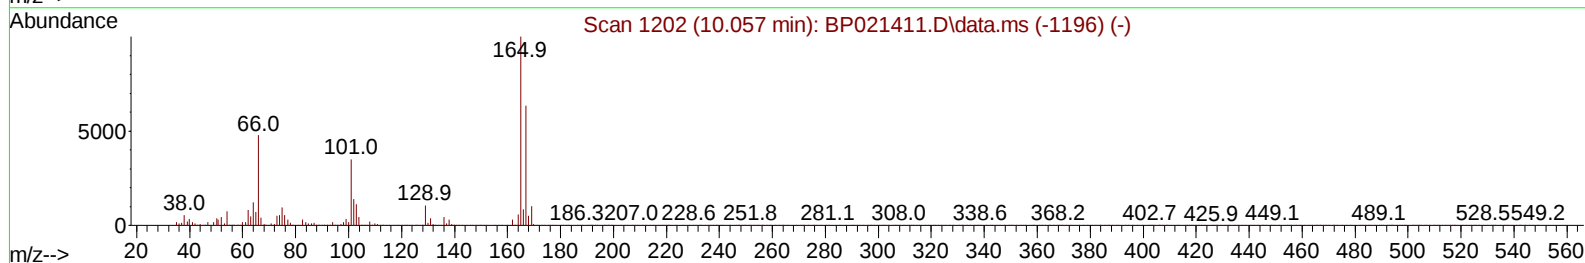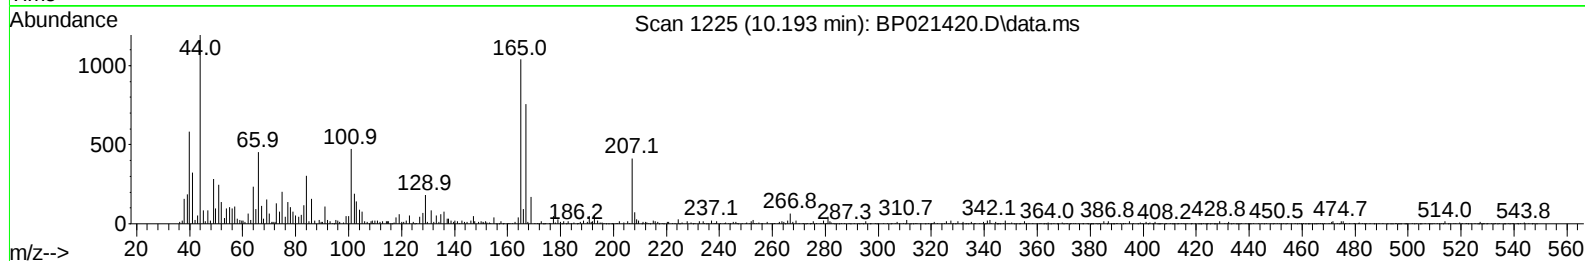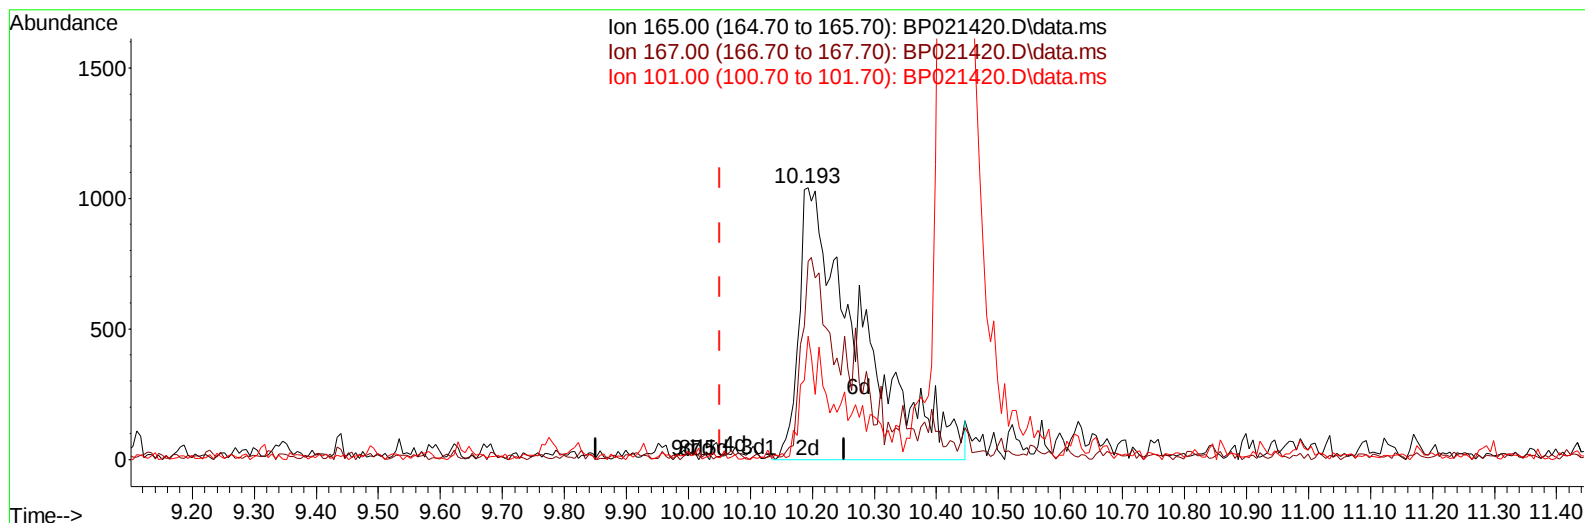

TIC: BP021420.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.193min (+ 0.142) 0.93 ng/ul m

response 7169

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	72.98
101.00	35.50	45.38#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:35:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

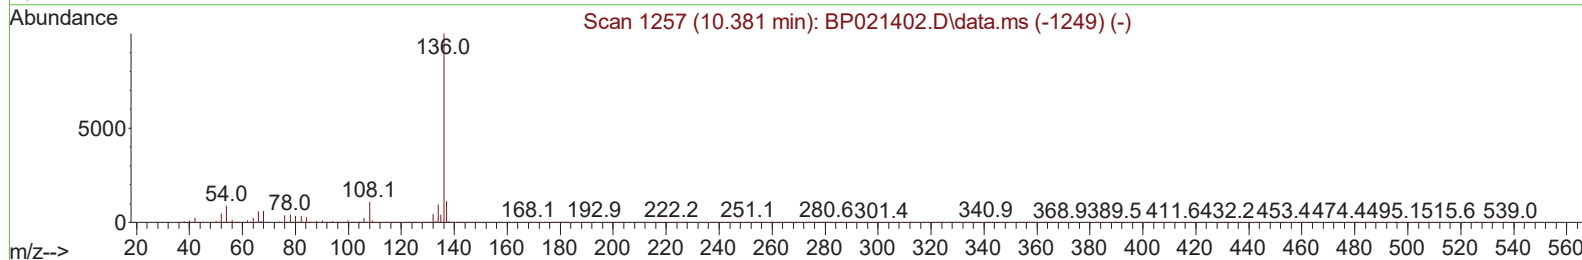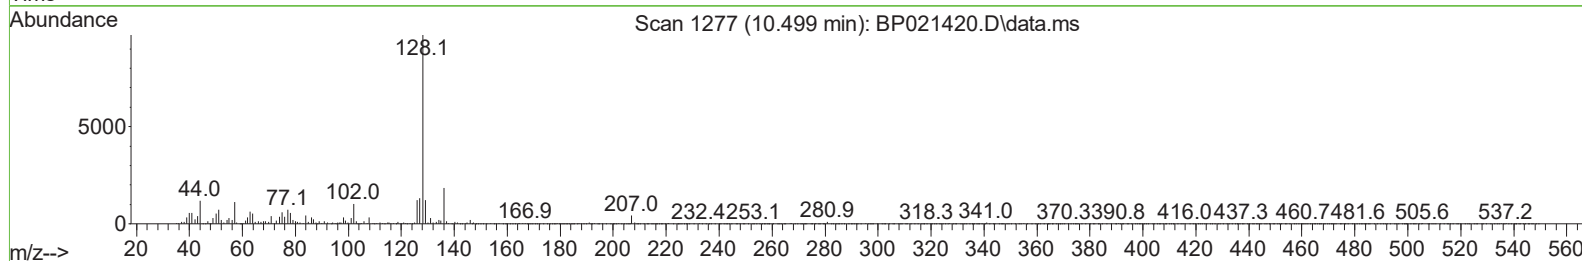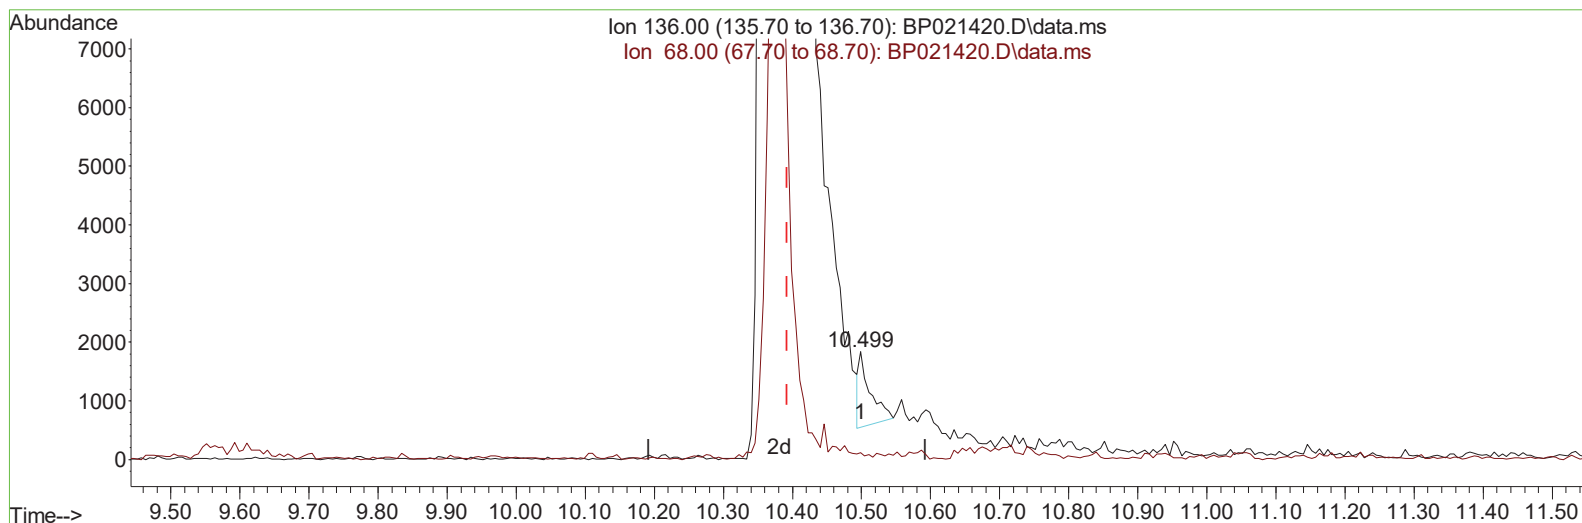

TIC: BP021420.D\data.ms

(20) Naphthalene-d8 (I)

10.499min (+ 0.106) 20.00 ng/u1

response 1499

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	6.10	6.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021420.D
 Acq On : 07 Aug 2024 14:50
 Operator : CG/JU
 Sample : P3329-02DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:35:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

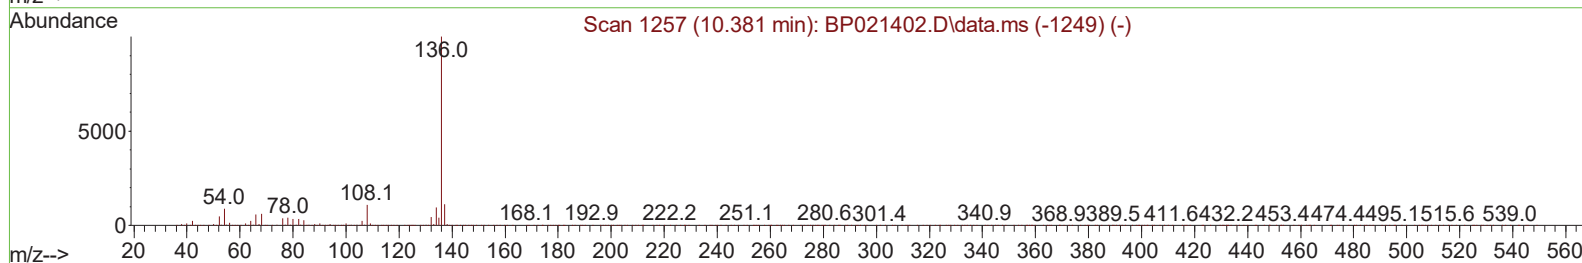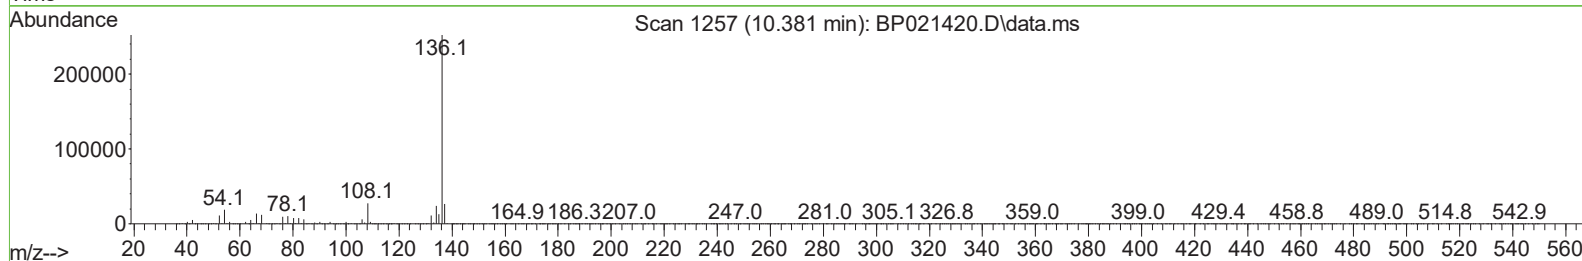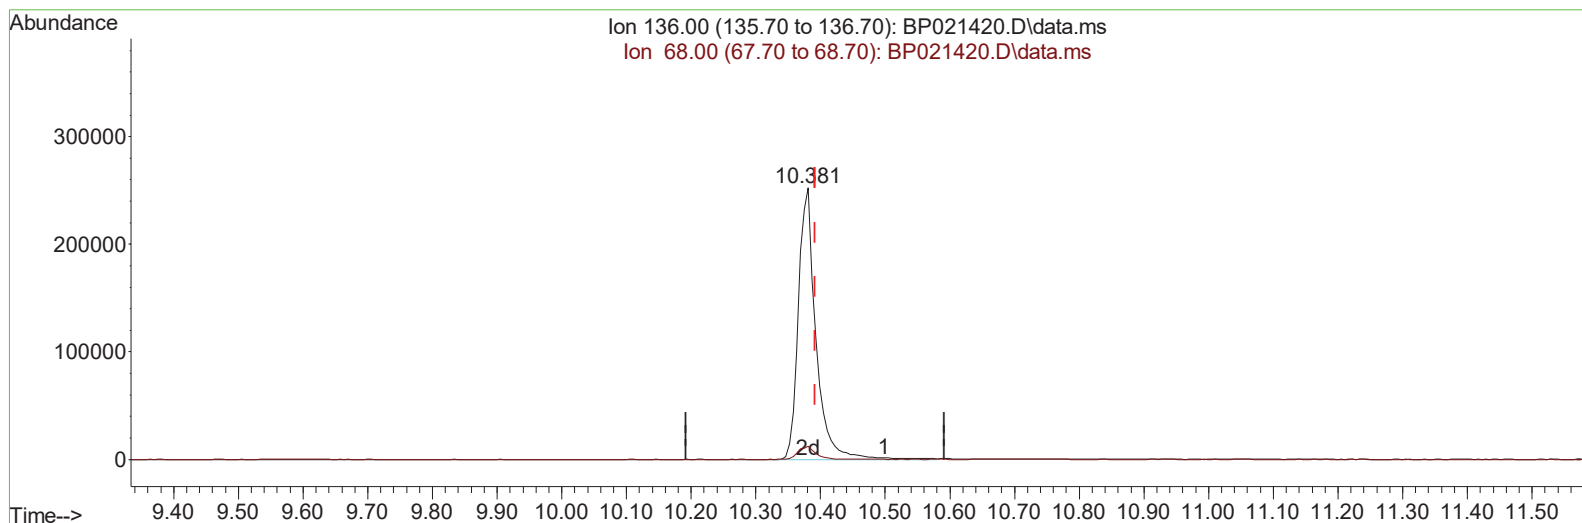

TIC: BP021420.D\data.ms

(20) Naphthalene-d8 (I)

10.381min (-0.011) 20.00 ng/ul m

response 477157

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	6.10	4.83#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 08 03:52:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

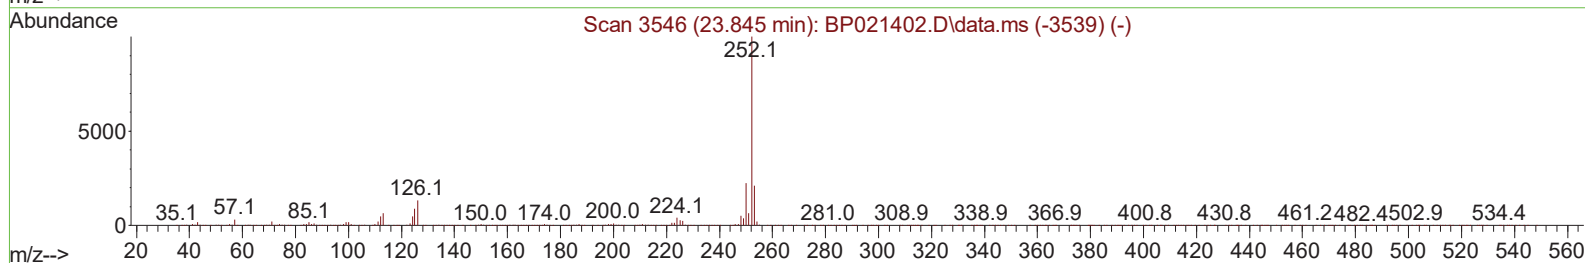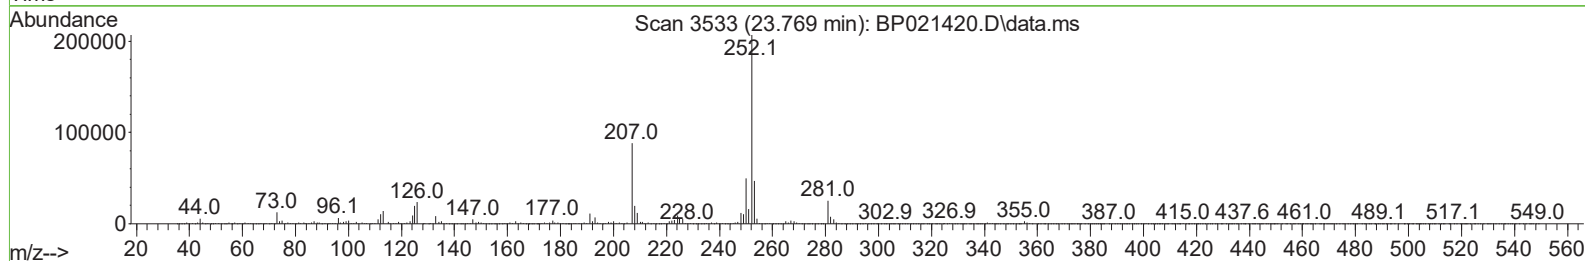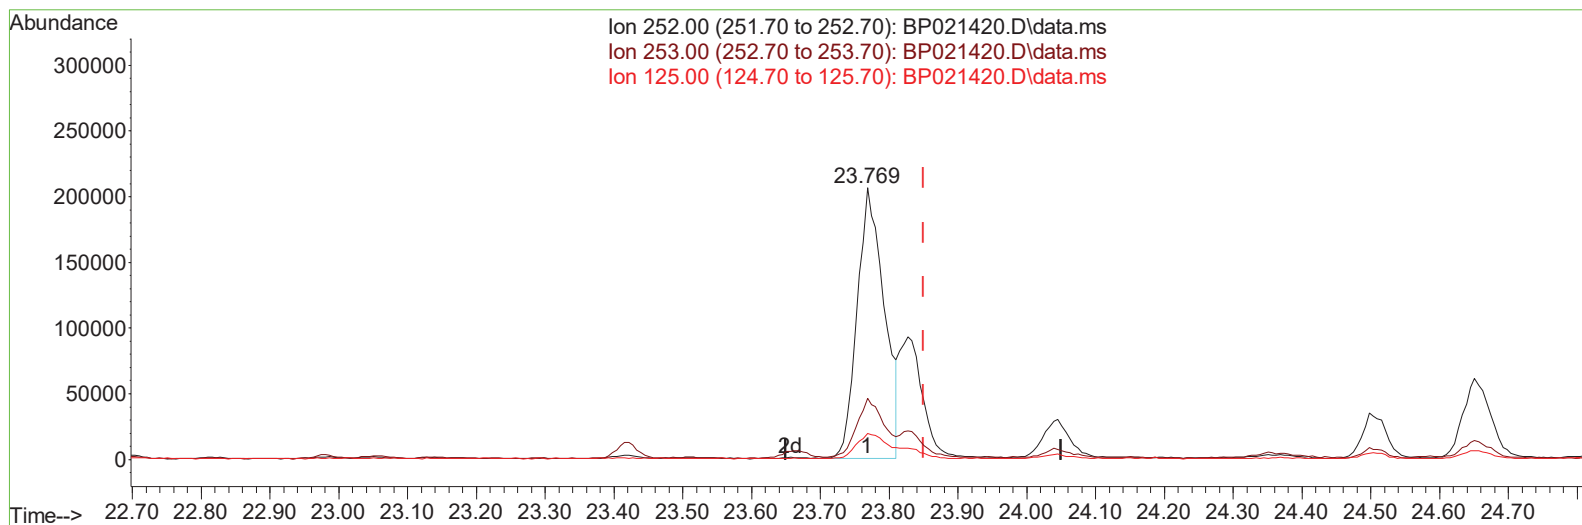

TIC: BP021420.D\data.ms

(91) Benzo(k)fluoranthene

23.769min (-0.082) 8.13 ng/u1

response 564158

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	22.62
125.00	9.20	9.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 08 03:52:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

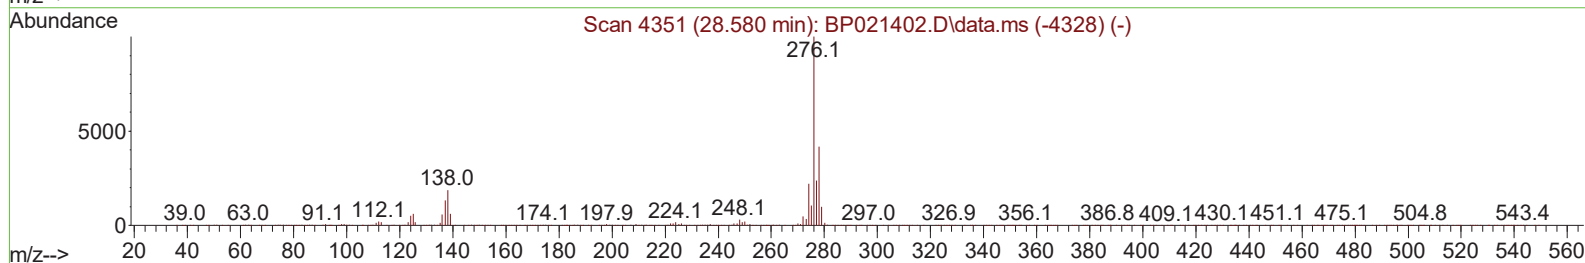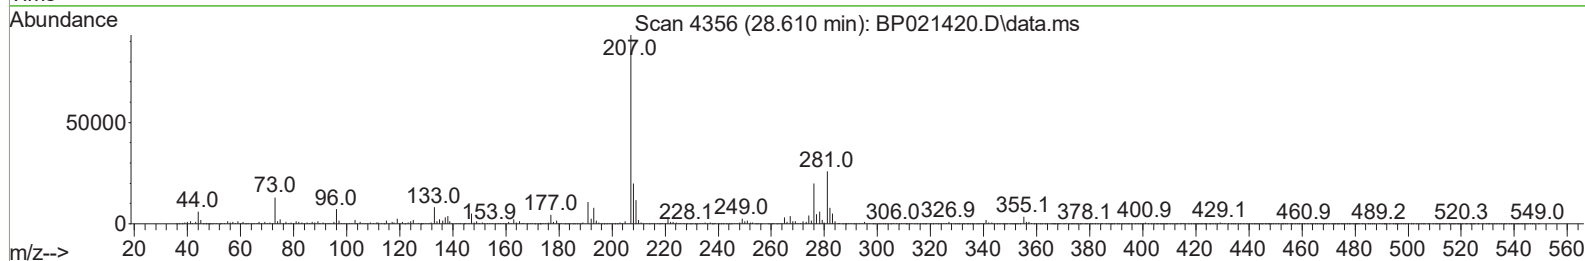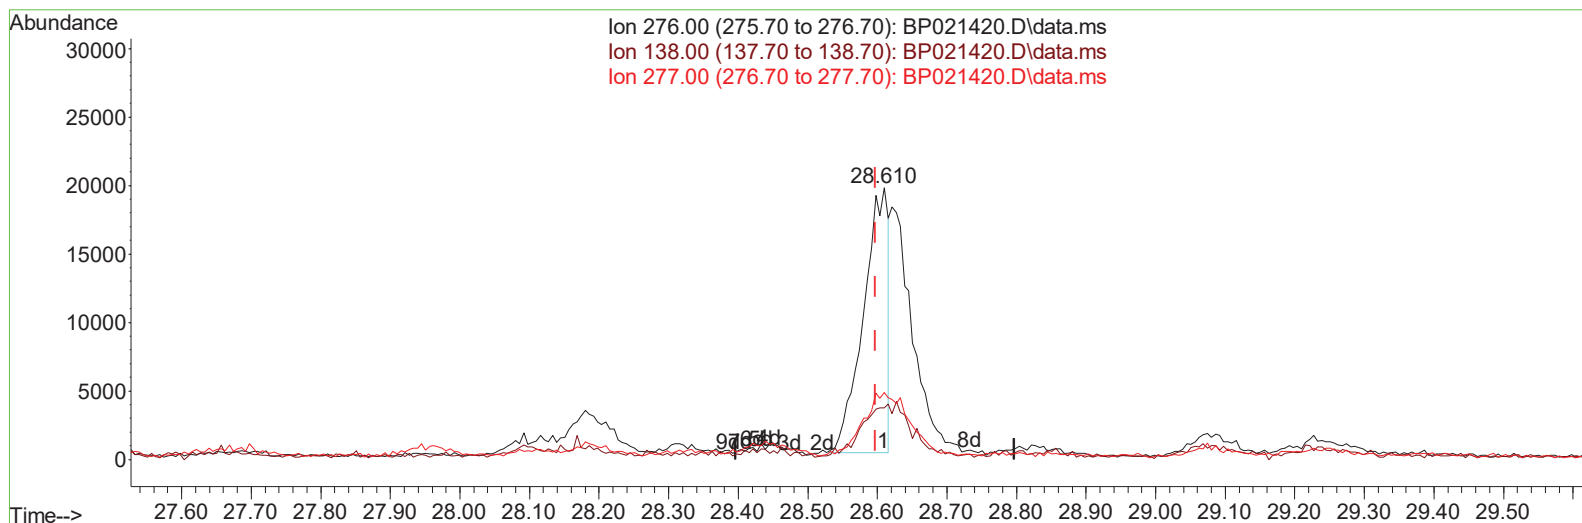

TIC: BP021420.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.610min (+ 0.012) 0.57 ng/u1

response 47919

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.90	18.96
277.00	24.00	24.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:52:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

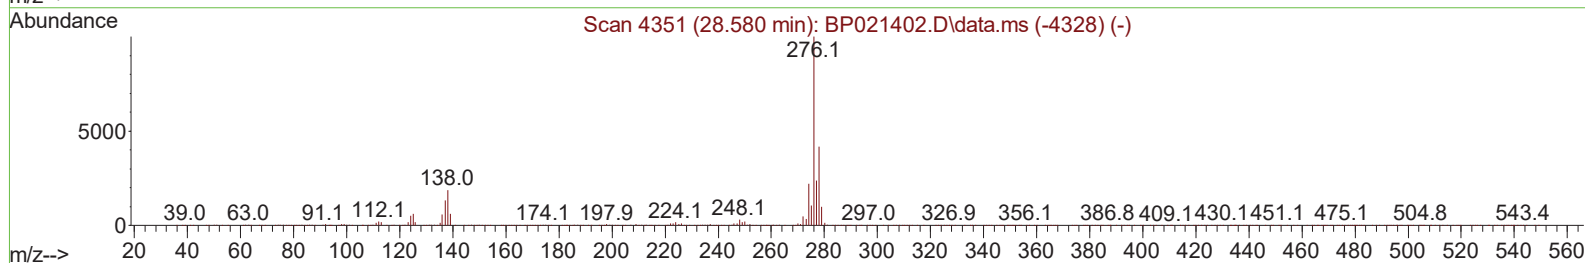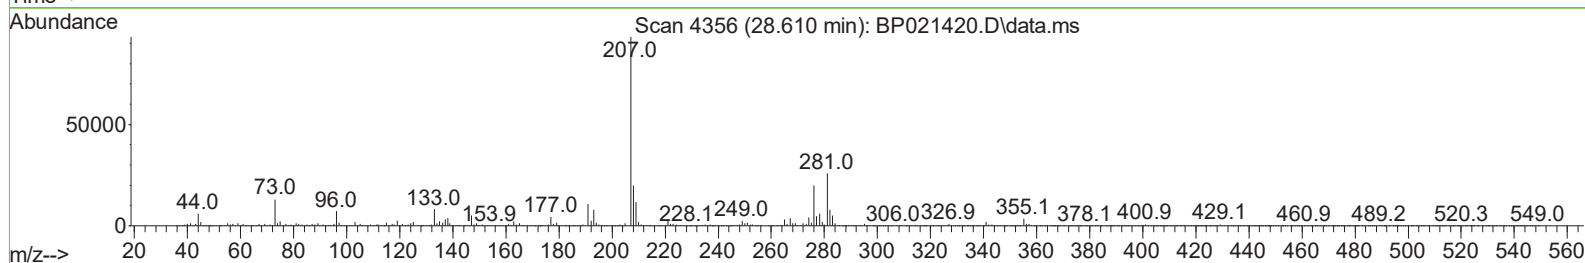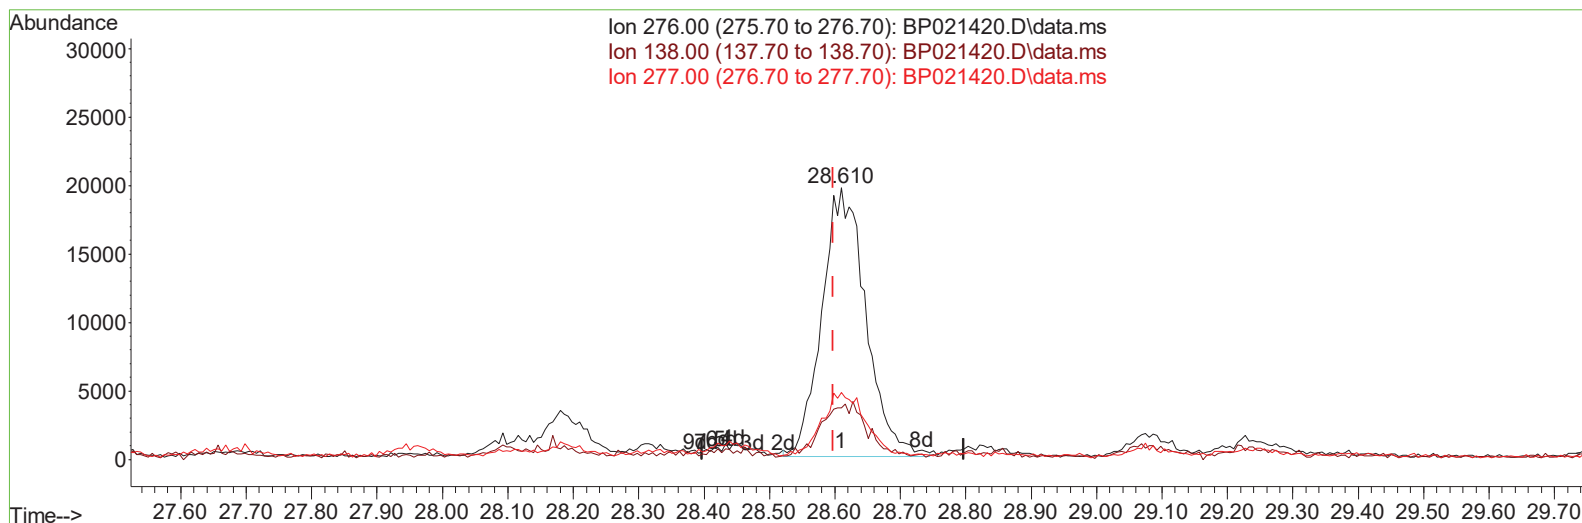

TIC: BP021420.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.610min (+ 0.012) 1.08 ng/ul m

response 91345

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.90	18.96
277.00	24.00	24.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021420.D
 Acq On : 07 Aug 2024 14:50
 Operator : CG/JU
 Sample : P3329-02DL2 30X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E01DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/08/2024
 Supervised By :mohammad ahmed 08/09/2024

Quant Time: Aug 08 03:53:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.622	152		126512	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.381	136		477157m	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.257	164		388683	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.081	188		885953	20.000	ng/ul	-0.01
79) Chrysene-d12	21.522	240		974192	20.000	ng/ul	-0.01
88) Perylene-d12	24.804	264		1146401	20.000	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	0.000	99		0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	7.064	67		6106m	0.977	ng/ul	0.08
11) 2-Chlorophenol-d4	7.293	132		7241m	0.852	ng/ul	0.11
15) 4-Methylphenol-d8	8.534	113		7698m	0.899	ng/ul	0.17
21) Nitrobenzene-d5	0.000	128		0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	9.558	143		3226m	0.761	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.193	165		7169m	0.935	ng/ul	0.14
31) 4-Chloroaniline-d4	0.000	131		0d	0.000	ng/ul	
46) Dimethylphthalate-d6	13.693	166		31820	1.126	ng/ul	0.01
49) Acenaphthylene-d8	13.963	160		32153	1.013	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.275	176		31055	1.340	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.187	188		49763	1.265	ng/ul	0.00
81) Pyrene-d10	19.569	212		54887	0.911	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.580	264		42284	0.748	ng/ul	-0.02
Target Compounds							
						Qvalue	
30) Naphthalene	10.428	128		1041646	41.502	ng/ul	99
36) 2-Methylnaphthalene	12.046	142		792156m	45.979	ng/ul	
37) 1-Methylnaphthalene	12.269	142		405525	22.886	ng/ul	99
43) 1,1'-Biphenyl	13.075	154		236510	8.326	ng/ul	98
52) Acenaphthene	14.322	153		939022	39.385	ng/ul	98
56) Dibenzofuran	14.681	168		1026611	31.444	ng/ul	98
61) Fluorene	15.334	166		1135158	42.607	ng/ul	98
72) Phenanthrene	17.128	178		4797432	104.383	ng/ul	99
74) Anthracene	17.222	178		1172827	25.031	ng/ul	98
77) Carbazole	17.540	167		194121	5.068	ng/ul	97
80) Fluoranthene	19.216	202		3221412	44.290	ng/ul	99
82) Pyrene	19.598	202		1691559	22.854	ng/ul	99
85) Benzo(a)anthracene	21.504	228		849539	12.449	ng/ul	98
87) Chrysene	21.563	228		774545	12.214	ng/ul	98
90) Benzo(b)fluoranthene	23.769	252		564158	8.109	ng/ul	98
91) Benzo(k)fluoranthene	23.827	252		215182m	3.099	ng/ul	
93) Benzo(a)pyrene	24.651	252		167175	2.543	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	28.610	276		91345m	1.078	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021420.D
Acq On : 07 Aug 2024 14:50
Operator : CG/JU
Sample : P3329-02DL2 30X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E01DL2

Manual IntegrationsAPPROVED

Quant Time: Aug 08 03:53:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/08/2024
Supervised By :mohammad ahmed 08/09/2024

