

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021412.D
 Acq On : 07 Aug 2024 09:00
 Operator : CG/JU
 Sample : PB162410BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK410

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	36	rVB	39261	55030	1.25%	0.143%
2	3.564	95	98	123	rBV	392971	789990	17.88%	2.048%
3	3.852	143	147	152	rVB2	7624	11513	0.26%	0.030%
4	4.152	193	198	200	rVV6	2850	5399	0.12%	0.014%
5	6.816	645	651	667	rBV	319614	891854	20.19%	2.313%
6	6.940	667	672	691	rVB	378105	742155	16.80%	1.924%
7	7.140	700	706	724	rBV	499286	928367	21.01%	2.407%
8	7.581	774	781	799	rBV	366842	781072	17.68%	2.025%
9	8.334	902	909	934	rBV	357144	1188350	26.90%	3.081%
10	8.757	974	981	1003	rBV	377441	934242	21.15%	2.422%
11	9.022	1023	1026	1033	rVB8	3641	8759	0.20%	0.023%
12	9.469	1092	1102	1130	rBV	233318	628116	14.22%	1.629%
13	10.052	1192	1201	1209	rBV	232432	645112	14.60%	1.673%
14	10.363	1247	1254	1271	rVB	451870	881536	19.95%	2.286%
15	10.546	1276	1285	1303	rBV2	245859	868454	19.66%	2.252%
16	12.016	1528	1535	1543	rBV8	5362	15517	0.35%	0.040%
17	13.669	1806	1816	1837	rBV	996437	1938278	43.87%	5.026%
18	13.934	1854	1861	1881	rBV	1394426	2220600	50.26%	5.758%
19	14.245	1905	1914	1932	rBV	1080925	1619207	36.65%	4.199%
20	14.634	1974	1980	1986	rBV	185837	407795	9.23%	1.057%
21	14.810	2008	2010	2019	rVB5	15176	27113	0.61%	0.070%
22	14.892	2019	2024	2030	rVB6	8838	19334	0.44%	0.050%
23	15.281	2083	2090	2105	rBV	1324785	2892960	65.48%	7.501%
24	15.469	2116	2122	2143	rBV3	220647	757466	17.14%	1.964%
25	16.081	2222	2226	2230	rBV6	5457	8109	0.18%	0.021%
26	16.739	2336	2338	2342	rBV5	4511	6194	0.14%	0.016%
27	16.881	2358	2362	2365	rBV6	3308	5974	0.14%	0.015%
28	17.075	2389	2395	2407	rBV	1342759	2029933	45.94%	5.264%
29	17.192	2407	2415	2438	rVV	1370220	3322003	75.19%	8.614%
30	18.033	2553	2558	2565	rBV7	35011	77450	1.75%	0.201%
31	19.116	2739	2742	2748	rVB3	23729	33854	0.77%	0.088%
32	19.210	2755	2758	2763	rBV	24415	37485	0.85%	0.097%
33	19.575	2813	2820	2835	rBV2	2012141	4205120	95.18%	10.904%
34	21.539	3148	3154	3173	rVB2	1082848	2463801	55.76%	6.389%
35	24.580	3662	3671	3691	rBV2	1424135	4418217	100.00%	11.456%
36	24.815	3703	3711	3736	rVB	792773	2698912	61.09%	6.998%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021412.D
Acq On : 07 Aug 2024 09:00
Operator : CG/JU
Sample : PB162410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK410

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 38565271

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021412.D
Acq On : 07 Aug 2024 09:00
Operator : CG/JU
Sample : PB162410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

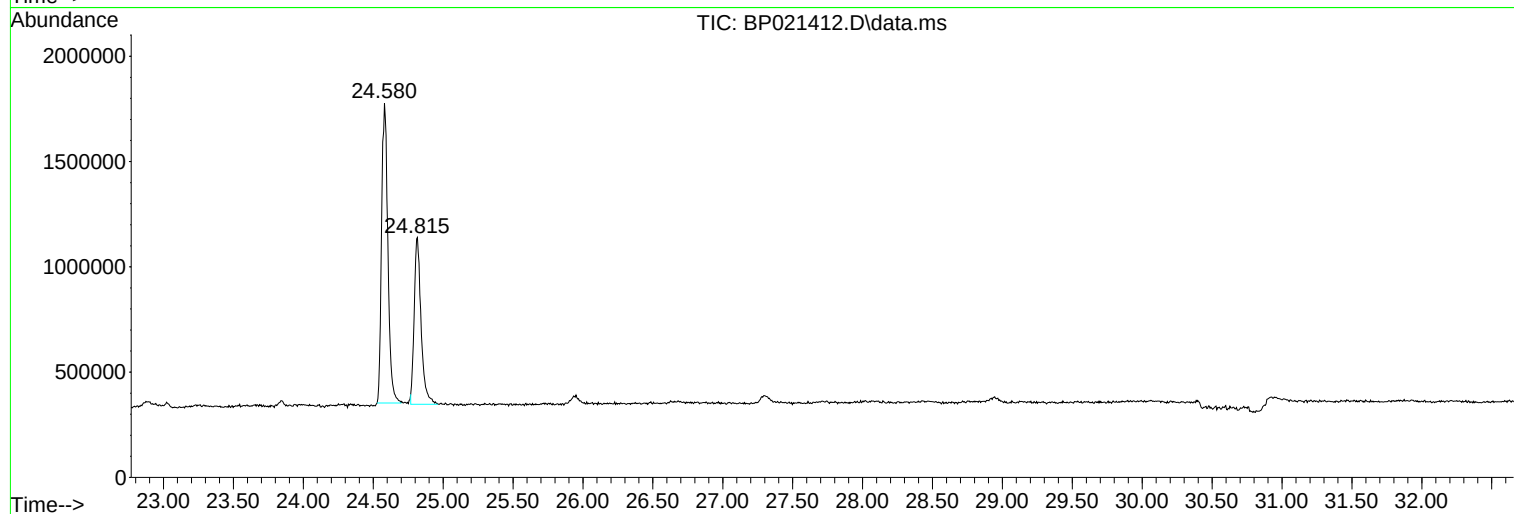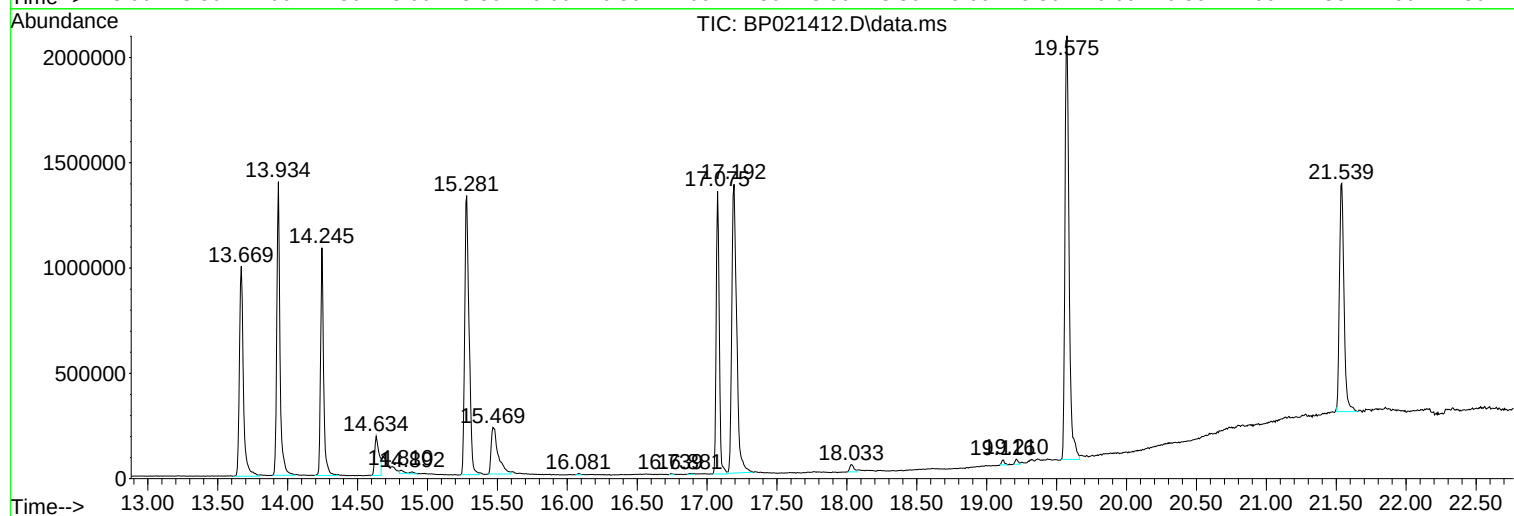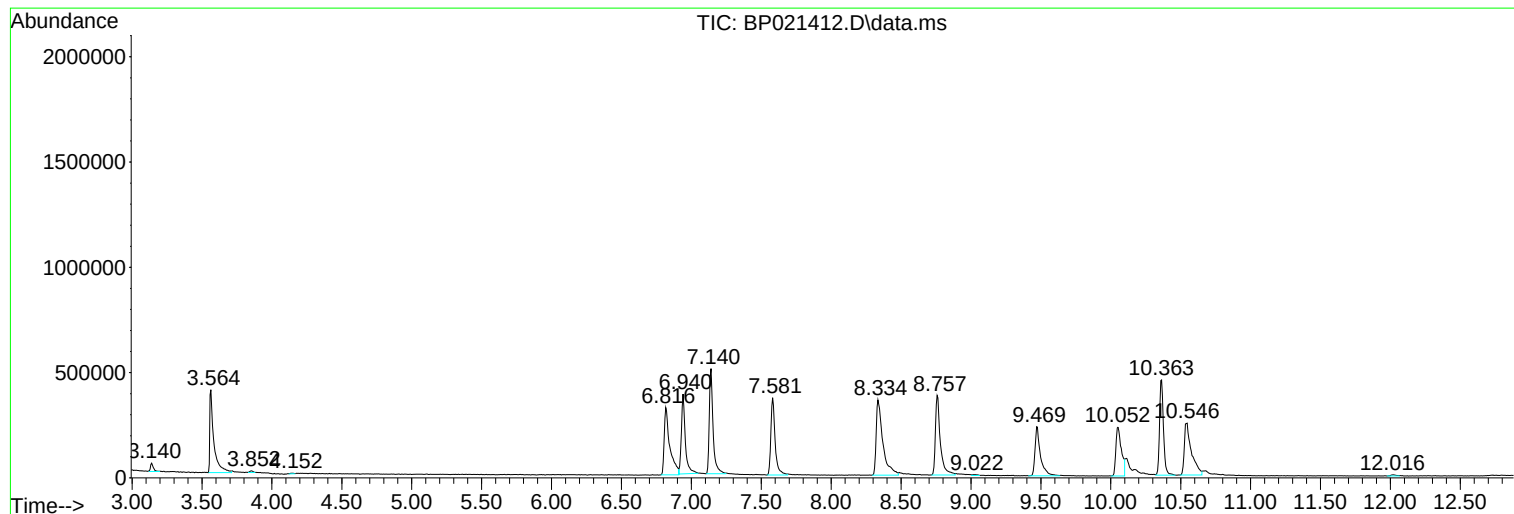

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021412.D
Acq On : 07 Aug 2024 09:00
Operator : CG/JU
Sample : PB162410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021412.D
Acq On : 07 Aug 2024 09:00
Operator : CG/JU
Sample : PB162410BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK410

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc