

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
 Data File : BP021413.D
 Acq On : 07 Aug 2024 09:44
 Operator : CG/JU
 Sample : PB162412BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK412

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	36	rBV	36095	51265	1.31%	0.143%
2	3.581	99	101	128	rBV	340596	748018	19.17%	2.081%
3	3.875	147	151	156	rVB	9405	13879	0.36%	0.039%
4	6.858	647	658	673	rBV	240977	717013	18.38%	1.995%
5	6.981	673	679	696	rVB	280990	543126	13.92%	1.511%
6	7.181	706	713	732	rBV	436639	822881	21.09%	2.289%
7	7.616	781	787	811	rBV	425295	840201	21.54%	2.338%
8	8.369	909	915	943	rBV	337608	1130752	28.98%	3.146%
9	8.793	980	987	1006	rBV	393154	887957	22.76%	2.470%
10	9.510	1102	1109	1136	rBV	283868	771646	19.78%	2.147%
11	10.087	1200	1207	1231	rBV	263483	1037928	26.60%	2.888%
12	10.393	1252	1259	1276	rVB	558846	1184045	30.35%	3.294%
13	10.575	1283	1290	1314	rBV	328250	1091224	27.97%	3.036%
14	10.857	1336	1338	1342	rVB5	3735	4062	0.10%	0.011%
15	12.051	1536	1541	1550	rBV4	5391	11848	0.30%	0.033%
16	13.681	1810	1818	1843	rBV	668347	1627710	41.72%	4.529%
17	13.951	1857	1864	1878	rBV2	1016254	1738480	44.56%	4.837%
18	14.263	1910	1917	1936	rBV	1023550	1664393	42.66%	4.631%
19	14.651	1977	1983	1989	rBV2	136118	363609	9.32%	1.012%
20	14.769	2000	2003	2011	rVB3	19760	37470	0.96%	0.104%
21	14.887	2022	2023	2029	rVB6	5850	8259	0.21%	0.023%
22	15.287	2084	2091	2115	rBV	1187822	2699968	69.20%	7.512%
23	15.475	2118	2123	2134	rBV2	188115	602790	15.45%	1.677%
24	16.092	2224	2228	2231	rBV5	5465	7726	0.20%	0.021%
25	17.086	2390	2397	2408	rBV	1364779	2101750	53.87%	5.848%
26	17.186	2408	2414	2440	rVB2	1447038	3100984	79.48%	8.628%
27	18.033	2555	2558	2563	rBV7	9577	15389	0.39%	0.043%
28	19.116	2739	2742	2751	rBV4	24676	44439	1.14%	0.124%
29	19.210	2755	2758	2762	rVV	18441	24906	0.64%	0.069%
30	19.575	2814	2820	2835	rBV	1973949	3901422	100.00%	10.855%
31	21.539	3148	3154	3170	rBV	1224291	2194934	56.26%	6.107%
32	24.586	3663	3672	3685	rBV2	1098075	3427481	87.85%	9.536%
33	24.810	3702	3710	3735	rVB	749698	2525077	64.72%	7.025%




Sum of corrected areas: 35942632

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021413.D
Acq On : 07 Aug 2024 09:44
Operator : CG/JU
Sample : PB162412BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

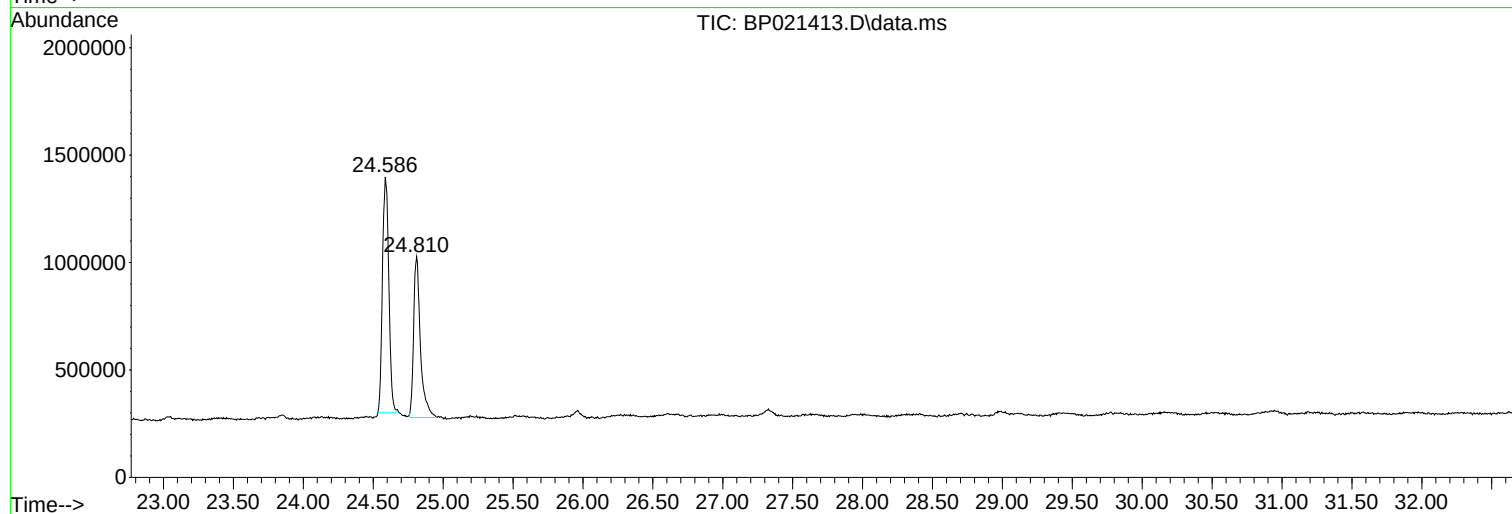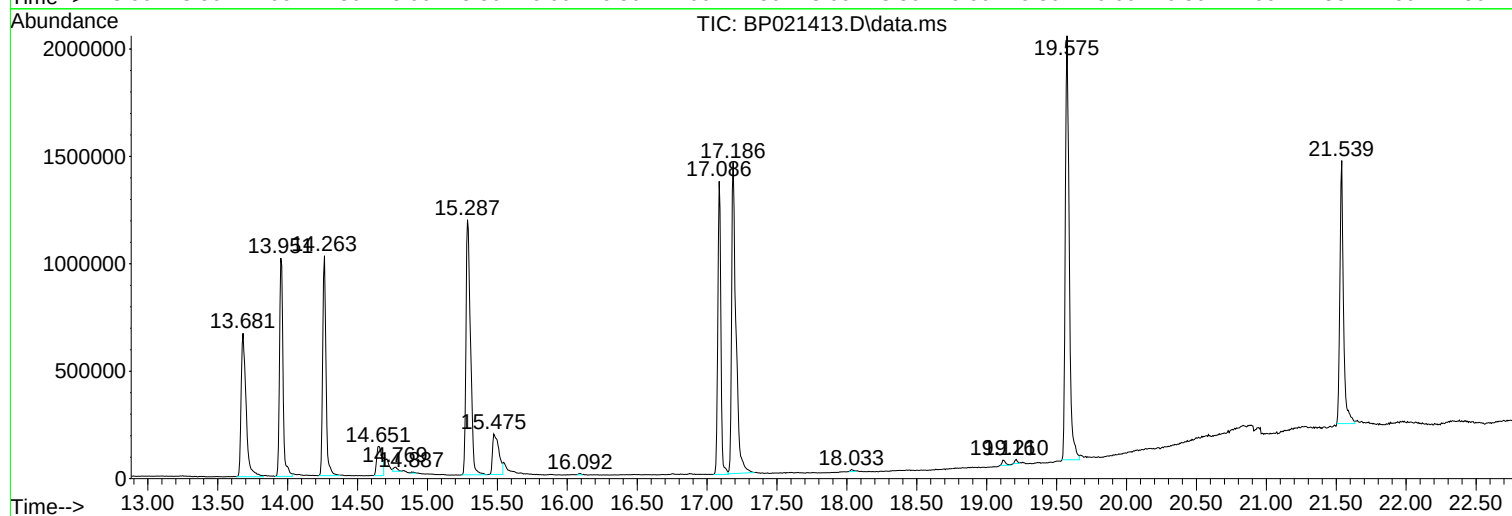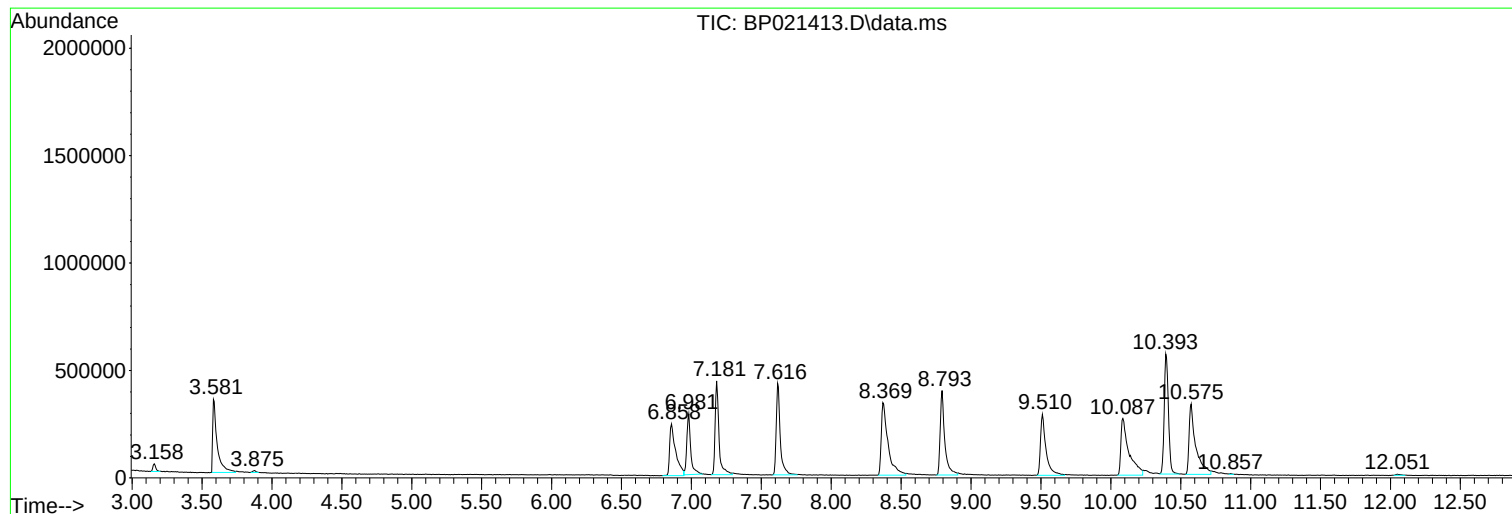

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021413.D
Acq On : 07 Aug 2024 09:44
Operator : CG/JU
Sample : PB162412BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080624\
Data File : BP021413.D
Acq On : 07 Aug 2024 09:44
Operator : CG/JU
Sample : PB162412BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------