
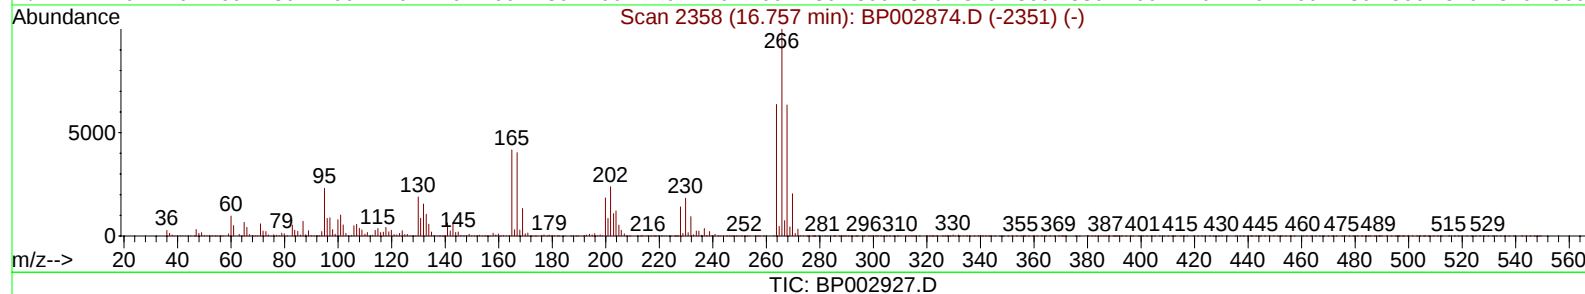
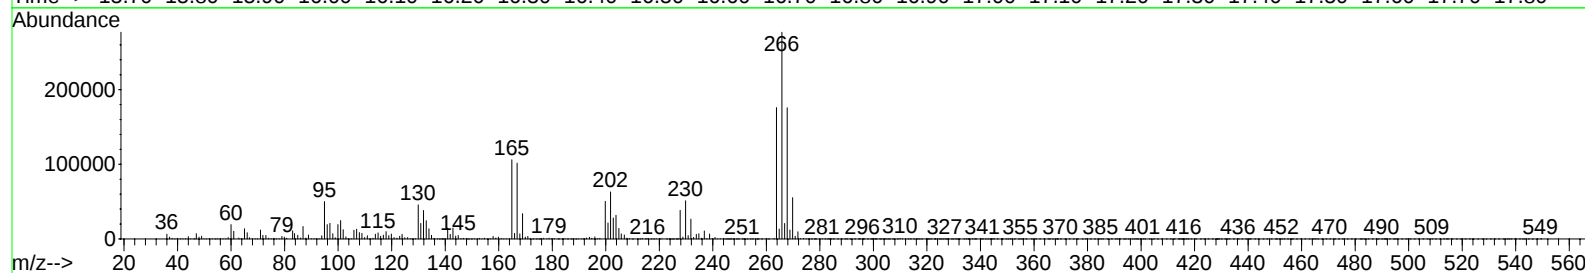


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP080720\
Data File : BP002927.D
Acq On : 07 Aug 2020 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 17:13:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 15:30:34 2020
Response via : Initial Calibration

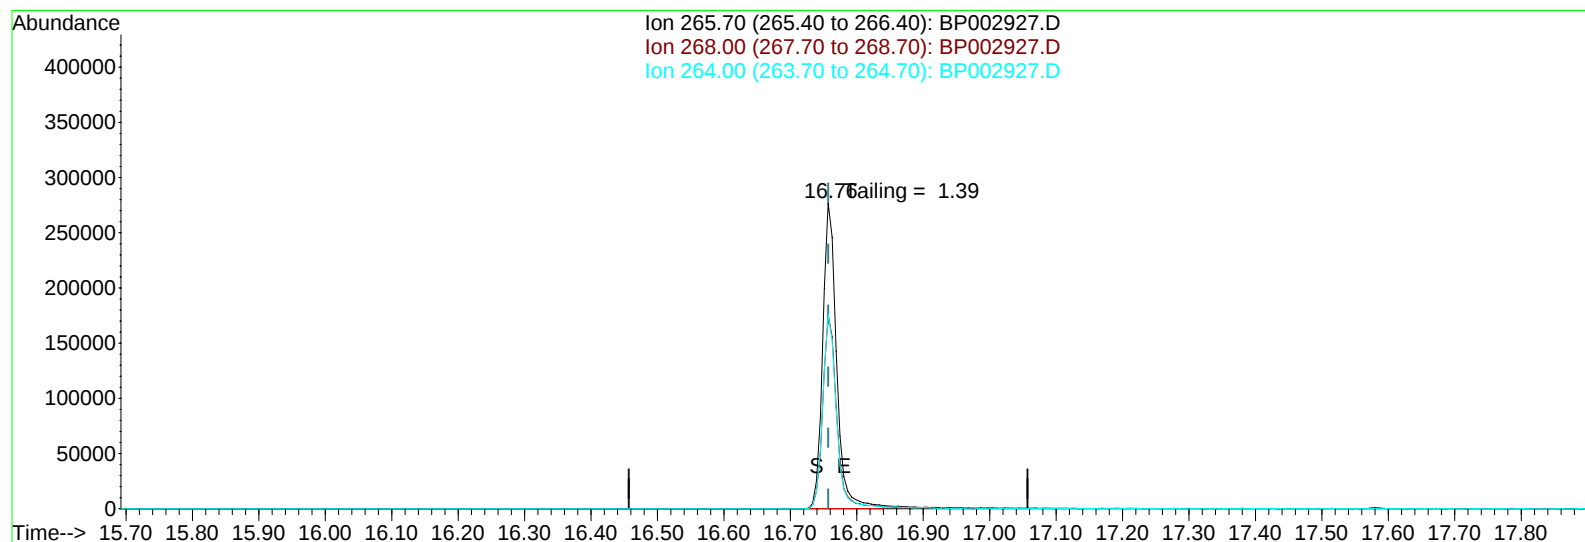

(70) Pentachlorophenol (C)




16.757min (+0.000) 43447.10ng

response 409295

Ion	Exp%	Act%
265.70	100	100
268.00	63.40	63.49
264.00	63.60	63.53
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP080720\
 Data File : BP002927.D
 Acq On : 07 Aug 2020 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 17:13:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 15:30:34 2020
 Response via : Initial Calibration

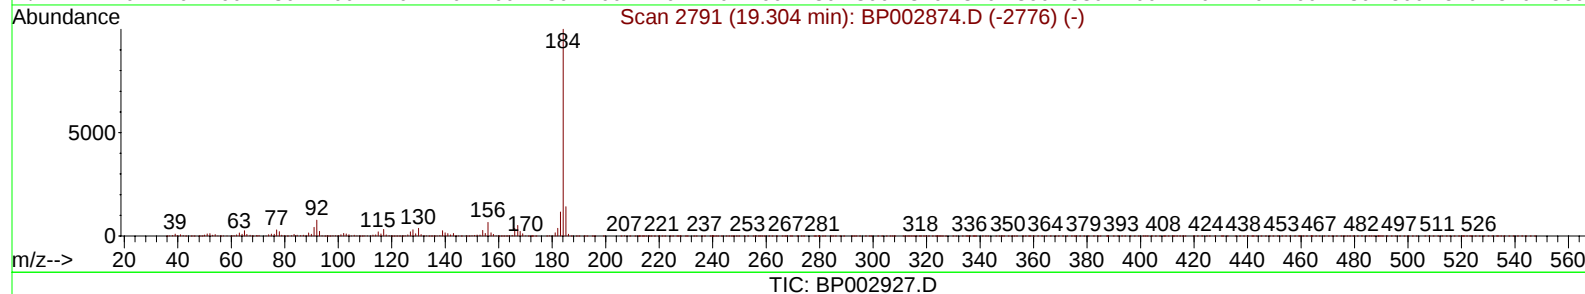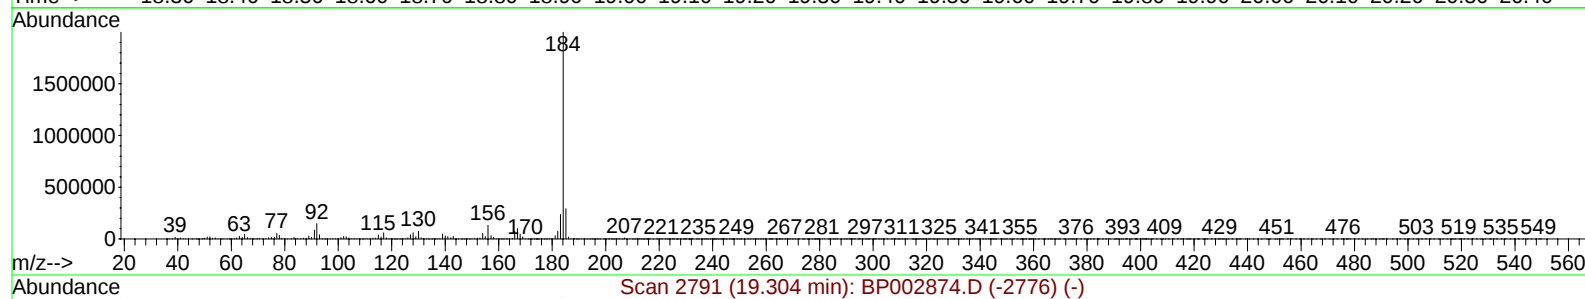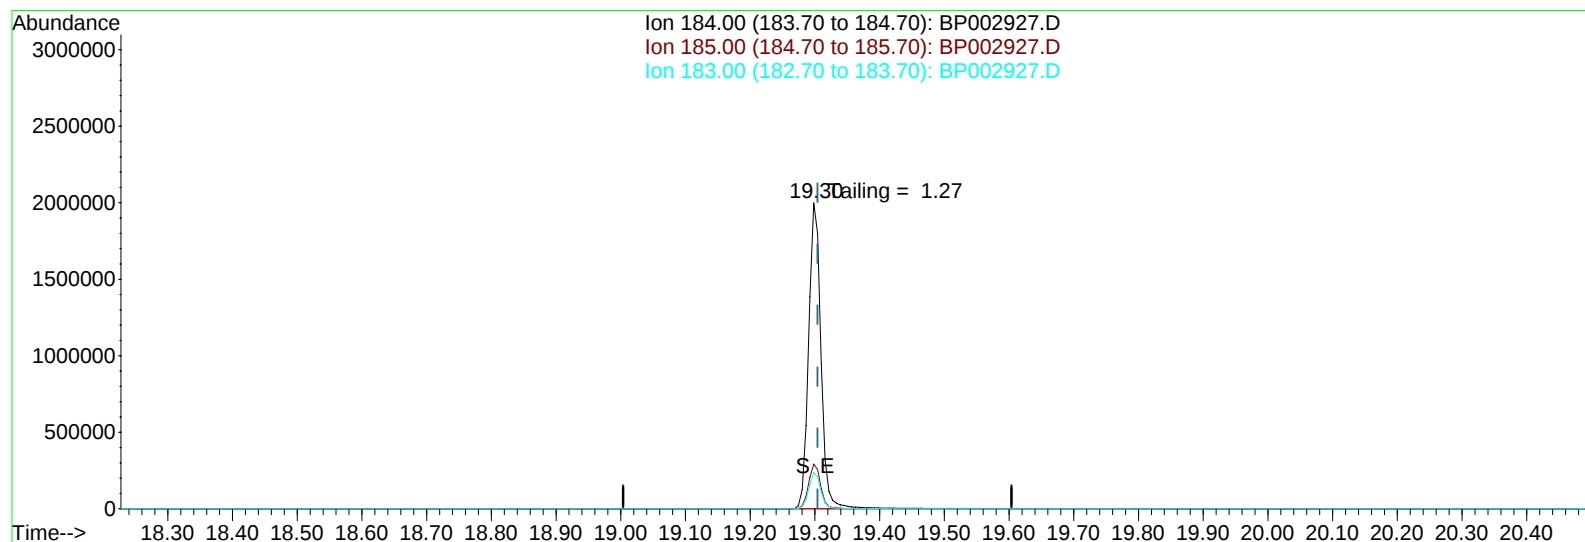

(77) Benzidine

19.298min (-0.006) 32410.14ng

response 2654573

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.59
183.00	11.60	11.83
0.00	0.00	0.00