


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080720\
 Data File : BP002927.D
 Acq On : 07 Aug 2020 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 15:30:34 2020

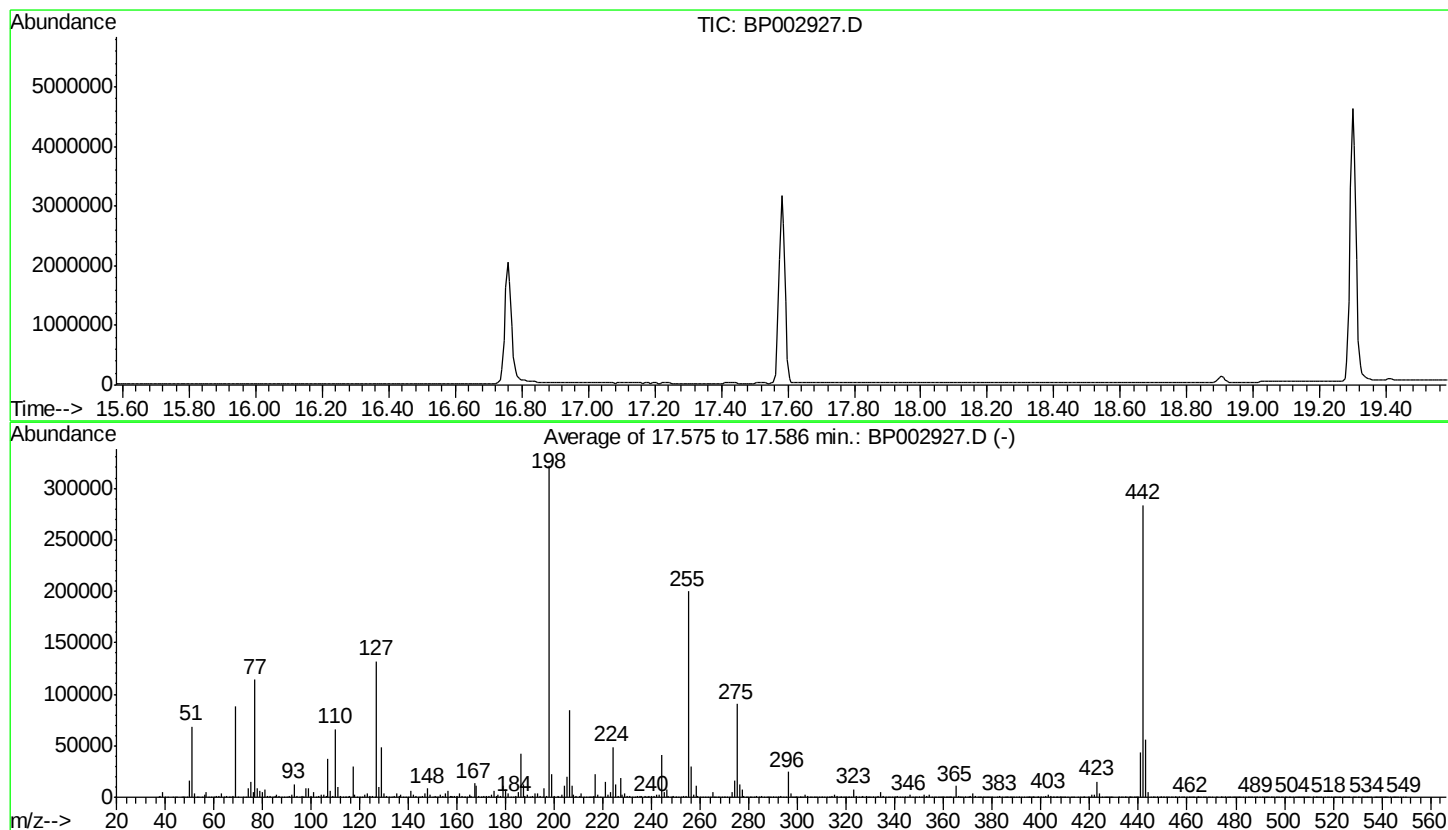

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	68581	PASS
68	69	0.00	2	1.9	1690	PASS
69	198	0.00	100	27.3	87776	PASS
70	69	0.00	2	0.4	343	PASS
127	198	10	80	41.1	132350	PASS
197	198	0.00	2	0.5	1632	PASS
198	198	100	100	100.0	321839	PASS
199	198	5	9	6.9	22296	PASS
275	198	10	60	28.1	90570	PASS
365	198	1	100	3.3	10727	PASS
441	198	0.01	100	13.7	44042	PASS
442	198	50	100	88.2	283916	PASS
443	442	15	24	19.6	55760	PASS