

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006567.D
 Acq On : 07 Aug 2021 14:24
 Operator : CG/JU
 Sample : M3163-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ6

Quant Time: Aug 07 17:40:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	168285	20.000	ng/ul	0.00
20) Naphthalene-d8	10.534	136	716735	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.381	164	397312	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	778388	20.000	ng/ul	0.00
79) Chrysene-d12	21.227	240	754871	20.000	ng/ul	0.00
88) Perylene-d12	23.557	264	797675	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	37427	8.302	ng/uL	0.00
4) Pyridine-d5	3.681	84	523969	39.150	ng/ul	0.00
7) Phenol-d5	6.928	99	663574	41.985	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	437911	44.530	ng/ul	0.00
11) 2-Chlorophenol-d4	7.287	132	512960	43.685	ng/ul	0.00
15) 4-Methylphenol-d8	8.457	113	529131	42.572	ng/ul	0.00
21) Nitrobenzene-d5	8.904	128	263902	49.450	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	261500	51.318	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.157	165	421653	42.226	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	657218	39.978	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1368496	48.395	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	1705707	49.097	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	214113	38.134	ng/ul	0.00
60) Fluorene-d10	15.375	176	1129063	47.496	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	152921	35.241	ng/ul	0.00
73) Anthracene-d10	17.233	188	1711354	48.704	ng/ul	0.00
81) Pyrene-d10	19.474	212	1874378	48.276	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.409	264	1906674	47.037	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.952	94	17316	1.072	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006567.D
Acq On : 07 Aug 2021 14:24
Operator : CG/JU
Sample : M3163-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ6

Quant Time: Aug 07 17:40:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

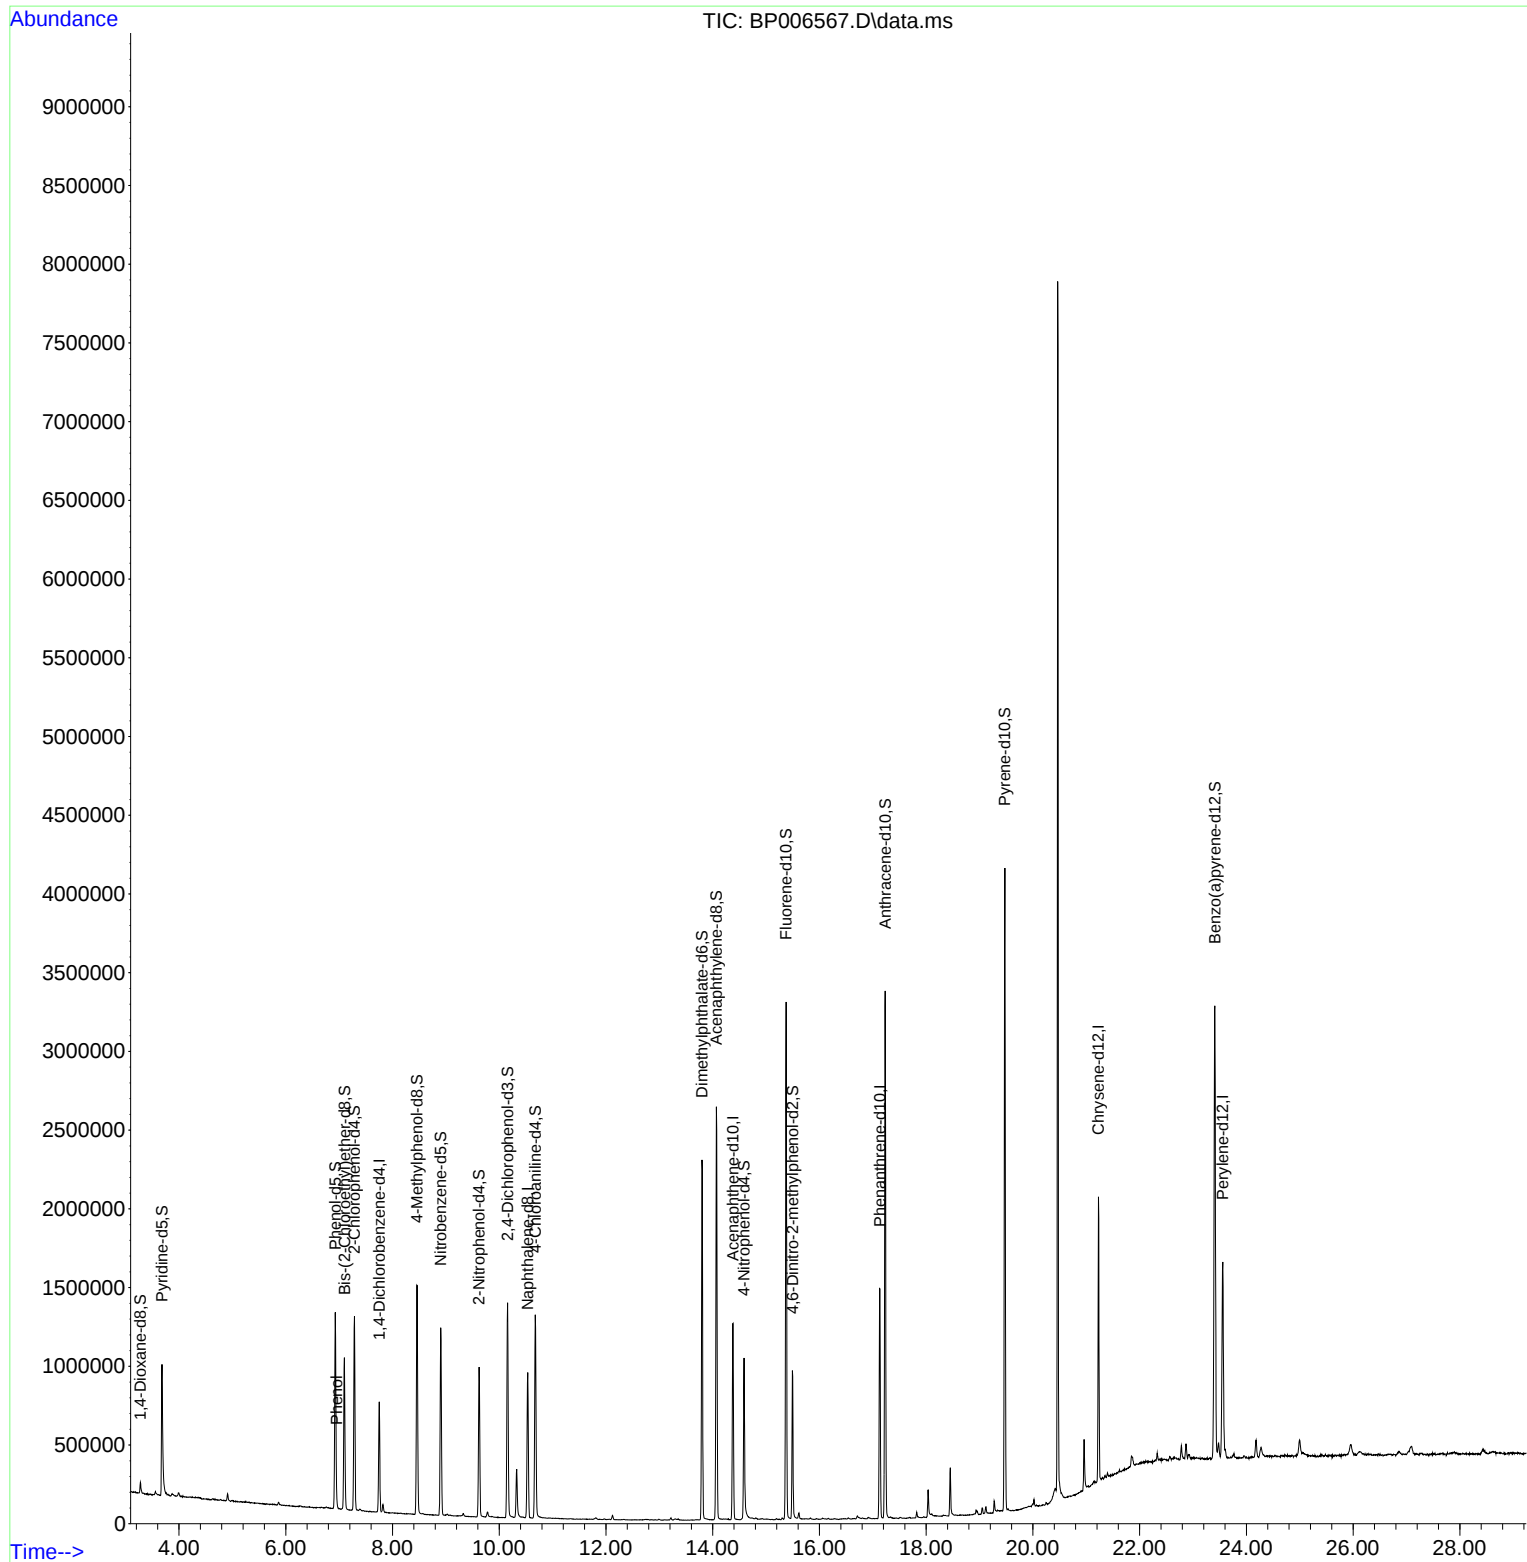

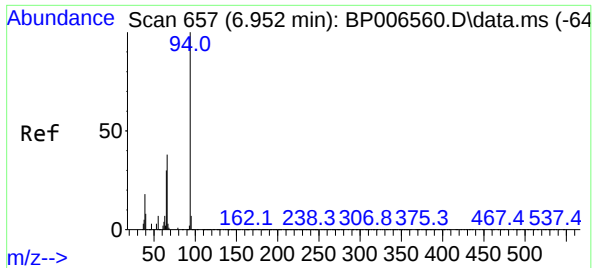

#8
Phenol
Concen: 1.072 ng/ul
RT: 6.952 min Scan# 657
Delta R.T. -0.000 min
Lab File: BP006567.D
Acq: 07 Aug 2021 14:24

Instrument :
BNA_P
ClientSampleId :
BGEZ6

Tgt Ion: 94 Resp: 17316
Ion Ratio Lower Upper
94 100
65 36.7 23.8 35.8#
66 55.9 30.9 46.3#

