

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006568.D
 Acq On : 07 Aug 2021 14:58
 Operator : CG/JU
 Sample : M3163-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEY4

Quant Time: Aug 07 17:44:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	166008	20.000	ng/u1	0.00
20) Naphthalene-d8	10.534	136	697465	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.381	164	396144	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.133	188	790766	20.000	ng/u1	0.00
79) Chrysene-d12	21.227	240	822051	20.000	ng/u1	0.00
88) Perylene-d12	23.557	264	895904	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	19857	4.465	ng/uL	0.00
4) Pyridine-d5	3.681	84	194708	14.748	ng/u1	0.00
7) Phenol-d5	6.928	99	324174	20.792	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	233763	24.097	ng/u1	0.00
11) 2-Chlorophenol-d4	7.287	132	265706	22.939	ng/u1	0.00
15) 4-Methylphenol-d8	8.457	113	226336	18.460	ng/u1	0.00
21) Nitrobenzene-d5	8.904	128	133815	25.767	ng/u1	0.00
24) 2-Nitrophenol-d4	9.622	143	132002	26.620	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.157	165	197972	20.374	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	320140	20.012	ng/u1	0.00
46) Dimethylphthalate-d6	13.798	166	724990	25.714	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	847258	24.459	ng/u1	0.00
54) 4-Nitrophenol-d4	14.592	143	86664	15.481	ng/u1	0.00
60) Fluorene-d10	15.375	176	594226	25.071	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	65467	14.851	ng/u1	0.00
73) Anthracene-d10	17.227	188	914597	25.622	ng/u1	0.00
81) Pyrene-d10	19.474	212	1059110	25.049	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.404	264	1030555	22.636	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.952	94	22065	1.384	ng/u1#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006568.D
Acq On : 07 Aug 2021 14:58
Operator : CG/JU
Sample : M3163-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEY4

Quant Time: Aug 07 17:44:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

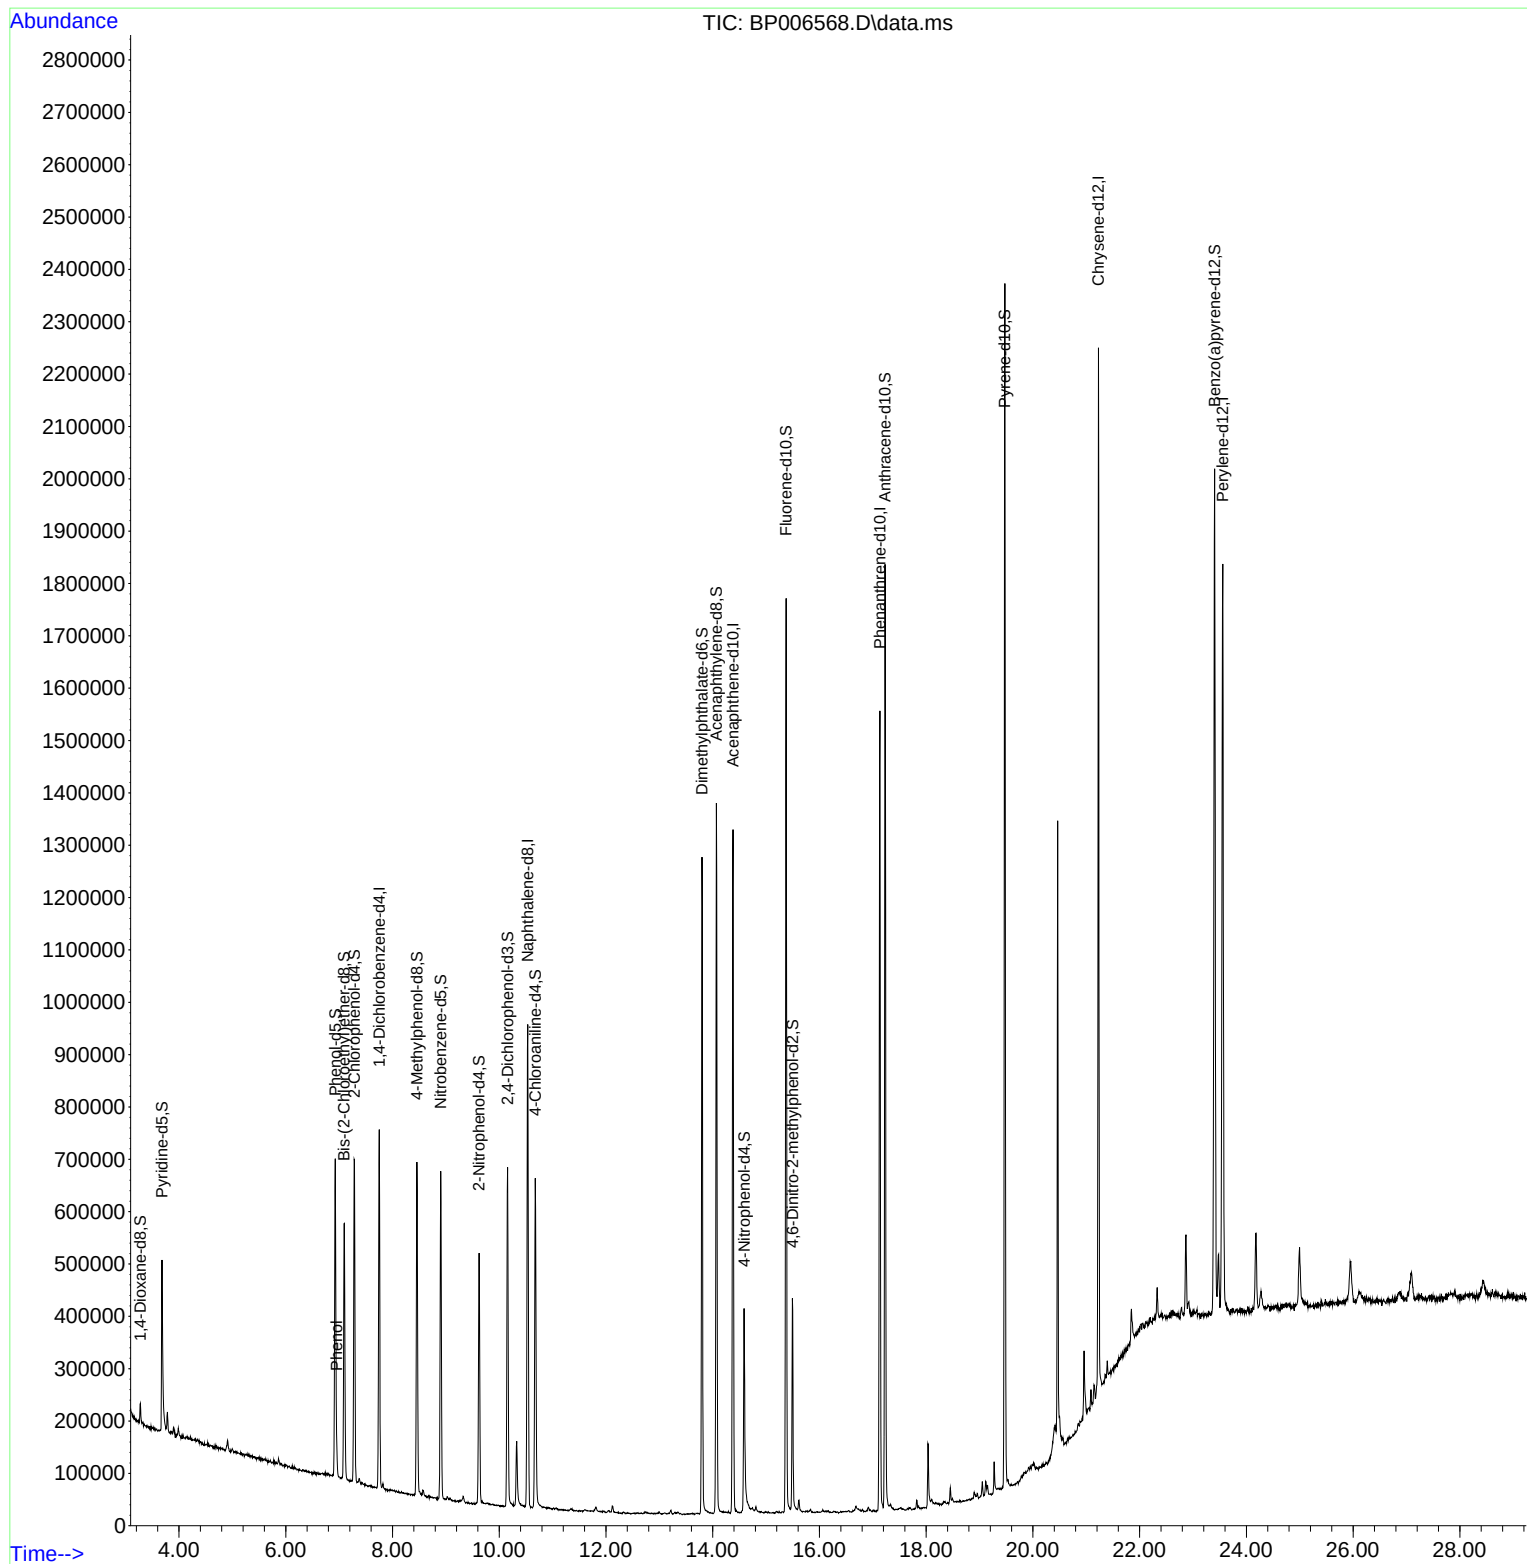

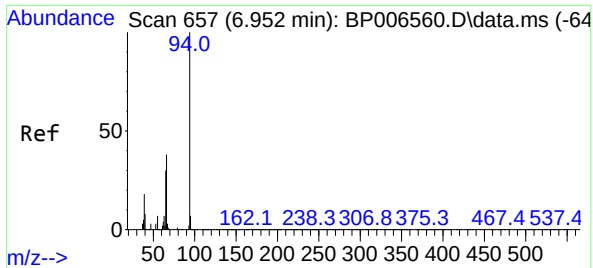

#8
Phenol
Concen: 1.384 ng/ul
RT: 6.952 min Scan# 657
Delta R.T. -0.000 min
Lab File: BP006568.D
Acq: 07 Aug 2021 14:58

Instrument :
BNA_P
ClientSampleId :
BGEY4

Tgt Ion: 94 Resp: 22065
Ion Ratio Lower Upper
94 100
65 31.0 23.8 35.8
66 49.0 30.9 46.3#

