

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006572.D
 Acq On : 07 Aug 2021 17:15
 Operator : CG/JU
 Sample : M3163-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ1

Quant Time: Aug 08 02:35:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	164680	20.000	ng/ul	0.00
20) Naphthalene-d8	10.534	136	706910	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.380	164	395461	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	778997	20.000	ng/ul	0.00
79) Chrysene-d12	21.227	240	755633	20.000	ng/ul	0.00
88) Perylene-d12	23.556	264	796214	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	31873	7.225	ng/uL	0.00
4) Pyridine-d5	3.681	84	461820	35.261	ng/ul	0.00
7) Phenol-d5	6.928	99	586147	37.898	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	374422	38.907	ng/ul	0.00
11) 2-Chlorophenol-d4	7.287	132	441603	38.431	ng/ul	0.00
15) 4-Methylphenol-d8	8.457	113	473576	38.936	ng/ul	0.00
21) Nitrobenzene-d5	8.904	128	226480	43.027	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	230705	45.904	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.157	165	376425	38.221	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	603010	37.191	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	1201317	42.682	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	1507179	43.586	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	197315	35.307	ng/ul	0.00
60) Fluorene-d10	15.374	176	995260	42.063	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	136812	31.504	ng/ul	0.00
73) Anthracene-d10	17.233	188	1524561	43.354	ng/ul	0.00
81) Pyrene-d10	19.474	212	1653948	42.555	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.403	264	1676659	41.438	ng/ul	0.00


Target Compounds					Qvalue	
8) Phenol	6.951	94	18634	1.179	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006572.D
Acq On : 07 Aug 2021 17:15
Operator : CG/JU
Sample : M3163-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ1

Quant Time: Aug 08 02:35:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

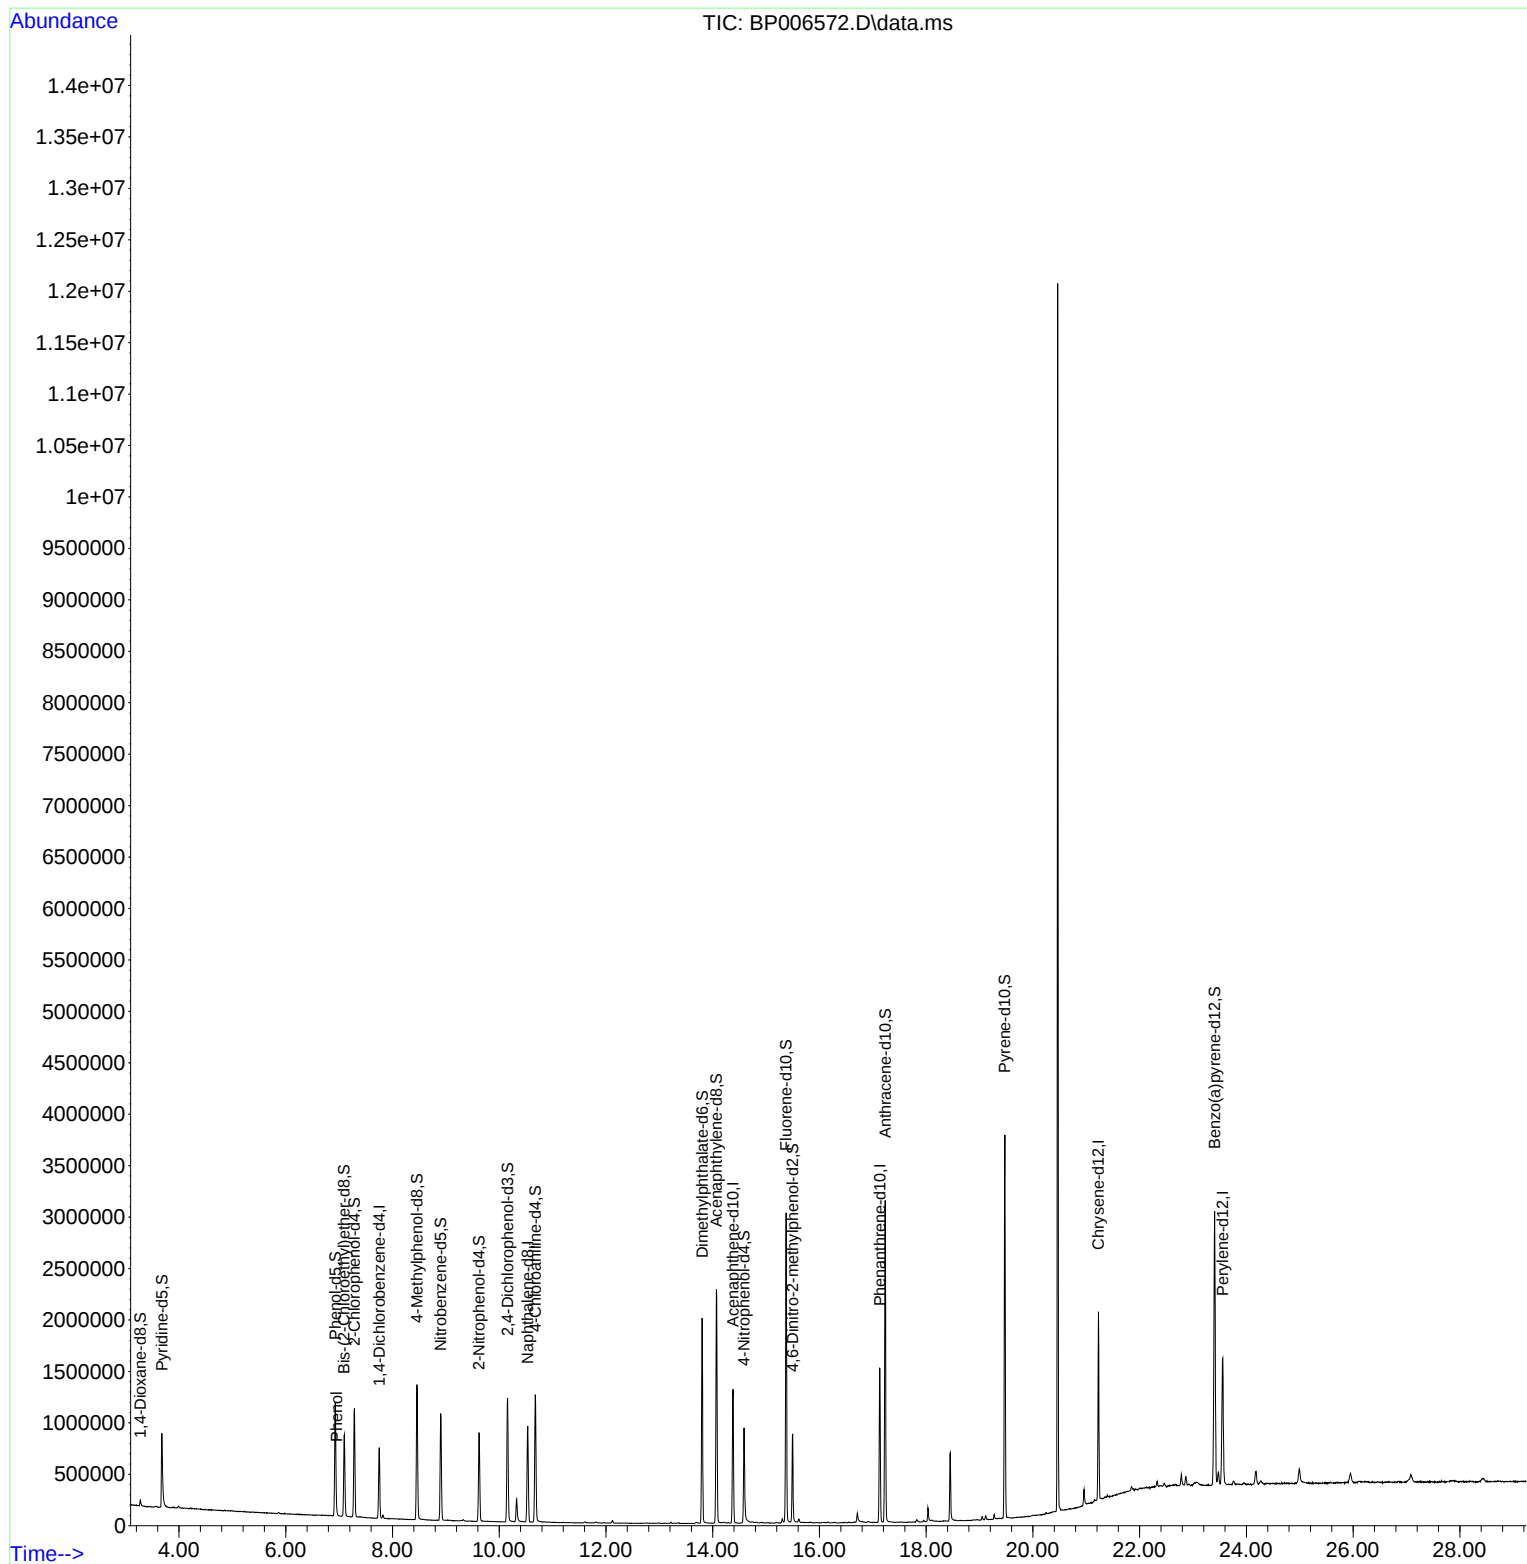

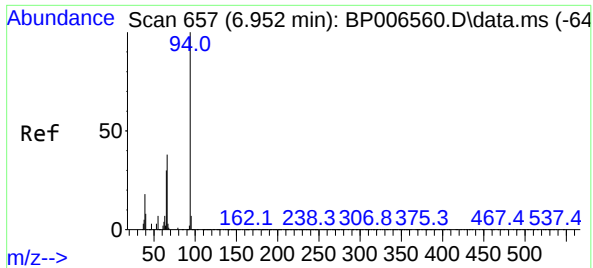

#8
Phenol
Concen: 1.179 ng/ul
RT: 6.951 min Scan# 657
Delta R.T. -0.000 min
Lab File: BP006572.D
Acq: 07 Aug 2021 17:15

Instrument :
BNA_P
ClientSampleId :
BGEZ1

Tgt Ion: 94 Resp: 18634

Ion	Ratio	Lower	Upper
94	100		
65	37.4	23.8	35.8#
66	55.2	30.9	46.3#

